

Data Path : Z:\HPCHEM1\HPLC\_L\Data\HL120314\  
 Data File : HL005873.D  
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
 Acq On : 03-Dec-2014, 16:35  
 Operator : TP  
 Sample : HSTDICC020  
 Misc :  
 ALS Vial : 67 Sample Multiplier: 1

Instrument :  
 HPLC\_L  
 ClientSampleId :  
 HSTDICC020

Integration File signal 1: AUTOINT1.E  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 12 05:48:09 2015  
 Quant Method : Z:\HPCHEM1\HPLC\_L\METHODS\HL1203NG.M  
 Quant Title :  
 QLast Update : Mon Mar 09 13:45:27 2015  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 50 u1  
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

| Compound                    | R.T.  | Response | Conc Units  |
|-----------------------------|-------|----------|-------------|
| -----                       |       |          |             |
| System Monitoring Compounds |       |          |             |
| Target Compounds            |       |          |             |
| 2) T Nitroglycerin          | 7.540 | 1544     | 0.000 ng/u1 |
| -----                       |       |          |             |

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC\_L\Data\HL120314\  
Data File : H1005873.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 03-Dec-2014, 16:35  
Operator : TP  
Sample : HSTDICC020  
Misc :  
ALS Vial : 67 Sample Multiplier: 1

Instrument :  
HPLC\_L  
ClientSampleId :  
HSTDICC020

Integration File signal 1: AUTOINT1.E  
Integration File signal 2: autoint2.e  
Quant Time: Mar 12 05:48:09 2015  
Quant Method : Z:\HPCHEM1\HPLC\_L\METHODS\HL1203NG.M  
Quant Title :  
QLast Update : Mon Mar 09 13:45:27 2015  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

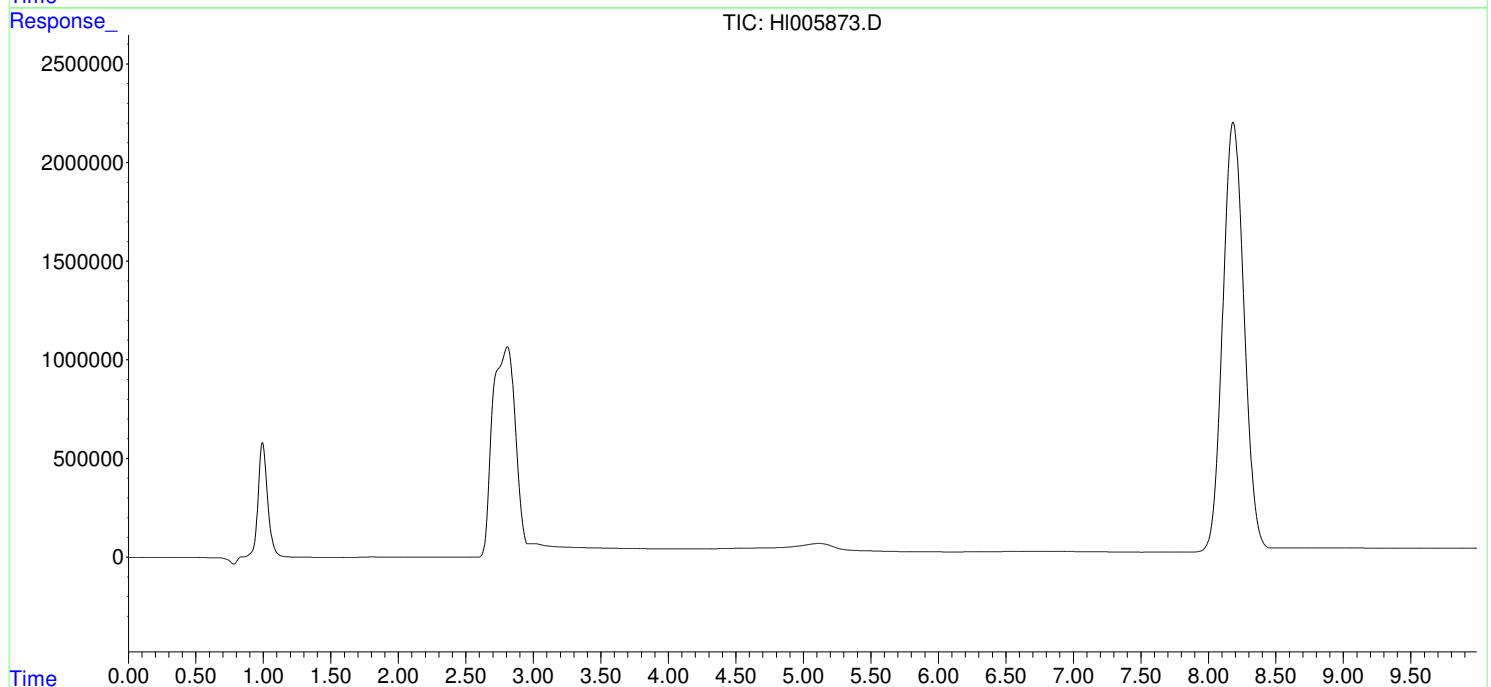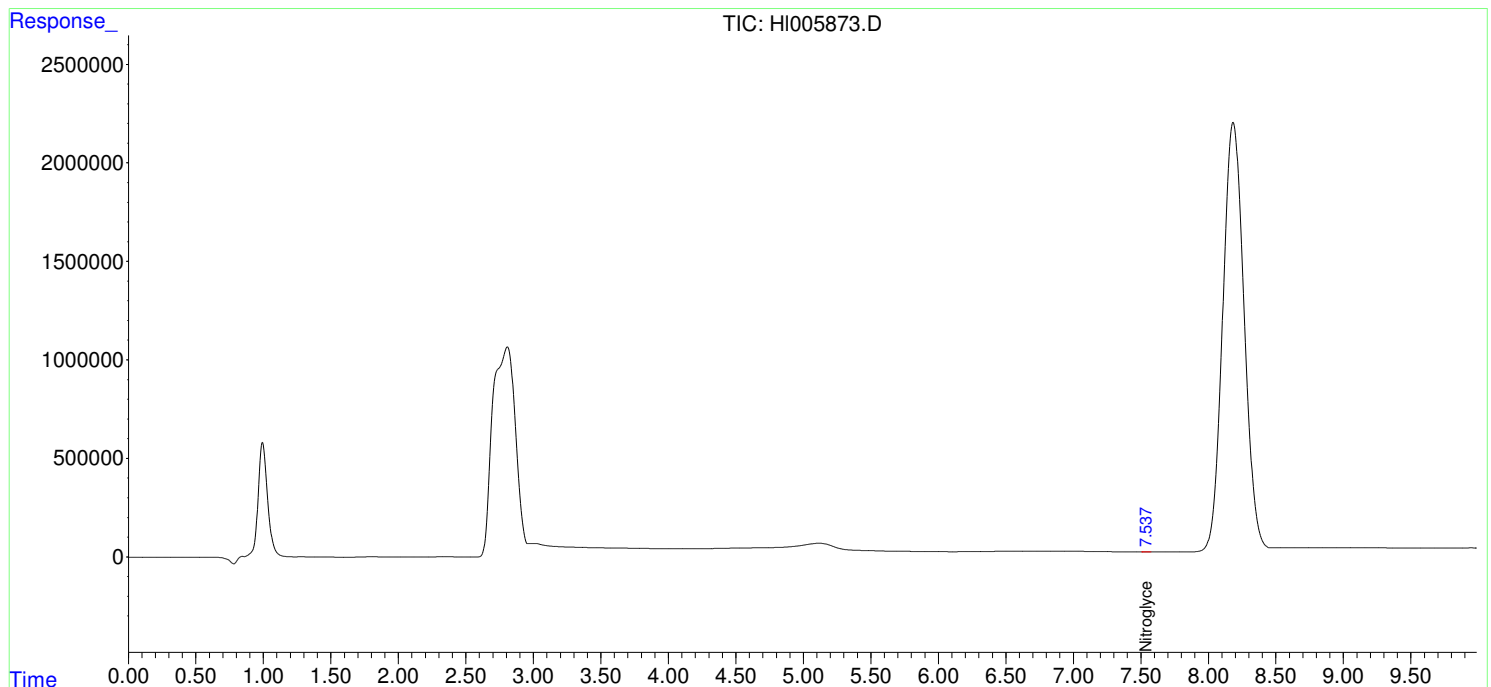


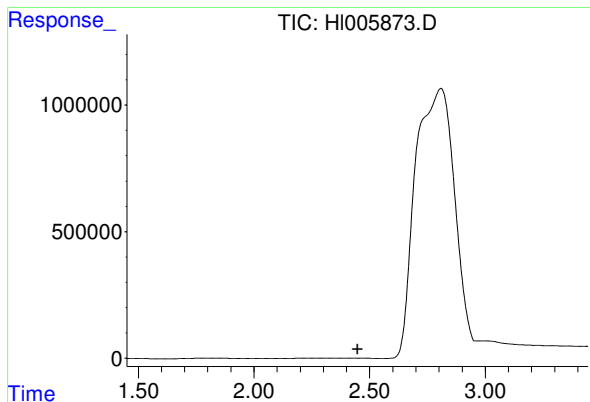

#1 4-Nitroaniline

R.T.: 0.000 min  
Exp R.T.: 2.448 min  
Response: 0  
Conc: N.D.

Instrument :  
HPLC\_L  
ClientSampleId :  
HSTDICC020

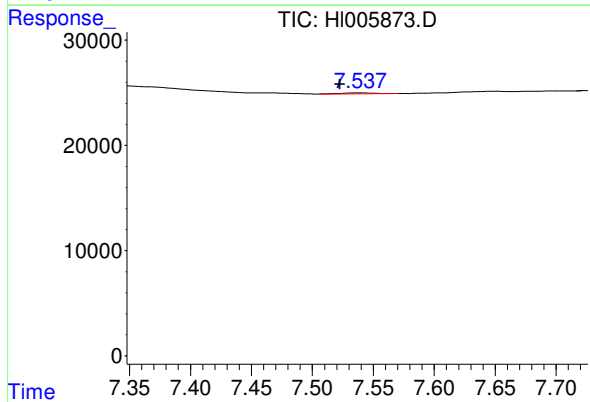

#2 Nitroglycerin

R.T.: 7.540 min  
Delta R.T.: 0.018 min  
Response: 1544  
Conc: 0.00 ng/u1