

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120314\
 Data File : HL005881.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 03-Dec-2014, 18:06
 Operator : TP
 Sample : HSTDICC5000
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 HSTDICC5000

Integration File signal 1: AUTOINT1.E
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 05:54:18 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120314.M
 Quant Title :
 QLast Update : Wed Mar 11 16:43:35 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.518	68070416	4787.309 ug/L
Target Compounds			
2) T HMX	1.463	29265752	4697.404 ug/L
3) T RDX	2.518	68070416	4787.309 ug/L
4) T 1,3,5-Trinitrobenzene	4.101	77076904	4588.638 ug/L
5) T 1,3-Dinitrobenzene	5.395	116151753	4777.811 ng/ml
6) T 3,5-Dinitroaniline	6.195	72073125	3821.522 ug/L
7) T Nitrobenzene	6.959	62012404	4283.099 ug/L
8) T Tetryl	9.275	49777644	4359.263 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120314\
Data File : H1005881.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 03-Dec-2014, 18:06
Operator : TP
Sample : HSTDICC5000
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HSTDICC5000

Integration File signal 1: AUTOINT1.E
Integration File signal 2: autoint2.e
Quant Time: Mar 12 05:54:18 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120314.M
Quant Title :
QLast Update : Wed Mar 11 16:43:35 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

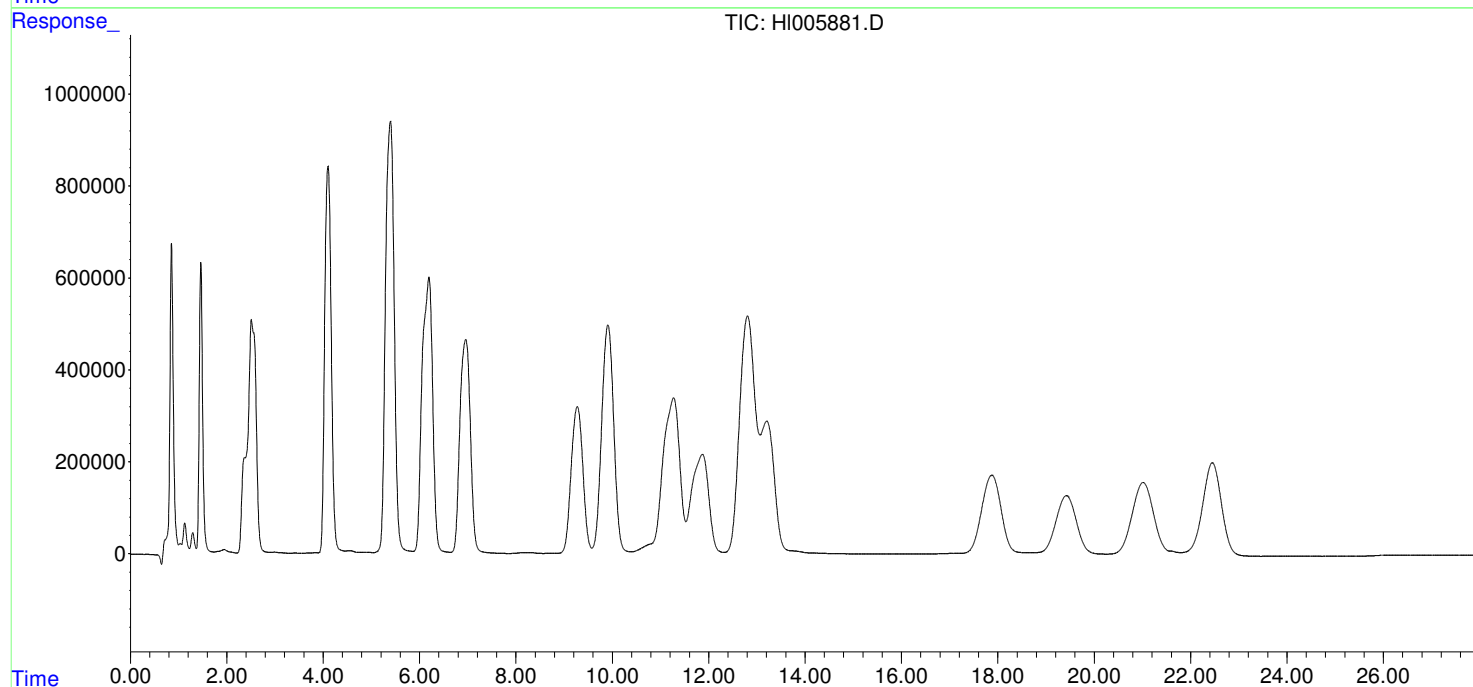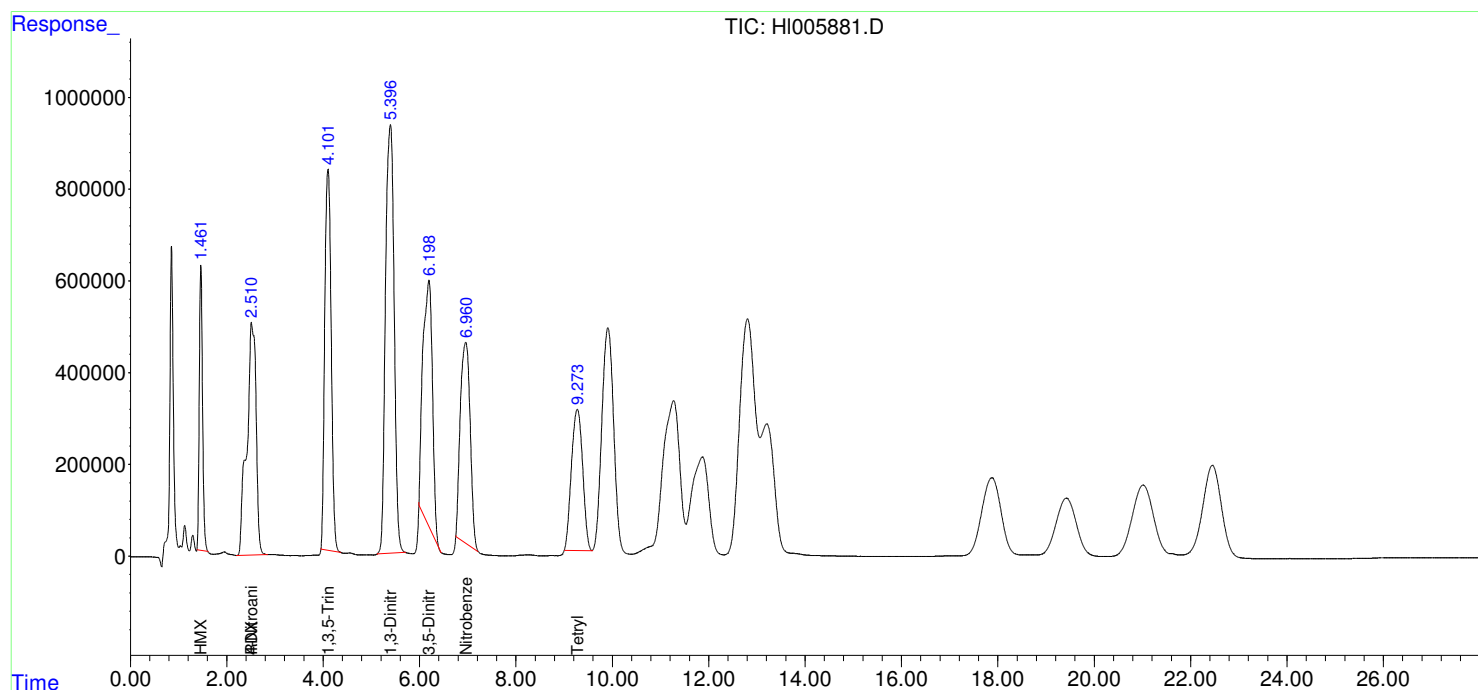


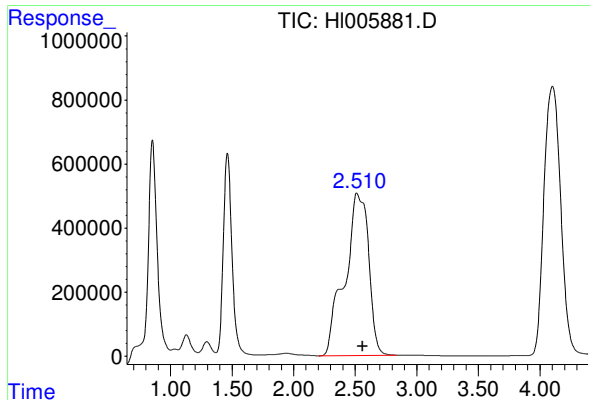

#1 4-Nitroaniline


R.T.: 2.518 min
Delta R.T.: -0.042 min
Response: 68070416
Conc: 4787.31 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC5000

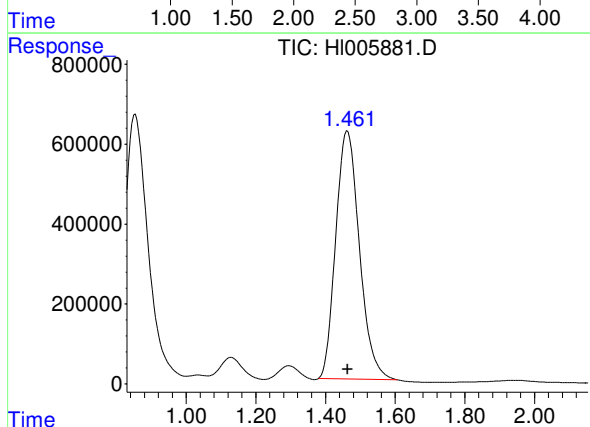


#2 HMX

R.T.: 1.463 min
Delta R.T.: 0.000 min
Response: 29265752
Conc: 4697.40 ug/L

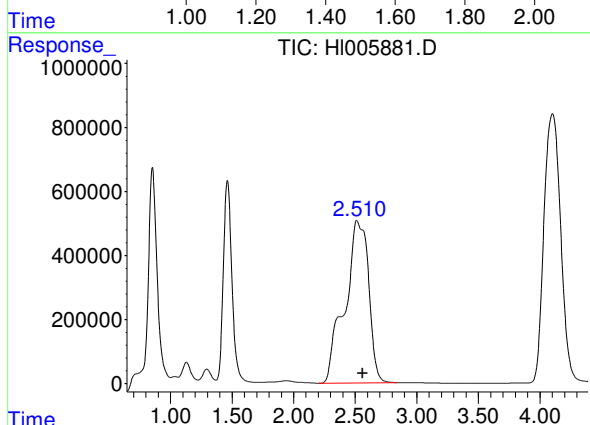


#3 RDX

R.T.: 2.518 min
Delta R.T.: -0.042 min
Response: 68070416
Conc: 4787.31 ug/L

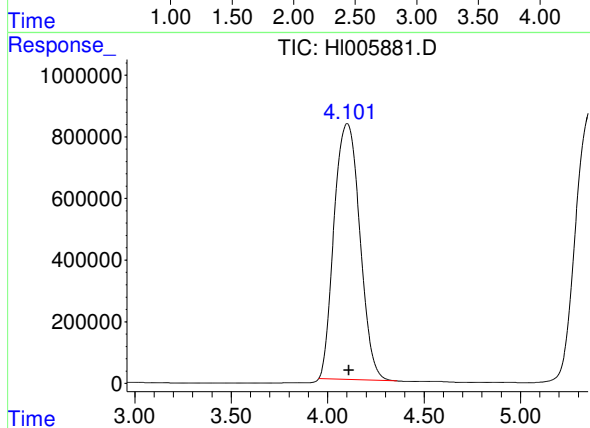

#4 1,3,5-Trinitrobenzene


R.T.: 4.101 min
Delta R.T.: -0.007 min
Response: 77076904
Conc: 4588.64 ug/L

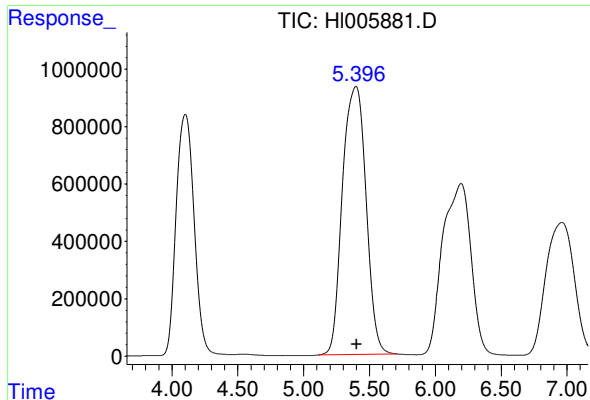

#5 1,3-Dinitrobenzene


R.T.: 5.395 min
Delta R.T.: -0.005 min
Response: 116151753
Conc: 4777.81 ng/ml

Instrument :
HPLC_L
ClientSampleId :
HSTDICC5000

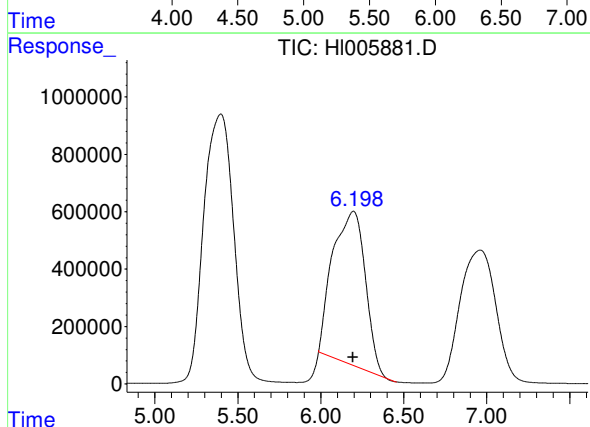


#6 3,5-Dinitroaniline

R.T.: 6.195 min
Delta R.T.: 0.001 min
Response: 72073125
Conc: 3821.52 ug/L

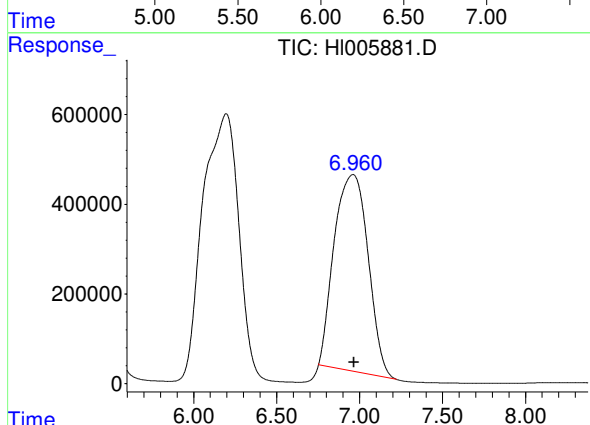

#7 Nitrobenzene

R.T.: 6.959 min
Delta R.T.: -0.007 min
Response: 62012404
Conc: 4283.10 ug/L

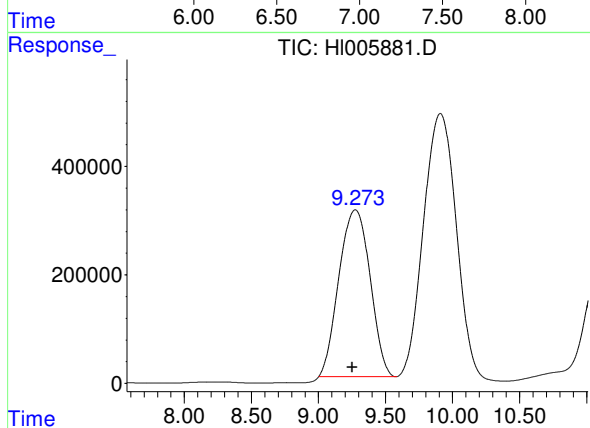

#8 Tetryl

R.T.: 9.275 min
Delta R.T.: 0.023 min
Response: 49777644
Conc: 4359.26 ug/L