

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120314\
 Data File : H1005882.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 03-Dec-2014, 18:35
 Operator : TP
 Sample : HSTDICC2000
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 HSTDICC2000

Integration File signal 1: AUTOINT1.E
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 05:54:22 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120314.M
 Quant Title :
 QLast Update : Wed Mar 11 16:43:35 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.551	27235945	1915.471 ug/L
Target Compounds			
2) T HMX	1.463	11777979	1890.467 ug/L
3) T RDX	2.551	27235945	1915.471 ug/L
4) T 1,3,5-Trinitrobenzene	4.102	31633117	1883.222 ug/L
5) T 1,3-Dinitrobenzene	5.394	46685087	1920.354 ng/ml
6) T 3,5-Dinitroaniline	6.186	34594575	1834.302 ug/L
7) T Nitrobenzene	7.018	27122521	1873.310 ug/L
13) T 2,6-Dinitrotoluene	12.853	24245560	2013.567 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120314\
Data File : H1005882.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 03-Dec-2014, 18:35
Operator : TP
Sample : HSTDICC2000
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HSTDICC2000

Integration File signal 1: AUTOINT1.E
Integration File signal 2: autoint2.e
Quant Time: Mar 12 05:54:22 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120314.M
Quant Title :
QLast Update : Wed Mar 11 16:43:35 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

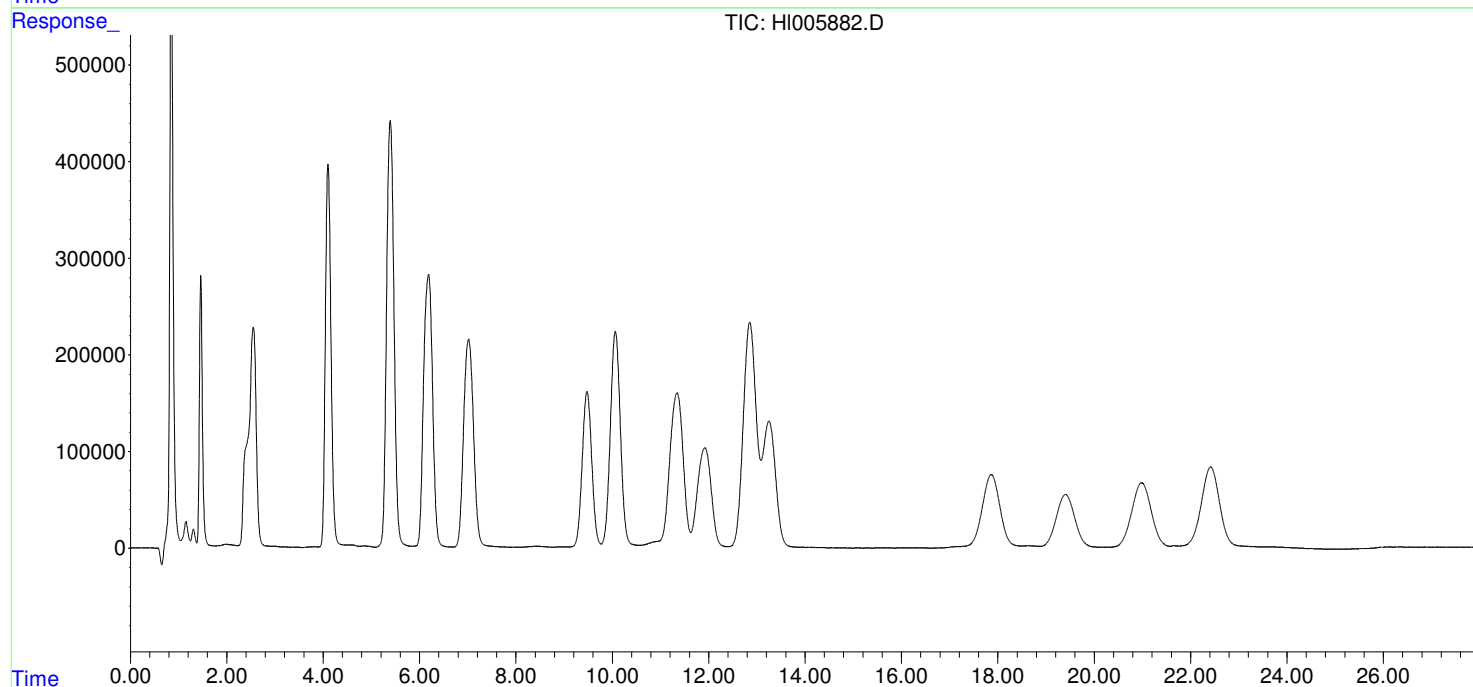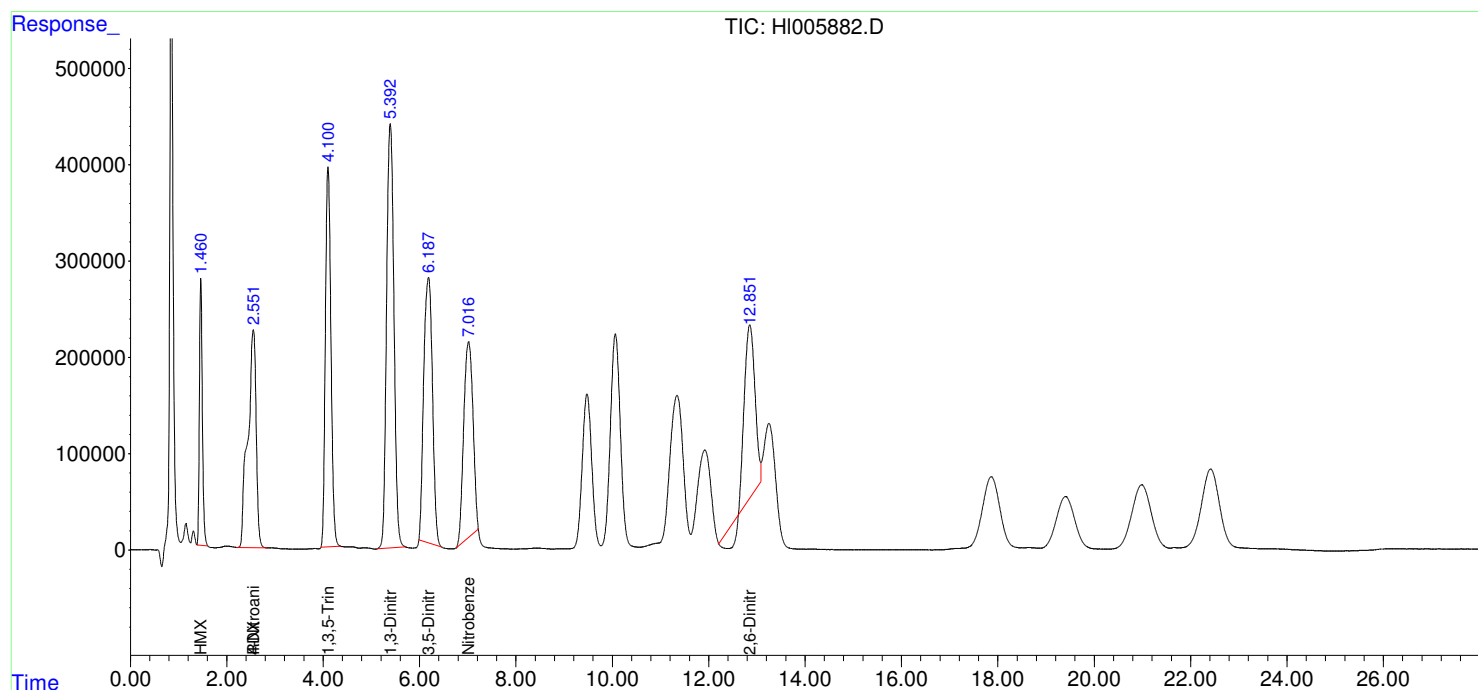


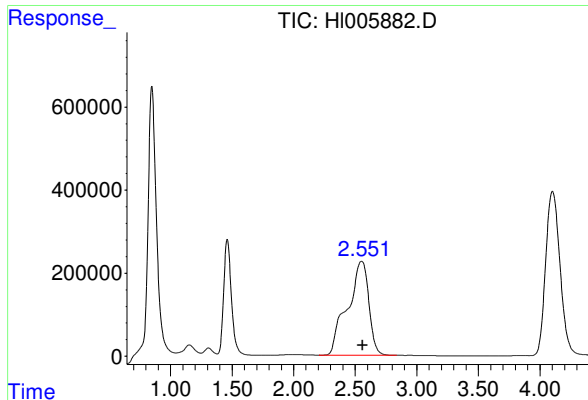

#1 4-Nitroaniline


R.T.: 2.551 min
Delta R.T.: -0.009 min
Response: 27235945
Conc: 1915.47 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC2000

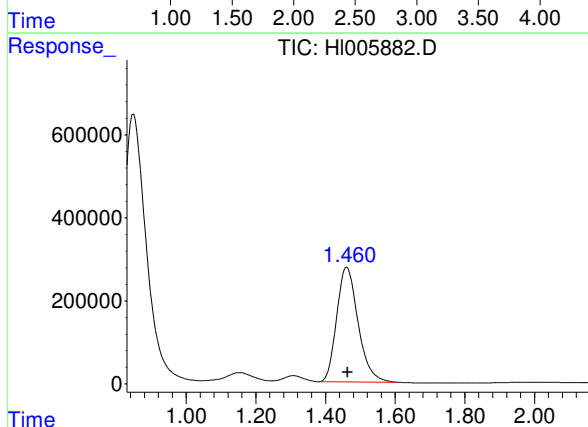


#2 HMX

R.T.: 1.463 min
Delta R.T.: 0.000 min
Response: 11777979
Conc: 1890.47 ug/L

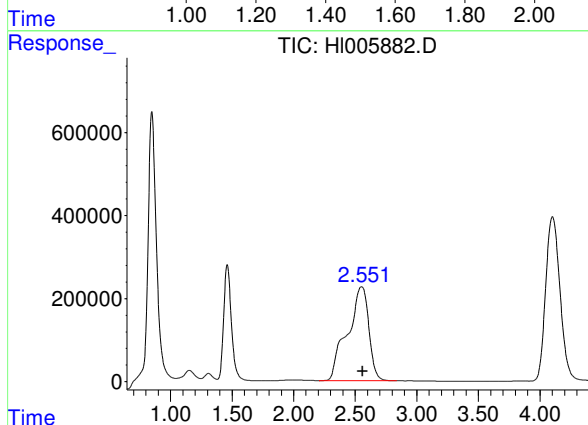


#3 RDX

R.T.: 2.551 min
Delta R.T.: -0.008 min
Response: 27235945
Conc: 1915.47 ug/L

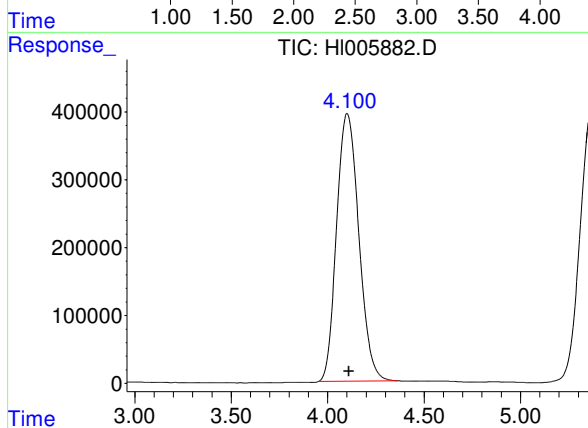

#4 1,3,5-Trinitrobenzene


R.T.: 4.102 min
Delta R.T.: -0.006 min
Response: 31633117
Conc: 1883.22 ug/L

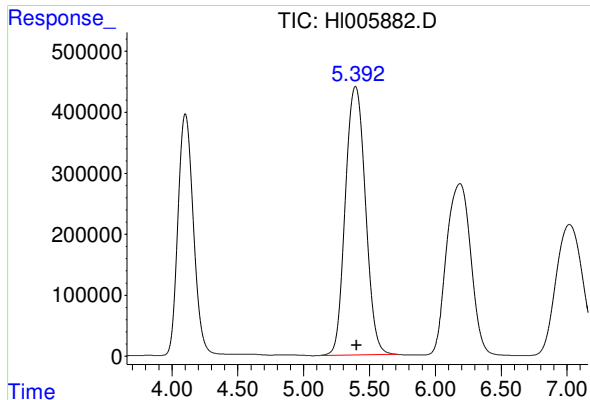

#5 1,3-Dinitrobenzene


R.T.: 5.394 min
Delta R.T.: -0.007 min
Response: 46685087
Conc: 1920.35 ng/ml

Instrument :
HPLC_L
ClientSampleId :
HSTDICC2000

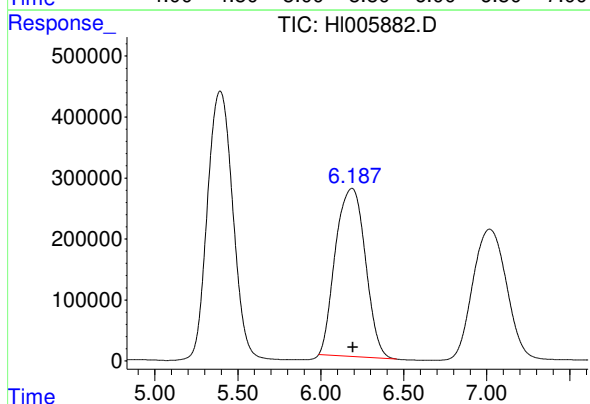


#6 3,5-Dinitroaniline

R.T.: 6.186 min
Delta R.T.: -0.007 min
Response: 34594575
Conc: 1834.30 ug/L

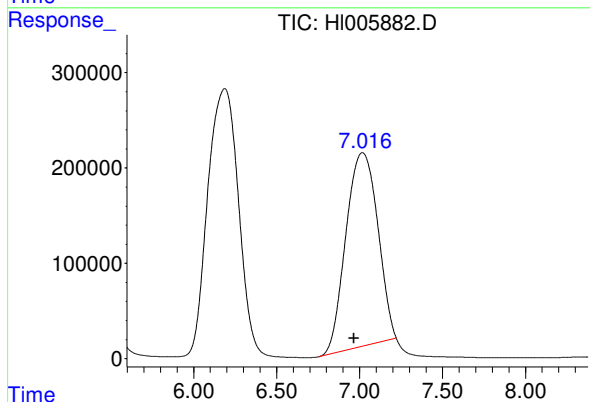

#7 Nitrobenzene

R.T.: 7.018 min
Delta R.T.: 0.052 min
Response: 27122521
Conc: 1873.31 ug/L

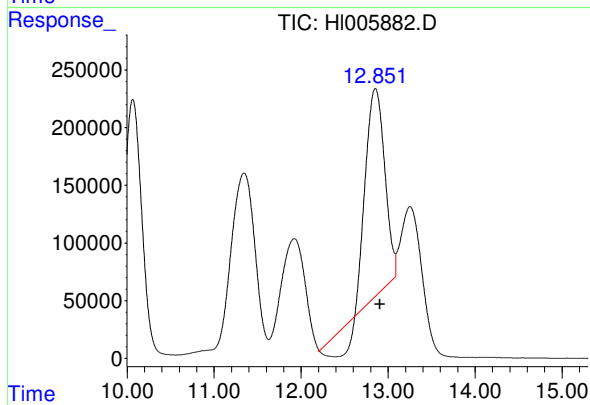

#13 2,6-Dinitrotoluene

R.T.: 12.853 min
Delta R.T.: -0.049 min
Response: 24245560
Conc: 2013.57 ug/L