

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120314\
 Data File : H1005883.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 03-Dec-2014, 19:05
 Operator : TP
 Sample : HSTDICC1000
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 HSTDICC1000

Integration File signal 1: AUTOINT1.E
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 05:54:26 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120314.M
 Quant Title :
 QLast Update : Wed Mar 11 16:43:35 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.563	14324503	1007.425 ug/L
Target Compounds			
2) T HMX	1.469	6197684	994.781 ug/L
3) T RDX	2.563	14324503	1007.425 ug/L
4) T 1,3,5-Trinitrobenzene	4.112	16801030	1000.220 ug/L
5) T 1,3-Dinitrobenzene	5.402	24557246	1010.143 ng/ml
6) T 3,5-Dinitroaniline	6.193	18568158	984.536 ug/L
7) T Nitrobenzene	6.969	13958855	964.116 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120314\
Data File : H1005883.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 03-Dec-2014, 19:05
Operator : TP
Sample : HSTDICC1000
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HSTDICC1000

Integration File signal 1: AUTOINT1.E
Integration File signal 2: autoint2.e
Quant Time: Mar 12 05:54:26 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120314.M
Quant Title :
QLast Update : Wed Mar 11 16:43:35 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

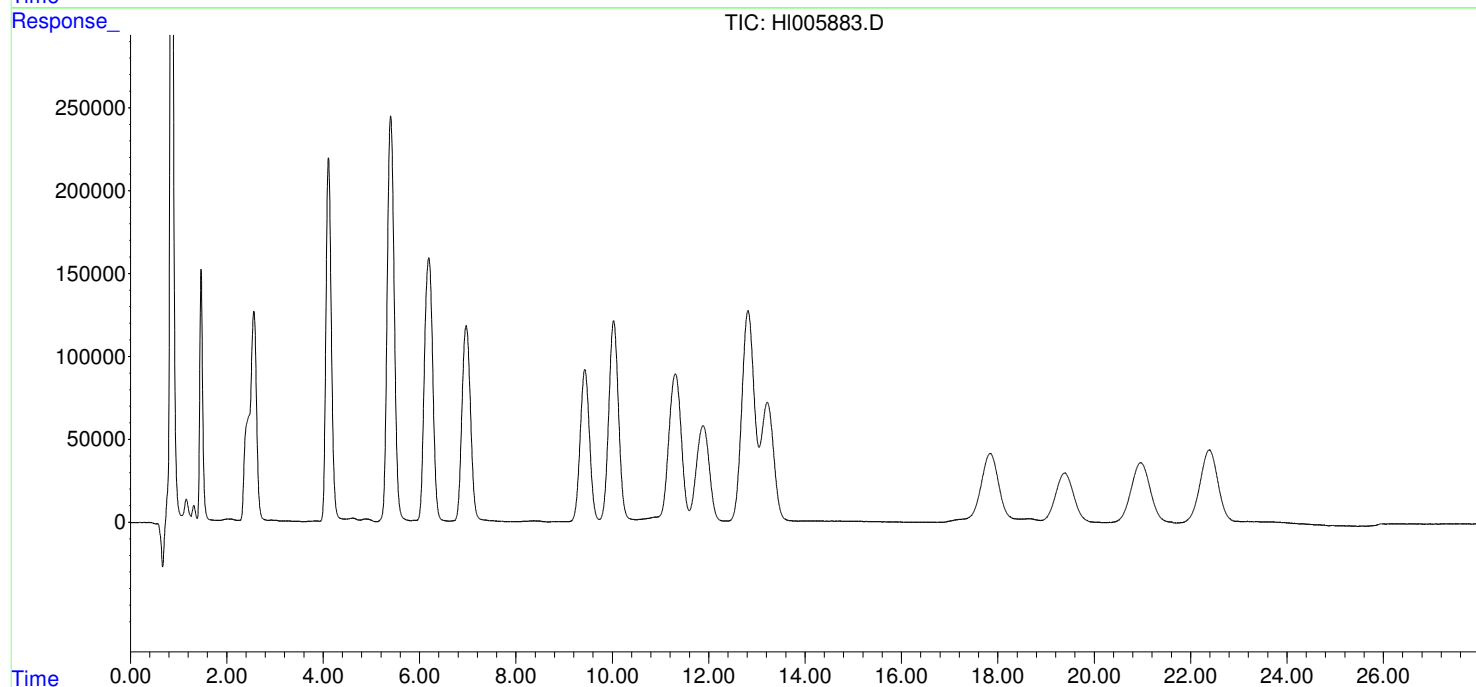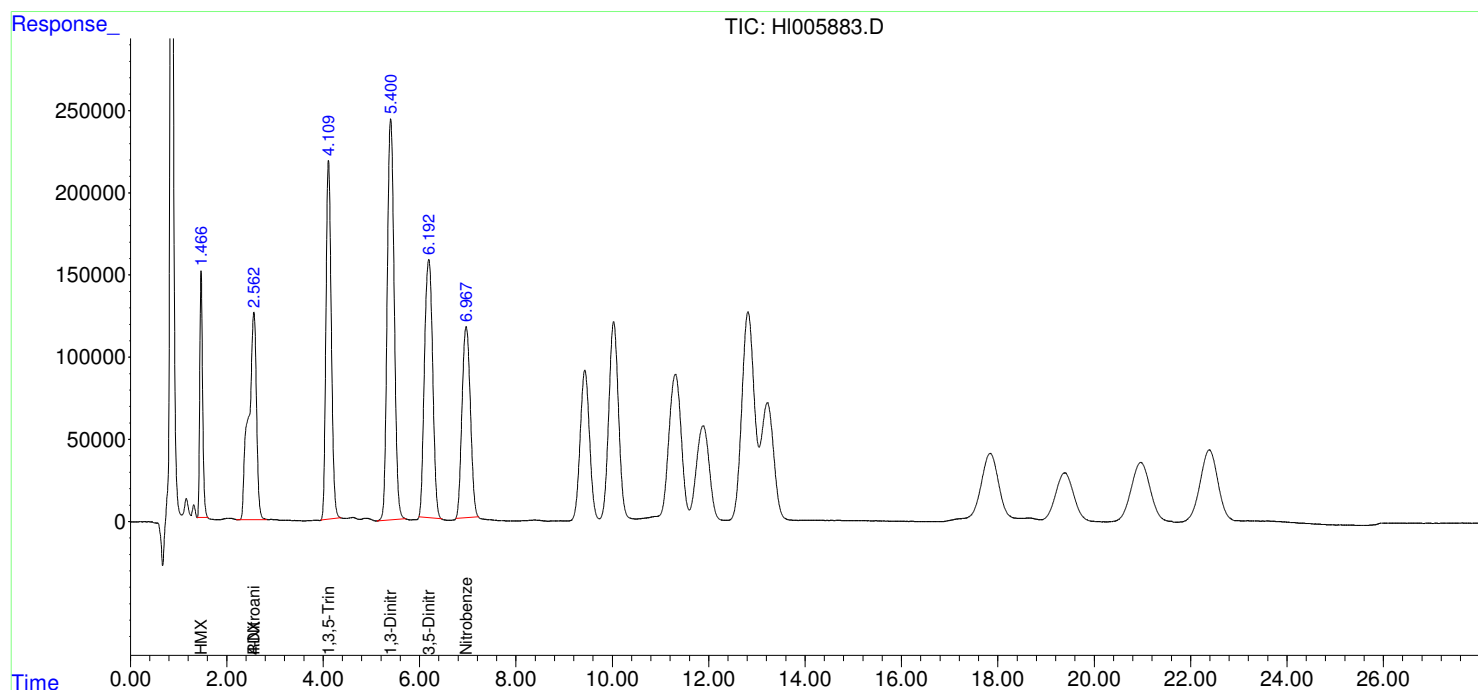


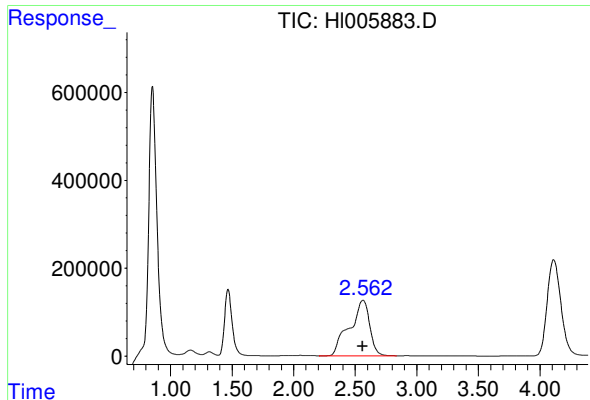

#1 4-Nitroaniline


R.T.: 2.563 min
Delta R.T.: 0.003 min
Response: 14324503
Conc: 1007.42 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC1000

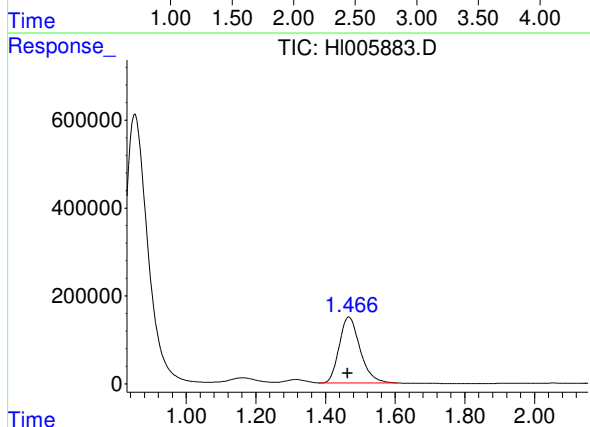


#2 HMX

R.T.: 1.469 min
Delta R.T.: 0.006 min
Response: 6197684
Conc: 994.78 ug/L

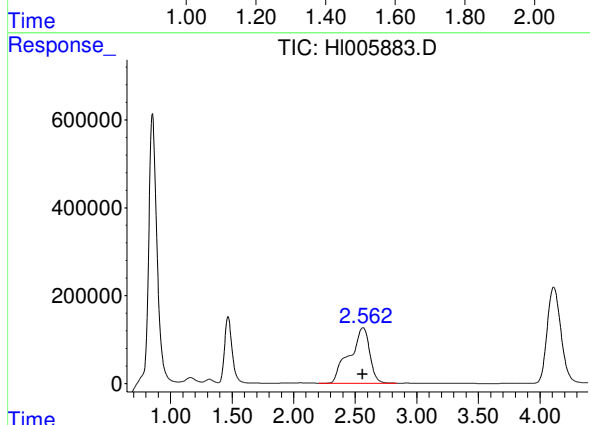


#3 RDX

R.T.: 2.563 min
Delta R.T.: 0.004 min
Response: 14324503
Conc: 1007.42 ug/L

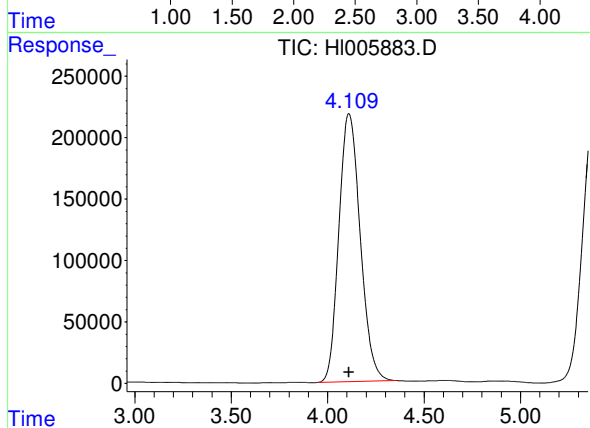

#4 1,3,5-Trinitrobenzene


R.T.: 4.112 min
Delta R.T.: 0.003 min
Response: 16801030
Conc: 1000.22 ug/L

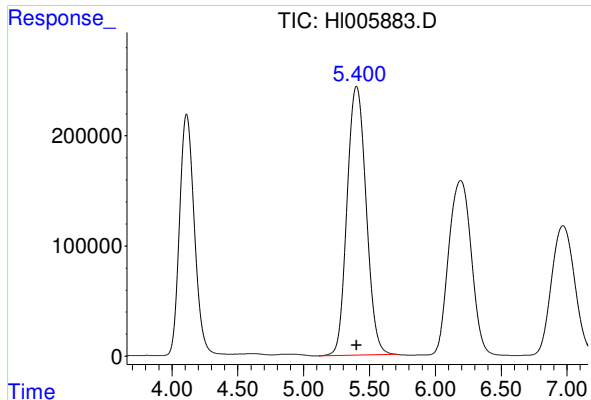

#5 1,3-Dinitrobenzene


R.T.: 5.402 min
Delta R.T.: 0.001 min
Response: 24557246
Conc: 1010.14 ng/ml

Instrument :
HPLC_L
ClientSampleId :
HSTDICC1000

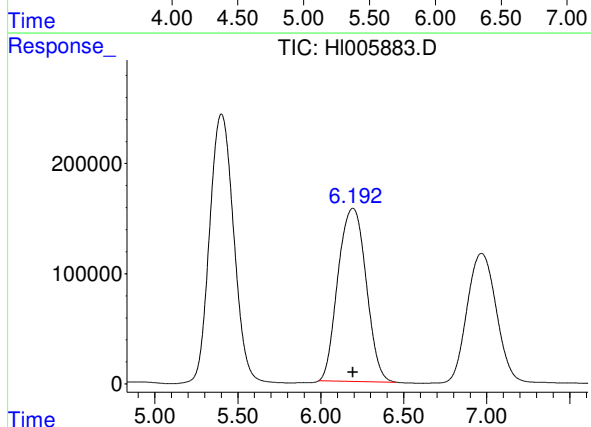

#6 3,5-Dinitroaniline

R.T.: 6.193 min
Delta R.T.: -0.001 min
Response: 18568158
Conc: 984.54 ug/L

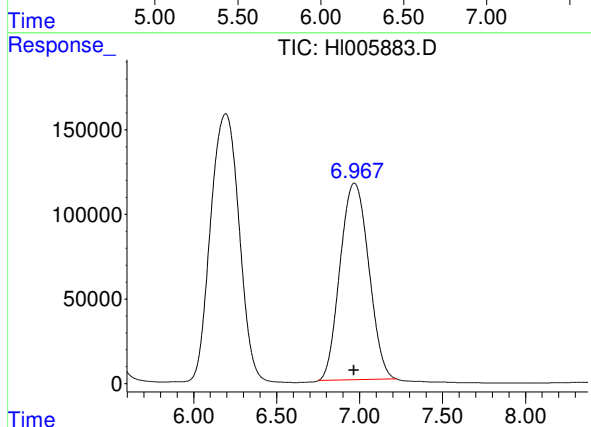

#7 Nitrobenzene

R.T.: 6.969 min
Delta R.T.: 0.003 min
Response: 13958855
Conc: 964.12 ug/L