

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120314\
 Data File : H1005890.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 03-Dec-2014, 22:30
 Operator : TP
 Sample : F4368-06
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 YS19-SB41-1014

Integration File signal 1: AUTOINT1.E
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 05:54:52 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120314.M
 Quant Title :
 QLast Update : Wed Mar 11 16:43:35 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.496	951565	66.922 ug/L
Target Compounds			
3) T RDX	2.496	951565	66.922 ug/L
4) T 1,3,5-Trinitrobenzene	4.164	786510	46.823 ug/L
10) T 2-Amino-4,6-dinitroto...	11.074	2690929	179.836 ug/L
11) T 4-Amino-2,6-dinitroto...	11.630	1659944	164.922 ug/L
12) T 2,4-Dinitrotoluene	12.546	309426	13.933 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120314\
Data File : H1005890.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 03-Dec-2014, 22:30
Operator : TP
Sample : F4368-06
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
YS19-SB41-1014

Integration File signal 1: AUTOINT1.E
Integration File signal 2: autoint2.e
Quant Time: Mar 12 05:54:52 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120314.M
Quant Title :
QLast Update : Wed Mar 11 16:43:35 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

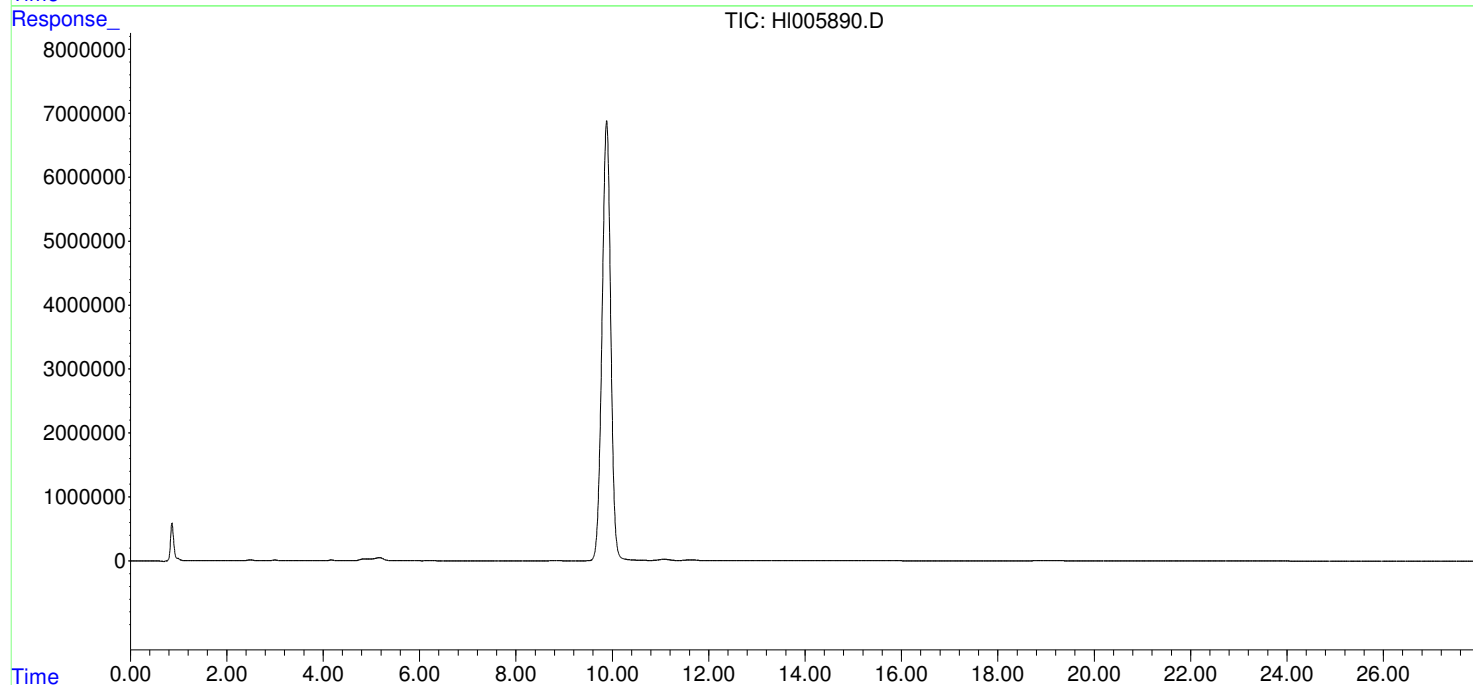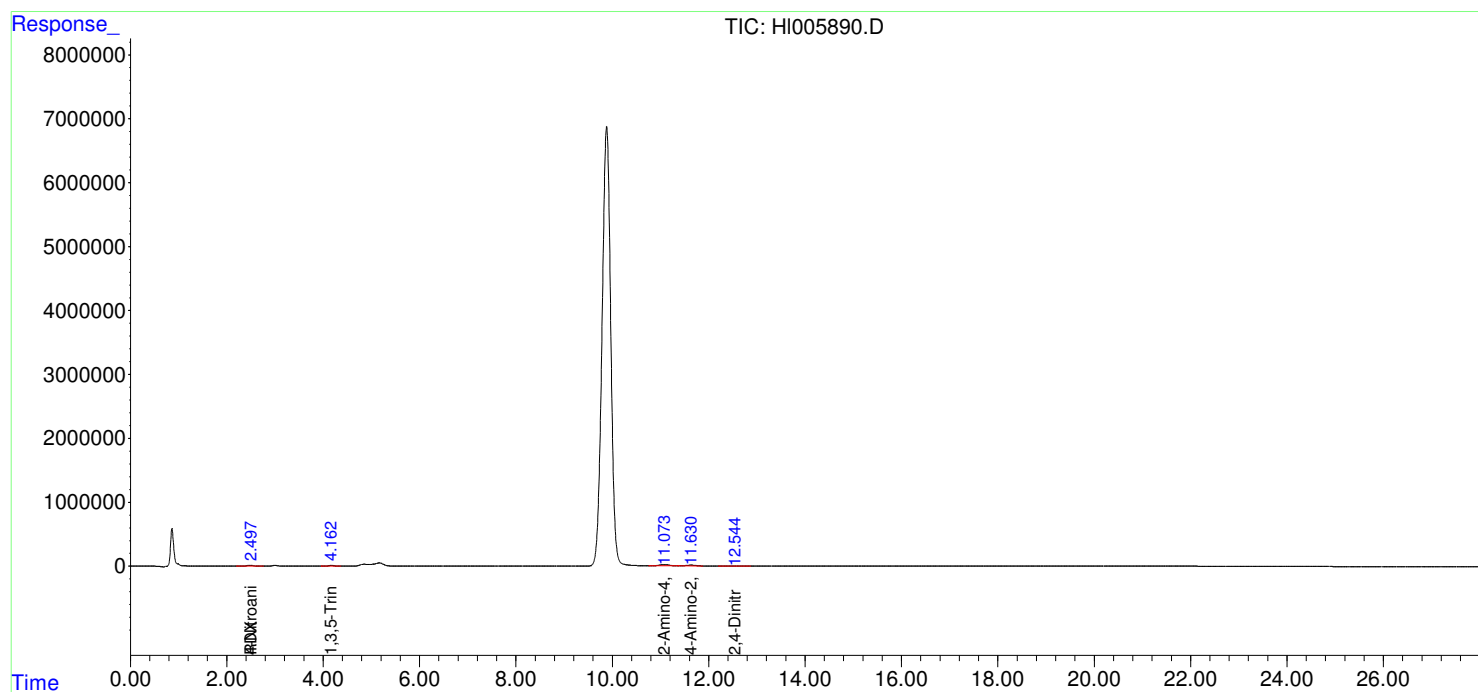


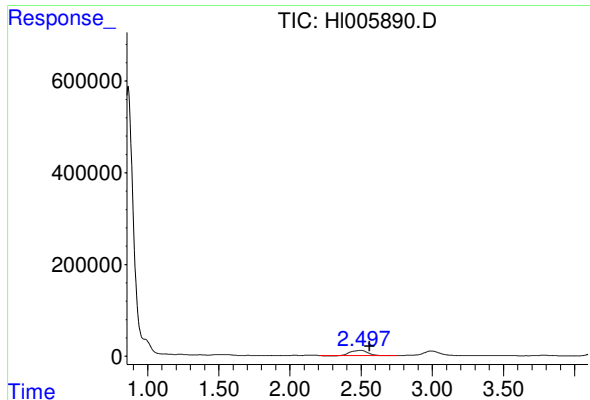

#1 4-Nitroaniline


R.T.: 2.496 min
Delta R.T.: -0.064 min
Response: 951565
Conc: 66.92 ug/L

Instrument :
HPLC_L
ClientSampleId :
YS19-SB41-1014

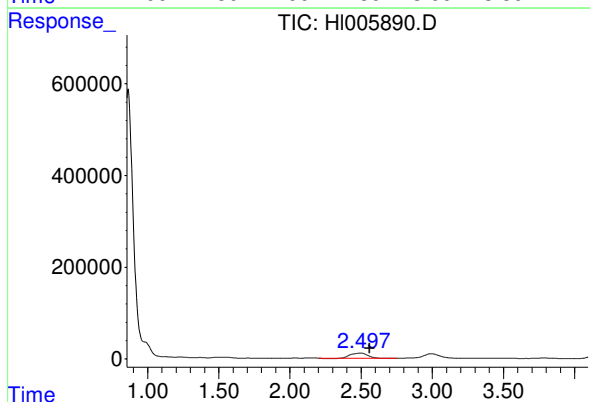


#3 RDX

R.T.: 2.496 min
Delta R.T.: -0.064 min
Response: 951565
Conc: 66.92 ug/L

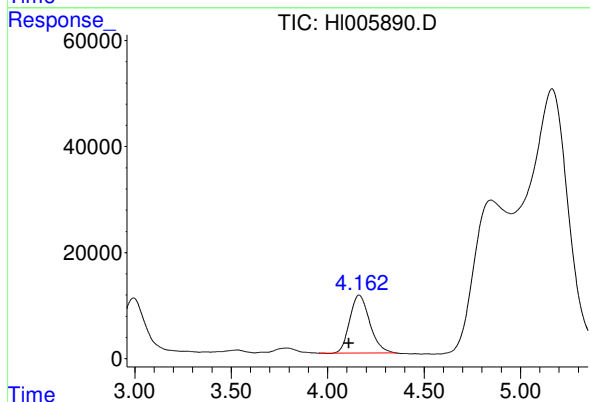


#4 1,3,5-Trinitrobenzene

R.T.: 4.164 min
Delta R.T.: 0.055 min
Response: 786510
Conc: 46.82 ug/L

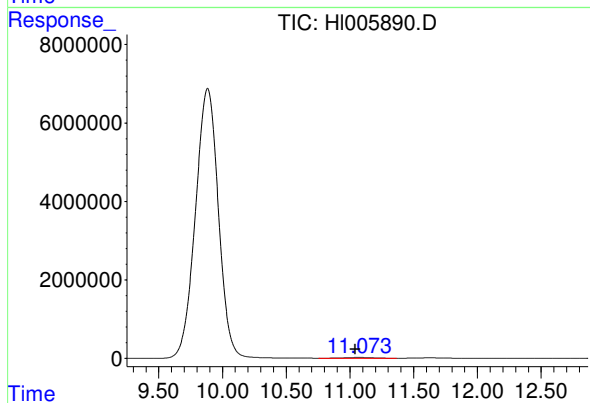

#10 2-Amino-4,6-dinitrotoluene


R.T.: 11.074 min
Delta R.T.: 0.032 min
Response: 2690929
Conc: 179.84 ug/L

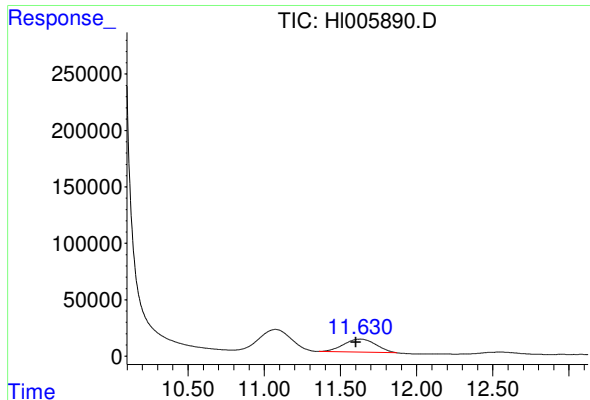

#11 4-Amino-2,6-dinitrotoluene

R.T.: 11.630 min
Delta R.T.: 0.031 min
Response: 1659944
Conc: 164.92 ug/L

Instrument :
HPLC_L
ClientSampleId :
YS19-SB41-1014

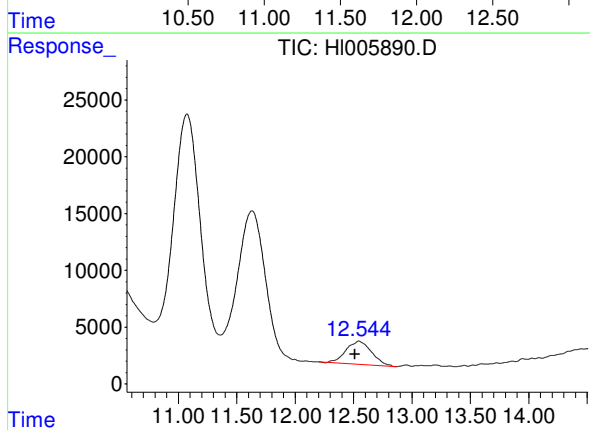

#12 2,4-Dinitrotoluene

R.T.: 12.546 min
Delta R.T.: 0.036 min
Response: 309426
Conc: 13.93 ug/L