

Data Path : Z:\HPCHEM1\HPLC\_L\Data\HL120314\  
 Data File : H1005895.D  
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
 Acq On : 04-Dec-2014, 00:57  
 Operator : TP  
 Sample : F4372-03  
 Misc :  
 ALS Vial : 55 Sample Multiplier: 1

Instrument :  
 HPLC\_L  
 ClientSampleId :  
 YS19-SD01-1014MSD

Integration File signal 1: AUTOINT1.E  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 12 05:55:11 2015  
 Quant Method : Z:\HPCHEM1\HPLC\_L\METHODS\HL120314.M  
 Quant Title :  
 QLast Update : Wed Mar 11 16:43:35 2015  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 50 uL  
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| 1) S 4-Nitroaniline         | 2.567  | 602122   | 42.347 ug/L  |
| Target Compounds            |        |          |              |
| 3) T RDX                    | 2.567  | 602122   | 42.347 ug/L  |
| 14) T 2-Nitrotoluene        | 17.653 | 1007077  | 111.927 ug/L |
| 15) T 4-Nitrotoluene        | 19.183 | 799240   | 114.179 ug/L |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC\_L\Data\HL120314\  
Data File : H1005895.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 04-Dec-2014, 00:57  
Operator : TP  
Sample : F4372-03  
Misc :  
ALS Vial : 55 Sample Multiplier: 1

Instrument :  
HPLC\_L  
ClientSampleId :  
YS19-SD01-1014MSD

Integration File signal 1: AUTOINT1.E  
Integration File signal 2: autoint2.e  
Quant Time: Mar 12 05:55:11 2015  
Quant Method : Z:\HPCHEM1\HPLC\_L\METHODS\HL120314.M  
Quant Title :  
QLast Update : Wed Mar 11 16:43:35 2015  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

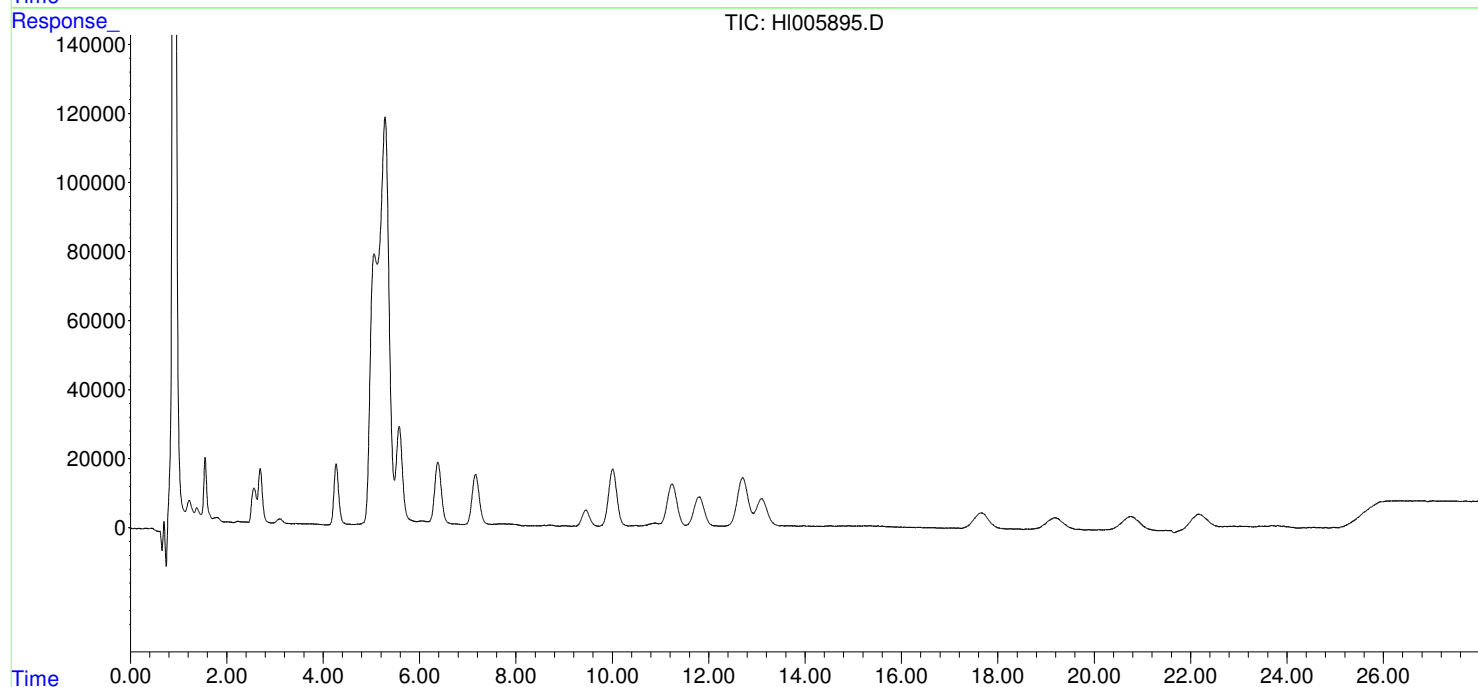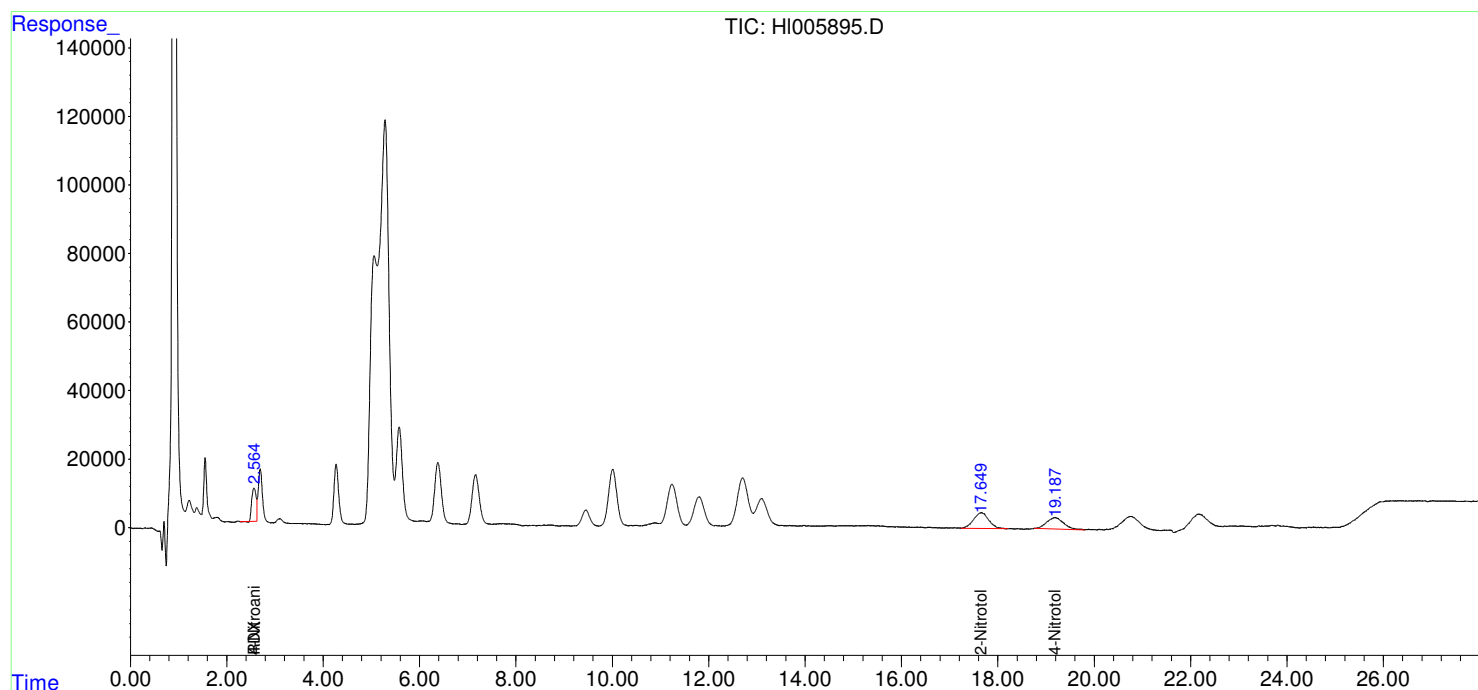


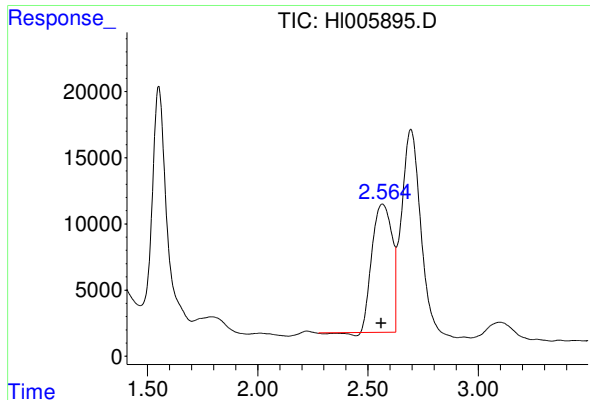

#1 4-Nitroaniline


R.T.: 2.567 min  
Delta R.T.: 0.007 min  
Response: 602122  
Conc: 42.35 ug/L

Instrument :  
HPLC\_L  
ClientSampleId :  
YS19-SD01-1014MSD

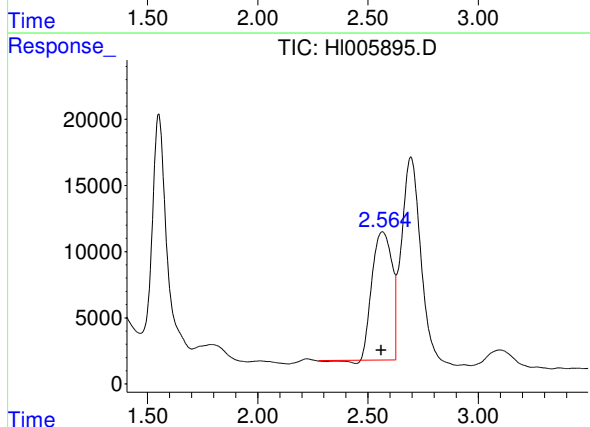


#3 RDX

R.T.: 2.567 min  
Delta R.T.: 0.007 min  
Response: 602122  
Conc: 42.35 ug/L

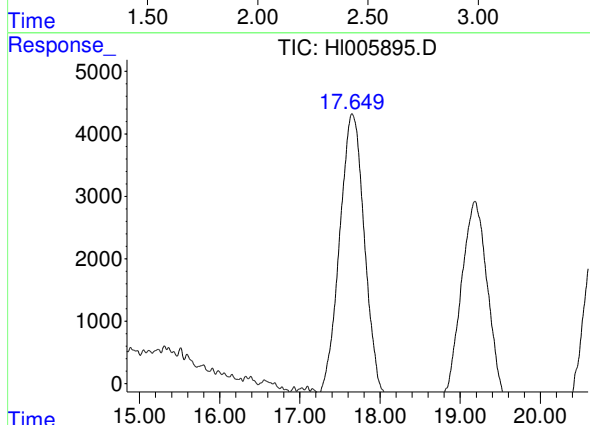

#14 2-Nitrotoluene

R.T.: 17.653 min  
Delta R.T.: 0.060 min  
Response: 1007077  
Conc: 111.93 ug/L

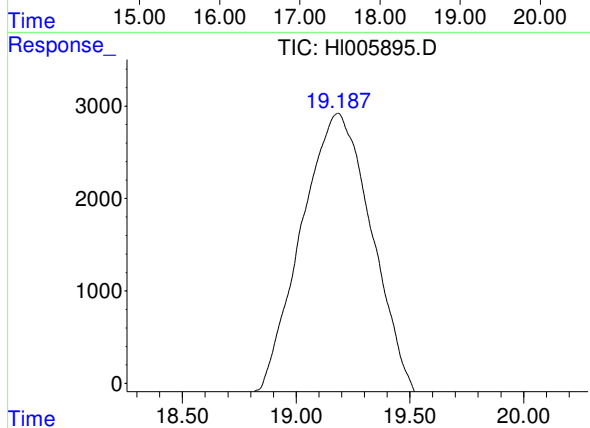

#15 4-Nitrotoluene

R.T.: 19.183 min  
Delta R.T.: -0.048 min  
Response: 799240  
Conc: 114.18 ug/L