

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120314\
 Data File : H1005896.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 04-Dec-2014, 01:26
 Operator : TP
 Sample : HSTDCCC0500
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 HSTDCCC0500

Integration File signal 1: AUTOINT1.E
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 05:55:15 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120314.M
 Quant Title :
 QLast Update : Wed Mar 11 16:43:35 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.565	6850725	481.803 ug/L
Target Compounds			
2) T HMX	1.470	2967971	476.385 ug/L
3) T RDX	2.565	6850725	481.803 ug/L
4) T 1,3,5-Trinitrobenzene	4.116	8101397	482.302 ug/L
5) T 1,3-Dinitrobenzene	5.408	11794333	485.151 ng/ml
6) T 3,5-Dinitroaniline	6.201	8987067	476.520 ug/L
7) T Nitrobenzene	6.976	6761774	467.025 ug/L
8) T Tetryl	9.261	5462253	478.355 ug/L
9) T 2,4,6-Trinitrotoluene	9.821	7543906	471.006 ug/L
10) T 2-Amino-4,6-dinitroto...	11.047	6791415	453.873 ug/L
11) T 4-Amino-2,6-dinitroto...	11.605	4355039	432.689 ug/L
12) T 2,4-Dinitrotoluene	12.564	11809796	531.774 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120314\
Data File : H1005896.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 04-Dec-2014, 01:26
Operator : TP
Sample : HSTDCCC0500
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HSTDCCC0500

Integration File signal 1: AUTOINT1.E
Integration File signal 2: autoint2.e
Quant Time: Mar 12 05:55:15 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120314.M
Quant Title :
QLast Update : Wed Mar 11 16:43:35 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

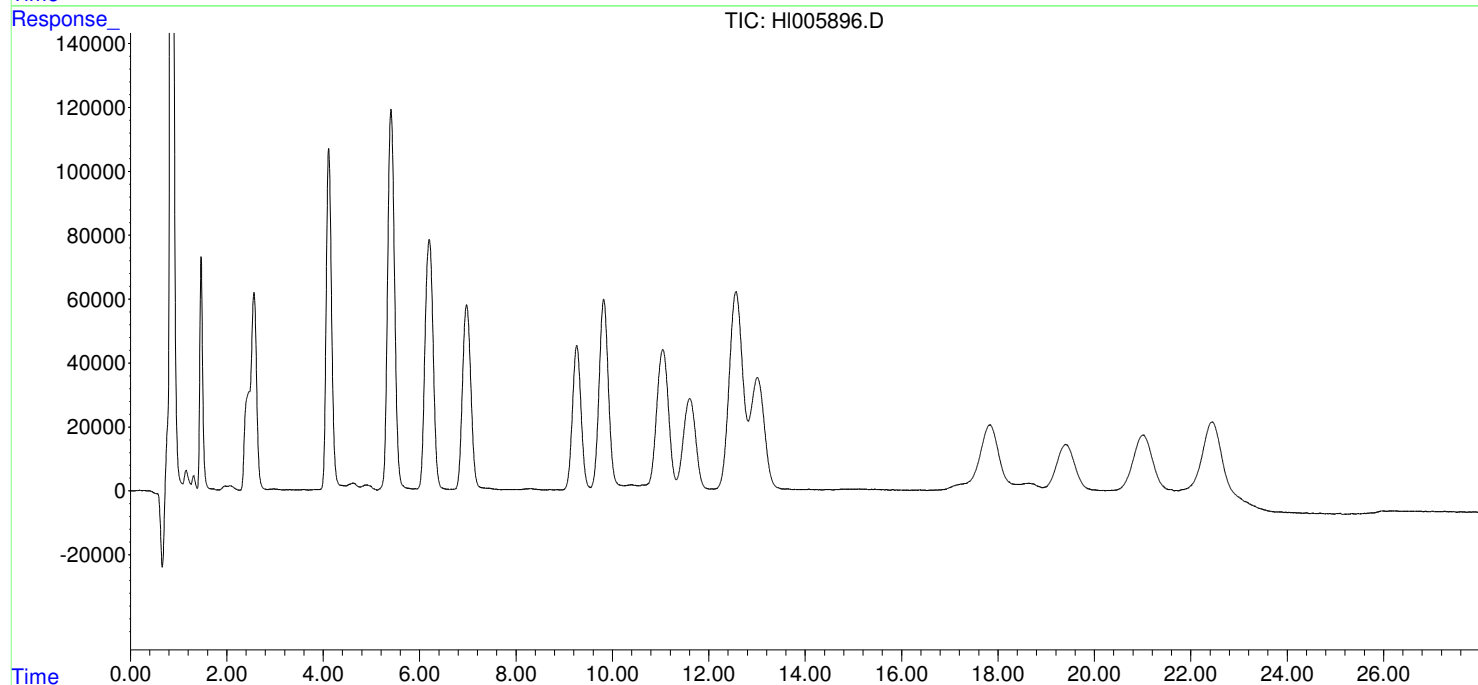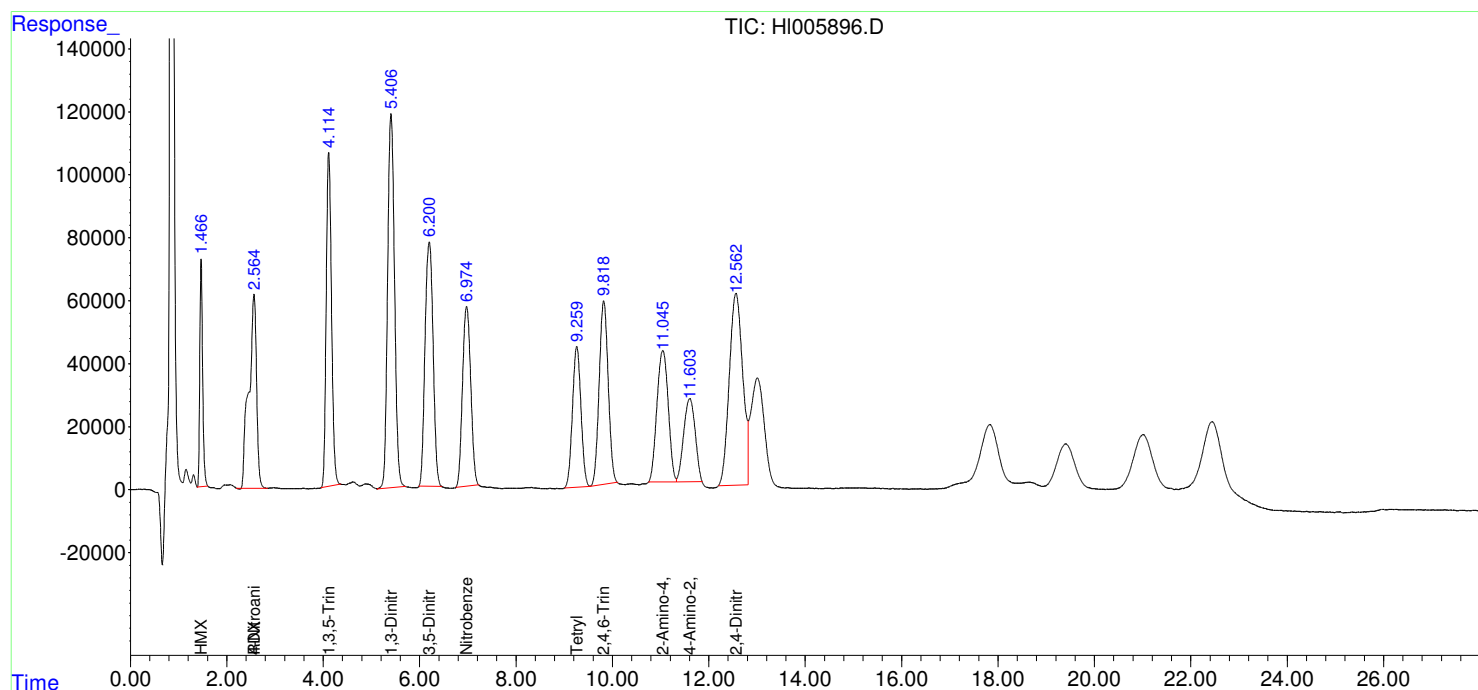


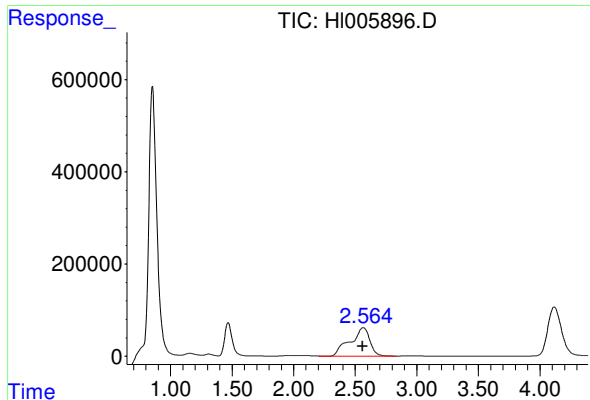

#1 4-Nitroaniline


R.T.: 2.565 min
Delta R.T.: 0.005 min
Response: 6850725
Conc: 481.80 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDCCC0500

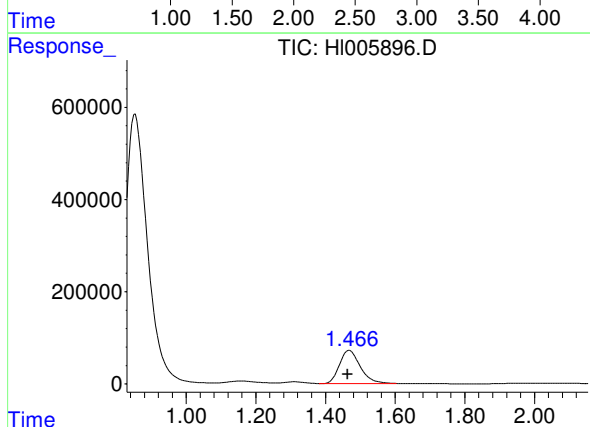


#2 HMX

R.T.: 1.470 min
Delta R.T.: 0.007 min
Response: 2967971
Conc: 476.38 ug/L

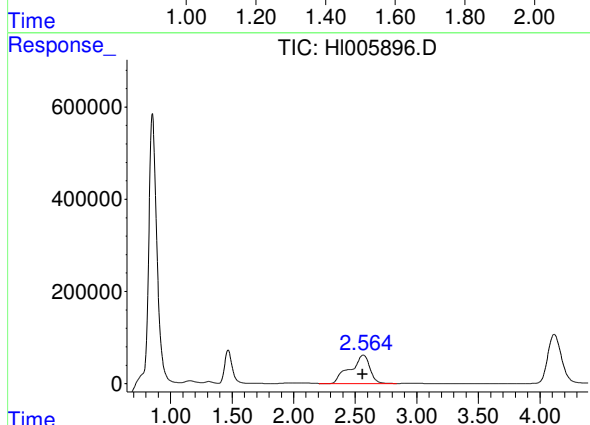


#3 RDX

R.T.: 2.565 min
Delta R.T.: 0.006 min
Response: 6850725
Conc: 481.80 ug/L

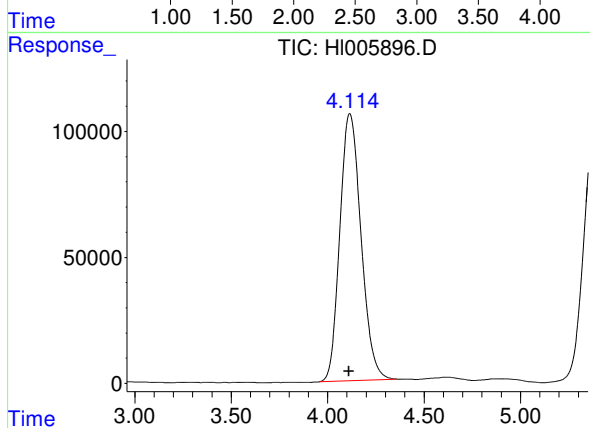

#4 1,3,5-Trinitrobenzene


R.T.: 4.116 min
Delta R.T.: 0.008 min
Response: 8101397
Conc: 482.30 ug/L

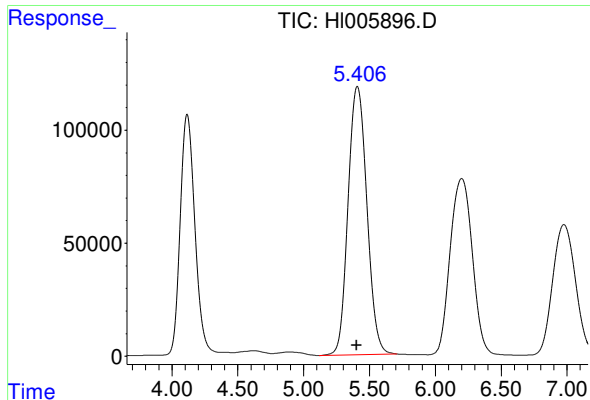

#5 1,3-Dinitrobenzene


R.T.: 5.408 min
Delta R.T.: 0.008 min
Response: 11794333
Conc: 485.15 ng/ml

Instrument :
HPLC_L
ClientSampleId :
HSTDCCC0500

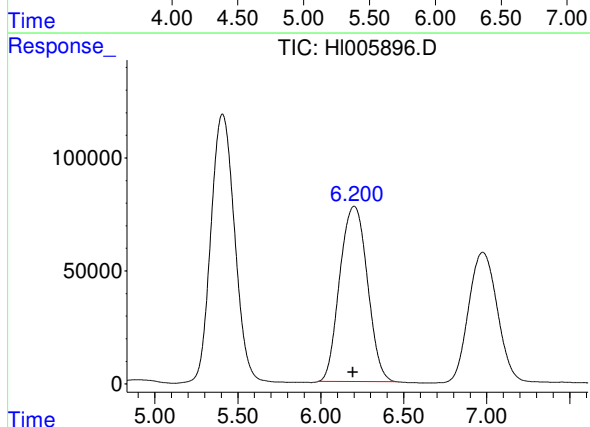


#6 3,5-Dinitroaniline

R.T.: 6.201 min
Delta R.T.: 0.007 min
Response: 8987067
Conc: 476.52 ug/L

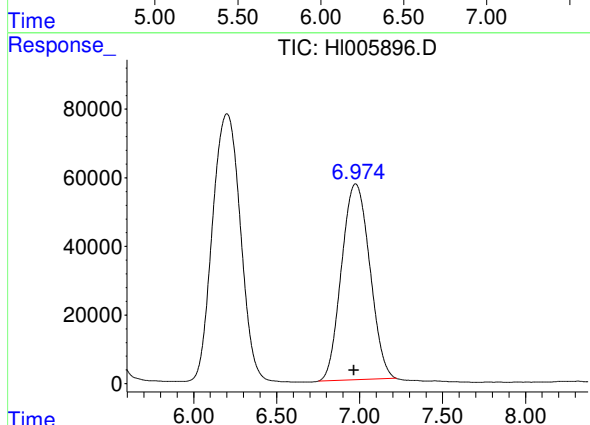


#7 Nitrobenzene

R.T.: 6.976 min
Delta R.T.: 0.010 min
Response: 6761774
Conc: 467.03 ug/L

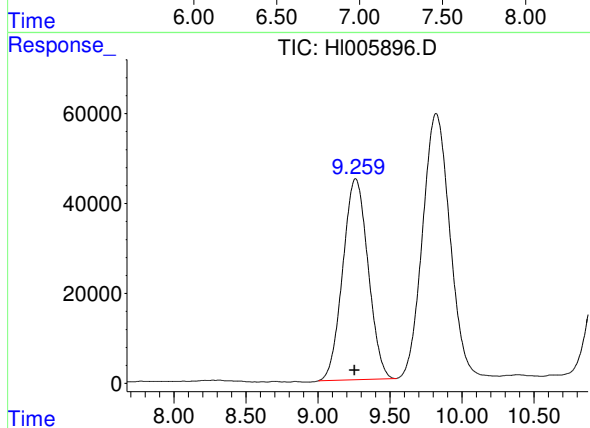

#8 Tetryl


R.T.: 9.261 min
Delta R.T.: 0.009 min
Response: 5462253
Conc: 478.36 ug/L

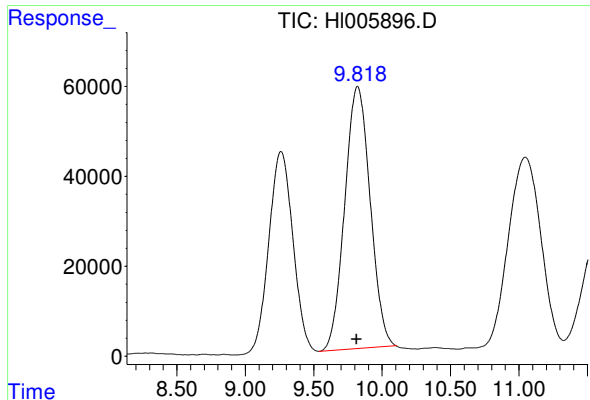

#9 2,4,6-Trinitrotoluene


R.T.: 9.821 min
Delta R.T.: 0.010 min
Response: 7543906
Conc: 471.01 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDCCC0500

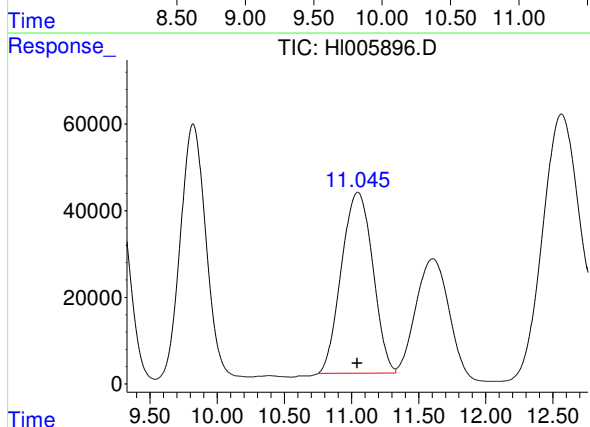


#10 2-Amino-4,6-dinitrotoluene

R.T.: 11.047 min
Delta R.T.: 0.005 min
Response: 6791415
Conc: 453.87 ug/L

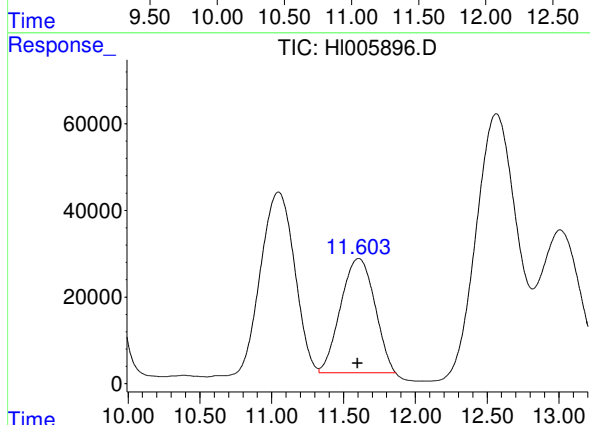

#11 4-Amino-2,6-dinitrotoluene

R.T.: 11.605 min
Delta R.T.: 0.005 min
Response: 4355039
Conc: 432.69 ug/L

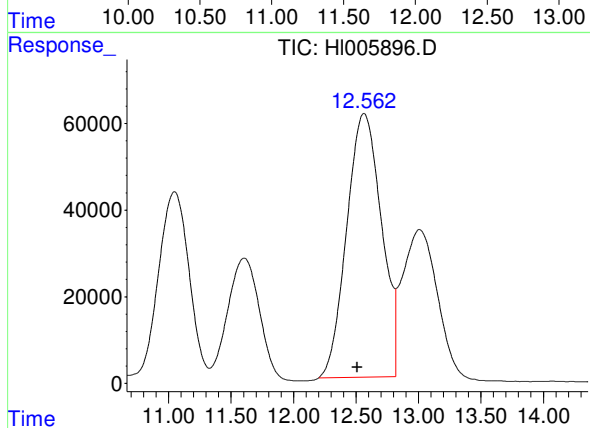

#12 2,4-Dinitrotoluene

R.T.: 12.564 min
Delta R.T.: 0.054 min
Response: 11809796
Conc: 531.77 ug/L