

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120314\
 Data File : H1005901.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 04-Dec-2014, 03:53
 Operator : TP
 Sample : F4372-08
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 YS19-SD09-1014

Integration File signal 1: AUTOINT1.E
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 05:55:31 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120314.M
 Quant Title :
 QLast Update : Wed Mar 11 16:43:35 2015
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 50 uL
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.554	759257	53.398 ug/L
Target Compounds			
3) T RDX	2.554	759257	53.398 ug/L
6) T 3,5-Dinitroaniline	6.258	368404	19.534 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.

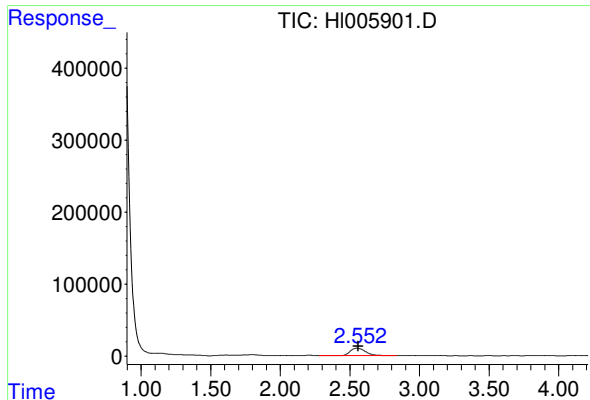

#1 4-Nitroaniline


R.T.: 2.554 min
Delta R.T.: -0.006 min
Response: 759257
Conc: 53.40 ug/L

Instrument :
HPLC_L
ClientSampleId :
YS19-SD09-1014

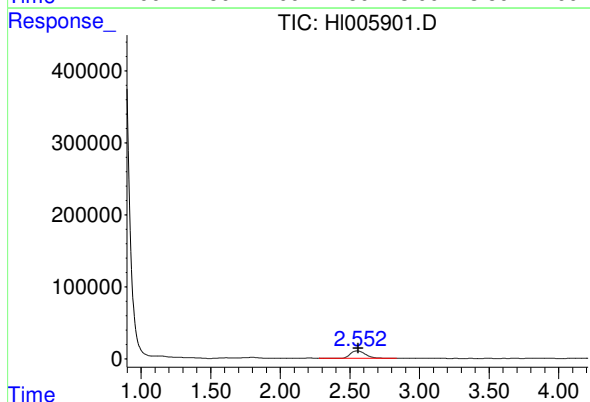

#3 RDX

R.T.: 2.554 min
Delta R.T.: -0.005 min
Response: 759257
Conc: 53.40 ug/L

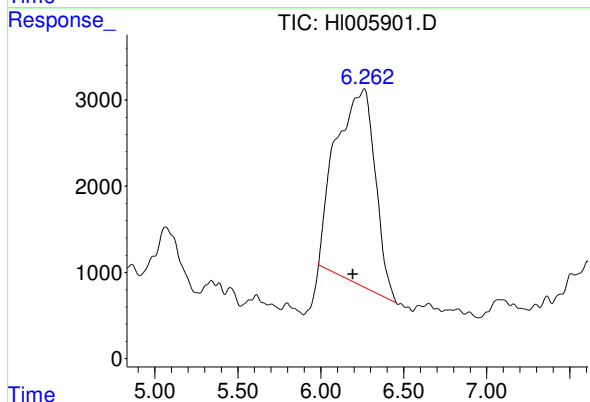

#6 3,5-Dinitroaniline

R.T.: 6.258 min
Delta R.T.: 0.064 min
Response: 368404
Conc: 19.53 ug/L