

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120814\
 Data File : HL005918.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 08-Dec-2014, 14:57
 Operator : TP
 Sample : HSTDICC5000
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 HSTDICC5000

Integration File signal 1: AUTOINT1.E
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 06:54:54 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120814.M
 Quant Title :
 QLast Update : Mon Mar 09 13:49:54 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.521	42324038	3129.200 ug/L
Target Compounds			
2) T HMX	1.464	29555422	4776.046 ug/L
3) T RDX	2.521	42324038	2995.721 ug/L
4) T 1,3,5-Trinitrobenzene	4.105	54207654	3262.477 ug/L
5) T 1,3-Dinitrobenzene	5.402	117834711	4827.348 ng/mL
6) T 3,5-Dinitroaniline	6.211	90411964	4761.341 ug/L
7) T Nitrobenzene	6.966	69044747	4817.291 ug/L
8) T Tetryl	9.254	39910179	3767.404 ug/L
9) T 2,4,6-Trinitrotoluene	9.810	81553599	4585.980 ug/L
10) T 2-Amino-4,6-dinitroto...	11.066	67859773	4286.909 ug/L
11) T 4-Amino-2,6-dinitroto...	11.630	45743267	4380.860 ug/L
12) T 2,4-Dinitrotoluene	12.514	110918442	4964.526 ug/L
13) T 2,6-Dinitrotoluene	12.894	48233546	4066.601 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120814\
Data File : H1005918.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 08-Dec-2014, 14:57
Operator : TP
Sample : HSTDICC5000
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HSTDICC5000

Integration File signal 1: AUTOINT1.E
Integration File signal 2: autoint2.e
Quant Time: Mar 12 06:54:54 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120814.M
Quant Title :
QLast Update : Mon Mar 09 13:49:54 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

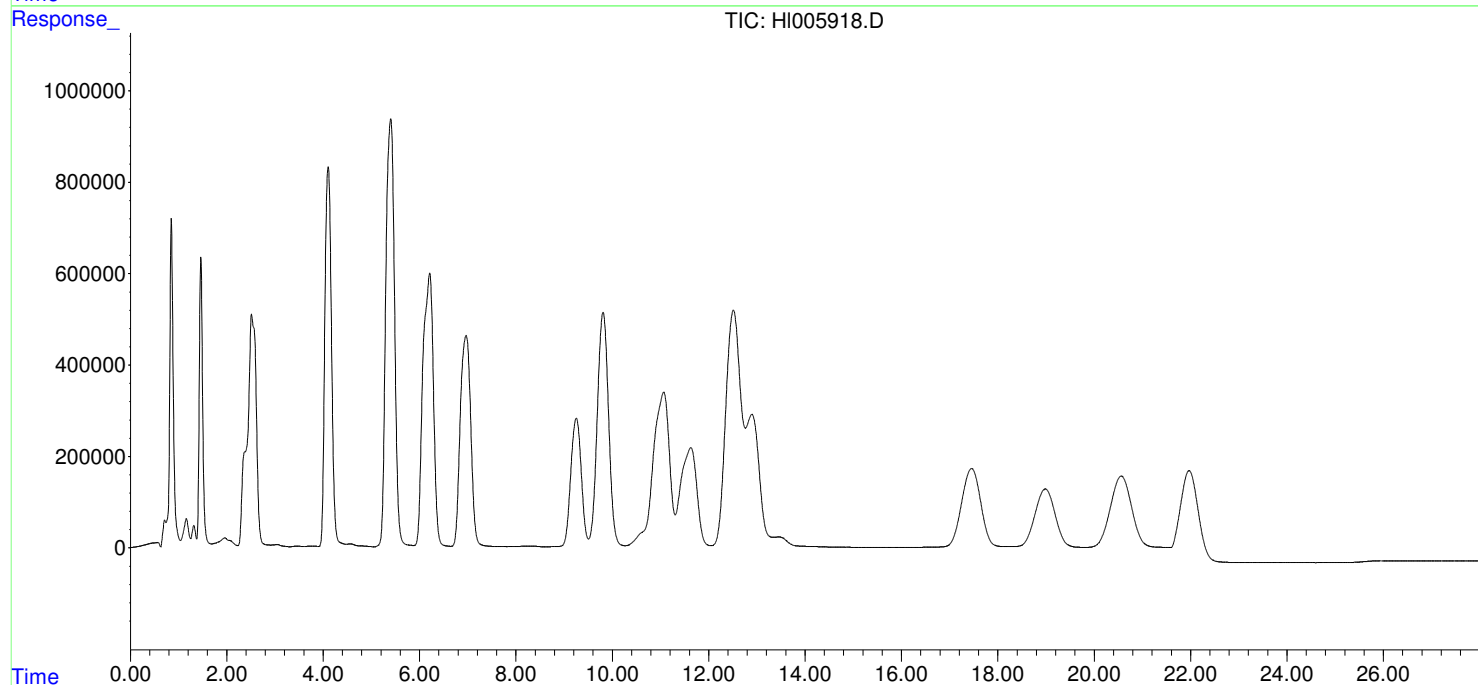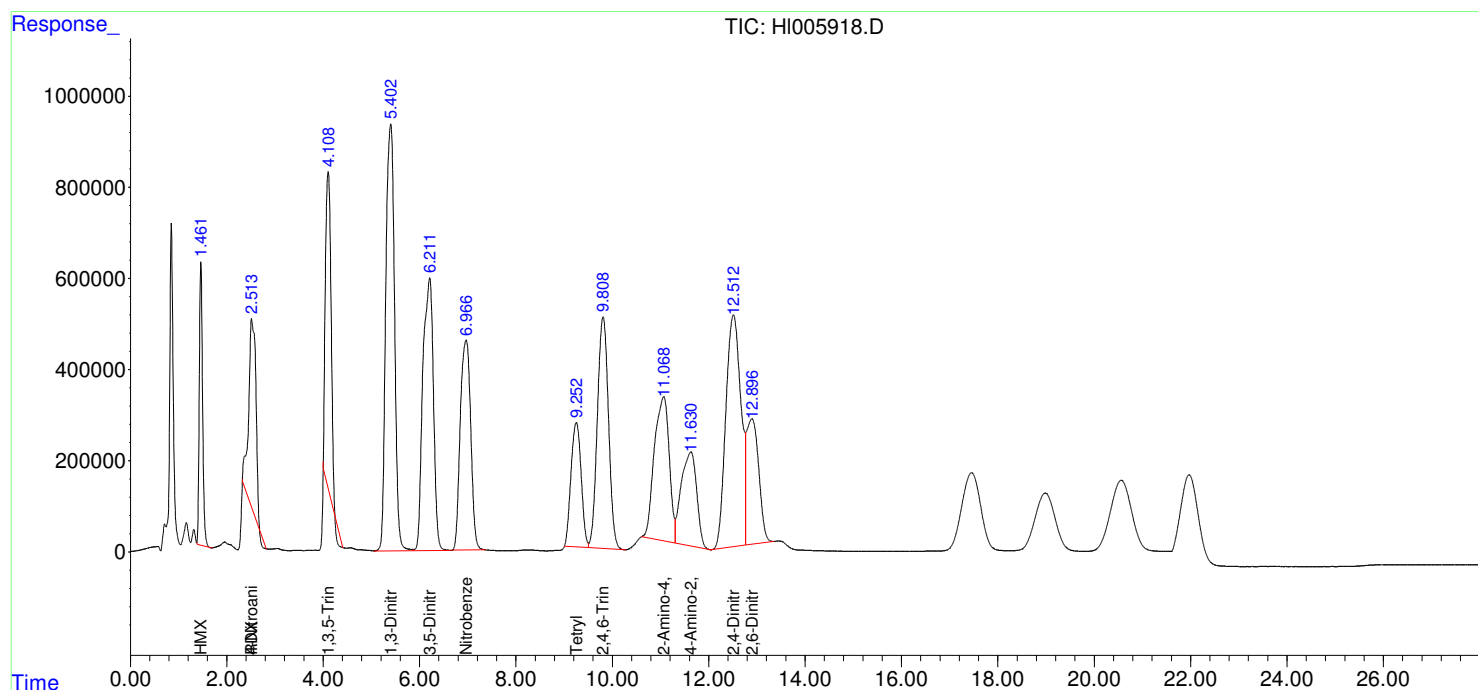


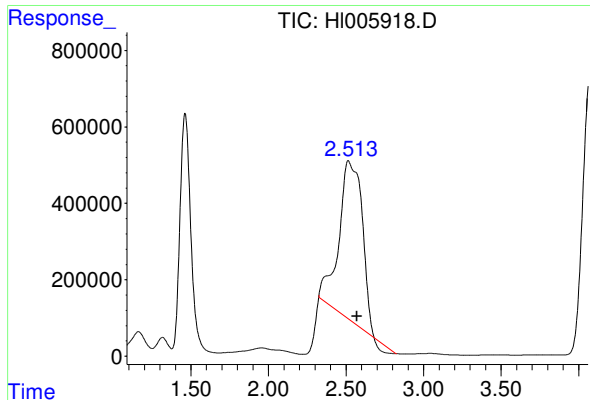

#1 4-Nitroaniline


R.T.: 2.521 min
Delta R.T.: -0.048 min
Response: 42324038
Conc: 3129.20 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC5000

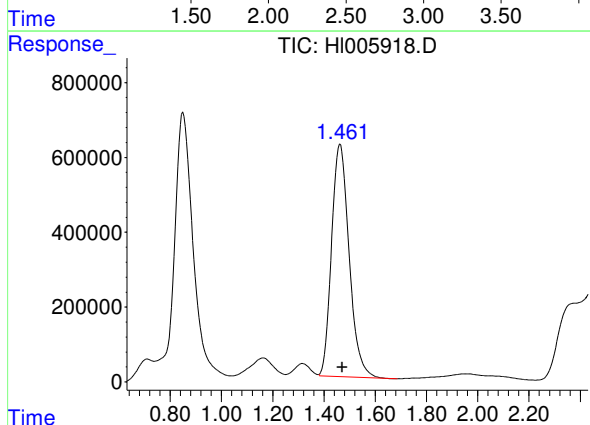


#2 HMX

R.T.: 1.464 min
Delta R.T.: -0.008 min
Response: 29555422
Conc: 4776.05 ug/L

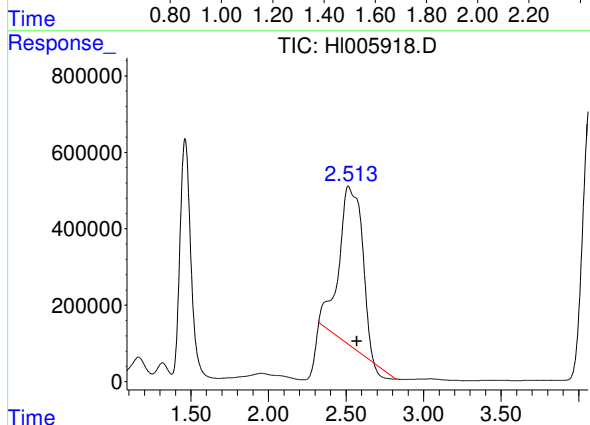


#3 RDX

R.T.: 2.521 min
Delta R.T.: -0.048 min
Response: 42324038
Conc: 2995.72 ug/L

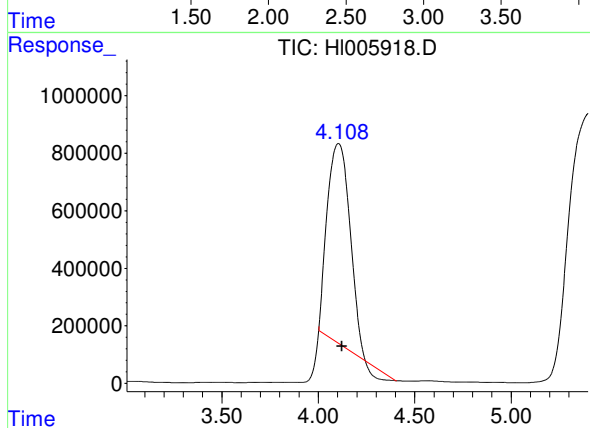

#4 1,3,5-Trinitrobenzene


R.T.: 4.105 min
Delta R.T.: -0.018 min
Response: 54207654
Conc: 3262.48 ug/L

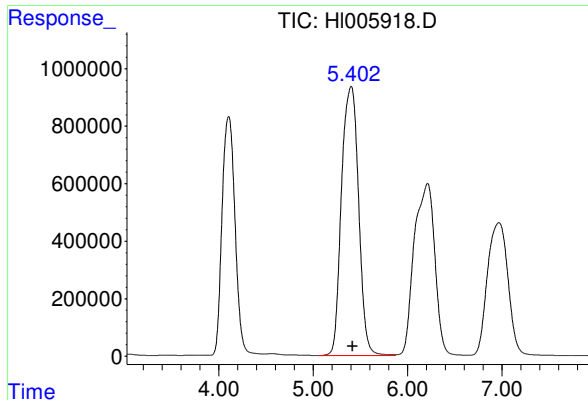

#5 1,3-Dinitrobenzene


R.T.: 5.402 min
Delta R.T.: -0.014 min
Response: 117834711
Conc: 4827.35 ng/ml

Instrument :
HPLC_L
ClientSampleId :
HSTDICC5000

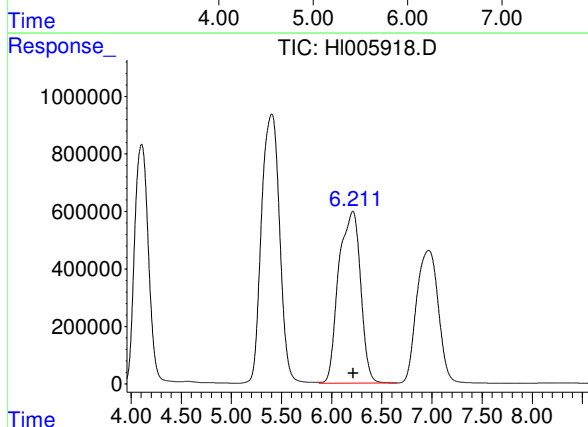


#6 3,5-Dinitroaniline

R.T.: 6.211 min
Delta R.T.: -0.004 min
Response: 90411964
Conc: 4761.34 ug/L

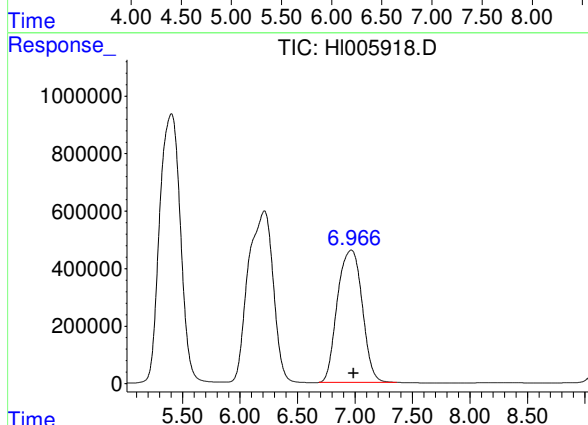


#7 Nitrobenzene

R.T.: 6.966 min
Delta R.T.: -0.020 min
Response: 69044747
Conc: 4817.29 ug/L

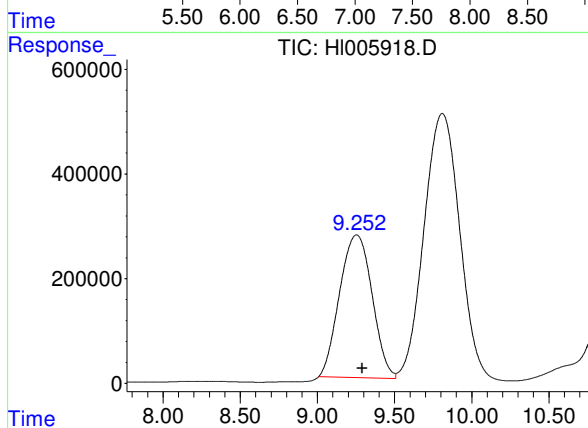

#8 Tetryl


R.T.: 9.254 min
Delta R.T.: -0.036 min
Response: 39910179
Conc: 3767.40 ug/L

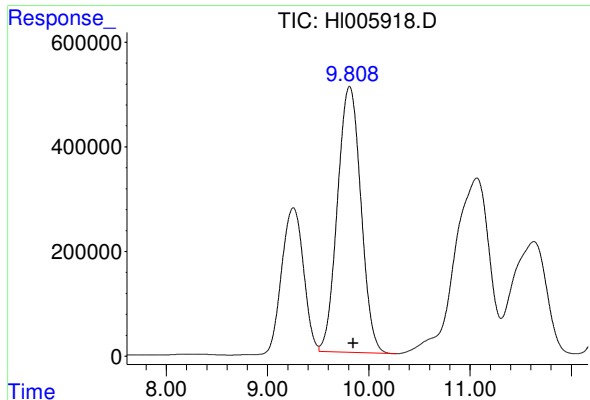

#9 2,4,6-Trinitrotoluene


R.T.: 9.810 min
Delta R.T.: -0.037 min
Response: 81553599
Conc: 4585.98 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC5000

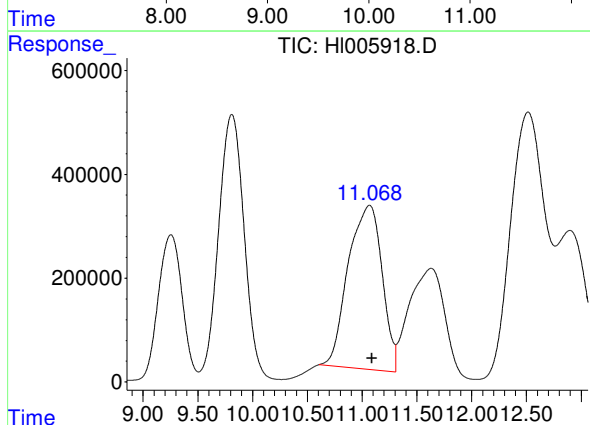


#10 2-Amino-4,6-dinitrotoluene

R.T.: 11.066 min
Delta R.T.: -0.023 min
Response: 67859773
Conc: 4286.91 ug/L

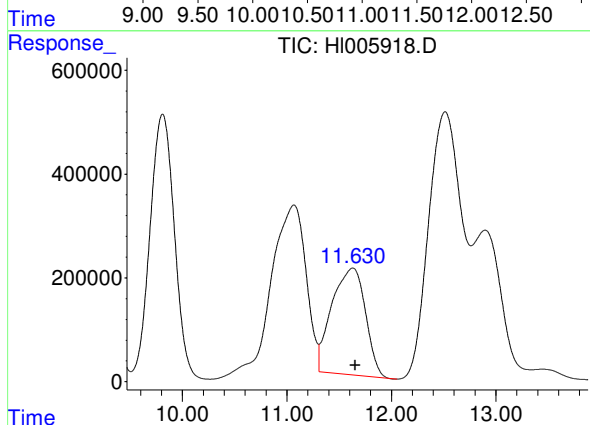


#11 4-Amino-2,6-dinitrotoluene

R.T.: 11.630 min
Delta R.T.: -0.023 min
Response: 45743267
Conc: 4380.86 ug/L

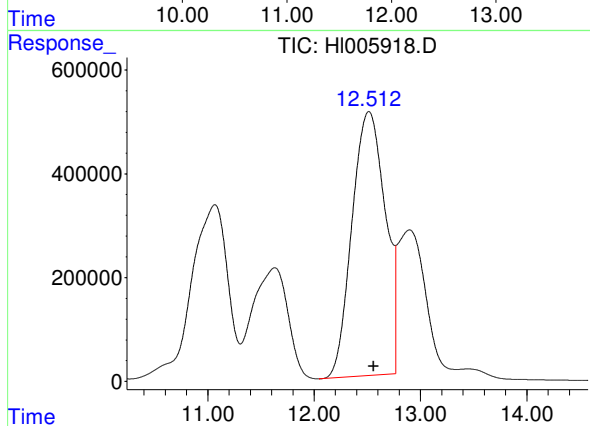

#12 2,4-Dinitrotoluene

R.T.: 12.514 min
Delta R.T.: -0.045 min
Response: 110918442
Conc: 4964.53 ug/L

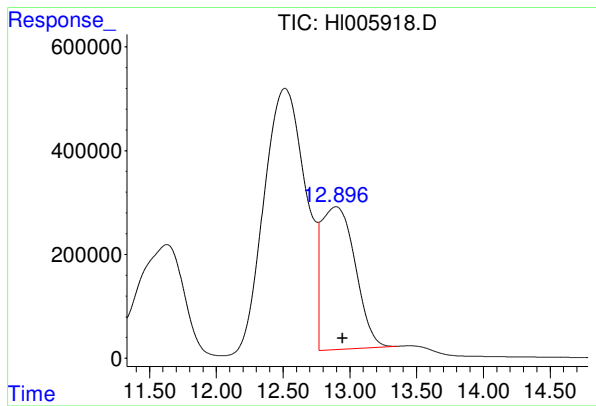

#13 2,6-Dinitrotoluene

R.T.: 12.894 min
Delta R.T.: -0.052 min
Response: 48233546
Conc: 4066.60 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC5000