

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120814\
 Data File : HL005919.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 08-Dec-2014, 15:27
 Operator : TP
 Sample : HSTDICC2000
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 HSTDICC2000

Integration File signal 1: AUTOINT1.E
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 06:54:59 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120814.M
 Quant Title :
 QLast Update : Mon Mar 09 13:49:54 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.557	23706920	1738.650 ug/L
Target Compounds			
2) T HMX	1.467	11852810	1915.370 ug/L
3) T RDX	2.557	23706920	1677.990 ug/L
4) T 1,3,5-Trinitrobenzene	4.112	28276381	1701.809 ug/L
5) T 1,3-Dinitrobenzene	5.404	47024274	1926.449 ng/mL
6) T 3,5-Dinitroaniline	6.204	36188896	1905.806 ug/L
7) T Nitrobenzene	6.973	27719035	1933.973 ug/L
8) T Tetryl	9.281	19911018	1879.542 ug/L
9) T 2,4,6-Trinitrotoluene	9.838	32327335	1817.854 ug/L
10) T 2-Amino-4,6-dinitroto...	11.079	28520942	1801.755 ug/L
11) T 4-Amino-2,6-dinitroto...	11.641	19304291	1848.783 ug/L
12) T 2,4-Dinitrotoluene	12.543	42807017	1915.971 ug/L
13) T 2,6-Dinitrotoluene	12.934	23356681	1969.217 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120814\
Data File : H1005919.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 08-Dec-2014, 15:27
Operator : TP
Sample : HSTDICC2000
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HSTDICC2000

Integration File signal 1: AUTOINT1.E
Integration File signal 2: autoint2.e
Quant Time: Mar 12 06:54:59 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120814.M
Quant Title :
QLast Update : Mon Mar 09 13:49:54 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

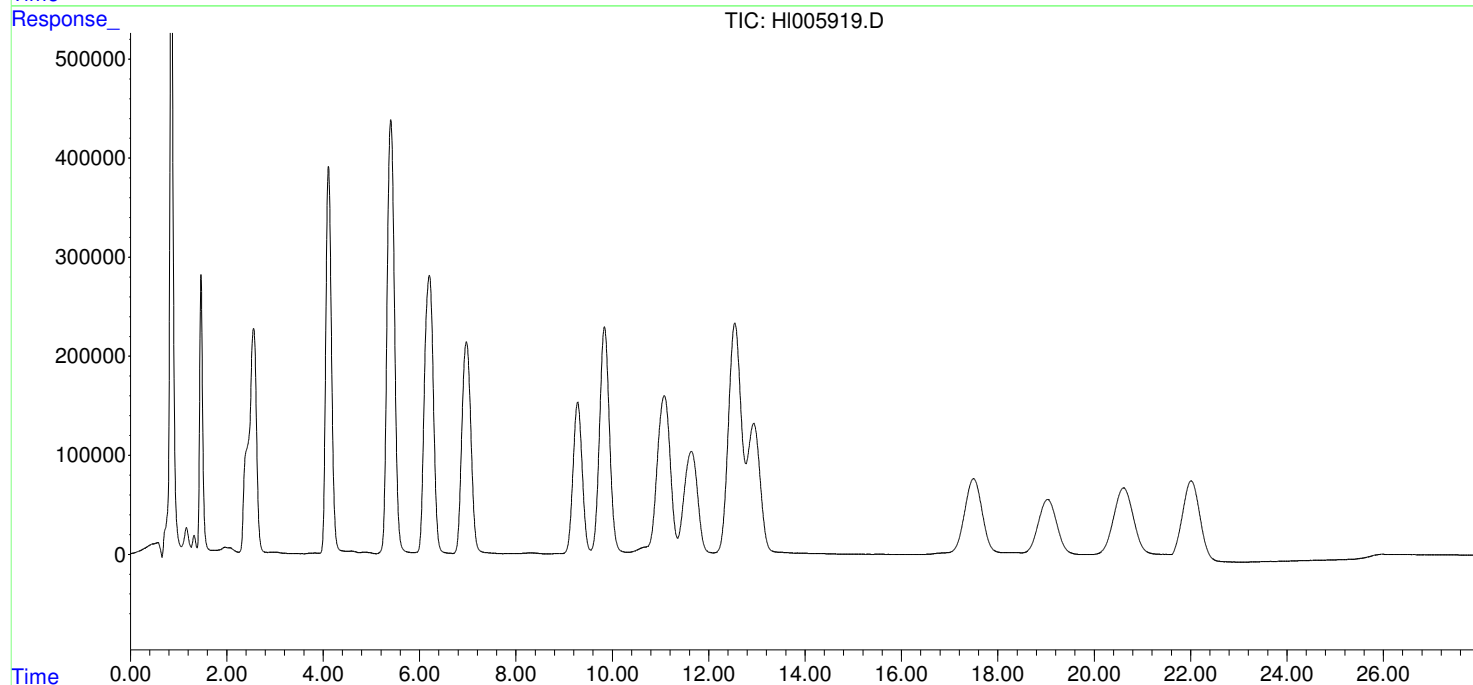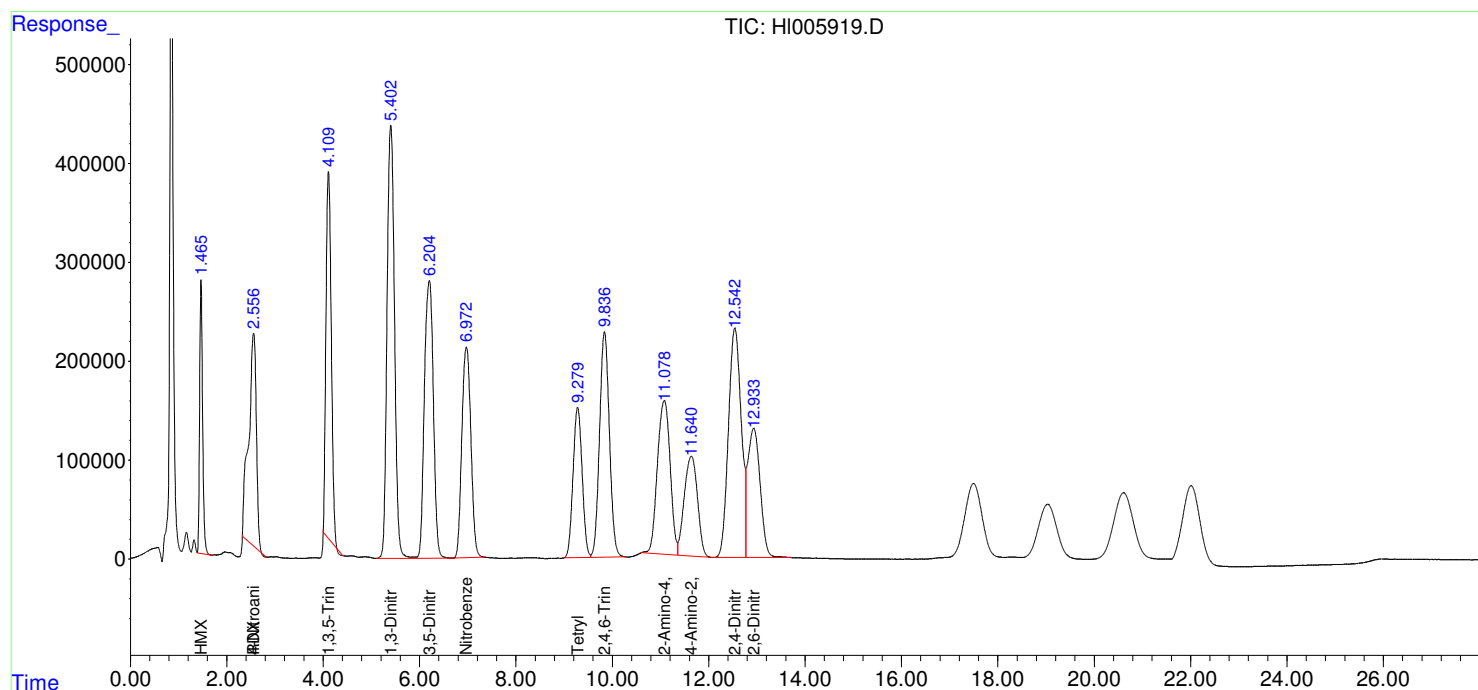


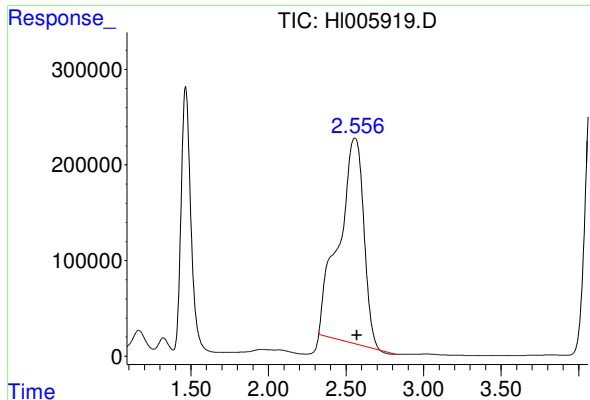

#1 4-Nitroaniline


R.T.: 2.557 min
Delta R.T.: -0.012 min
Response: 23706920
Conc: 1738.65 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC2000

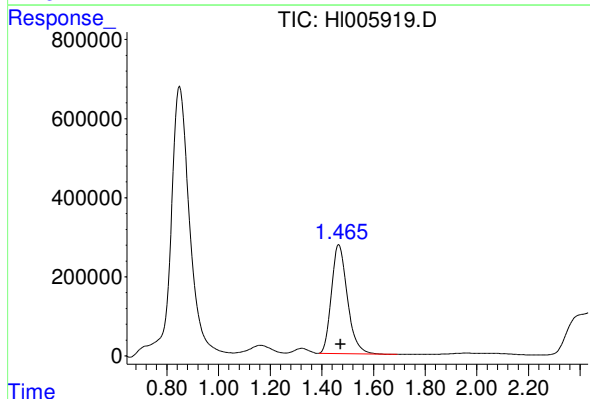


#2 HMX

R.T.: 1.467 min
Delta R.T.: -0.004 min
Response: 11852810
Conc: 1915.37 ug/L

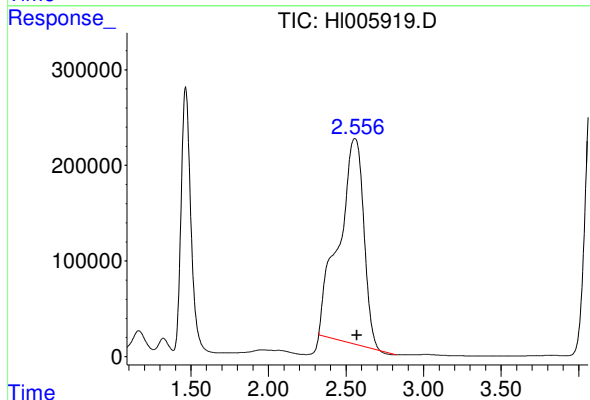


#3 RDX

R.T.: 2.557 min
Delta R.T.: -0.012 min
Response: 23706920
Conc: 1677.99 ug/L

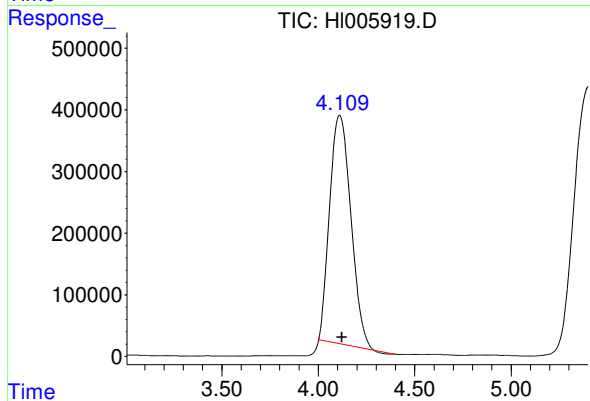

#4 1,3,5-Trinitrobenzene


R.T.: 4.112 min
Delta R.T.: -0.011 min
Response: 28276381
Conc: 1701.81 ug/L

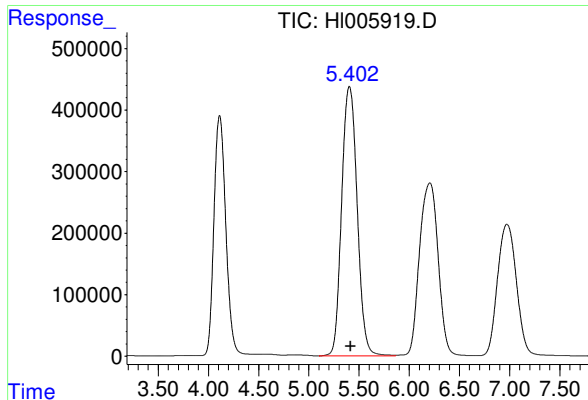

#5 1,3-Dinitrobenzene


R.T.: 5.404 min
Delta R.T.: -0.012 min
Response: 47024274
Conc: 1926.45 ng/ml

Instrument :
HPLC_L
ClientSampleId :
HSTDICC2000

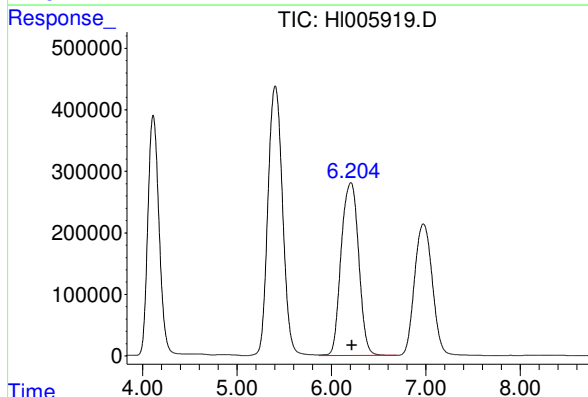


#6 3,5-Dinitroaniline

R.T.: 6.204 min
Delta R.T.: -0.010 min
Response: 36188896
Conc: 1905.81 ug/L

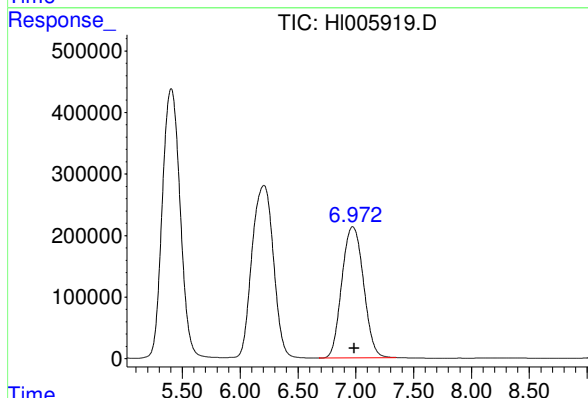


#7 Nitrobenzene

R.T.: 6.973 min
Delta R.T.: -0.013 min
Response: 27719035
Conc: 1933.97 ug/L

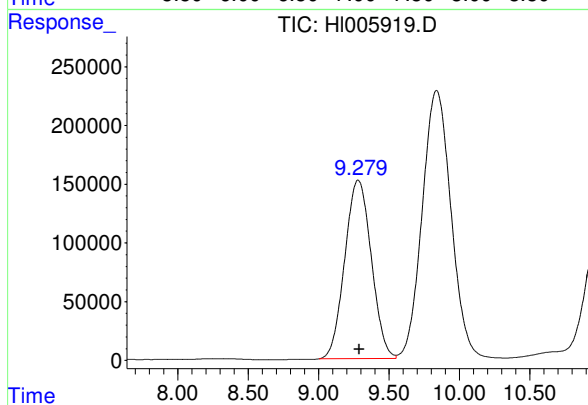

#8 Tetryl


R.T.: 9.281 min
Delta R.T.: -0.008 min
Response: 19911018
Conc: 1879.54 ug/L

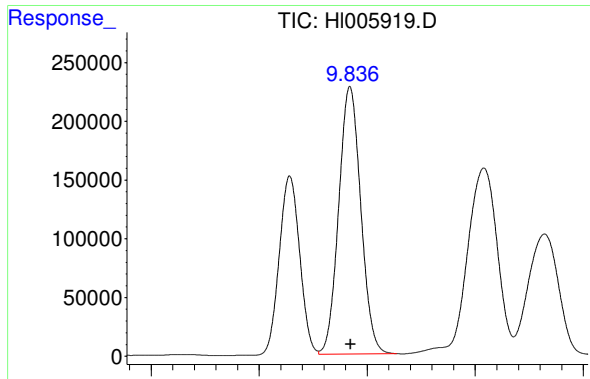

#9 2,4,6-Trinitrotoluene


R.T.: 9.838 min
Delta R.T.: -0.008 min
Response: 32327335
Conc: 1817.85 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC2000

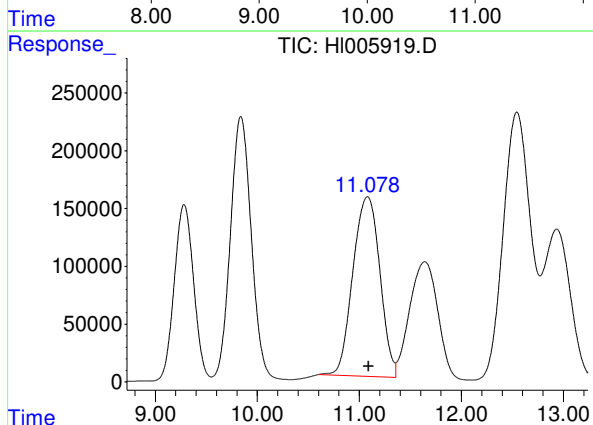


#10 2-Amino-4,6-dinitrotoluene

R.T.: 11.079 min
Delta R.T.: -0.010 min
Response: 28520942
Conc: 1801.75 ug/L

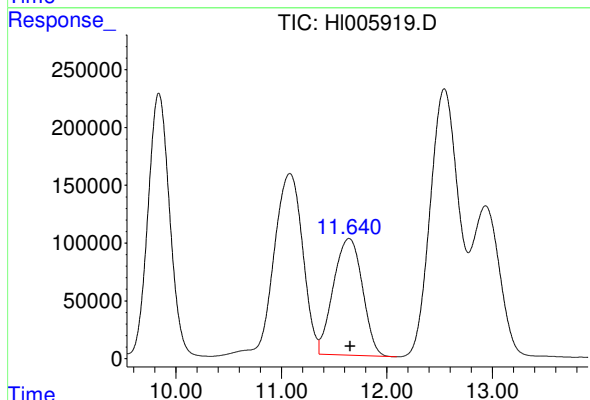


#11 4-Amino-2,6-dinitrotoluene

R.T.: 11.641 min
Delta R.T.: -0.012 min
Response: 19304291
Conc: 1848.78 ug/L

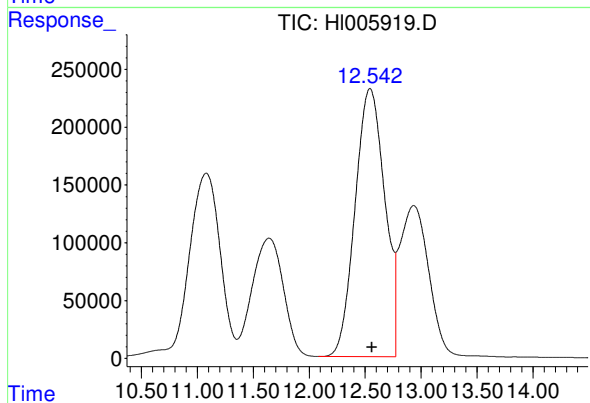

#12 2,4-Dinitrotoluene

R.T.: 12.543 min
Delta R.T.: -0.015 min
Response: 42807017
Conc: 1915.97 ug/L

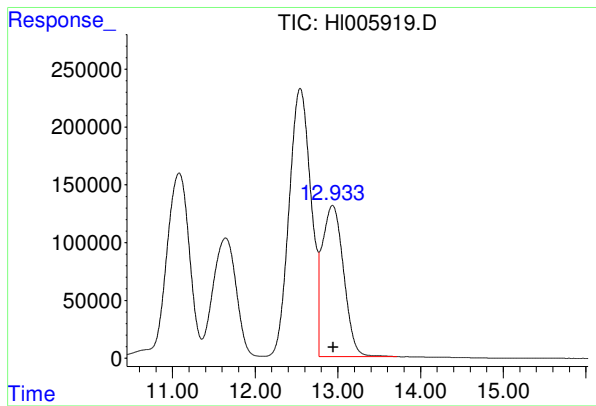

#13 2,6-Dinitrotoluene

R.T.: 12.934 min
Delta R.T.: -0.011 min
Response: 23356681
Conc: 1969.22 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC2000