

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120814\
 Data File : H1005927.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 08-Dec-2014, 19:21
 Operator : TP
 Sample : F4368-06
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 YS19-SB41-1014

Integration File signal 1: AUTOINT1.E
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 06:55:34 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120814.M
 Quant Title :
 QLast Update : Mon Mar 09 13:49:54 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds				
4) T	1,3,5-Trinitrobenzene	4.123	1543851	92.916 ug/L
9) T	2,4,6-Trinitrotoluene	9.869	857995786	48247.425 ug/L
10) T	2-Amino-4,6-dinitroto...	11.091	2715754	171.562 ug/L
11) T	4-Amino-2,6-dinitroto...	11.656	1793663	171.780 ug/L
12) T	2,4-Dinitrotoluene	12.555	299272	13.395 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120814\
Data File : H1005927.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 08-Dec-2014, 19:21
Operator : TP
Sample : F4368-06
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
YS19-SB41-1014

Integration File signal 1: AUTOINT1.E
Integration File signal 2: autoint2.e
Quant Time: Mar 12 06:55:34 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120814.M
Quant Title :
QLast Update : Mon Mar 09 13:49:54 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

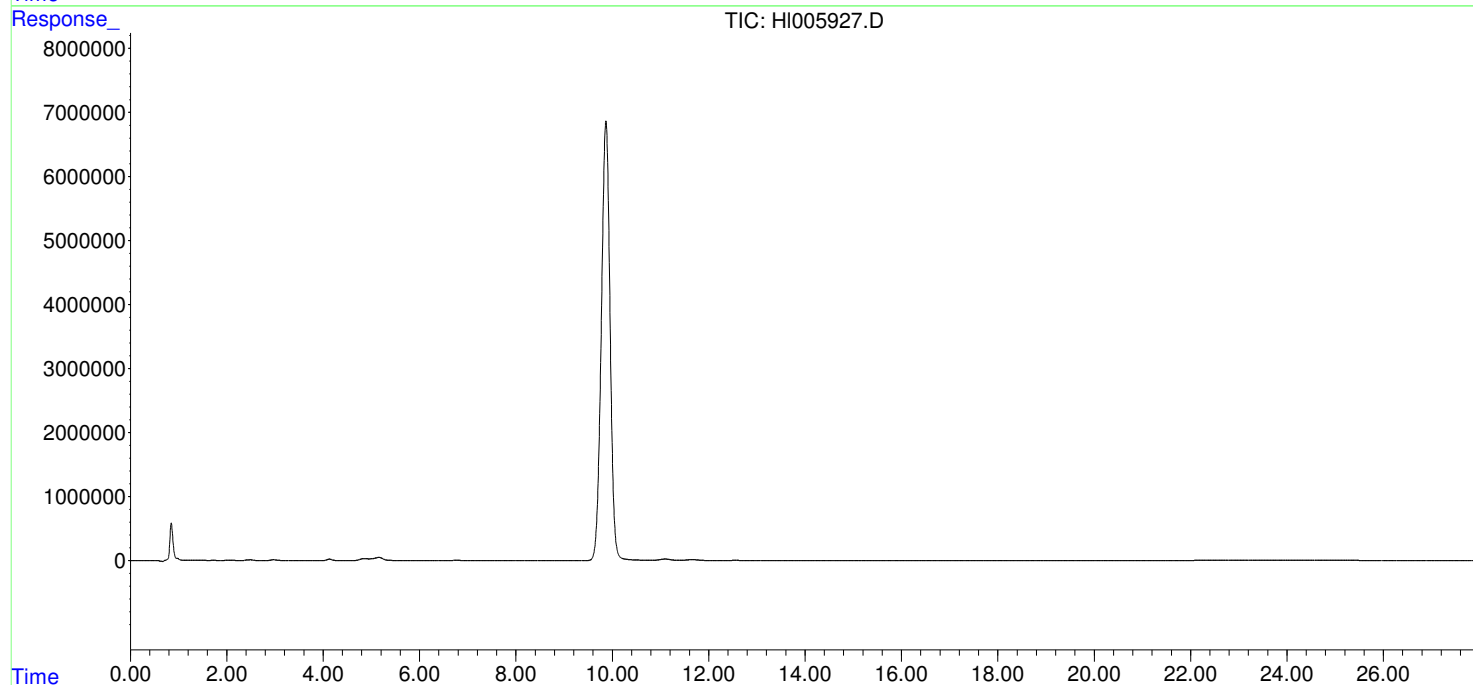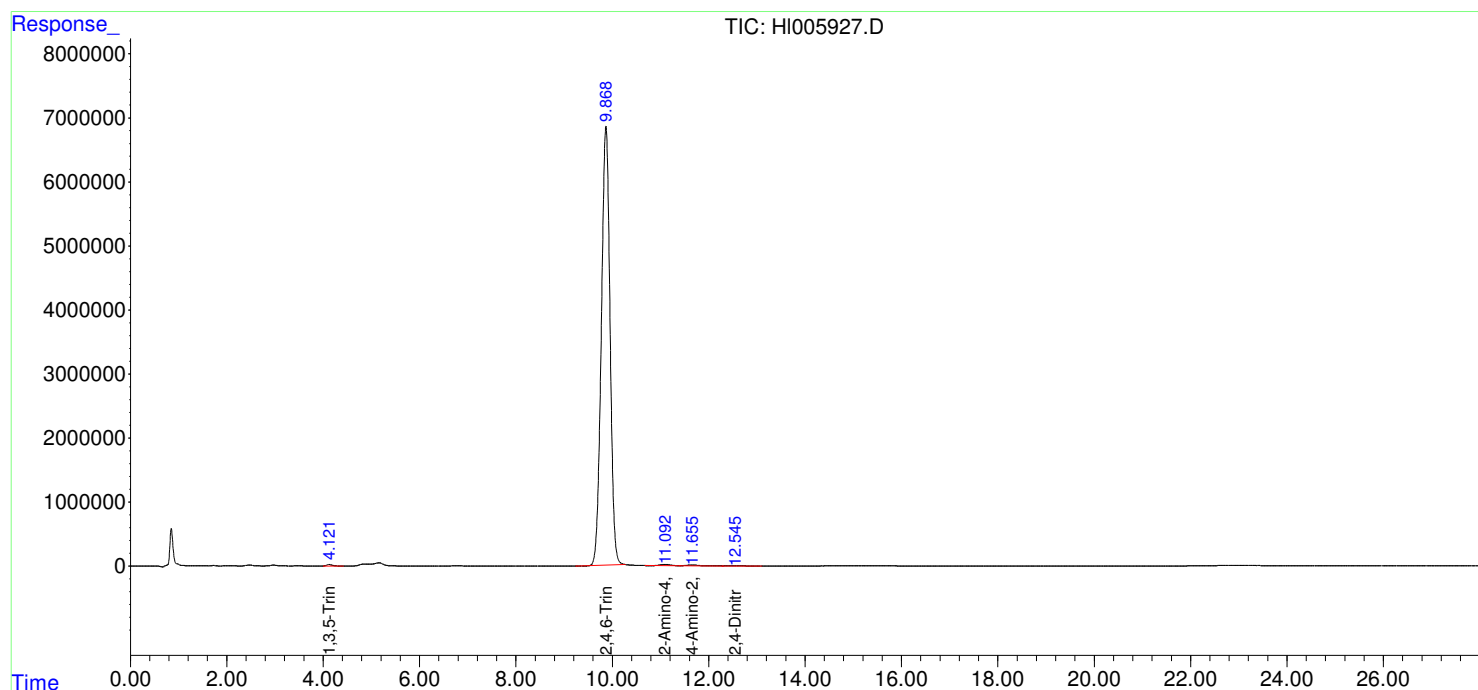


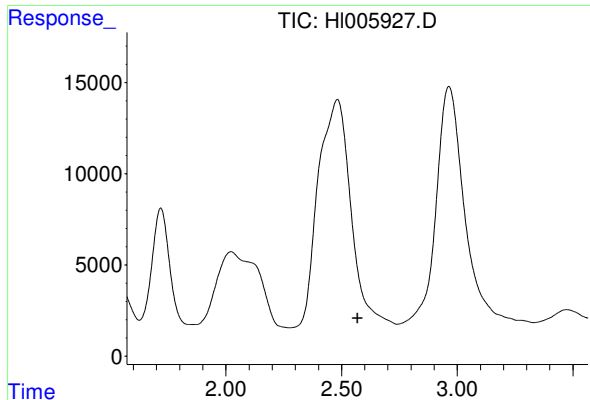

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 2.569 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
YS19-SB41-1014

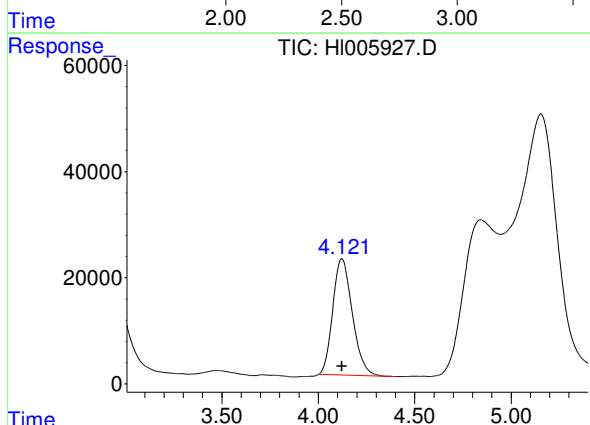


#4 1,3,5-Trinitrobenzene

R.T.: 4.123 min
Delta R.T.: 0.000 min
Response: 1543851
Conc: 92.92 ug/L

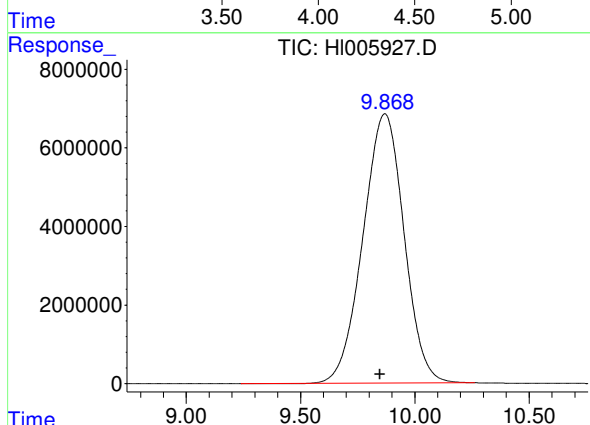


#9 2,4,6-Trinitrotoluene

R.T.: 9.869 min
Delta R.T.: 0.023 min
Response: 857995786
Conc: 48247.43 ug/L

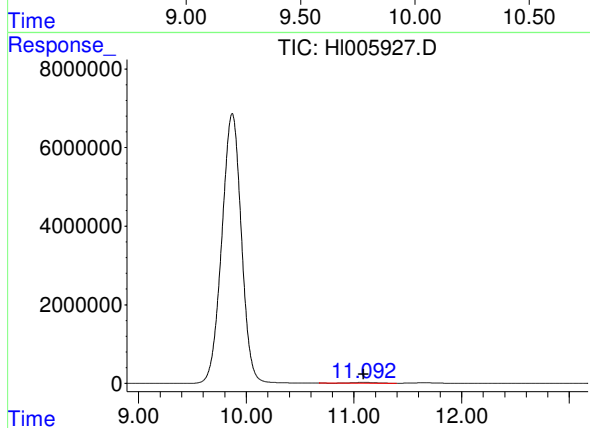

#10 2-Amino-4,6-dinitrotoluene


R.T.: 11.091 min
Delta R.T.: 0.002 min
Response: 2715754
Conc: 171.56 ug/L

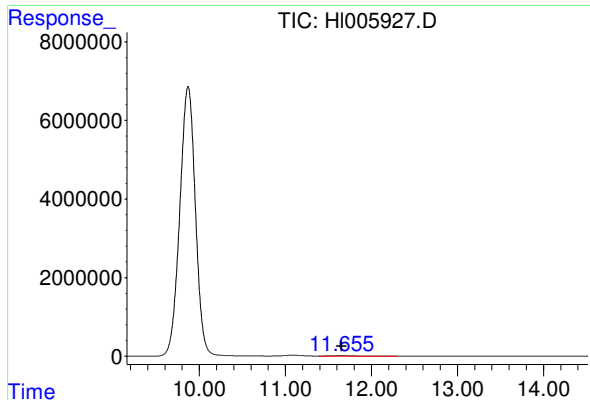

#11 4-Amino-2,6-dinitrotoluene

R.T.: 11.656 min
Delta R.T.: 0.003 min
Response: 1793663
Conc: 171.78 ug/L

Instrument :
HPLC_L
ClientSampleId :
YS19-SB41-1014

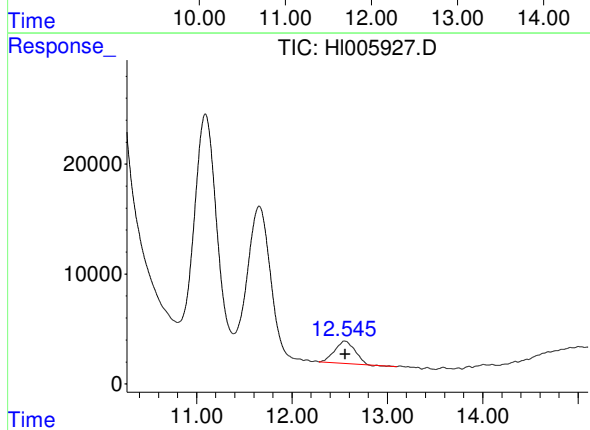

#12 2,4-Dinitrotoluene

R.T.: 12.555 min
Delta R.T.: -0.004 min
Response: 299272
Conc: 13.39 ug/L