

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120814\
 Data File : H1005932.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 08-Dec-2014, 21:48
 Operator : TP
 Sample : F4372-03
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 YS19-SD01-1014MSD

Integration File signal 1: AUTOINT1.E
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 06:55:54 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120814.M
 Quant Title :
 QLast Update : Mon Mar 09 13:49:54 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.578	968878	40.301 ug/L
Target Compounds			
2) T HMX	1.473	692879	111.967 ug/L
3) T RDX	2.578	968878	68.578 ug/L
4) T 1,3,5-Trinitrobenzene	4.130	1196066	71.985 ug/L
5) T 1,3-Dinitrobenzene	5.445	3047997	124.868 ng/ml
13) T 2,6-Dinitrotoluene	12.968	2241960	189.021 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120814\
Data File : H1005932.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 08-Dec-2014, 21:48
Operator : TP
Sample : F4372-03
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
YS19-SD01-1014MSD

Integration File signal 1: AUTOINT1.E
Integration File signal 2: autoint2.e
Quant Time: Mar 12 06:55:54 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120814.M
Quant Title :
QLast Update : Mon Mar 09 13:49:54 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

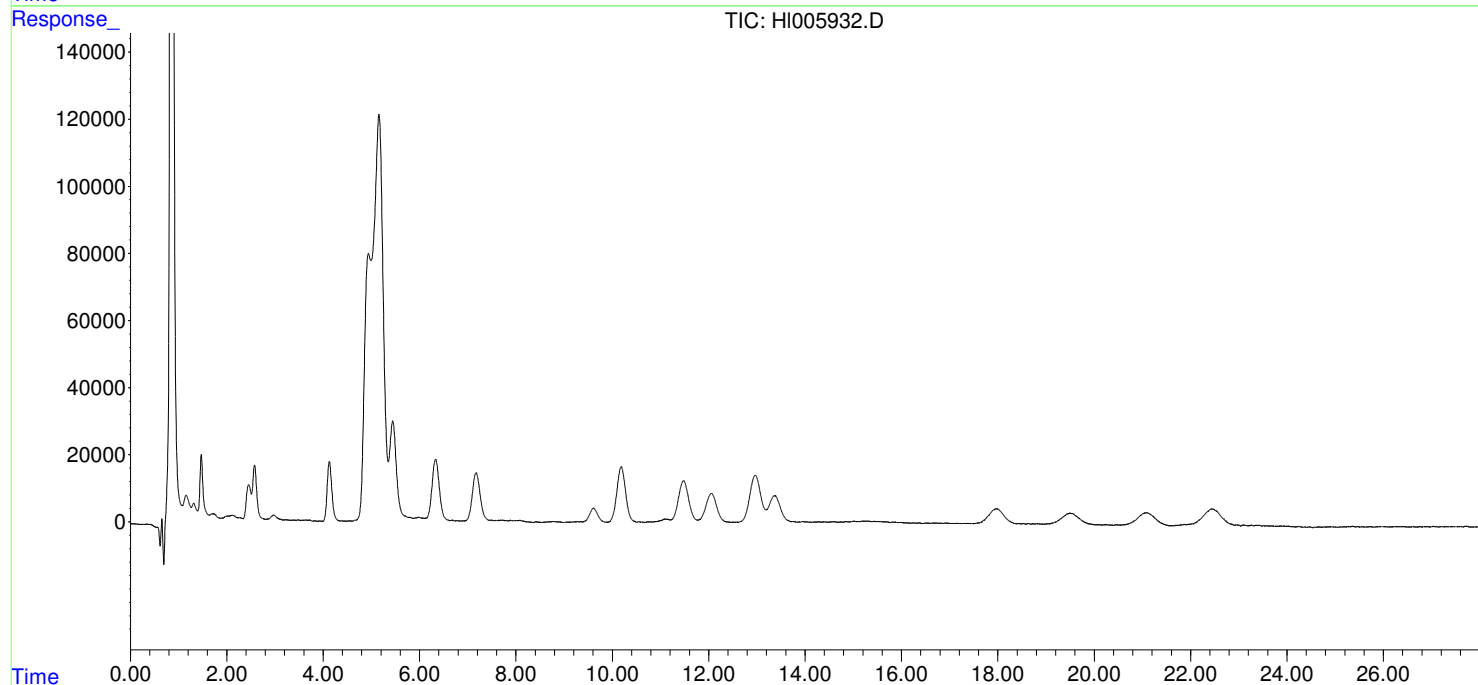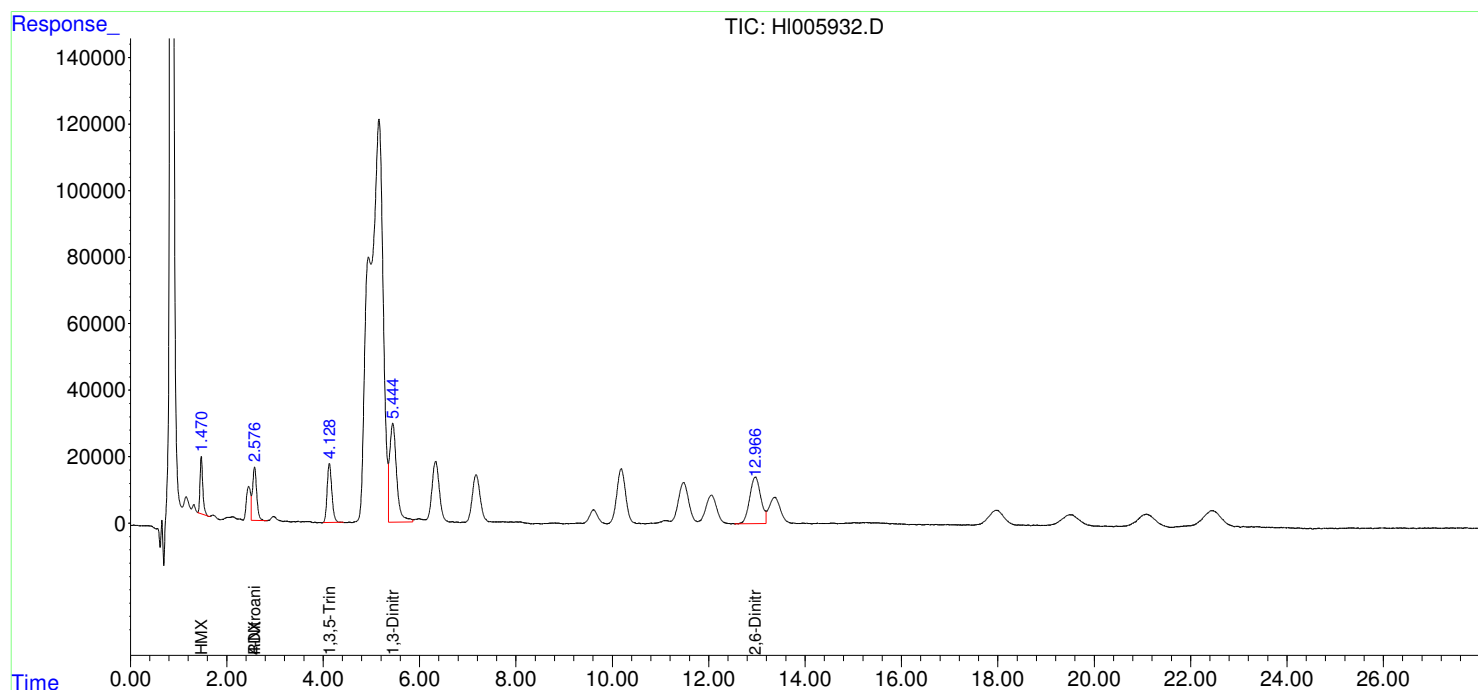


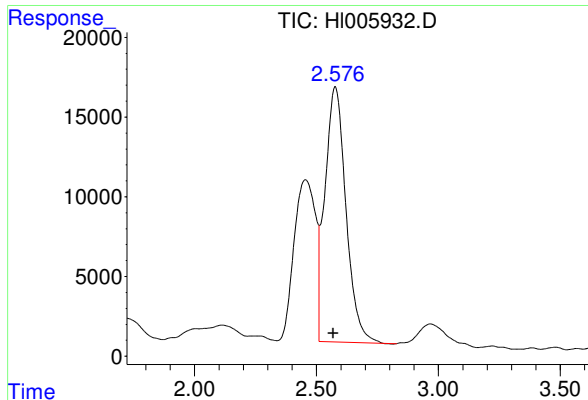

#1 4-Nitroaniline


R.T.: 2.578 min
Delta R.T.: 0.009 min
Response: 968878
Conc: 40.30 ug/L

Instrument :
HPLC_L
ClientSampleId :
YS19-SD01-1014MSD

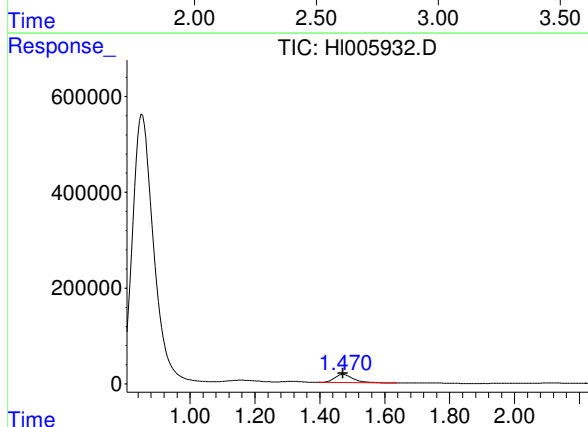


#2 HMX

R.T.: 1.473 min
Delta R.T.: 0.001 min
Response: 692879
Conc: 111.97 ug/L

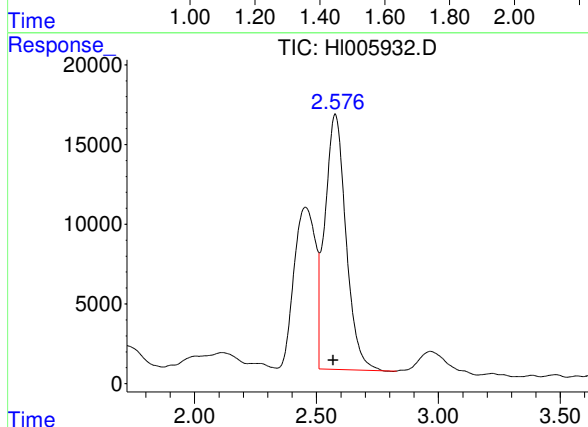


#3 RDX

R.T.: 2.578 min
Delta R.T.: 0.009 min
Response: 968878
Conc: 68.58 ug/L

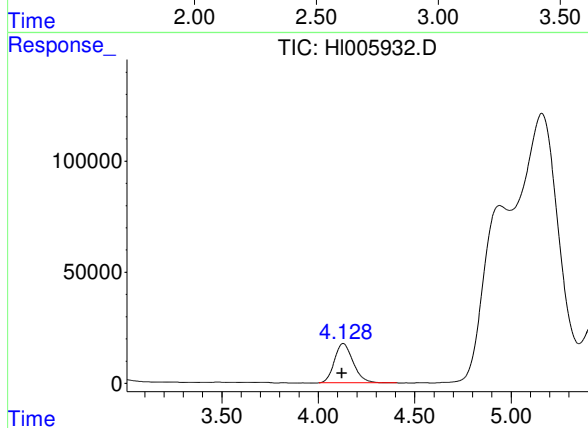

#4 1,3,5-Trinitrobenzene


R.T.: 4.130 min
Delta R.T.: 0.008 min
Response: 1196066
Conc: 71.98 ug/L

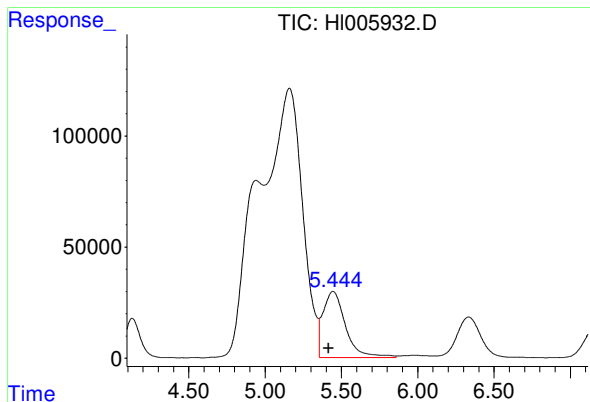

#5 1,3-Dinitrobenzene

R.T.: 5.445 min
Delta R.T.: 0.029 min
Response: 3047997
Conc: 124.87 ng/ml

Instrument :
HPLC_L
ClientSampleId :
YS19-SD01-1014MSD

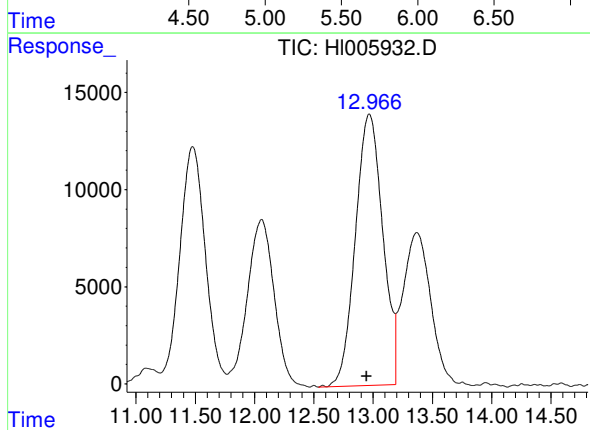

#13 2,6-Dinitrotoluene

R.T.: 12.968 min
Delta R.T.: 0.022 min
Response: 2241960
Conc: 189.02 ug/L