

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120814\
 Data File : H1005933.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 08-Dec-2014, 22:18
 Operator : TP
 Sample : HSTDCCC0500
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 HSTDCCC0500

Integration File signal 1: AUTOINT1.E
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 06:55:58 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120814.M
 Quant Title :
 QLast Update : Mon Mar 09 13:49:54 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.566	6656085	465.089 ug/L
Target Compounds			
2) T HMX	1.469	3063937	495.121 ug/L
3) T RDX	2.566	6656085	471.122 ug/L
4) T 1,3,5-Trinitrobenzene	4.122	7776214	468.010 ug/L
5) T 1,3-Dinitrobenzene	5.416	11974058	490.543 ng/ml
6) T 3,5-Dinitroaniline	6.216	9204696	484.744 ug/L
7) T Nitrobenzene	6.986	6974080	486.585 ug/L
13) T 2,6-Dinitrotoluene	12.966	11005582	927.888 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120814\
Data File : H1005933.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 08-Dec-2014, 22:18
Operator : TP
Sample : HSTDCCC0500
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HSTDCCC0500

Integration File signal 1: AUTOINT1.E
Integration File signal 2: autoint2.e
Quant Time: Mar 12 06:55:58 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120814.M
Quant Title :
QLast Update : Mon Mar 09 13:49:54 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

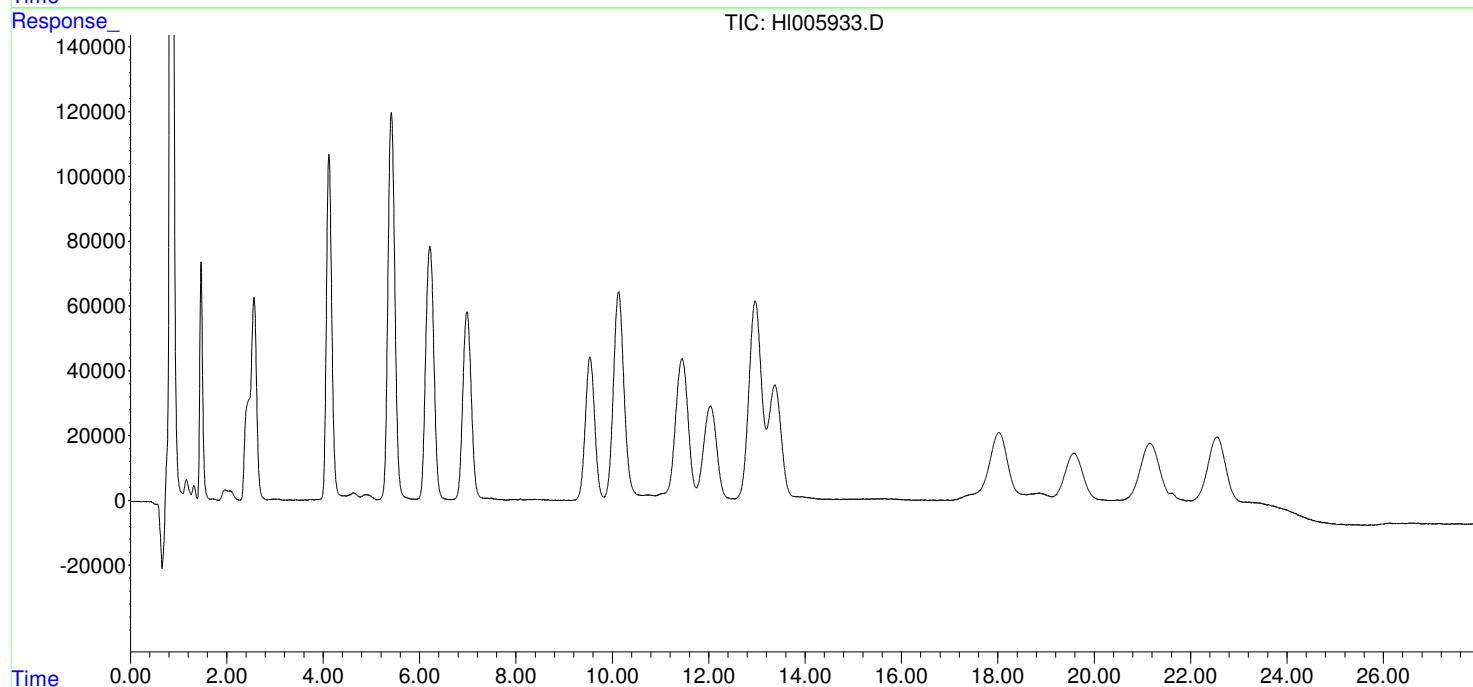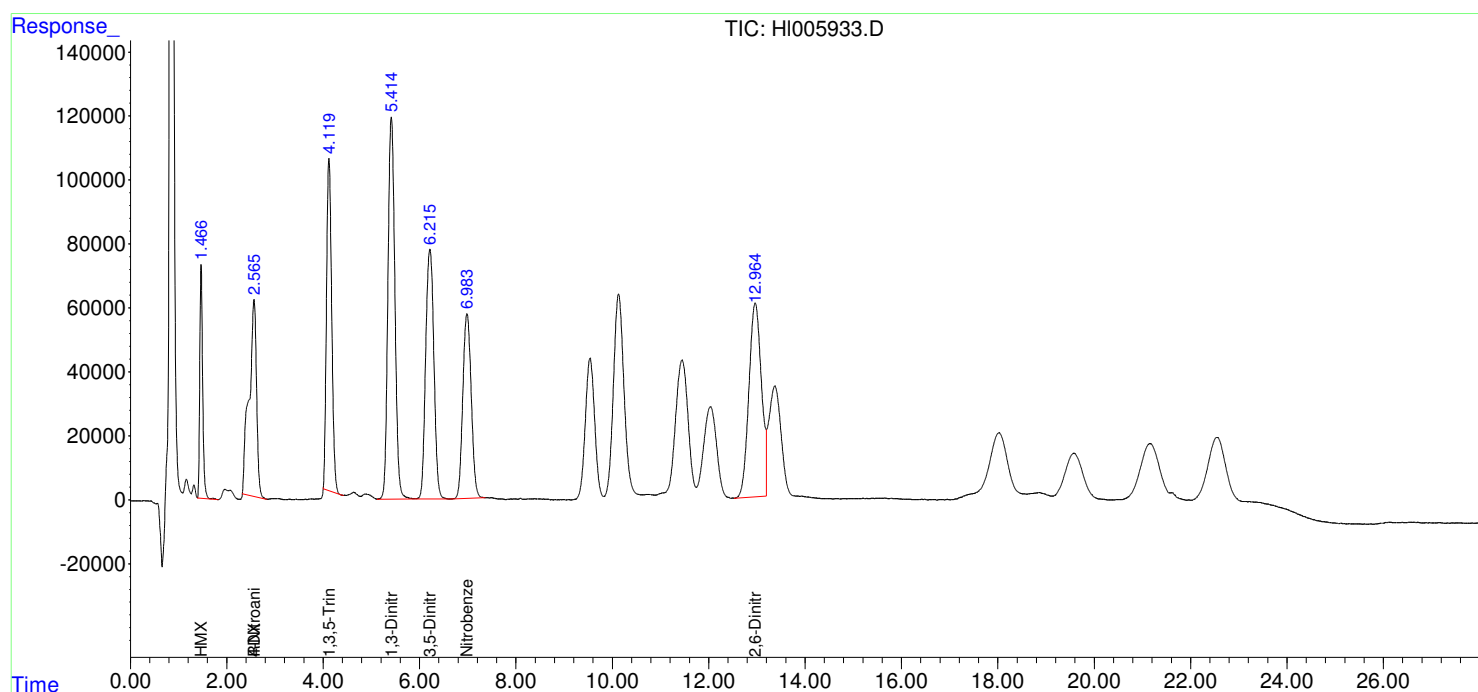


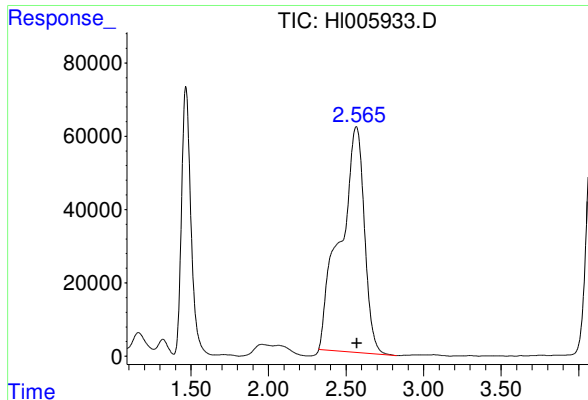

#1 4-Nitroaniline


R.T.: 2.566 min
Delta R.T.: -0.003 min
Response: 6656085
Conc: 465.09 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDCCC0500

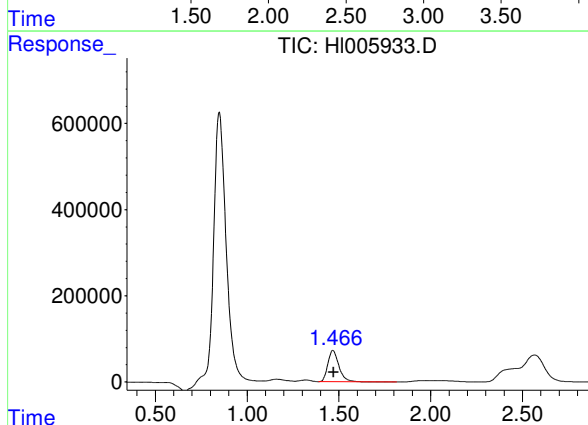


#2 HMX

R.T.: 1.469 min
Delta R.T.: -0.002 min
Response: 3063937
Conc: 495.12 ug/L

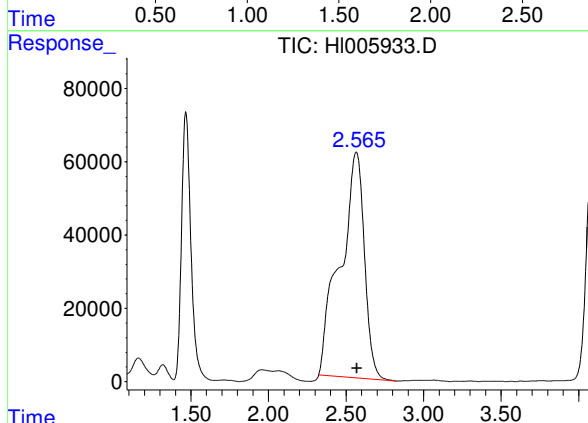


#3 RDX

R.T.: 2.566 min
Delta R.T.: -0.003 min
Response: 6656085
Conc: 471.12 ug/L

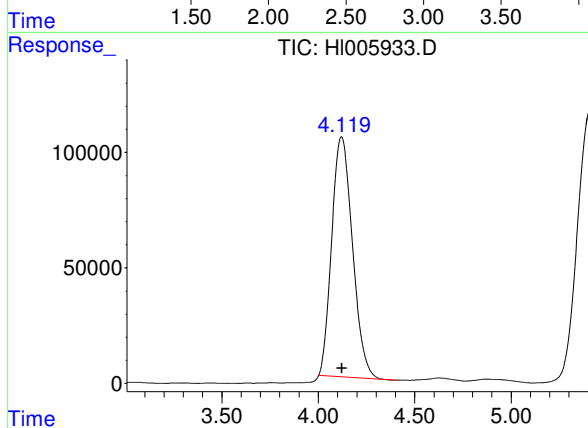

#4 1,3,5-Trinitrobenzene


R.T.: 4.122 min
Delta R.T.: -0.001 min
Response: 7776214
Conc: 468.01 ug/L

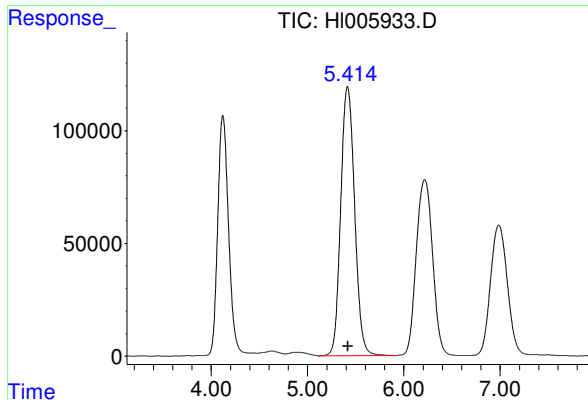

#5 1,3-Dinitrobenzene


R.T.: 5.416 min
Delta R.T.: 0.000 min
Response: 11974058
Conc: 490.54 ng/ml

Instrument :
HPLC_L
ClientSampleId :
HSTDCCC0500

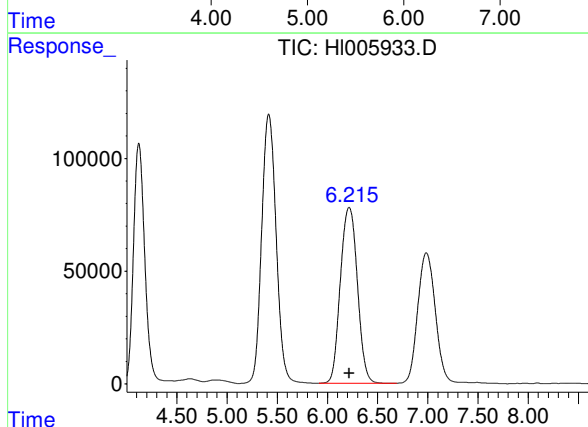


#6 3,5-Dinitroaniline

R.T.: 6.216 min
Delta R.T.: 0.002 min
Response: 9204696
Conc: 484.74 ug/L

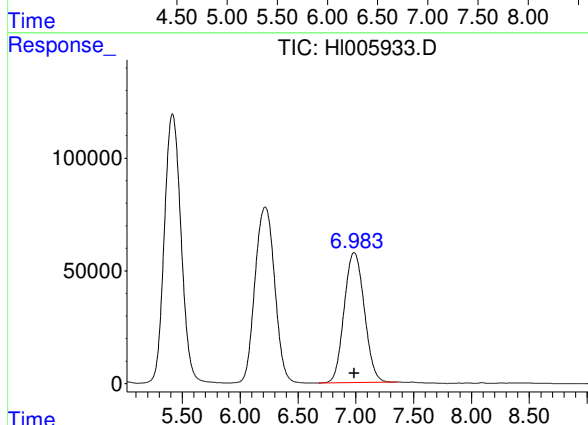

#7 Nitrobenzene

R.T.: 6.986 min
Delta R.T.: 0.000 min
Response: 6974080
Conc: 486.59 ug/L

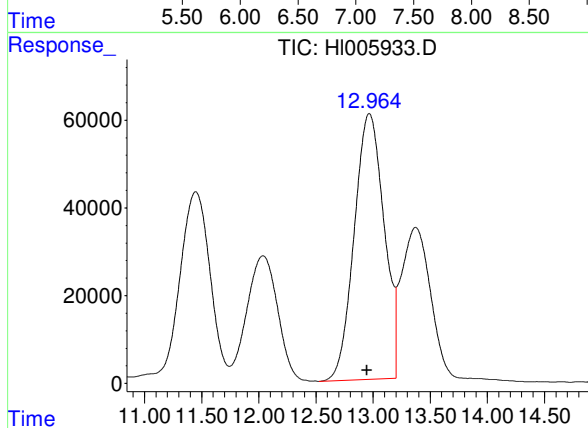

#13 2,6-Dinitrotoluene

R.T.: 12.966 min
Delta R.T.: 0.021 min
Response: 11005582
Conc: 927.89 ug/L