

Data Path : Z:\HPCHEM1\HPLC\_L\Data\HL120814\  
Data File : HL005929.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 08-Dec-2014, 20:20  
Operator : TP  
Sample : F4368-06DL2 200X  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
HPLC\_L  
ClientSampleId :  
YS19-SB41-1014DL2

Integration File signal 1: AUTOINT1.E  
Integration File signal 2: autoint2.e  
Quant Time: Dec 10 08:40:42 2014  
Quant Method : Z:\HPCHEM1\HPLC\_L\METHODS\HL120814.M  
Quant Title :  
QLast Update : Tue Dec 09 09:49:22 2014  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 uL  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

| Compound                    | R.T.   | Response | Conc Units      |
|-----------------------------|--------|----------|-----------------|
| -----                       |        |          |                 |
| System Monitoring Compounds |        |          |                 |
| Target Compounds            |        |          |                 |
| 9) T 2,4,6-Trinitrotoluene  | 10.027 | 45434413 | 2539.662 ug/L m |
| -----                       |        |          |                 |

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC\_L\Data\HL120814\  
Data File : H1005929.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 08-Dec-2014, 20:20  
Operator : TP  
Sample : F4368-06DL2 200X  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
HPLC\_L  
ClientSampleId :  
YS19-SB41-1014DL2

Integration File signal 1: AUTOINT1.E  
Integration File signal 2: autoint2.e  
Quant Time: Dec 10 08:40:42 2014  
Quant Method : Z:\HPCHEM1\HPLC\_L\METHODS\HL120814.M  
Quant Title :  
QLast Update : Tue Dec 09 09:49:22 2014  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

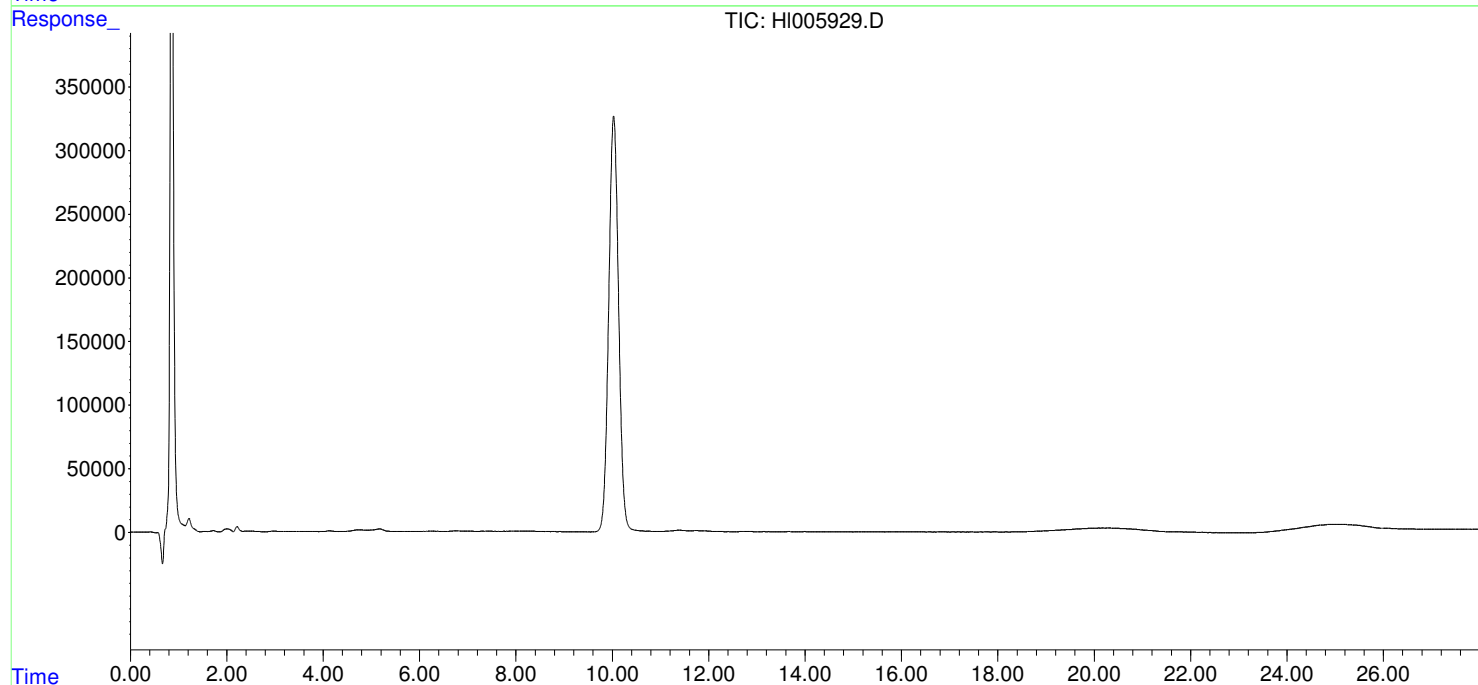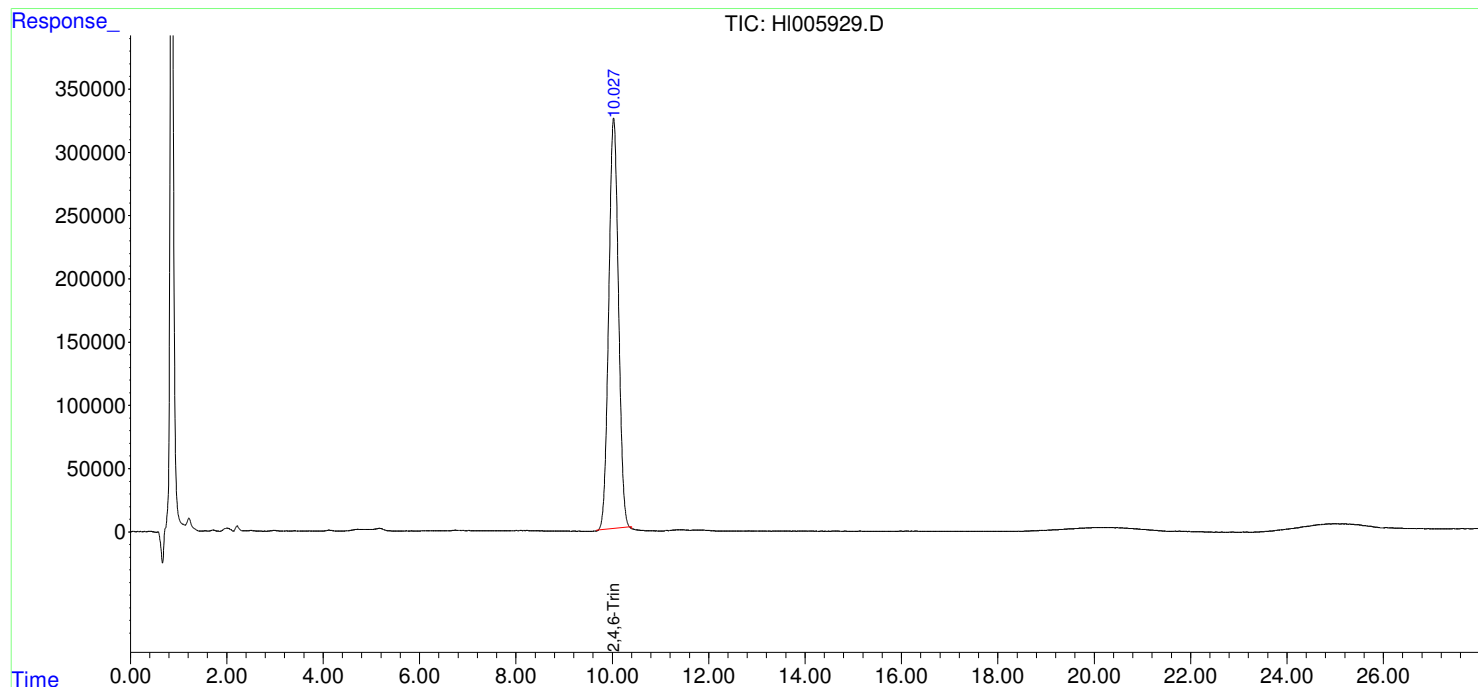


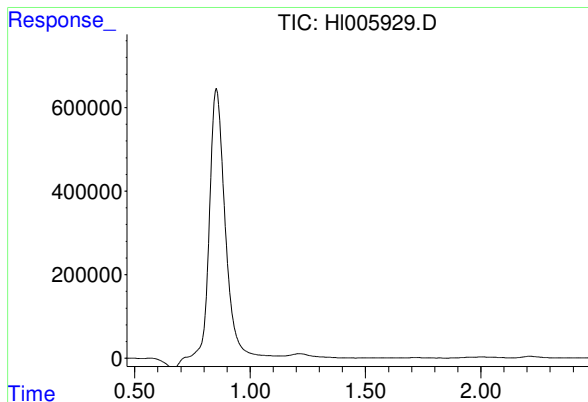

#1 4-Nitroaniline

R.T.: 0.000 min  
Exp R.T.: 1.464 min  
Response: 0  
Conc: N.D.

Instrument :  
HPLC\_L  
ClientSampleId :  
YS19-SB41-1014DL2

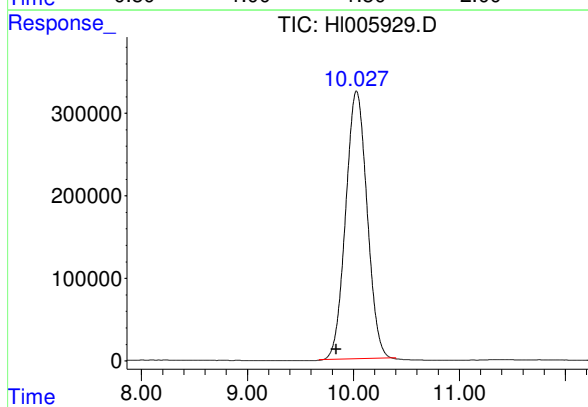

#9 2,4,6-Trinitrotoluene

R.T.: 10.027 min  
Delta R.T.: 0.190 min  
Response: 45434413  
Conc: 2539.66 ug/L m