

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120814\
 Data File : HL005936.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 08-Dec-2014, 23:46
 Operator : TP
 Sample : F4372-06
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 YS19-SD16-1014

Integration File signal 1: AUTOINT1.E
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 15:16:42 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120814.M
 Quant Title :
 QLast Update : Mon Mar 09 13:49:54 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.456	853052	31.649 ug/L
Target Compounds			
4) T 1,3,5-Trinitrobenzene	4.133	175951	10.590 ug/L
9) T 2,4,6-Trinitrotoluene	9.862	3402239	191.317 ug/L
10) T 2-Amino-4,6-dinitroto...	11.113	977883	61.776 ug/L
11) T 4-Amino-2,6-dinitroto...	11.687	1664403	159.401 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL120814\
Data File : H1005936.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 08-Dec-2014, 23:46
Operator : TP
Sample : F4372-06
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampled :
YS19-SD16-1014

Integration File signal 1: AUTOINT1.E
Integration File signal 2: autoint2.e
Quant Time: Mar 09 15:16:42 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL120814.M
Quant Title :
QLast Update : Mon Mar 09 13:49:54 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

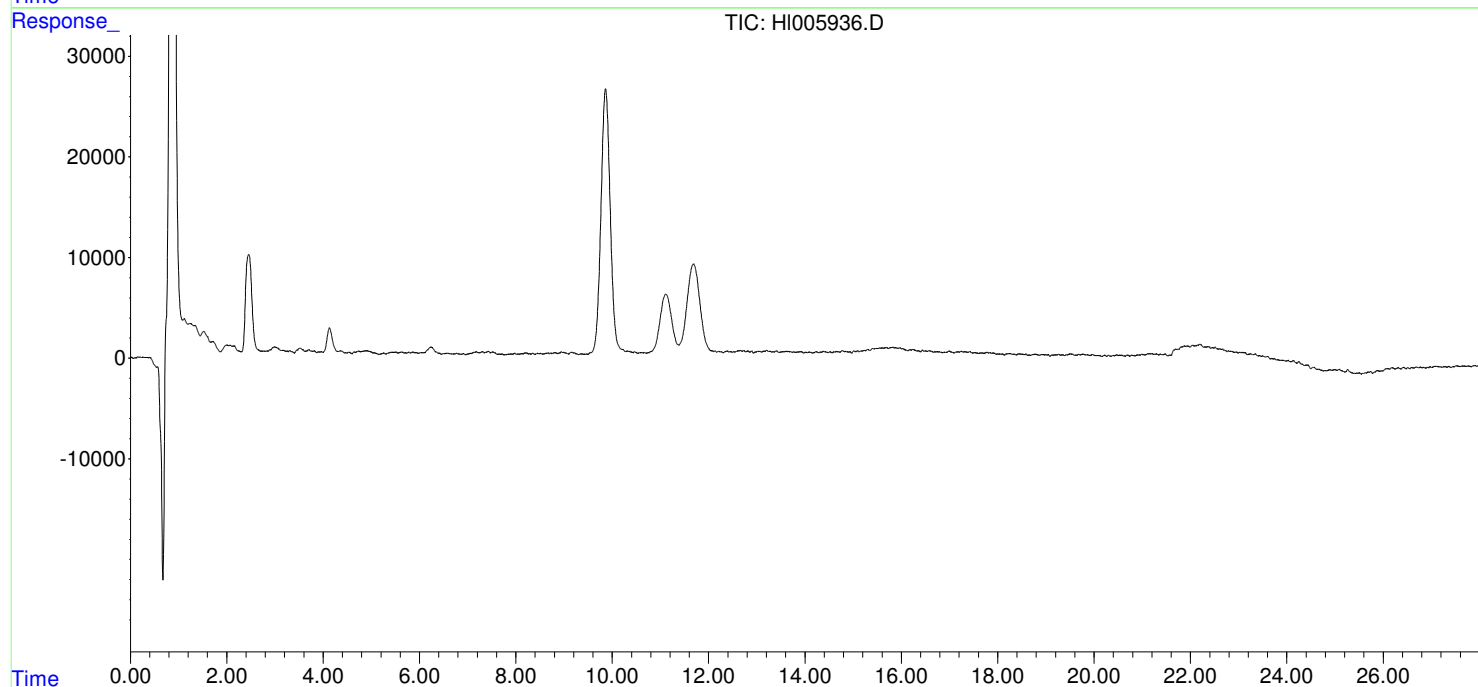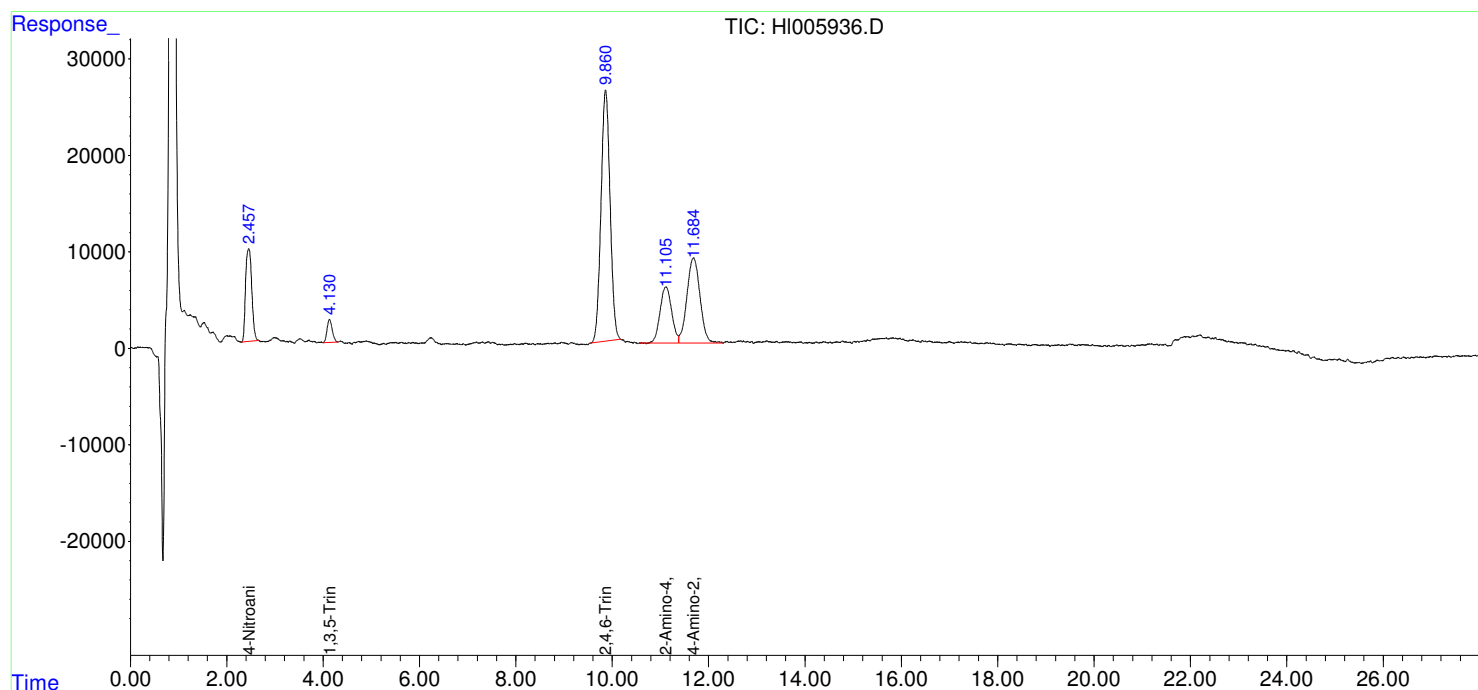


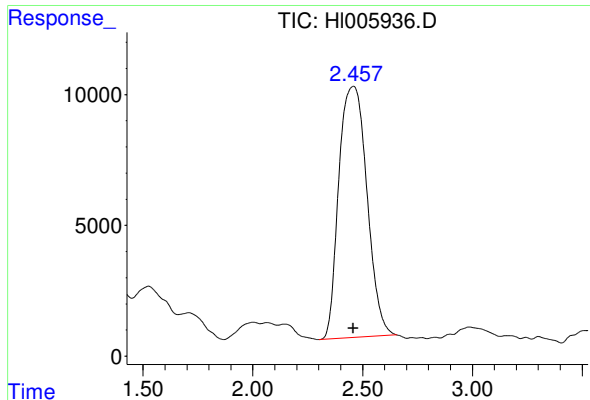

#1 4-Nitroaniline


R.T.: 2.456 min
Delta R.T.: -0.001 min
Response: 853052
Conc: 31.65 ug/L

Instrument :
HPLC_L
ClientSampleId :
YS19-SD16-1014

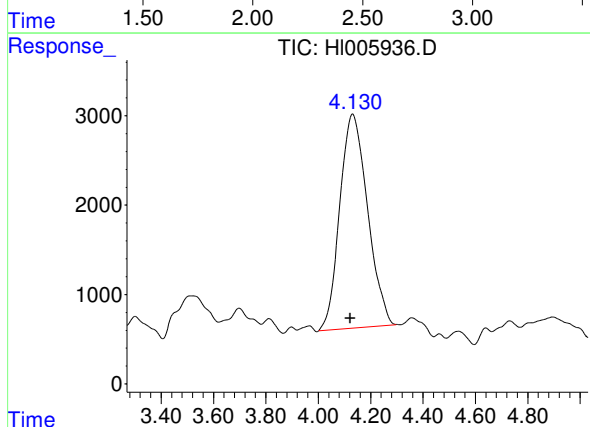


#4 1,3,5-Trinitrobenzene

R.T.: 4.133 min
Delta R.T.: 0.011 min
Response: 175951
Conc: 10.59 ug/L

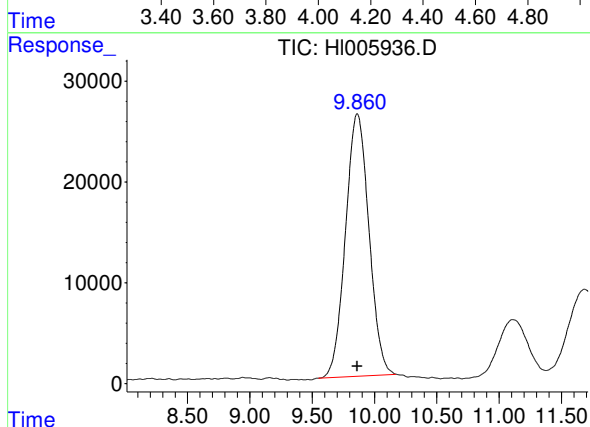


#9 2,4,6-Trinitrotoluene

R.T.: 9.862 min
Delta R.T.: 0.002 min
Response: 3402239
Conc: 191.32 ug/L

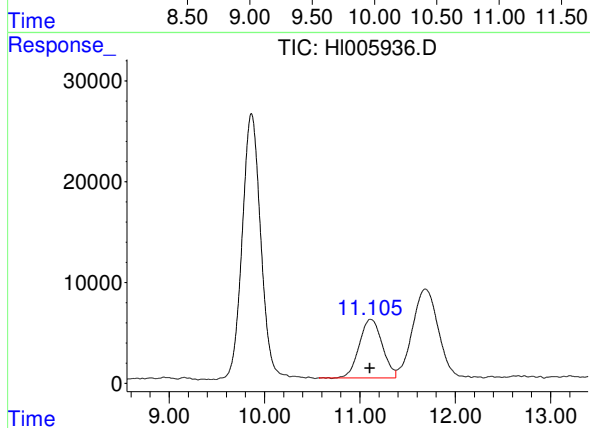

#10 2-Amino-4,6-dinitrotoluene

R.T.: 11.113 min
Delta R.T.: 0.008 min
Response: 977883
Conc: 61.78 ug/L

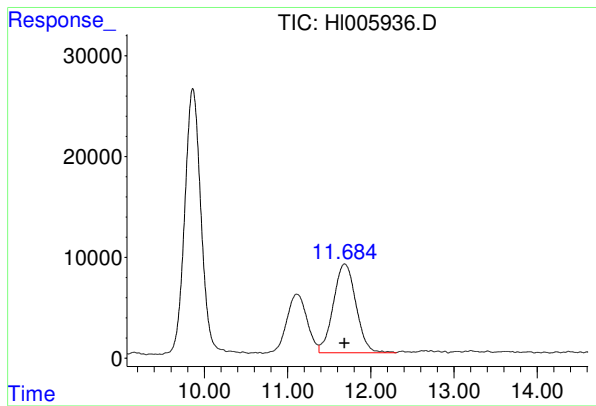

#11 4-Amino-2,6-dinitrotoluene

R.T.: 11.687 min
Delta R.T.: 0.003 min
Response: 1664403
Conc: 159.40 ug/L

Instrument :
HPLC_L
ClientSampleId :
YS19-SD16-1014