

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL122314\HL006046.D Vial: 10
Acq On : 24-Dec-2014, 00:25 Operator: TP/IZ
Sample : LOQ/LOD-WATER-BL Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Dec 26 4:30 2014 Quant Results File: HL122314.RES

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL122314.M
Title :
Last Update : Wed Dec 24 13:10:02 2014
Response via : Initial Calibration
DataAcq Meth : 8330CONF.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.48f	3112069	249.945 ug/L m

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL006046.D HL122314.M

Fri Jan 02 16:06:54 2015


RPT1


Quantitation Report

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL122314\HL006046.D Vial: 10
Acq On : 24-Dec-2014, 00:25 Operator: TP/IZ
Sample : LOQ/LOD-WATER-BL Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Dec 26 4:30 2014 Quant Results File: HL122314.RES

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL122314.M
Title :
Last Update : Wed Dec 24 13:10:02 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330CONF.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

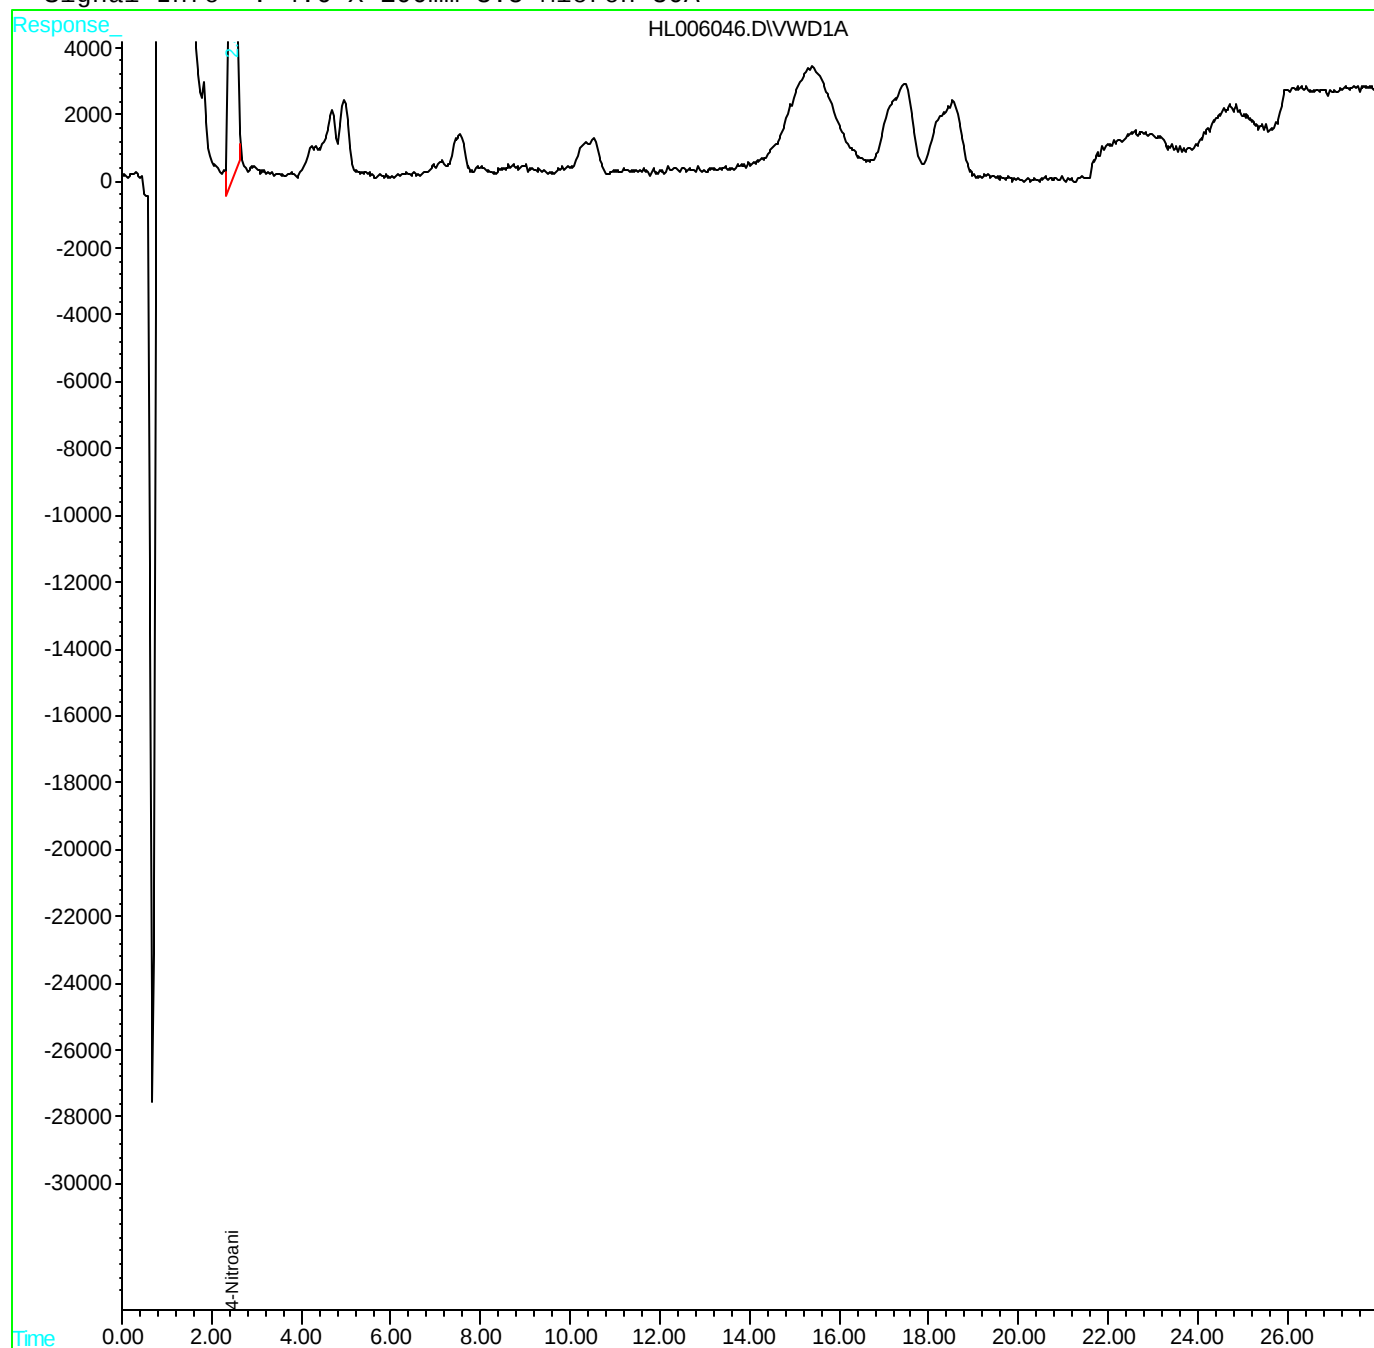

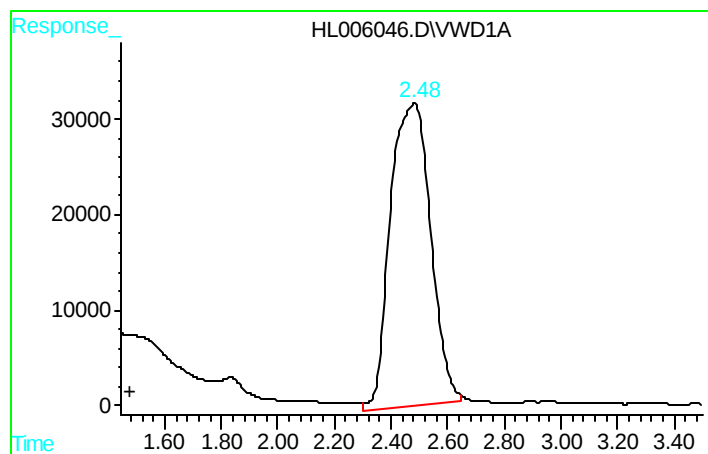

#1 4-Nitroaniline

R.T.: 2.481 min
Delta R.T.: 1.006 min
Response: 3112069
Conc: 249.94 ug/L m