

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN060514\HN006088.D Vial: 6
Acq On : 05-Jun-2014, 15:35 Operator: HNP
Sample : HSTDICC0020 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jun 5 17:41 2014 Quant Results File: HN060514.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Title :
Last Update : Tue May 20 07:20:33 2014
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.


HN006088.D HN060514.M Thu Jun 05 17:41:02 2014 RPT1


Quantitation Report

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN060514\HN006088.D Vial: 6
Acq On : 05-Jun-2014, 15:35 Operator: HNP
Sample : HSTDICC0020 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jun 5 17:41 2014 Quant Results File: HN060514.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Title :
Last Update : Tue May 20 07:20:33 2014
Response via : Single Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

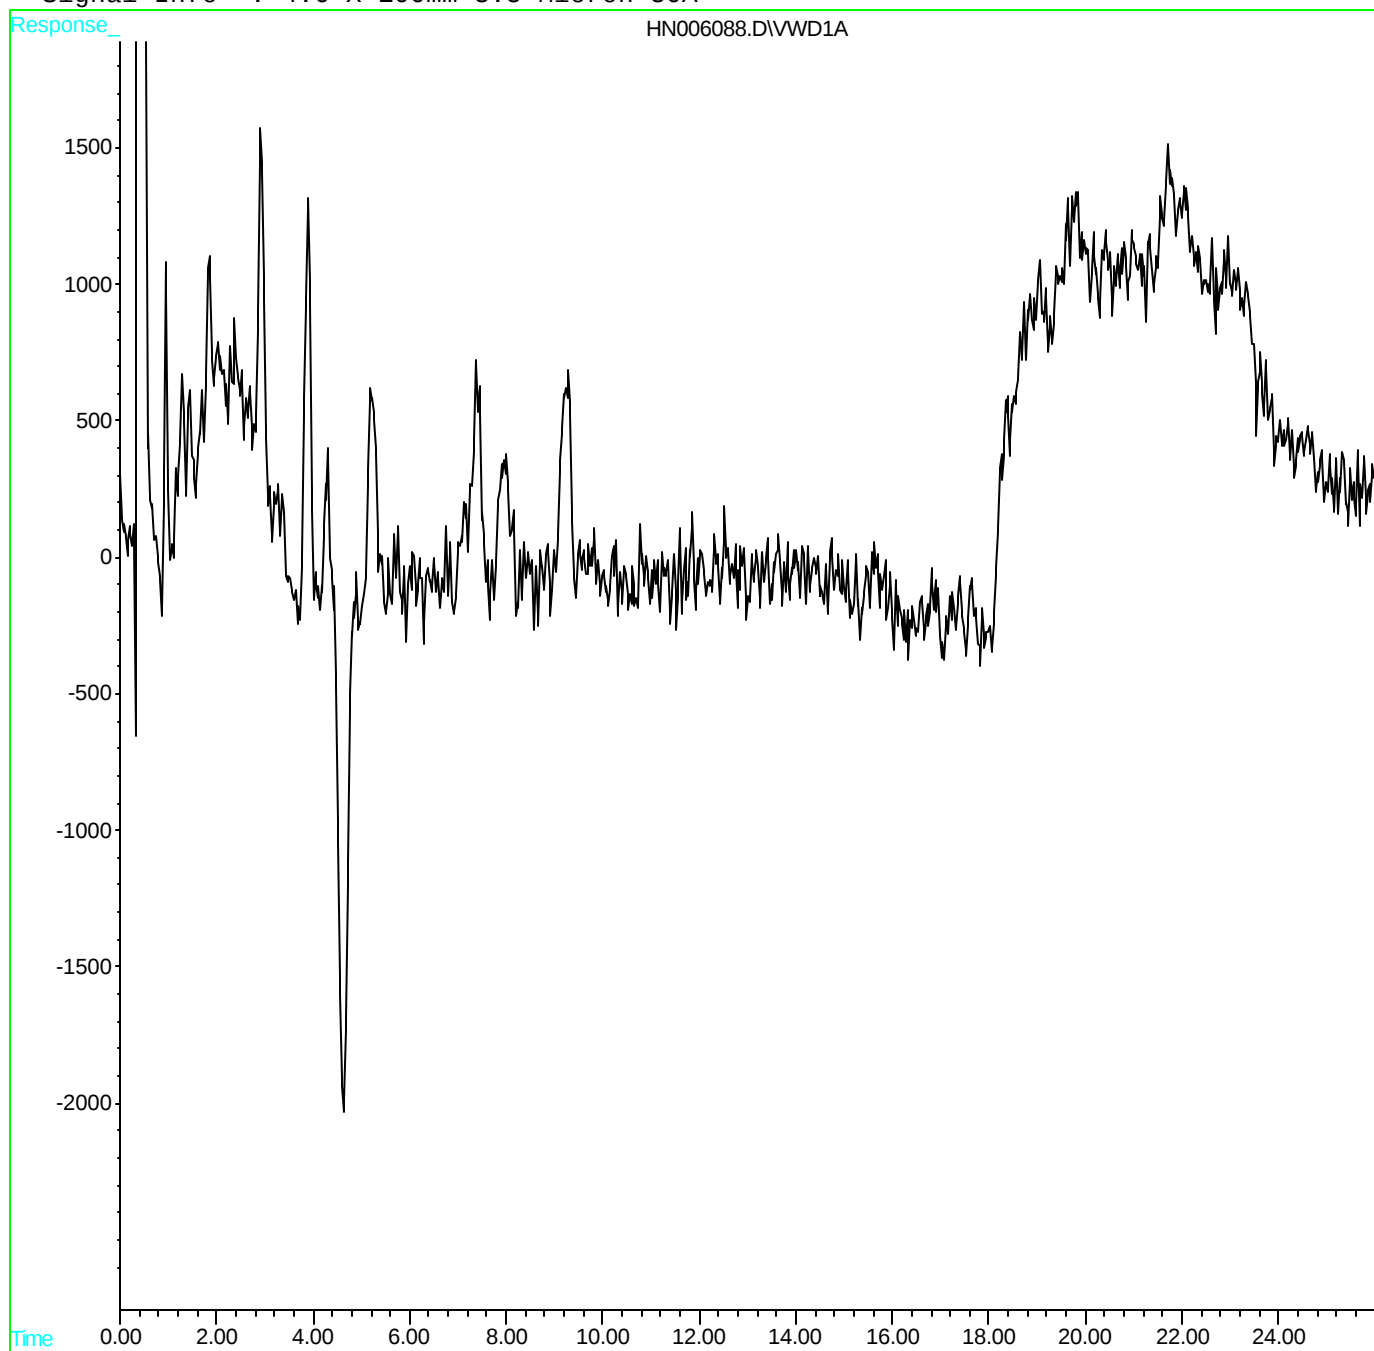

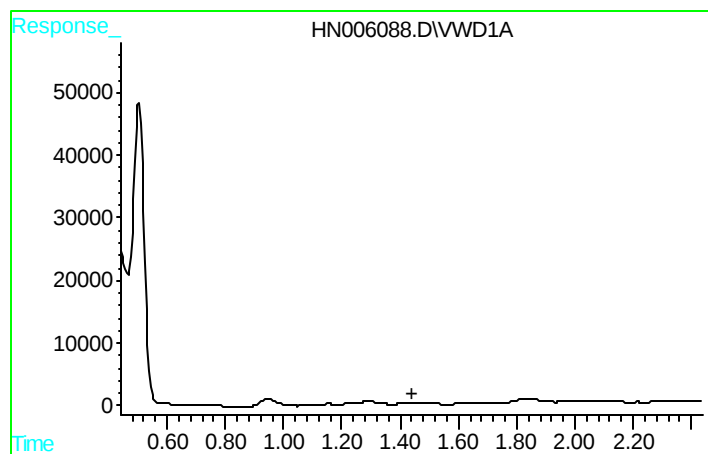

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T. : 1.440 min
Response: 0
Conc: N.D.