



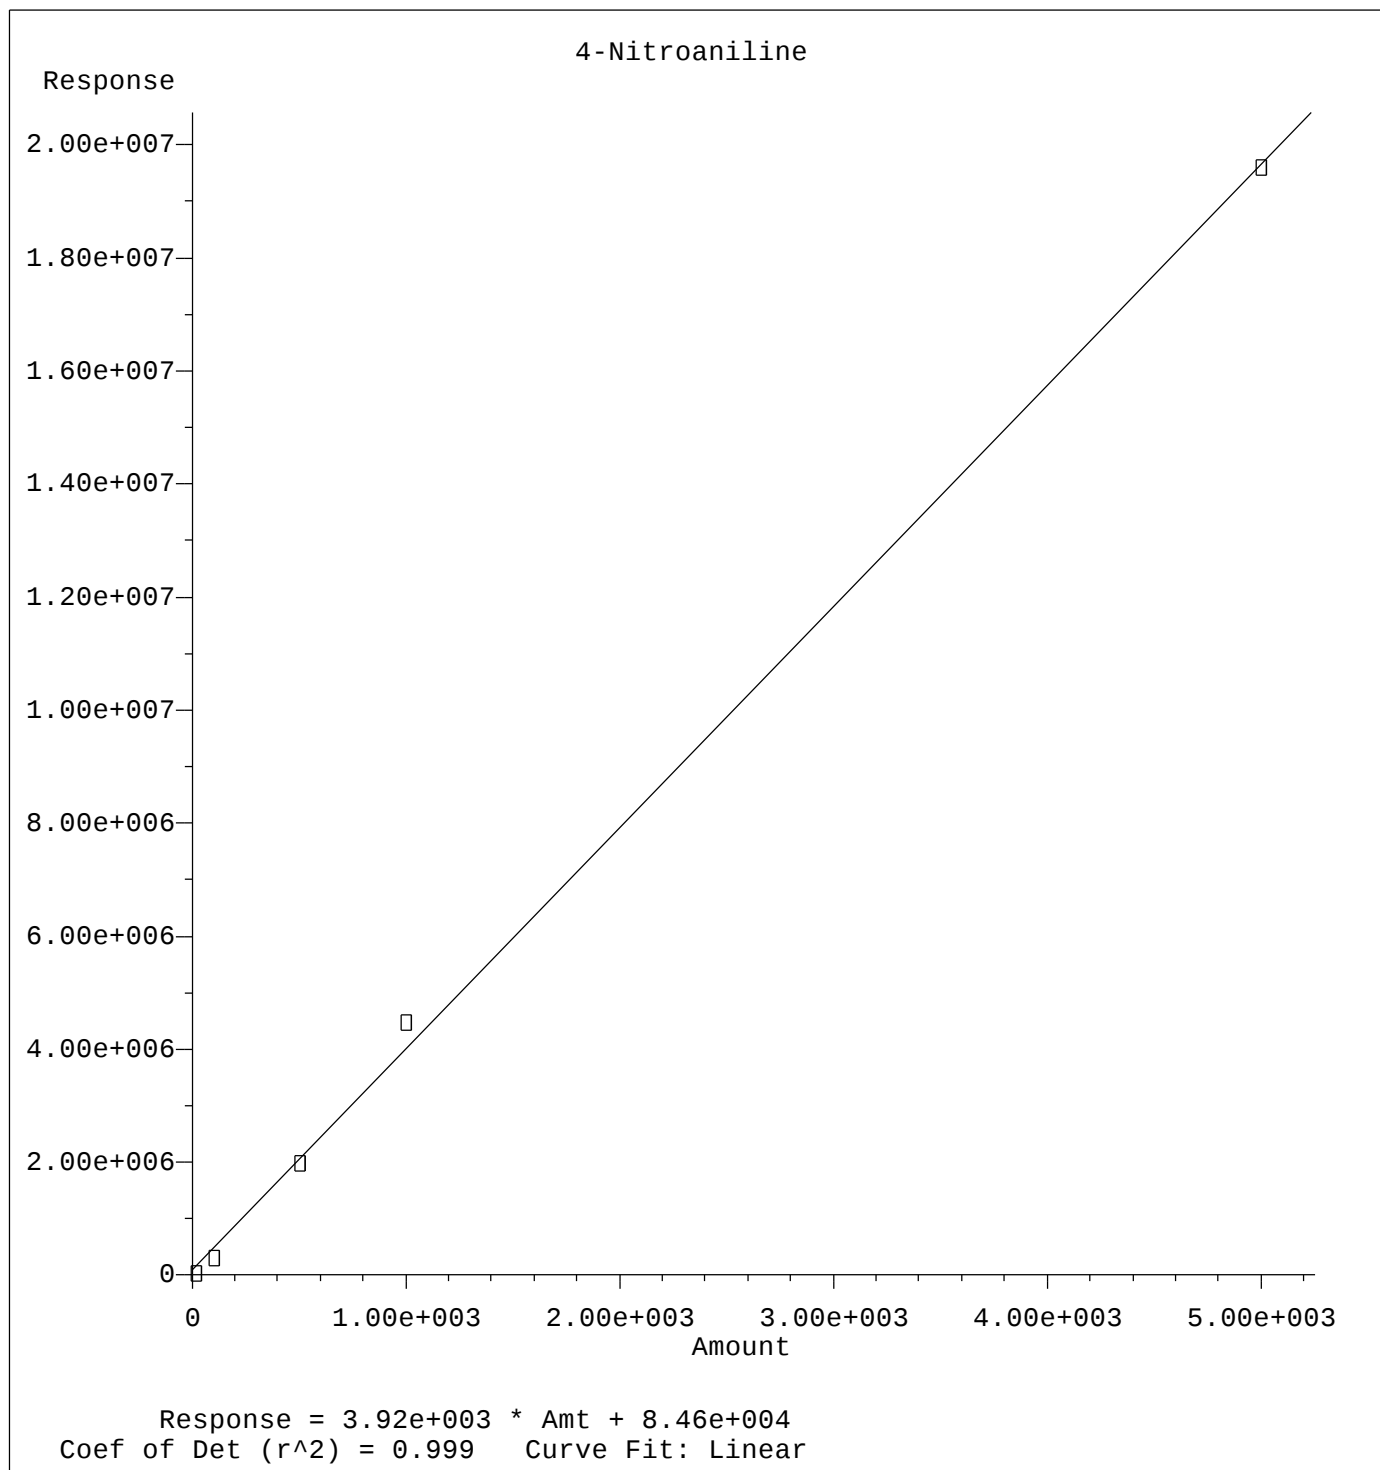


Method Name: Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Calibration Table Last Updated: Wed Jun 11 17:35:58 2014

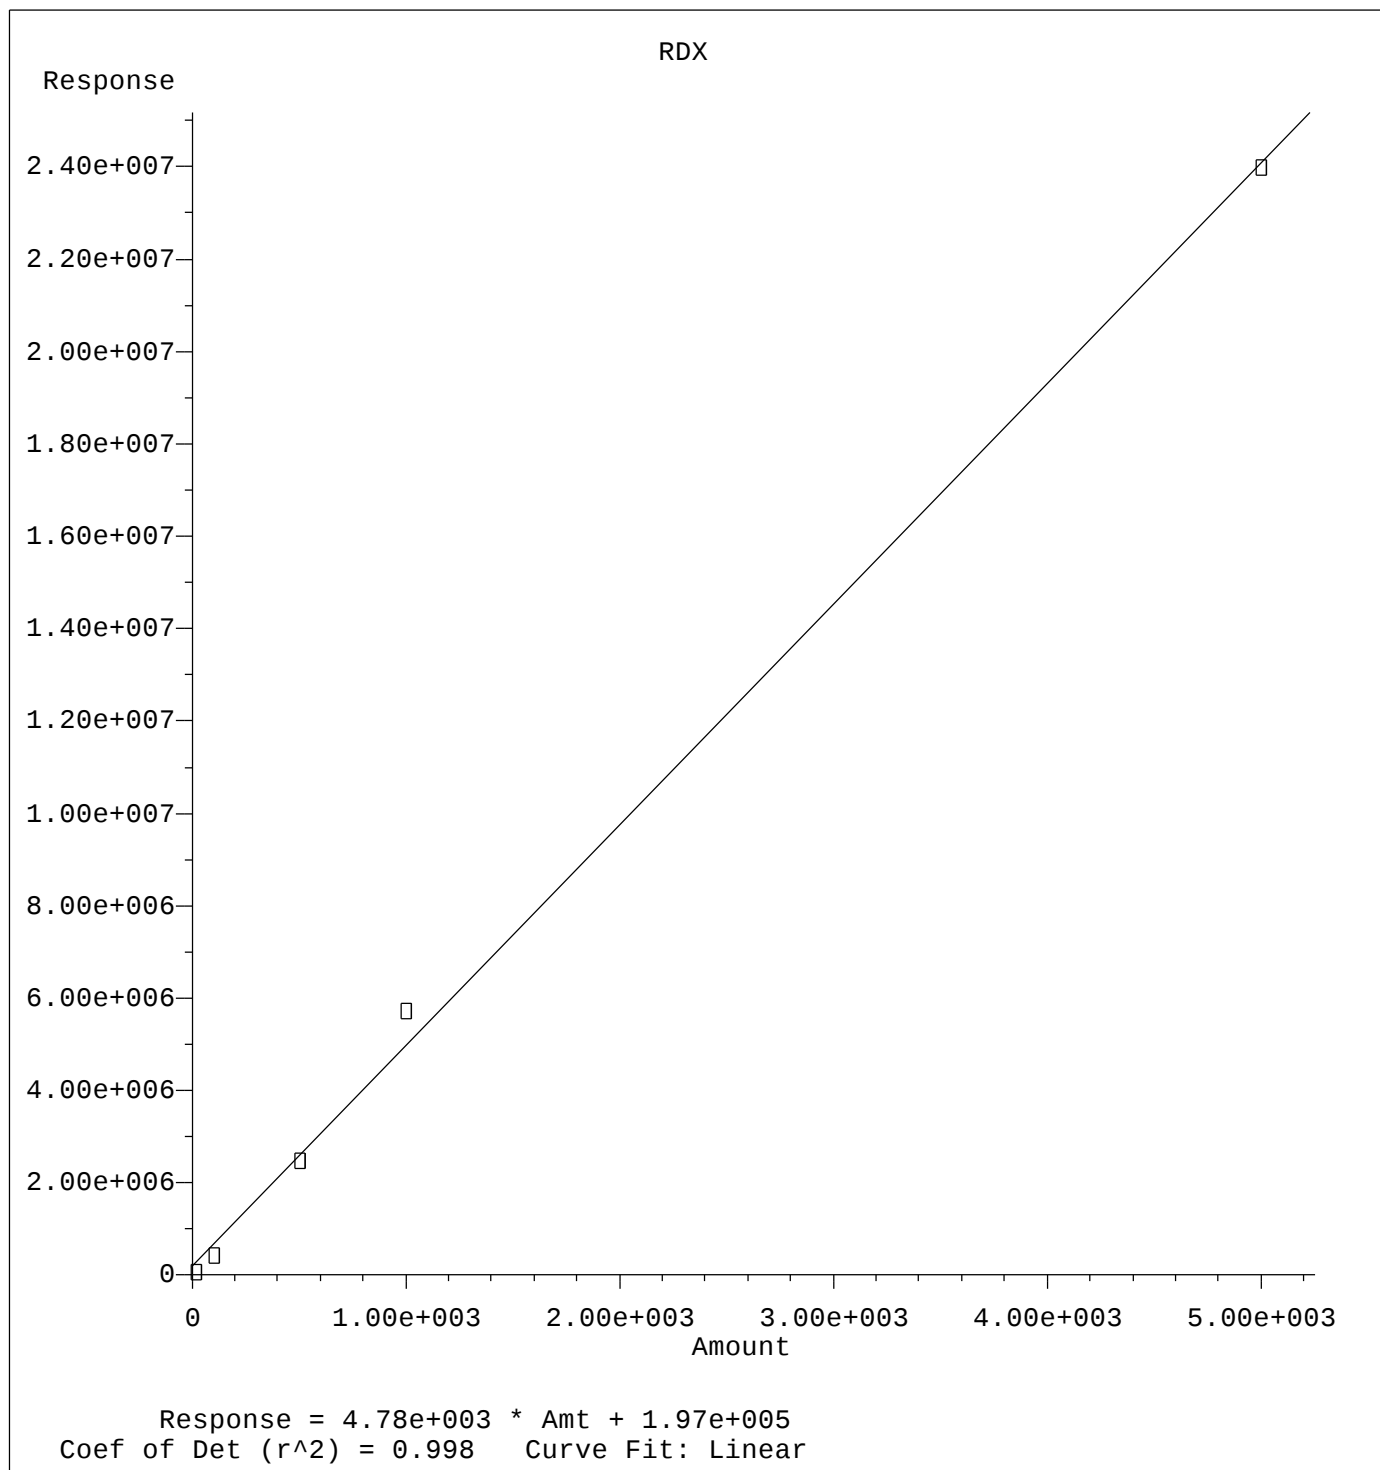


Method Name: Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Calibration Table Last Updated: Wed Jun 11 17:35:58 2014

1,3,5-Trinitrobenzene

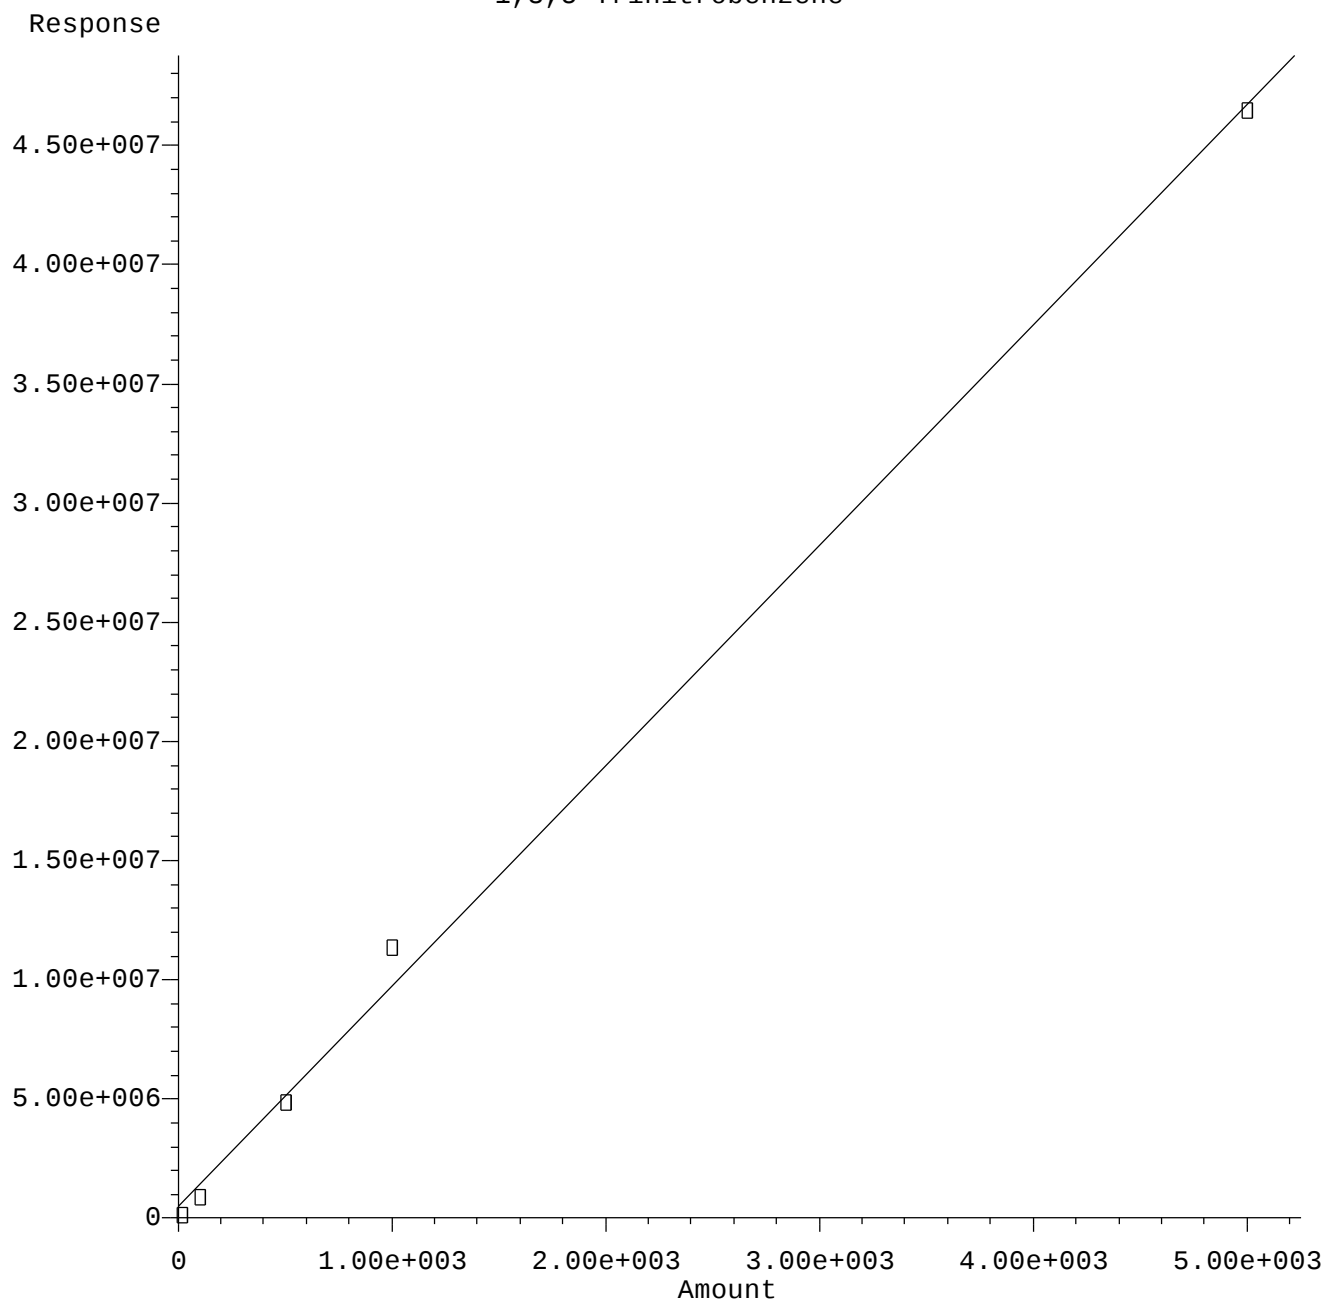


Response = $9.25 \times 10^3 \times \text{Amt} + 4.62 \times 10^5$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Calibration Table Last Updated: Wed Jun 11 17:35:58 2014

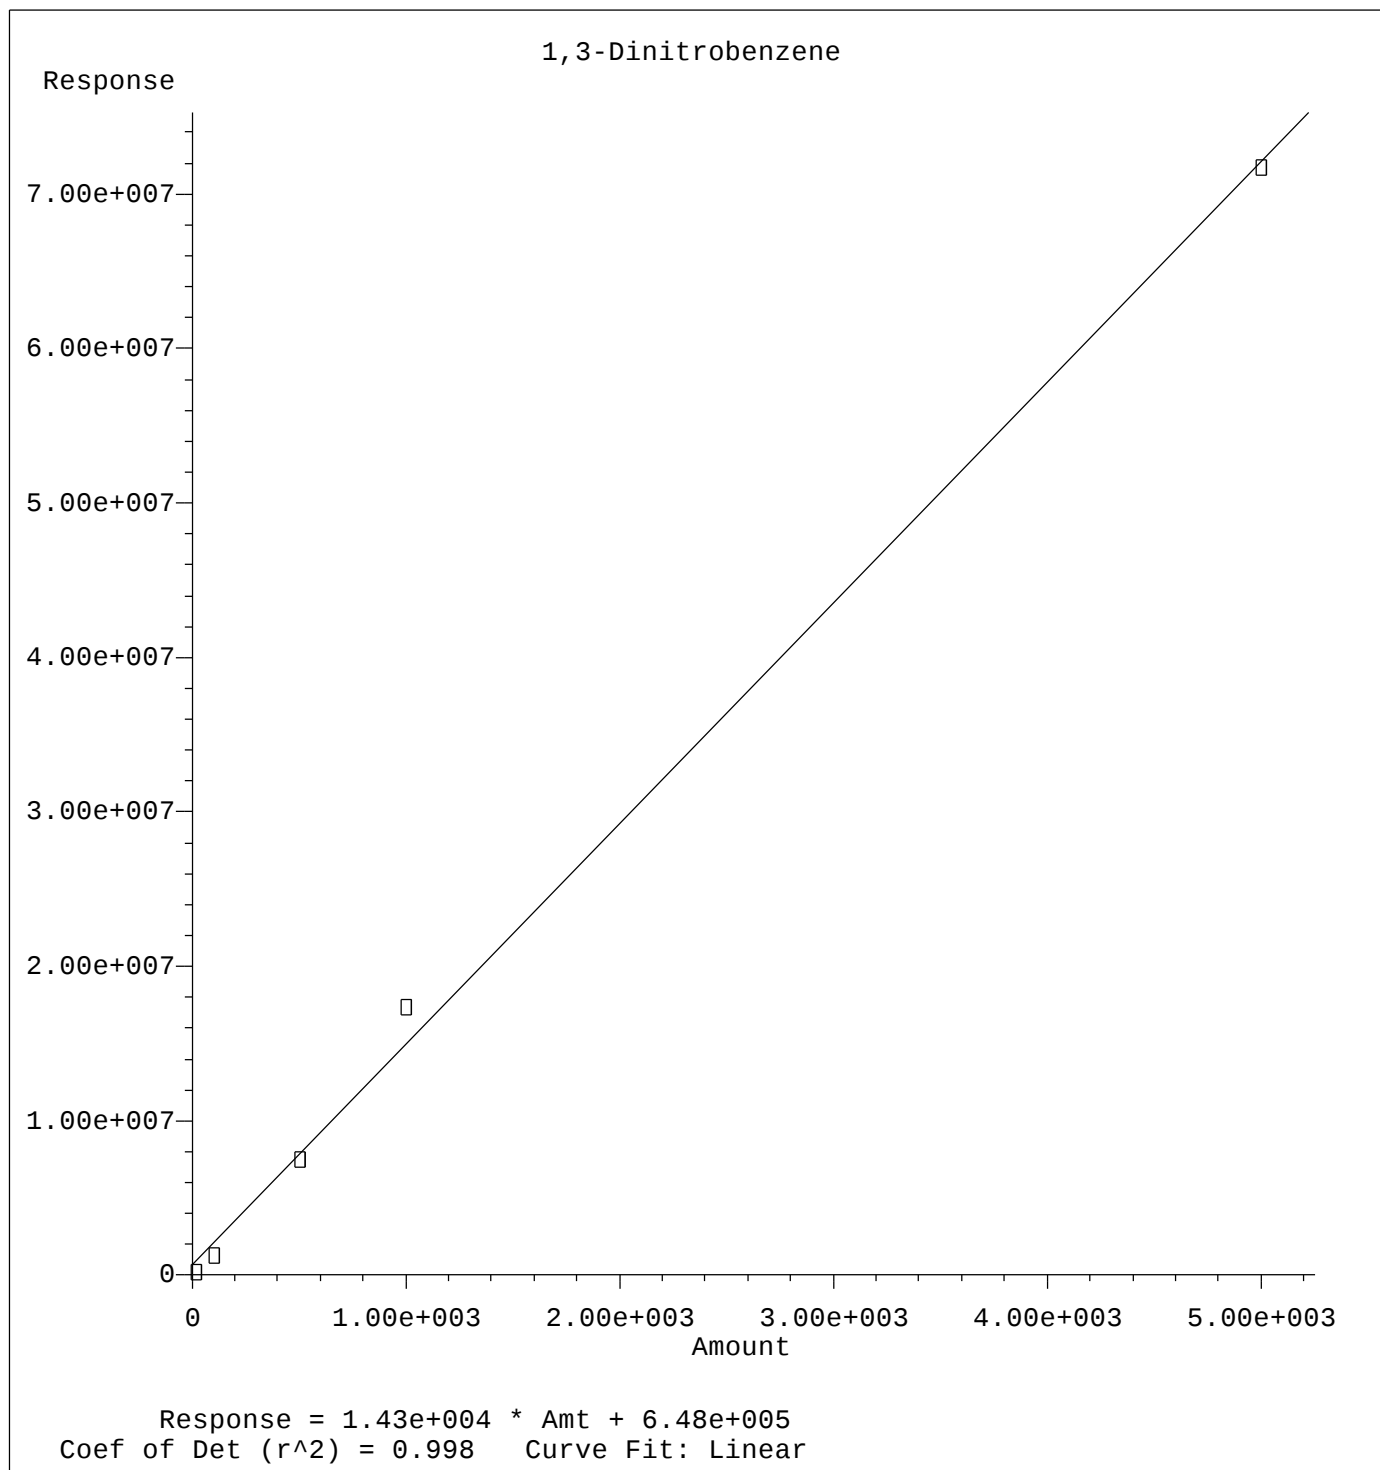


Method Name: Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Calibration Table Last Updated: Wed Jun 11 17:35:58 2014

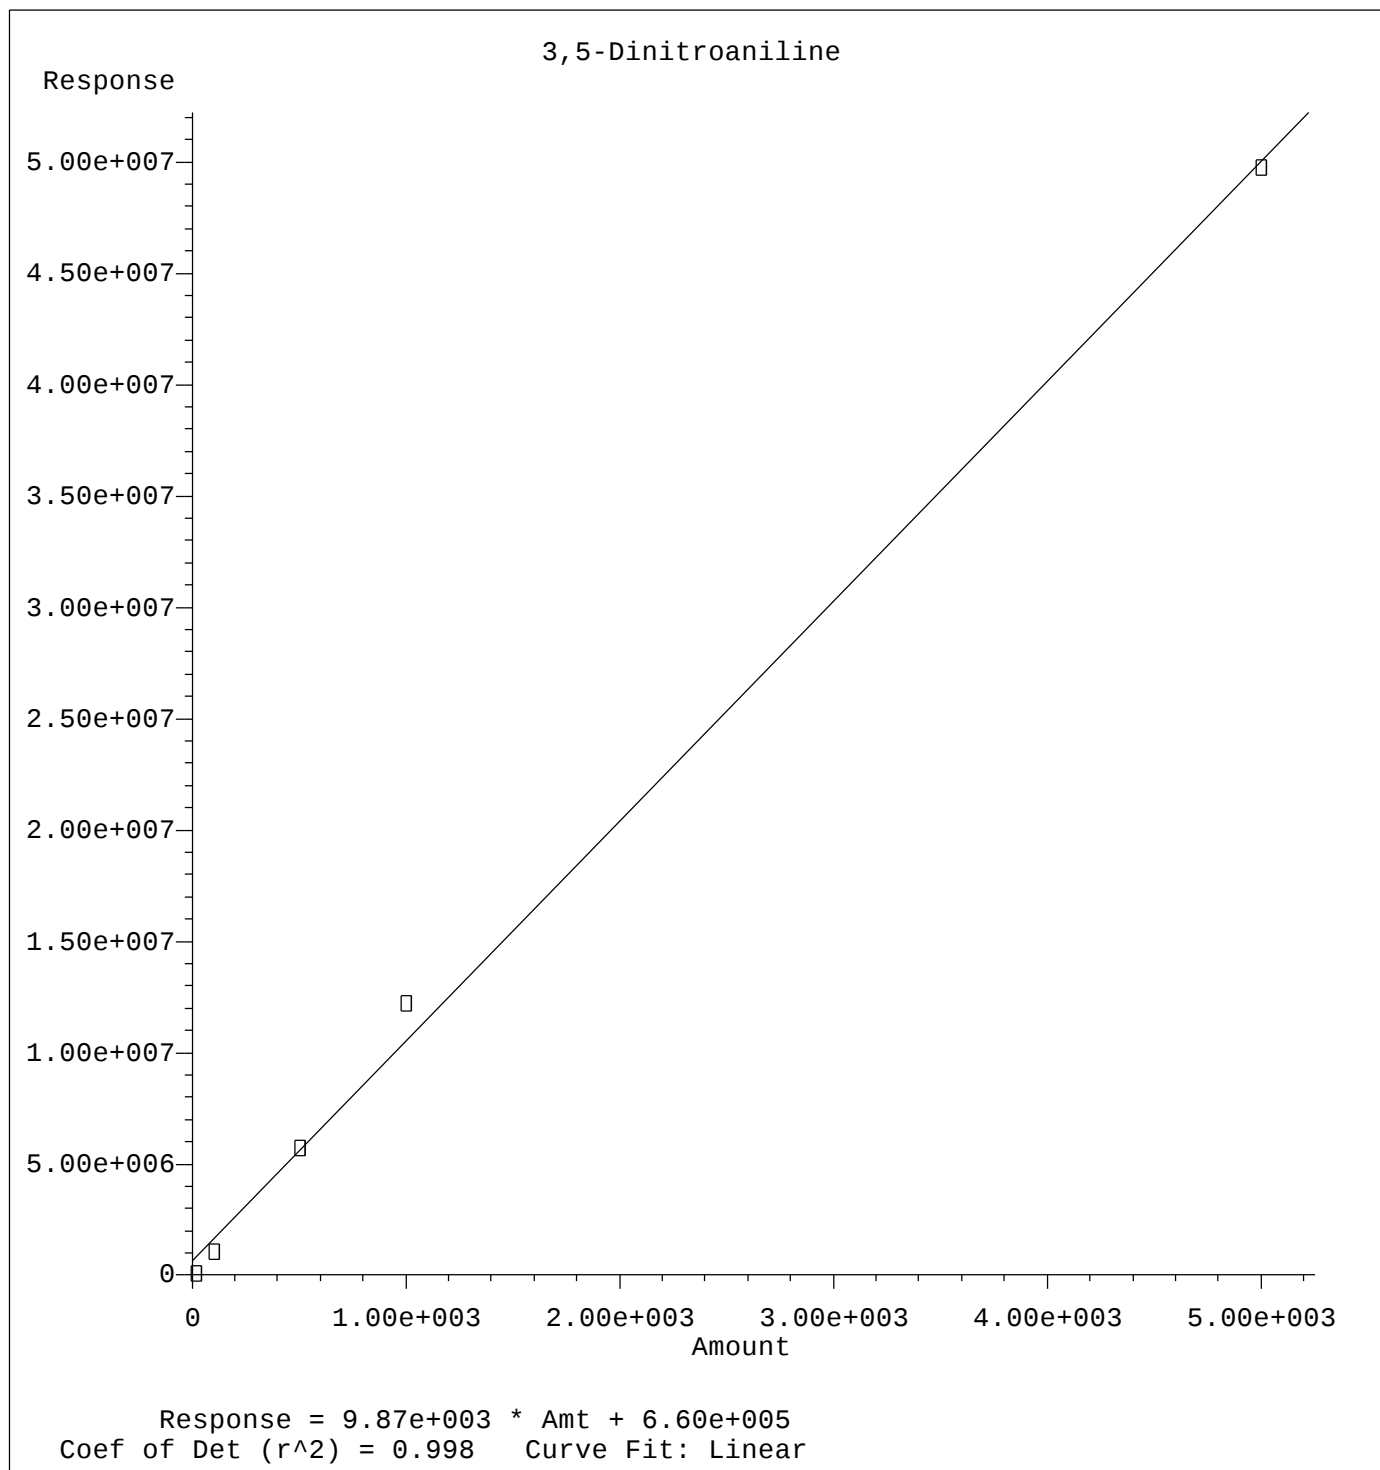


Method Name: Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Calibration Table Last Updated: Wed Jun 11 17:35:58 2014

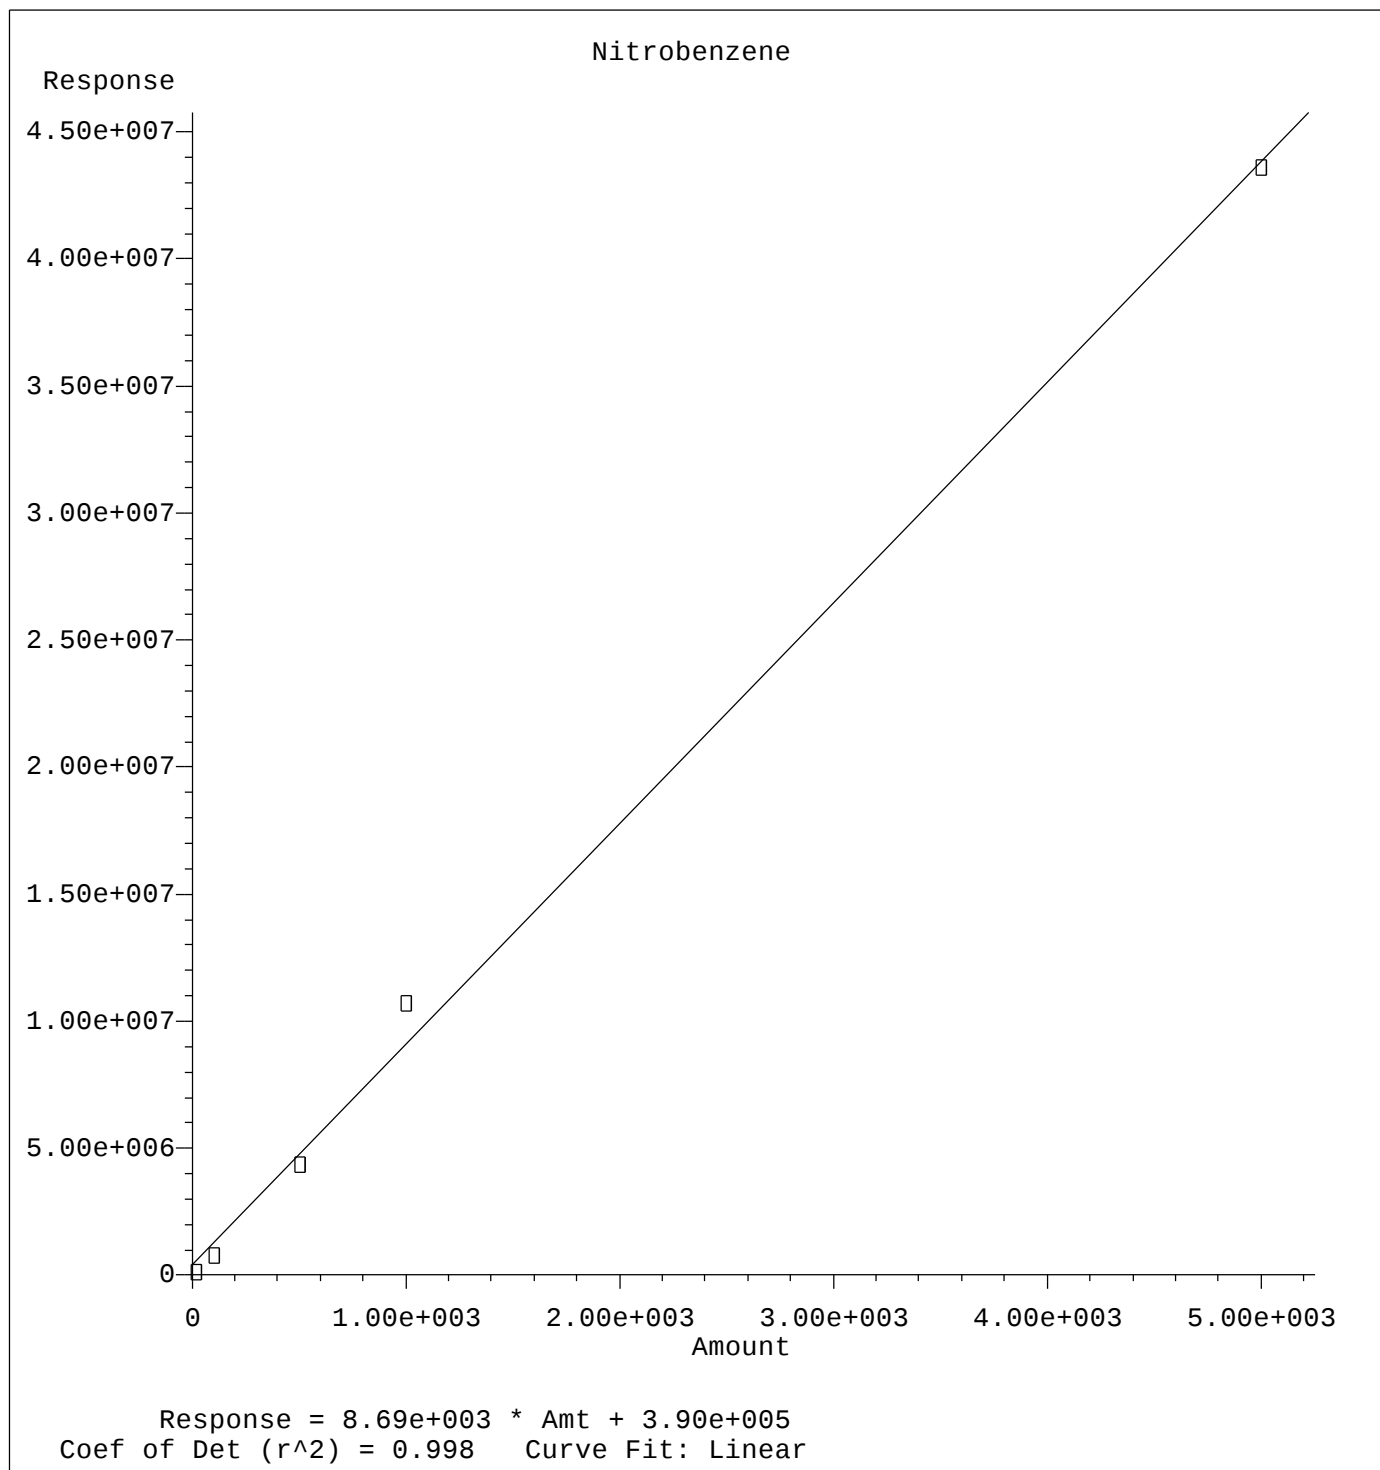


Method Name: Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Calibration Table Last Updated: Wed Jun 11 17:35:58 2014

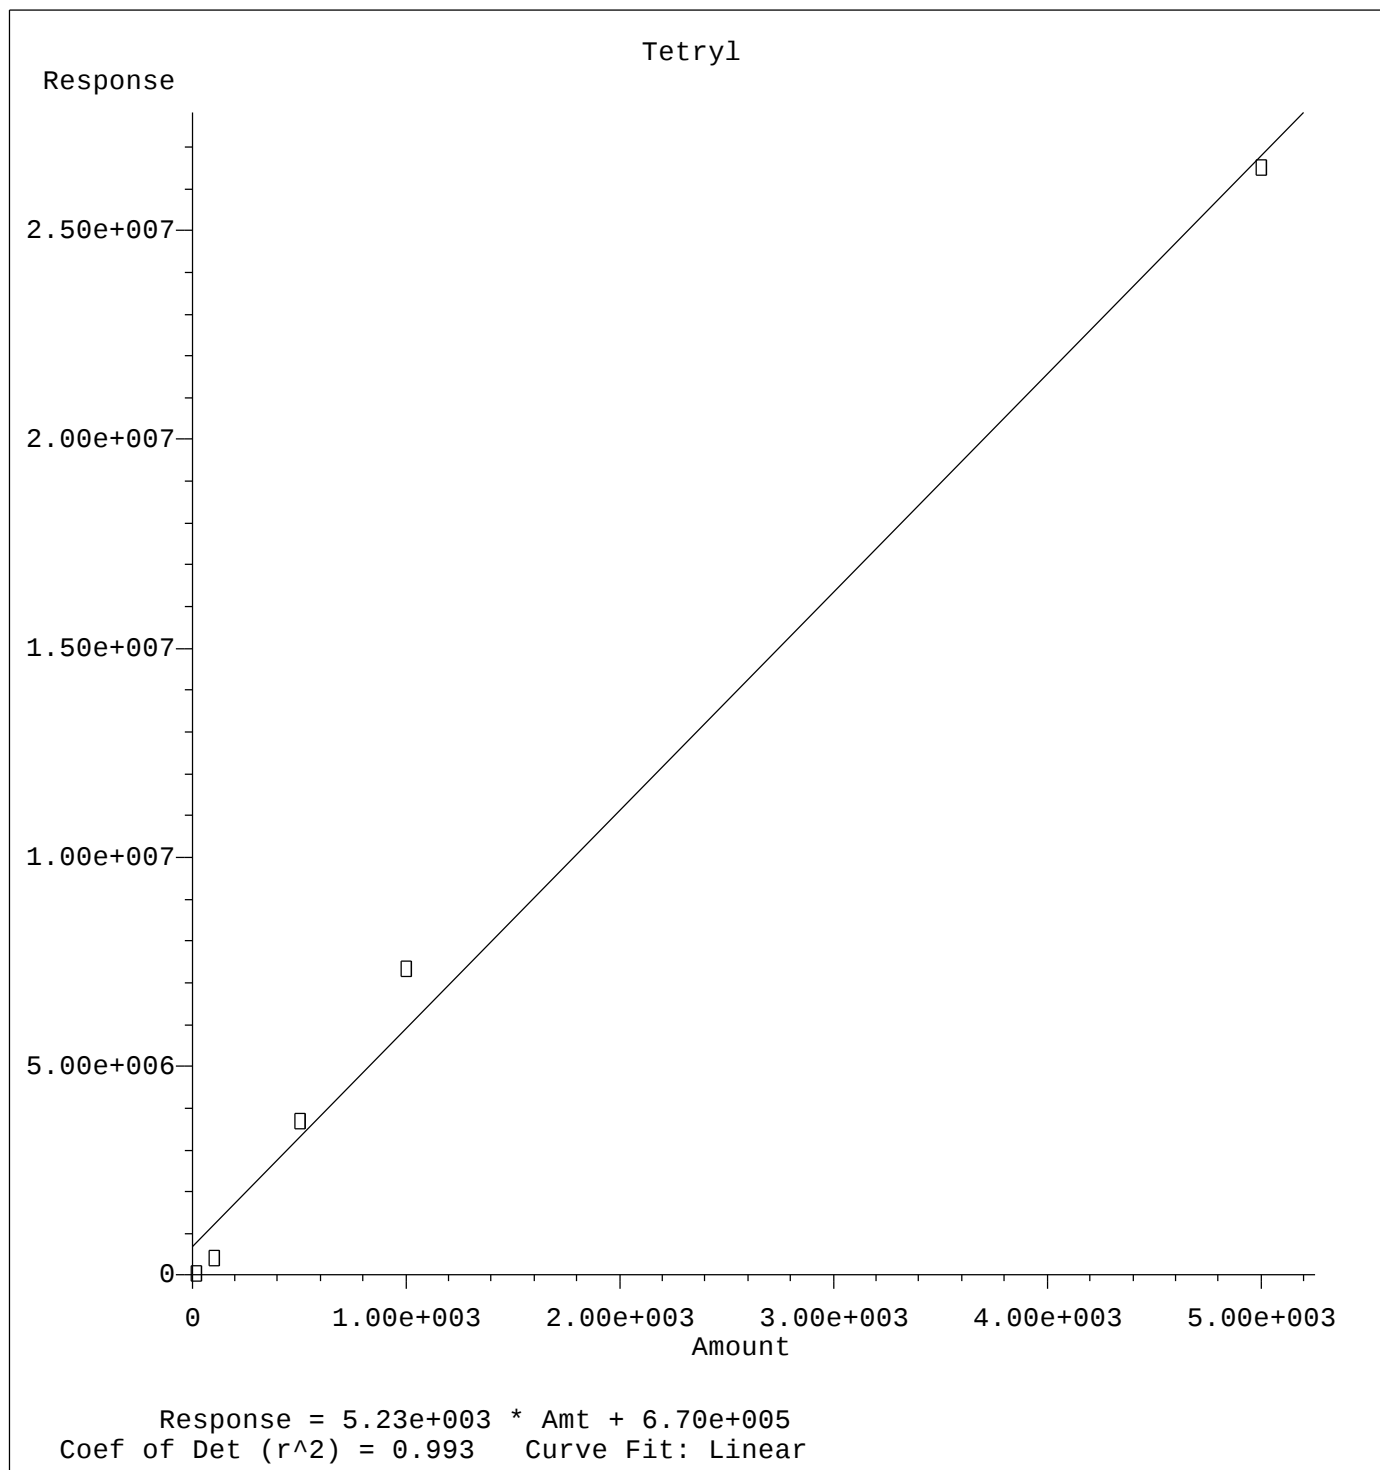


Method Name: Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Calibration Table Last Updated: Wed Jun 11 17:35:58 2014

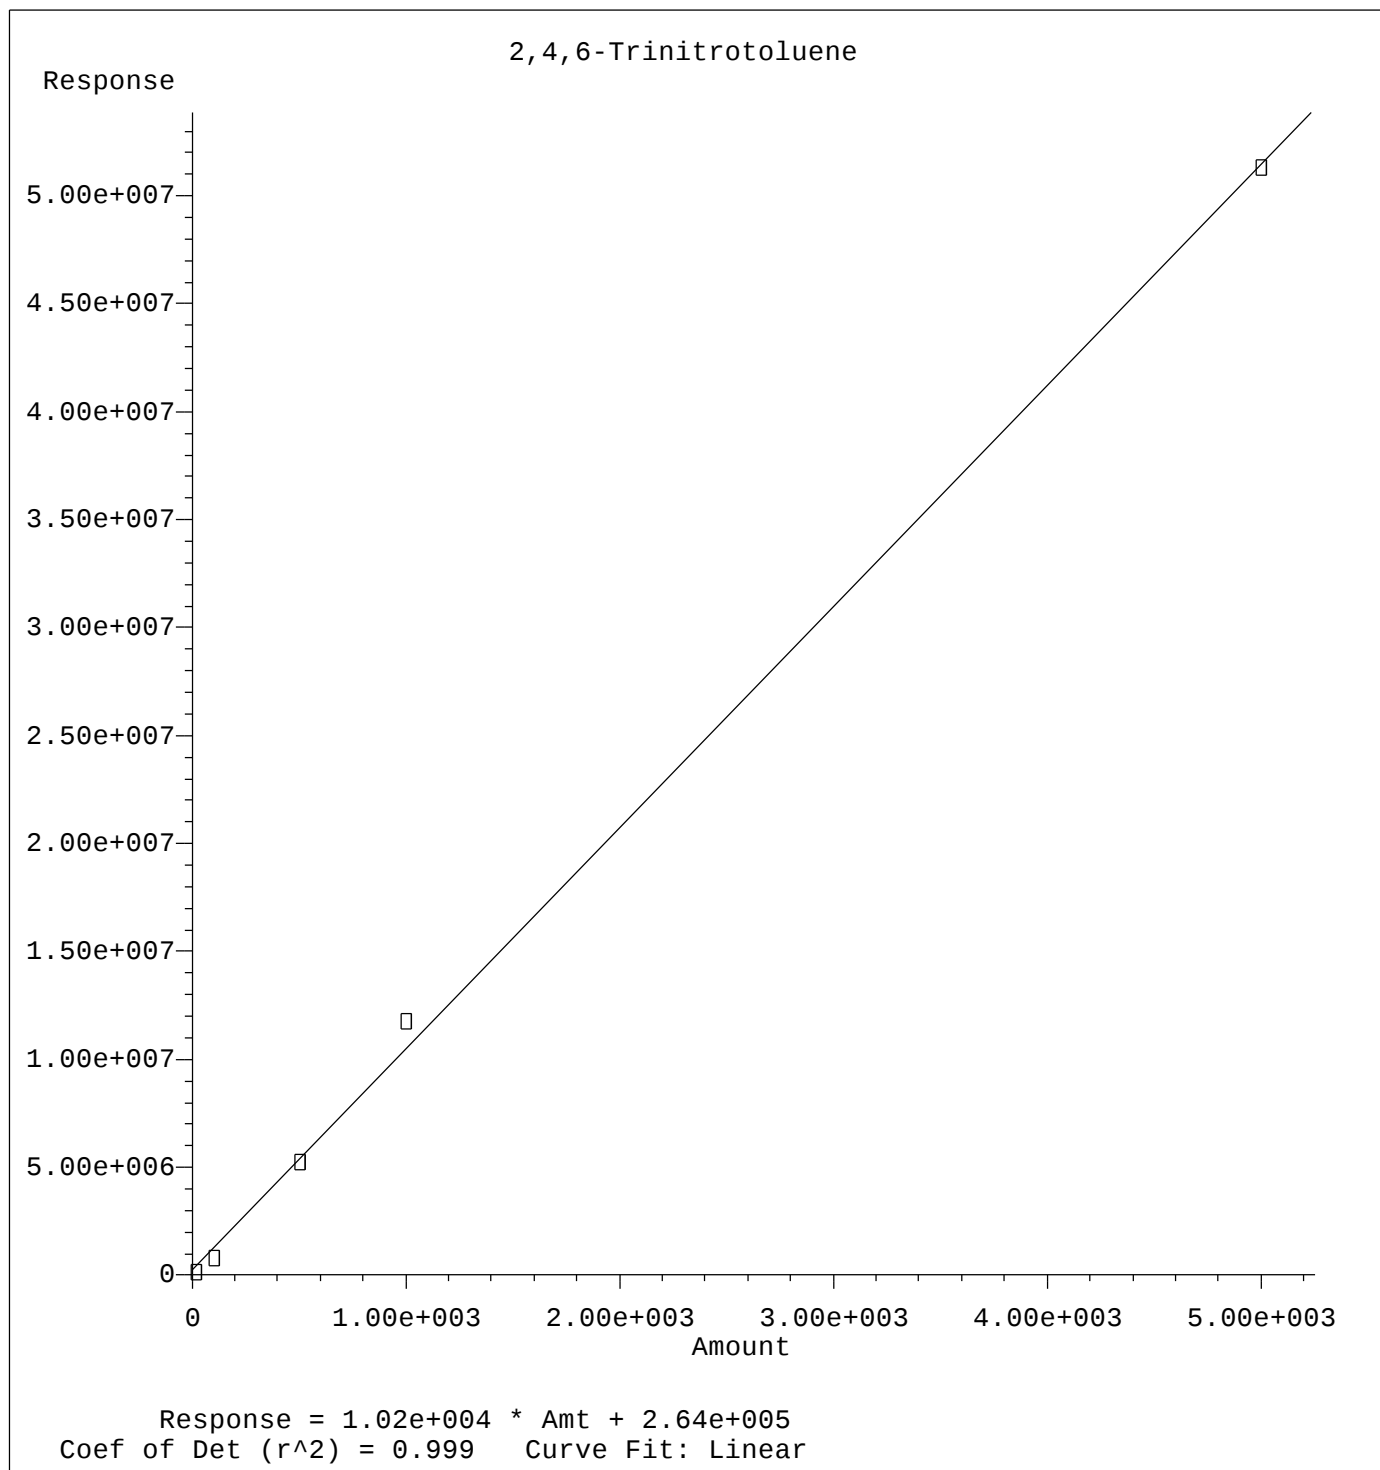


Method Name: Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Calibration Table Last Updated: Wed Jun 11 17:35:58 2014

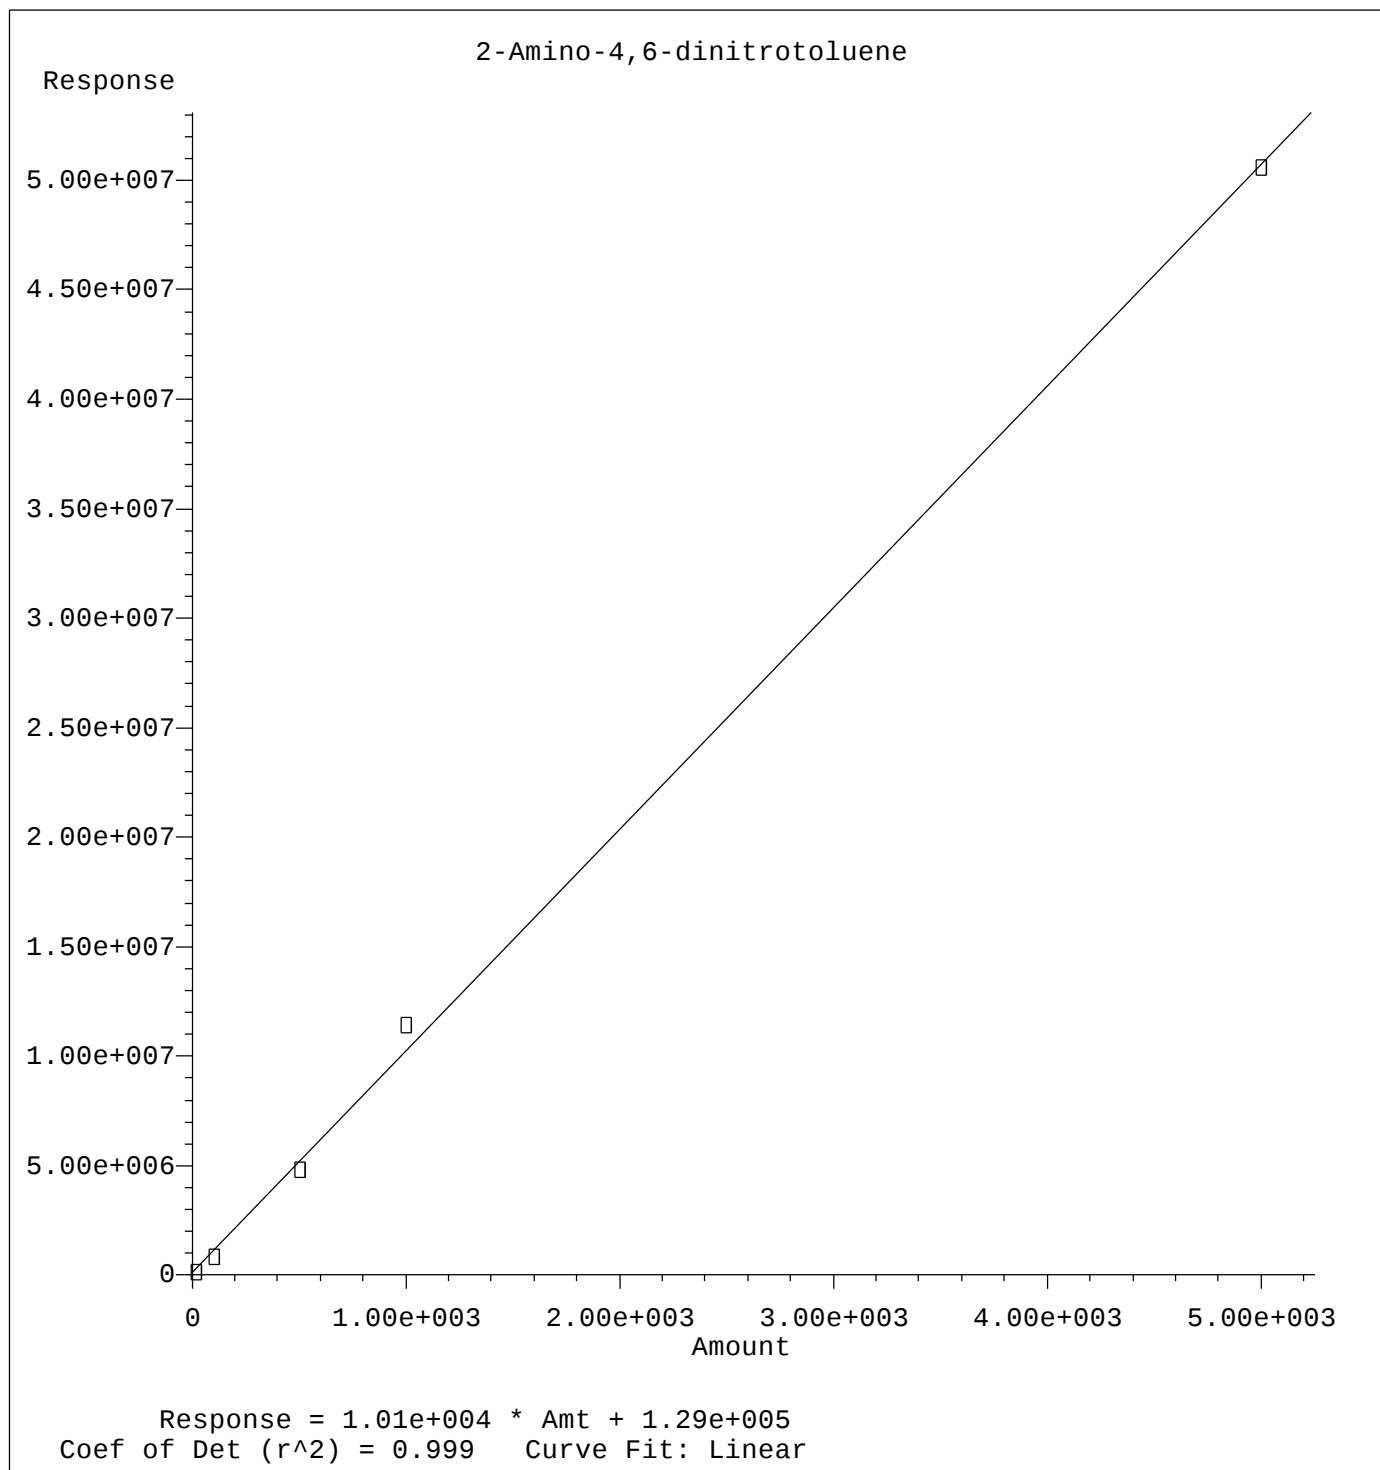


Method Name: Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Calibration Table Last Updated: Wed Jun 11 17:35:58 2014

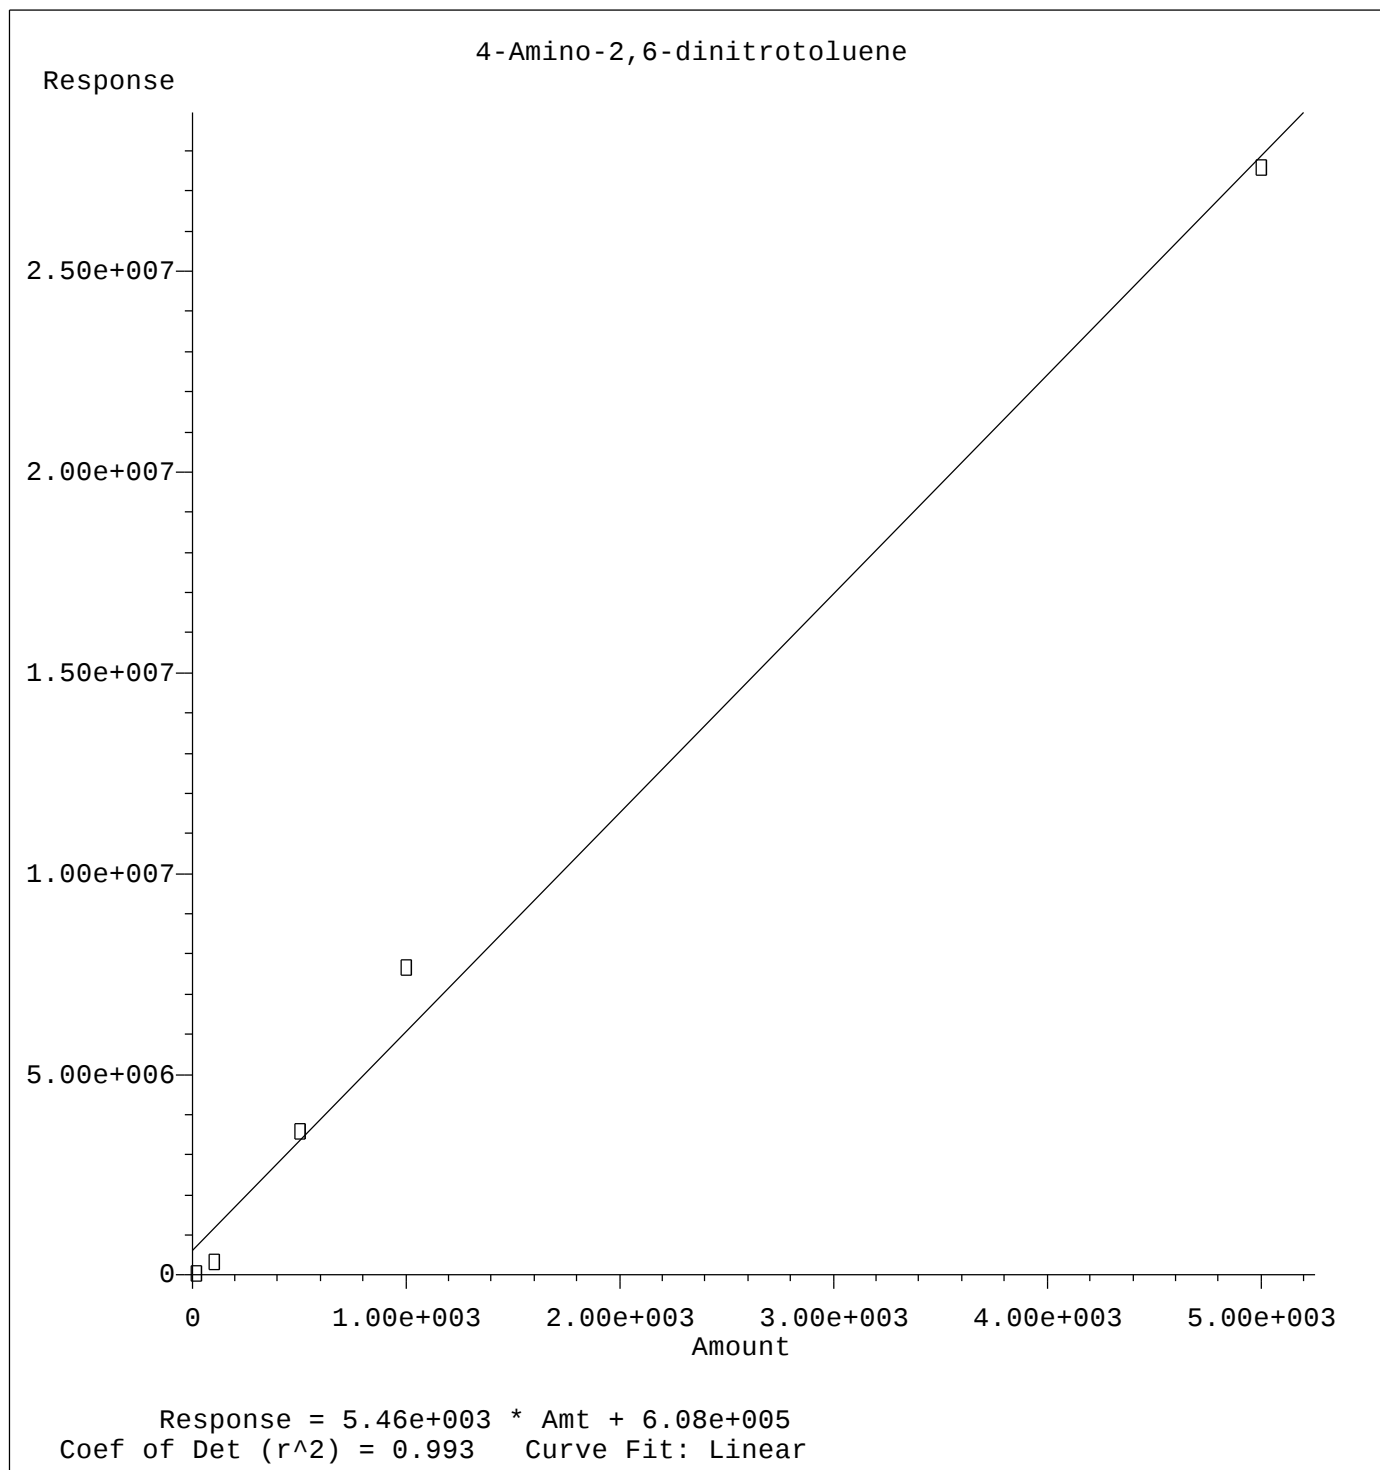


Method Name: Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Calibration Table Last Updated: Wed Jun 11 17:35:58 2014

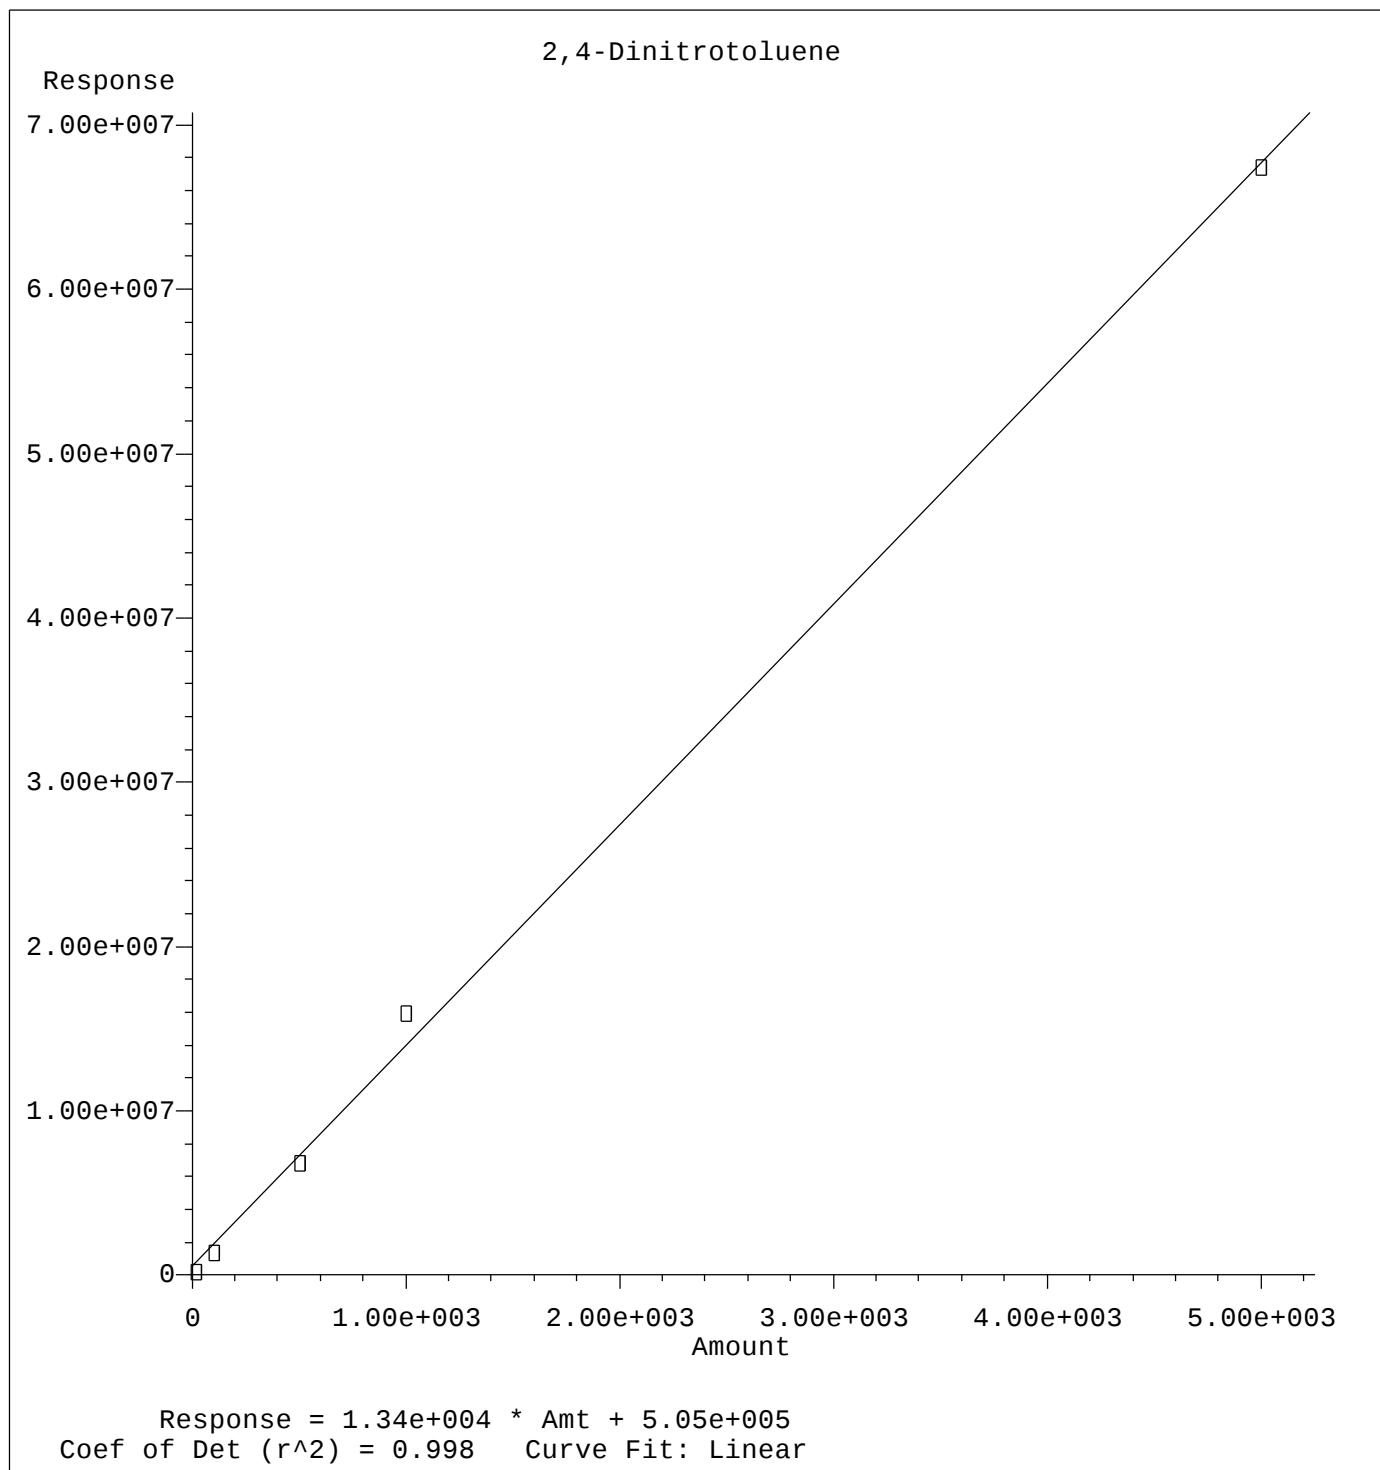

Method Name: Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Calibration Table Last Updated: Wed Jun 11 17:35:58 2014

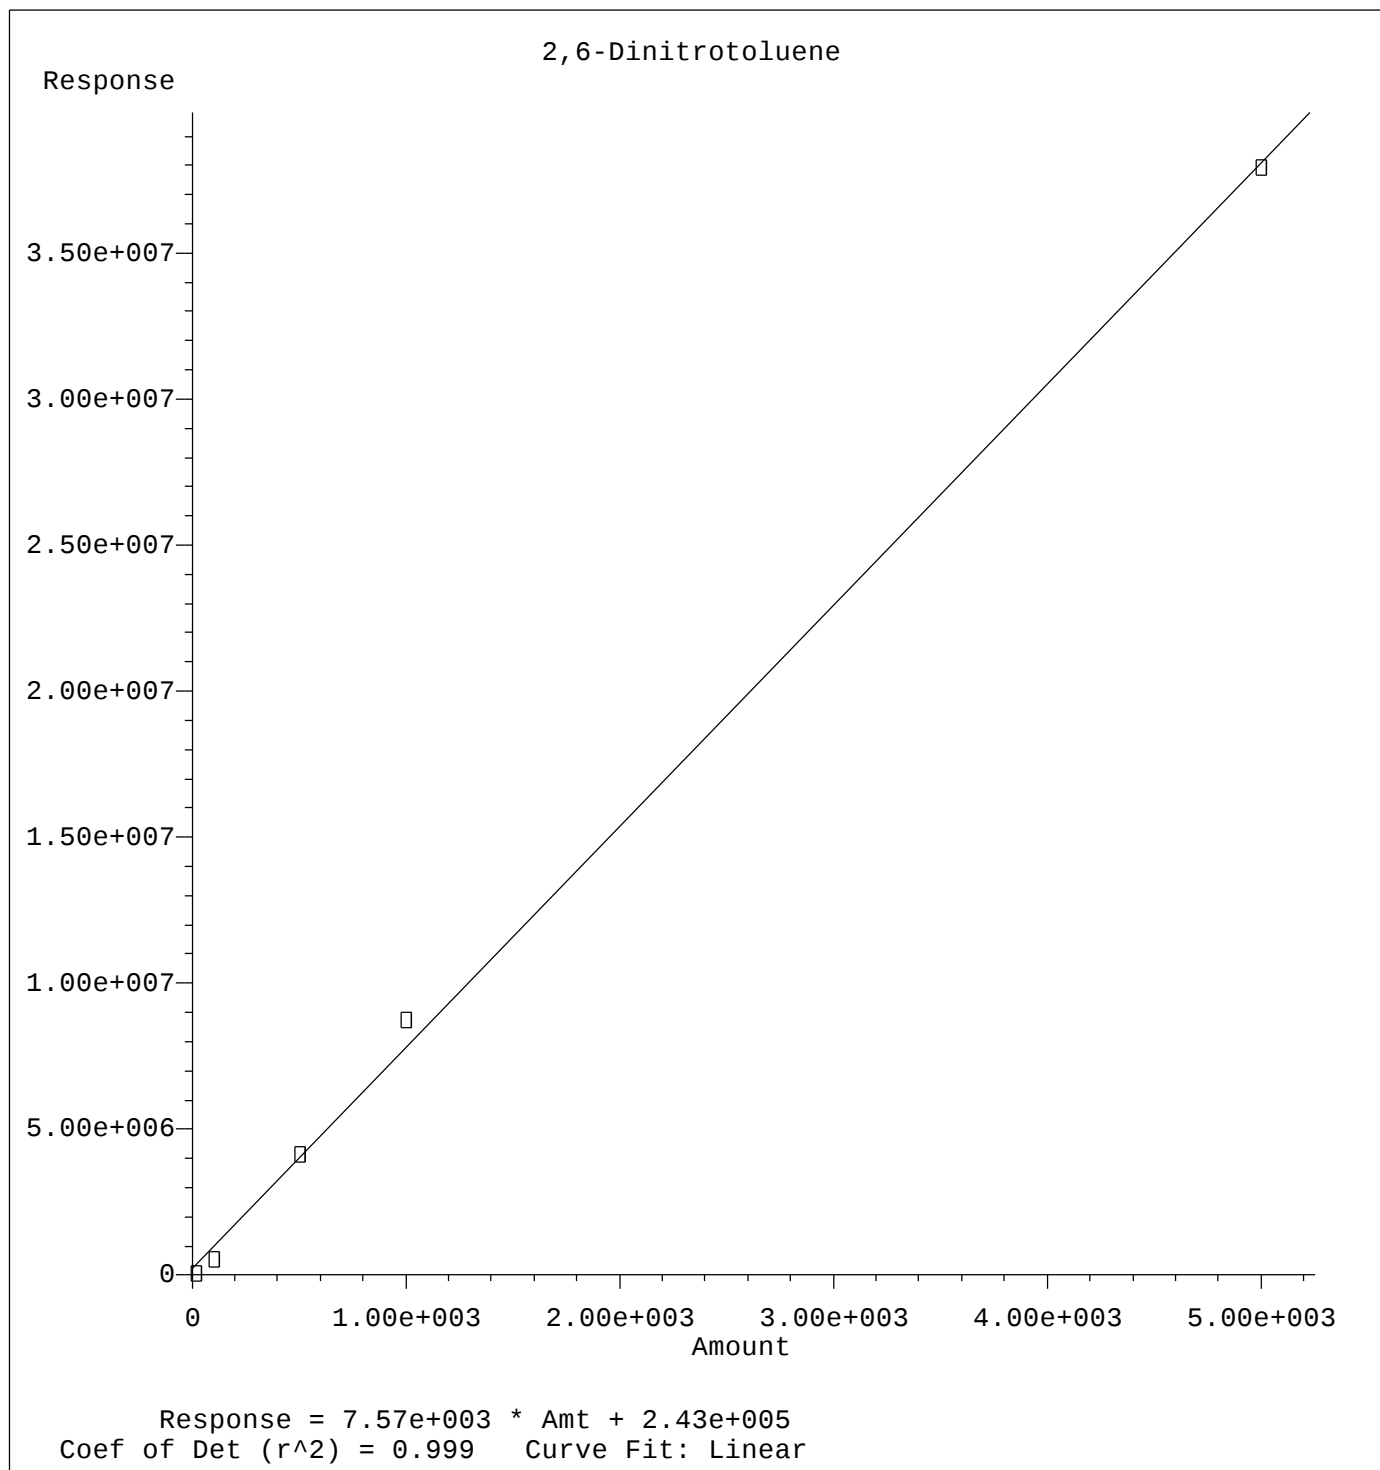

Method Name: Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Calibration Table Last Updated: Wed Jun 11 17:35:58 2014

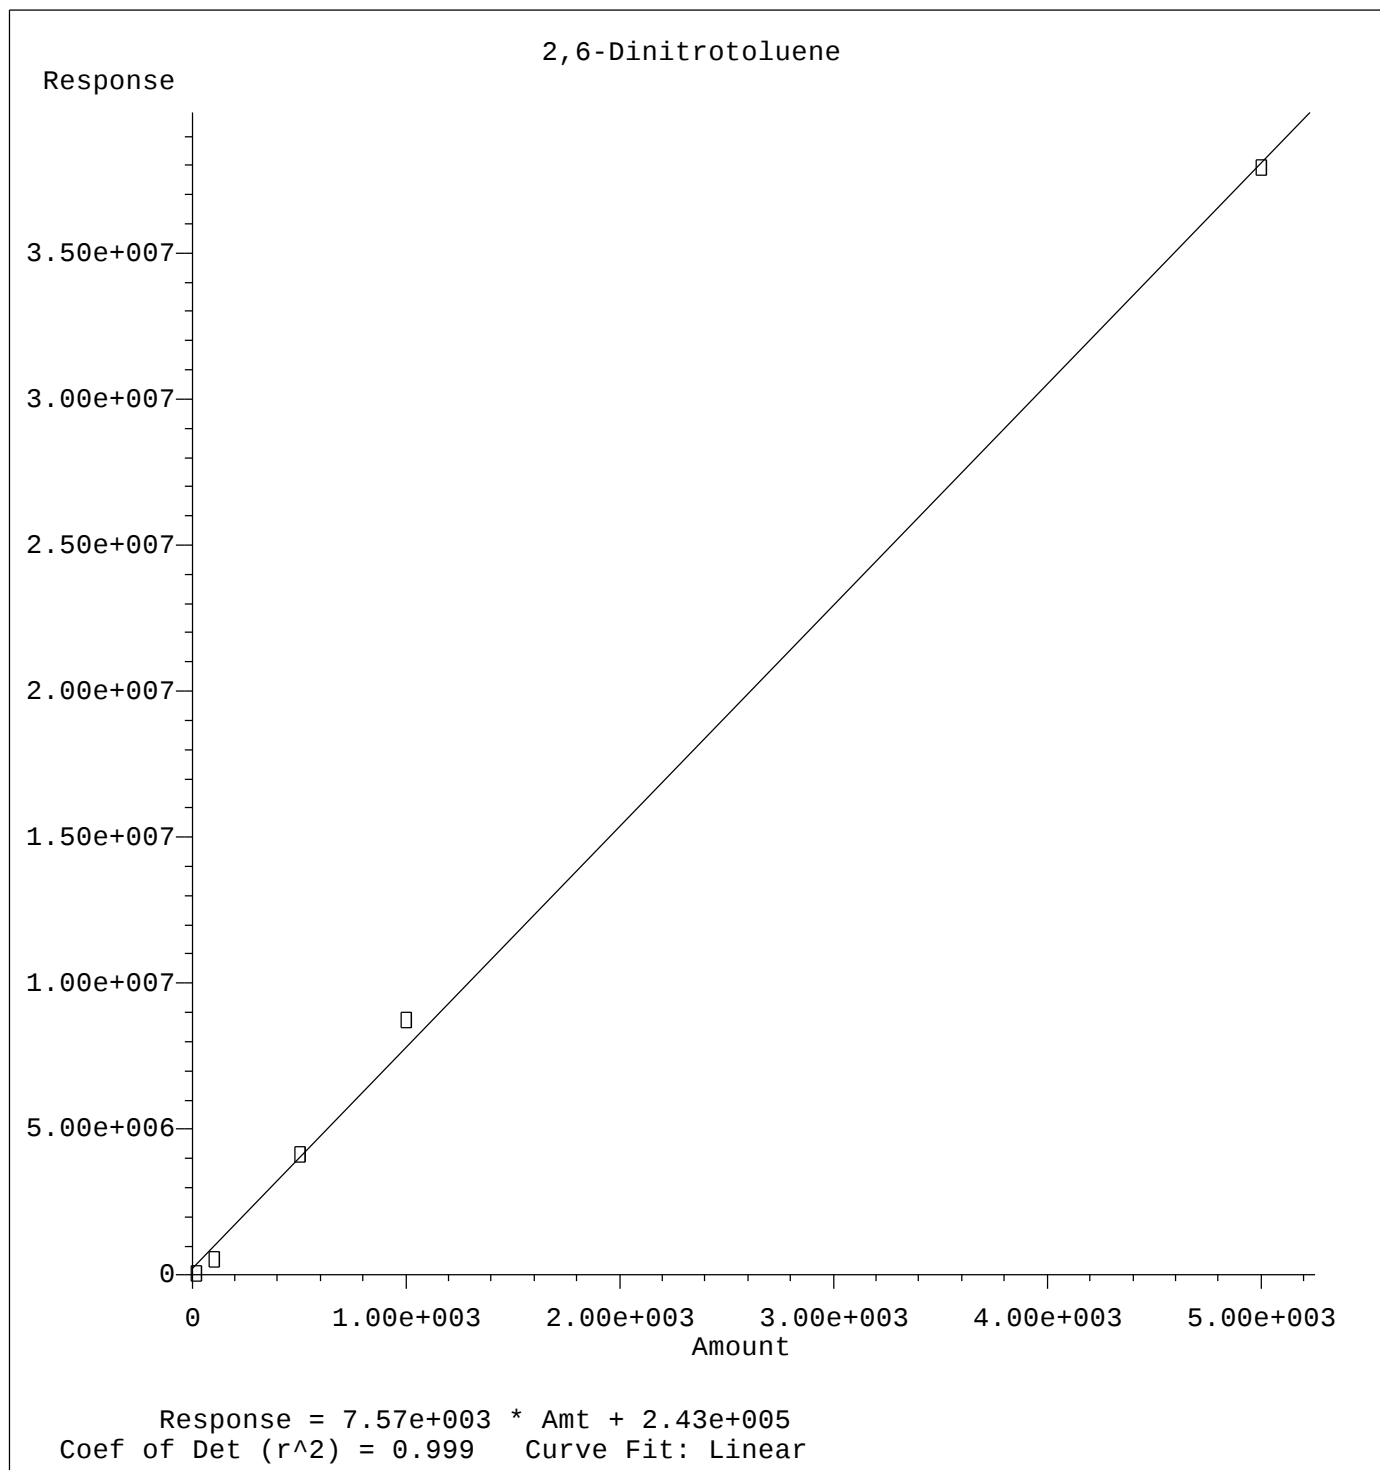

Method Name: Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Calibration Table Last Updated: Wed Jun 11 17:35:58 2014