

Data Path : Z:\HPCHEM1\HPLC_N\DATA\HN060514\
Data File : HN006081.D
Signal(s) : VWD1A.CH
Acq On : 05-Jun-2014, 09:56
Operator : HNP
Sample : HSTDICC5000
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDICC5000

Integration File: autoint1.e
Quant Time: Jan 10 01:04:28 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Quant Title :
QLast Update : Tue May 20 07:20:33 2014
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.44	19257321	4177.799 ug/L
Target Compounds			
2) T HMX	0.94	21106392	3817.595 ug/L
3) T RDX	1.85	23813471	3465.865 ug/L
4) T 1,3,5-Trinitrobenzene	2.91	46143886	3501.008 ug/L
11) T 4-Amino-2,6-dinitrotoluene	7.30	75831303	11330.628 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\DATA\HN060514\
Data File : HN006081.D
Signal(s) : VWD1A.CH
Acq On : 05-Jun-2014, 09:56
Operator : HNP
Sample : HSTDICC5000
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDICC5000

Integration File: autoint1.e
Quant Time: Jan 10 01:04:28 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Quant Title :
QLast Update : Tue May 20 07:20:33 2014
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

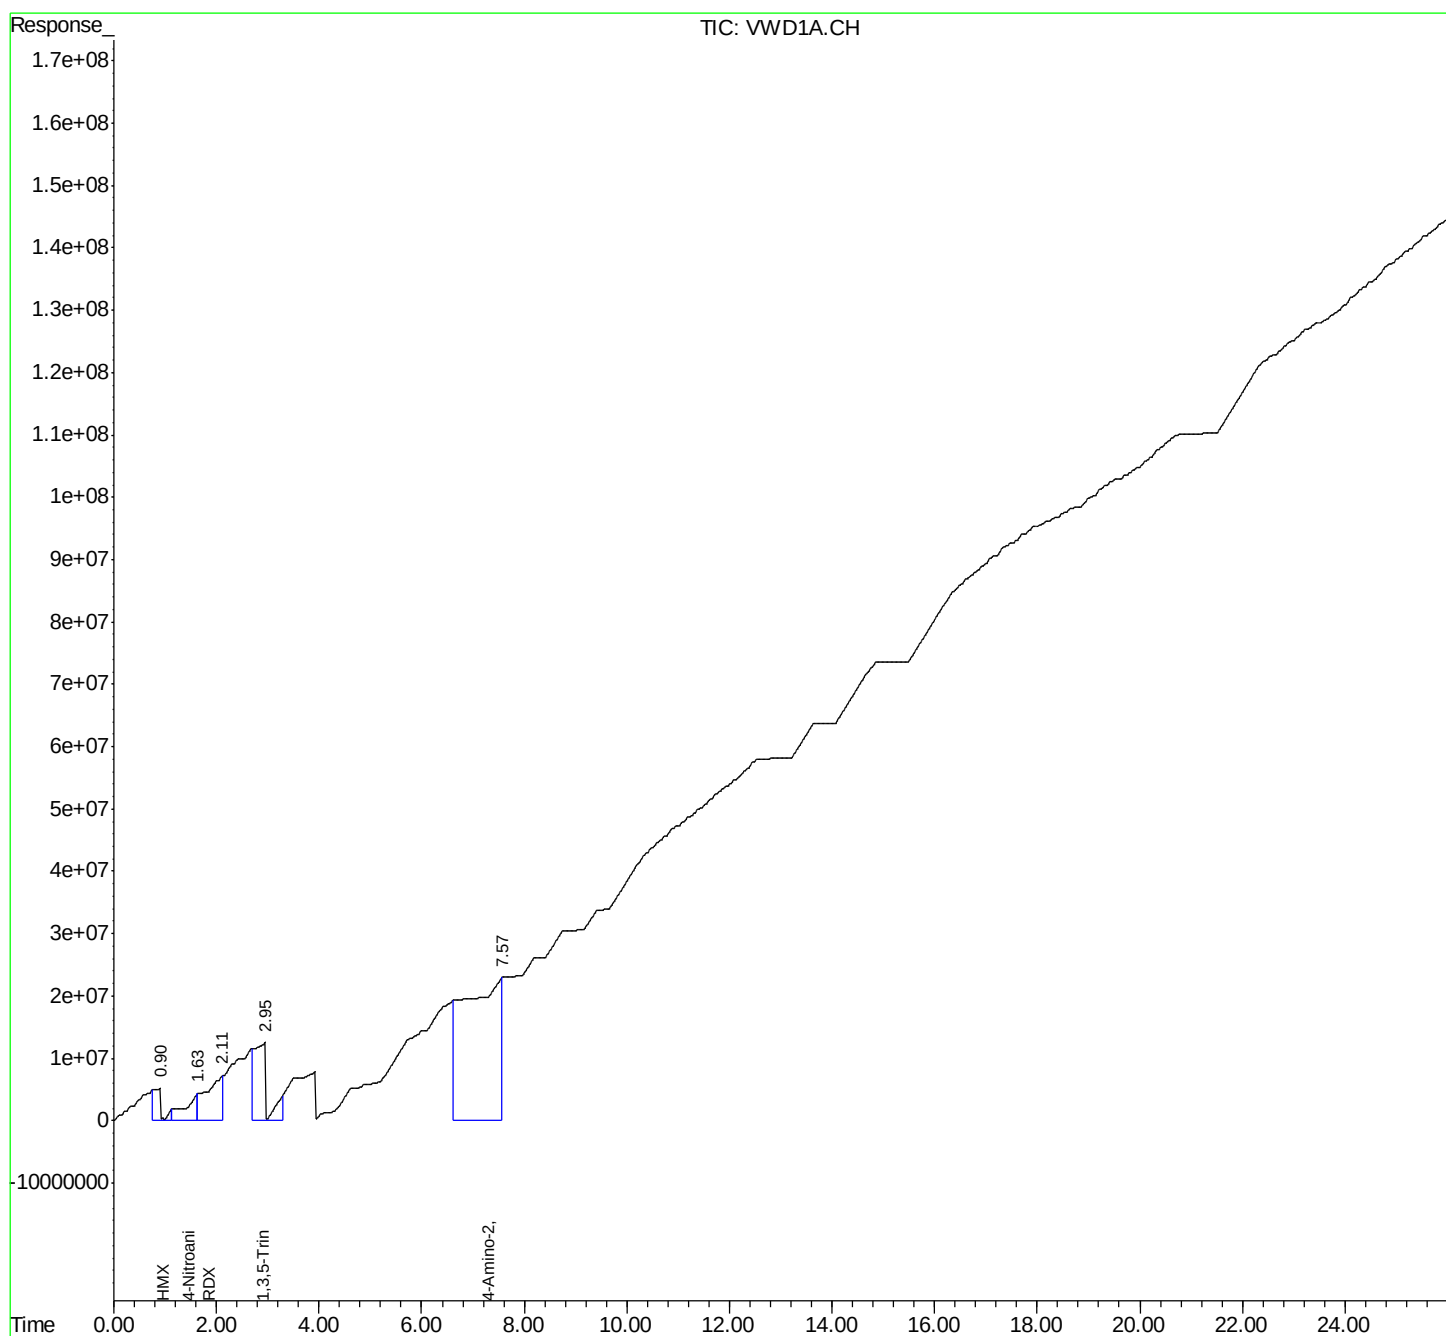


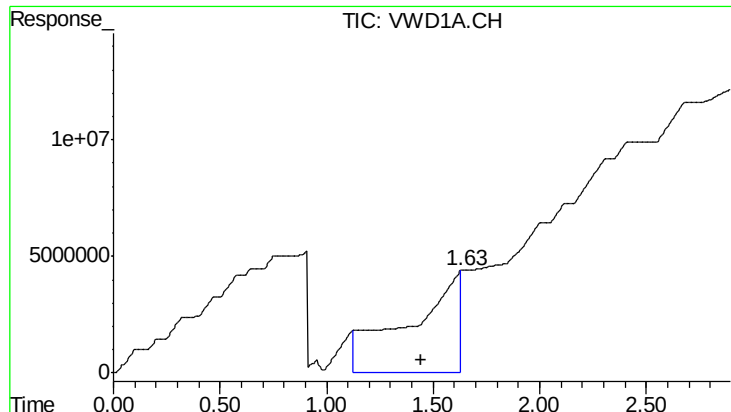

#1 4-Nitroaniline


R.T.: 1.443 min
Delta R.T.: 0.000 min
Response: 19257321
Conc: 4177.80 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDICC5000

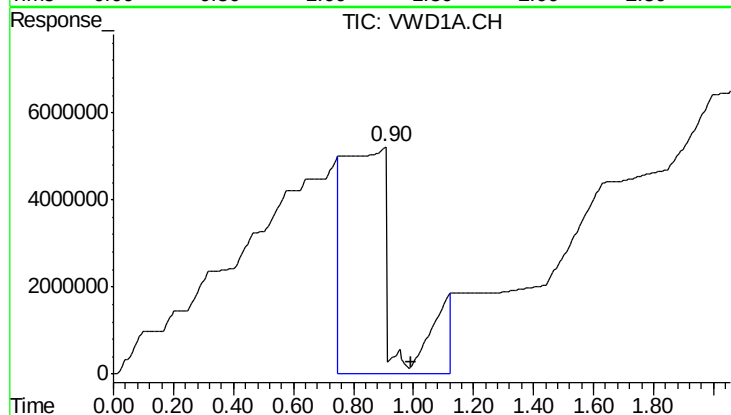


#2 HMX

R.T.: 0.944 min
Delta R.T.: -0.047 min
Response: 21106392
Conc: 3817.59 ug/L

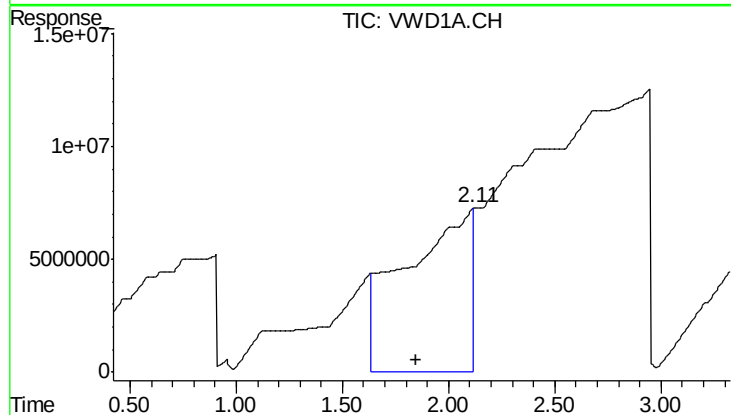


#3 RDX

R.T.: 1.847 min
Delta R.T.: 0.000 min
Response: 23813471
Conc: 3465.87 ug/L

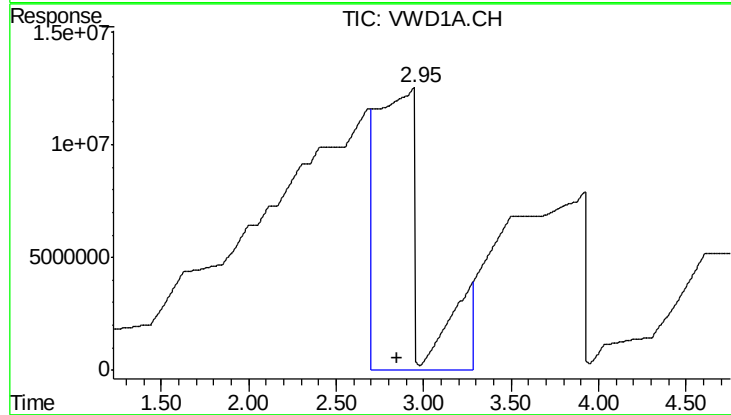

#4 1,3,5-Trinitrobenzene

R.T.: 2.912 min
Delta R.T.: 0.067 min
Response: 46143886
Conc: 3501.01 ug/L

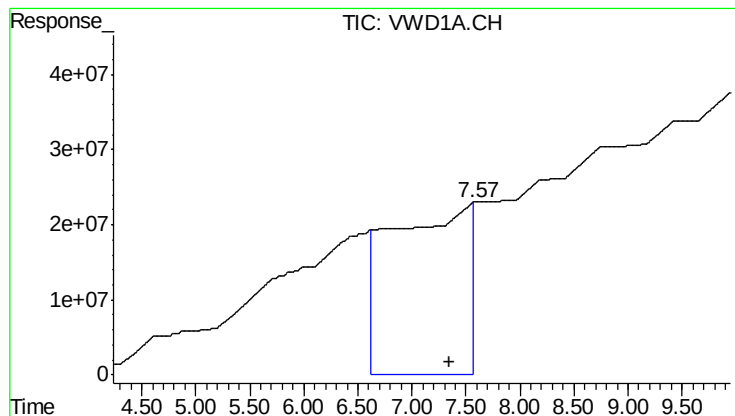

#11 4-Amino-2,6-dinitrotoluene

R.T.: 7.300 min
Delta R.T.: -0.042 min
Response: 75831303
Conc: 11330.63 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDICC5000