

Data Path : Z:\HPCHEM1\HPLC_N\DATA\HN060514\
 Data File : HN006084.D
 Signal(s) : VWD1A.CH
 Acq On : 05-Jun-2014, 13:43
 Operator : HNP
 Sample : HSTDICC2000
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDICC2000

Manual Integrations
 APPROVED

TEJASKUMAR
 10/13/2014 4:13:55 PM

Integration File: autoint1.e
 Quant Time: Jan 10 01:04:41 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
 Quant Title :
 QLast Update : Tue May 20 07:20:33 2014
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.43	4974334	1269.670 ug/L
Target Compounds			
2) T HMX	0.95	3388838	764.591 ug/L
3) T RDX	1.85	2352561	490.871 ug/L
4) T 1,3,5-Trinitrobenzene	2.92	7394680	796.300 ug/L
5) T 1,3-Dinitrobenzene	3.89	13513448	942.802 ng/ml
6) T 3,5-Dinitroaniline	4.30	8905827	895.802 ug/L
7) T Nitrobenzene	5.21	9337836	1071.625 ug/L
8) T Tetryl	7.19	3264206	582.902 ug/L
9) T 2,4,6-Trinitrotoluene	7.38	6229868	682.090 ug/L
10) T 2-Amino-4,6-dinitrotoluene	7.97	7539549	745.978 ug/L
11) T 4-Amino-2,6-dinitrotoluene	8.43	5090438	923.164 ug/L
12) T 2,4-Dinitrotoluene	9.22	10673085	792.322 ug/L
13) T 2,6-Dinitrotoluene	9.70	5965841	815.863 ug/L
14) T 2-Nitrotoluene	13.30	5313839	925.399 ug/L
15) T 4-Nitrotoluene	14.17	4228860	909.294 ug/L
16) T 3-Nitrotoluene	15.60	5351646	890.496 ug/L
17) T PETN	21.66	2338178	349.845 ug/L m

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\HPCHEM1\HPLC_N\DATA\HN060514\
Data File : HN006084.D
Signal(s) : VWD1A.CH
Acq On : 05-Jun-2014, 13:43
Operator : HNP
Sample : HSTDICC2000
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
HPLC_N
ClientSampleId :
HSTDICC2000


Manual Integrations
APPROVED

TEJASKUMAR
10/13/2014 4:13:55 PM

Integration File: autoint1.e
Quant Time: Jan 10 01:04:41 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN060514.M
Quant Title :
QLast Update : Tue May 20 07:20:33 2014
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

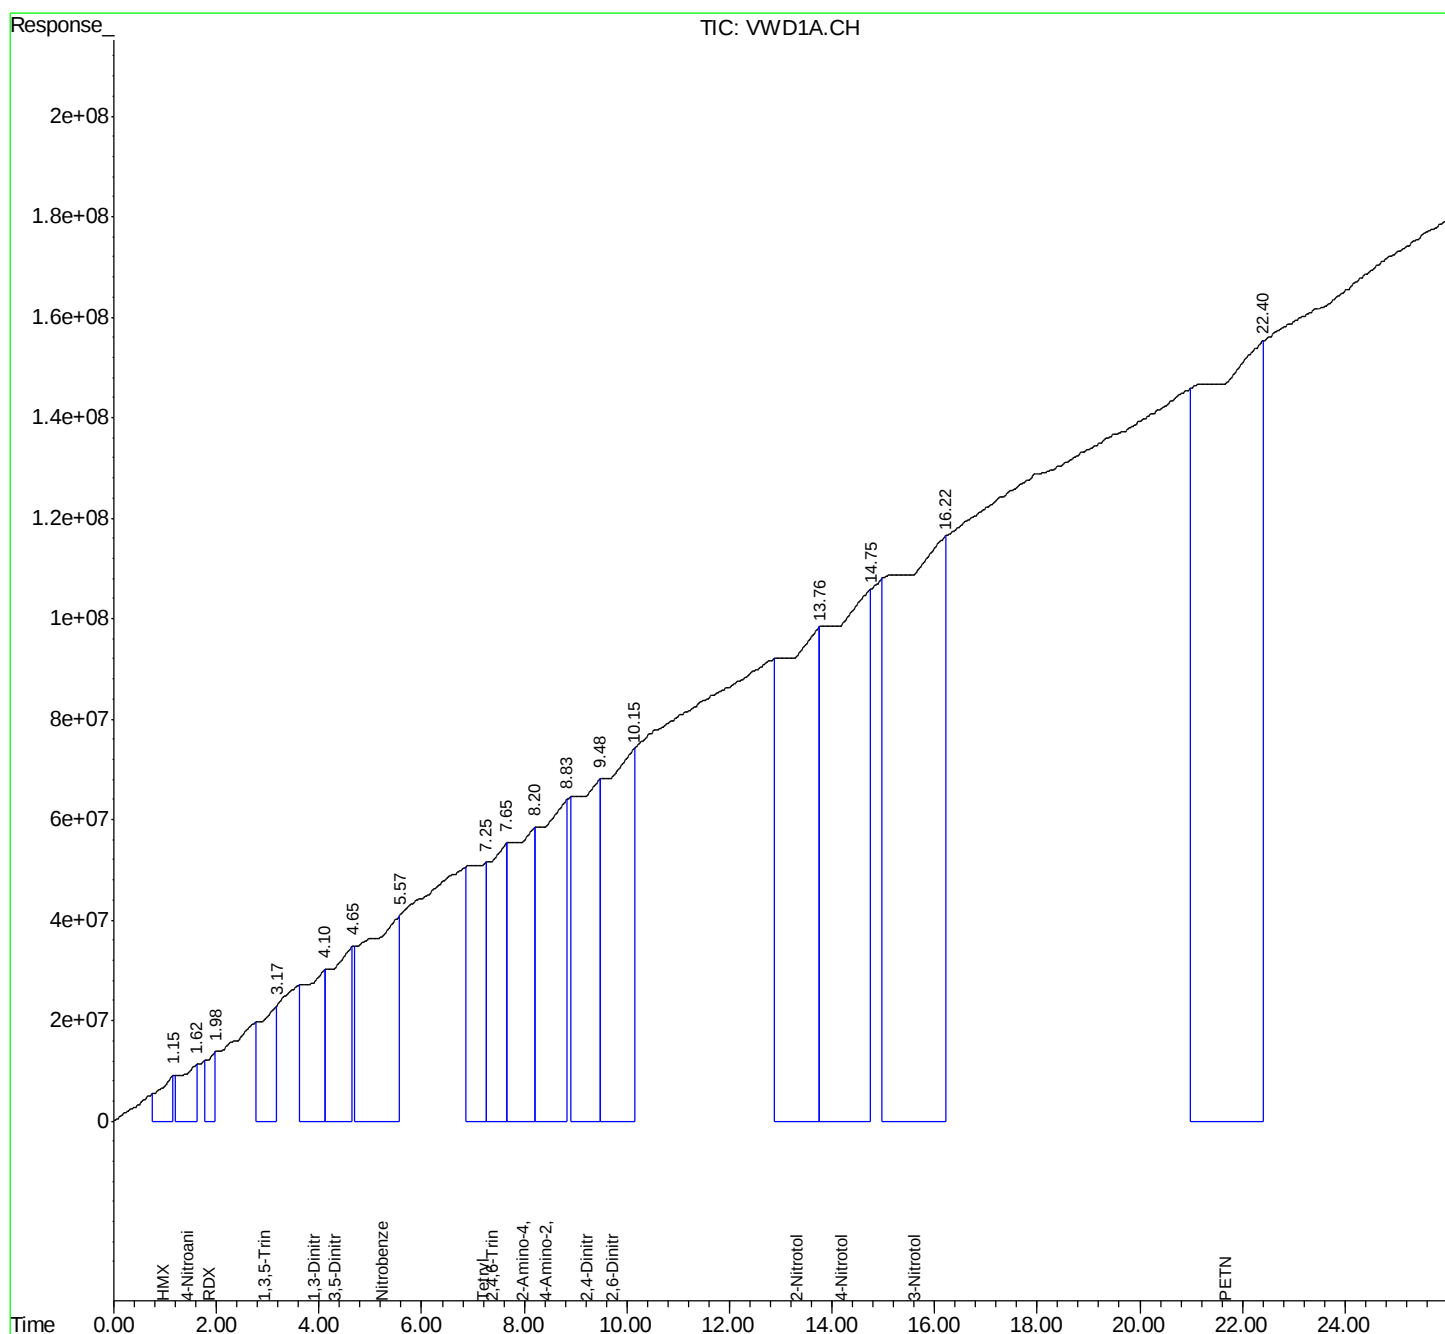

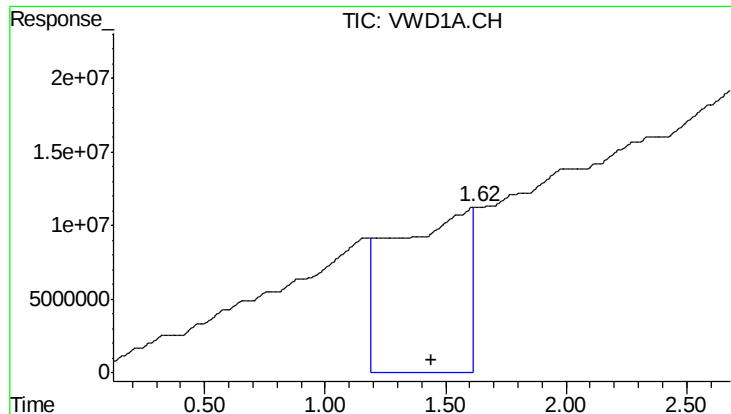


#1 4-Nitroaniline

R.T.: 1.429 min
Delta R.T.: -0.011 min
Response: 4974334
Conc: 1269.67 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDICC2000


Manual Integrations
APPROVED

TEJASKUMAR
10/13/2014 4:13:55 PM

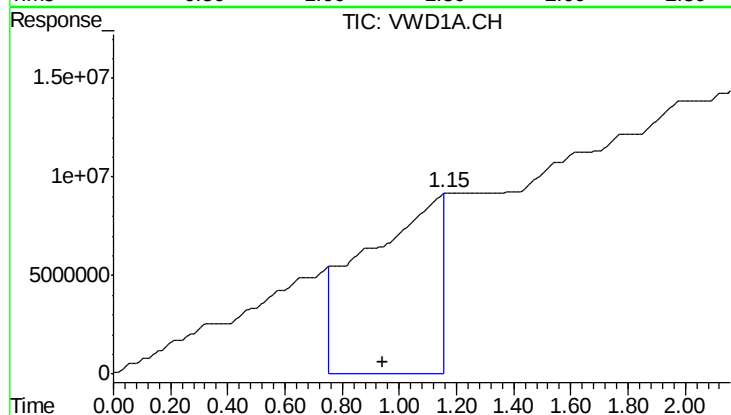


#2 HMX

R.T.: 0.946 min
Delta R.T.: 0.004 min
Response: 3388838
Conc: 764.59 ug/L

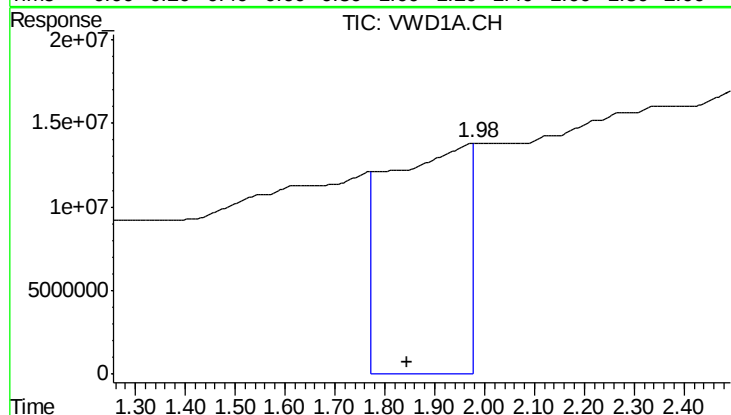


#3 RDX

R.T.: 1.852 min
Delta R.T.: 0.007 min
Response: 2352561
Conc: 490.87 ug/L

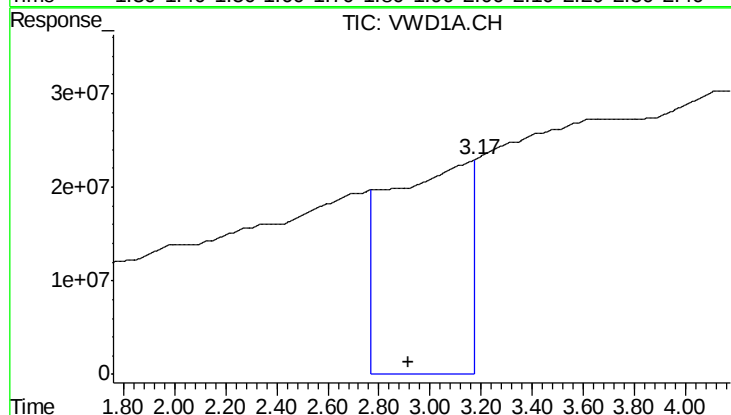

#4 1,3,5-Trinitrobenzene

R.T.: 2.925 min
Delta R.T.: 0.010 min
Response: 7394680
Conc: 796.30 ug/L

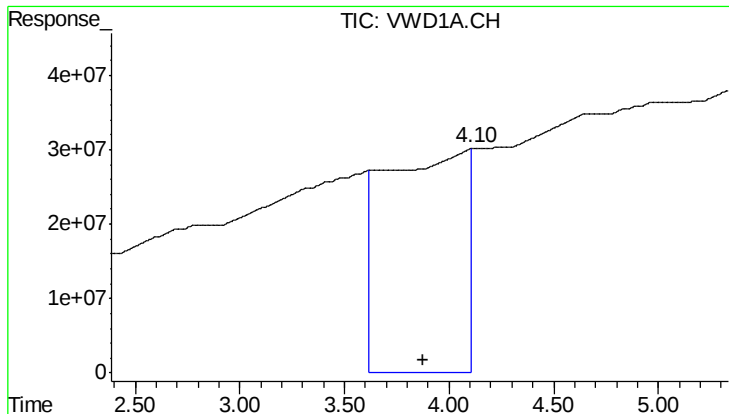


#5 1,3-Dinitrobenzene

R.T.: 3.887 min
 Delta R.T.: 0.009 min
 Response: 13513448
 Conc: 942.80 ng/ml

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDICC2000


Manual Integrations
 APPROVED

TEJASKUMAR
 10/13/2014 4:13:55 PM

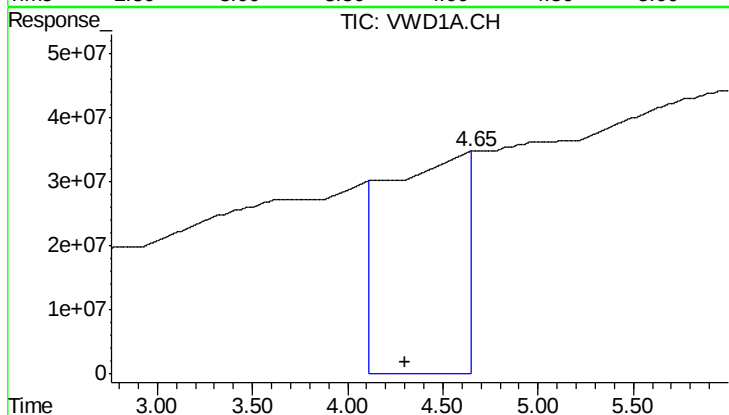


#6 3,5-Dinitroaniline

R.T.: 4.303 min
 Delta R.T.: -0.002 min
 Response: 8905827
 Conc: 895.80 ug/L

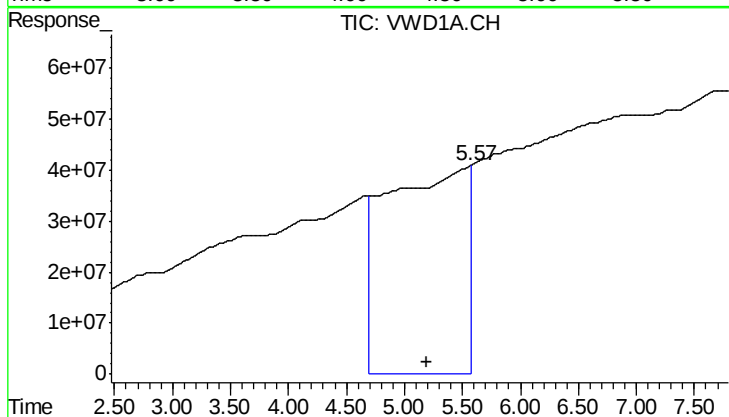


#7 Nitrobenzene

R.T.: 5.214 min
 Delta R.T.: 0.019 min
 Response: 9337836
 Conc: 1071.63 ug/L

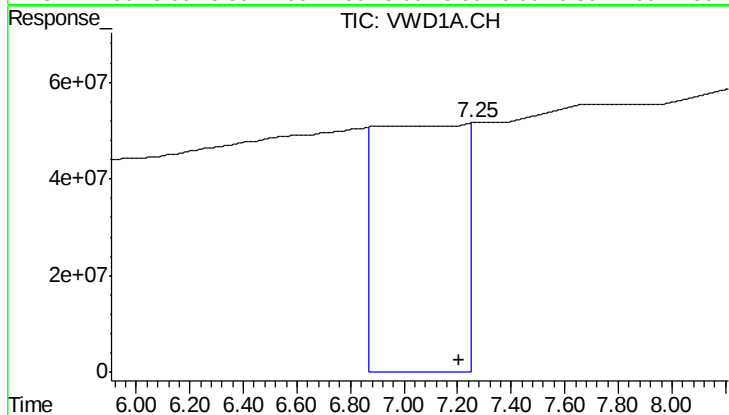

#8 Tetryl

R.T.: 7.195 min
 Delta R.T.: -0.012 min
 Response: 3264206
 Conc: 582.90 ug/L

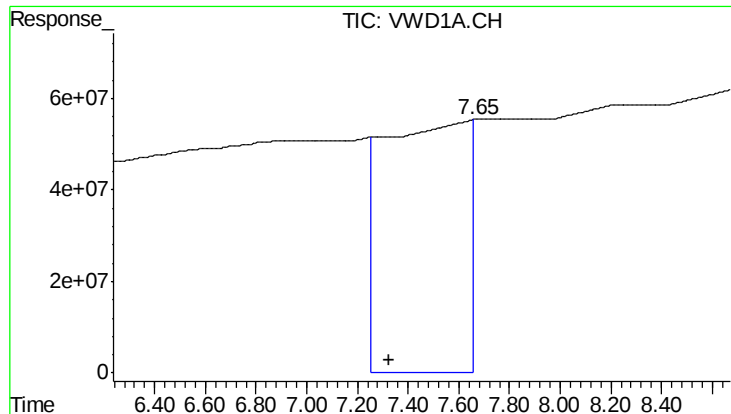


#9 2,4,6-Trinitrotoluene

R.T.: 7.379 min
Delta R.T.: 0.056 min
Response: 6229868
Conc: 682.09 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDICC2000


Manual Integrations
APPROVED

TEJASKUMAR
10/13/2014 4:13:55 PM

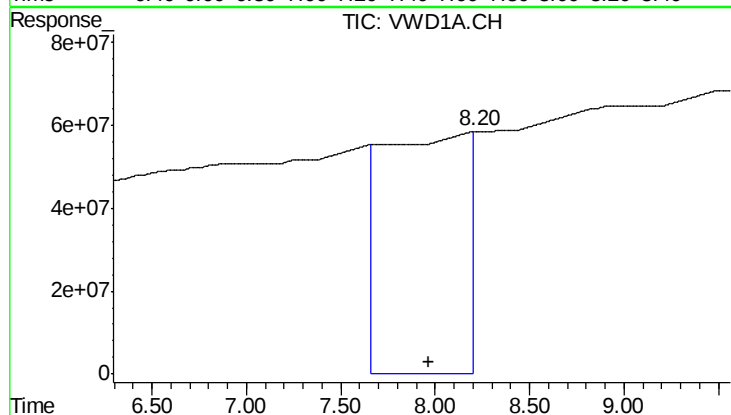


#10 2-Amino-4,6-dinitrotoluene

R.T.: 7.969 min
Delta R.T.: 0.002 min
Response: 7539549
Conc: 745.98 ug/L

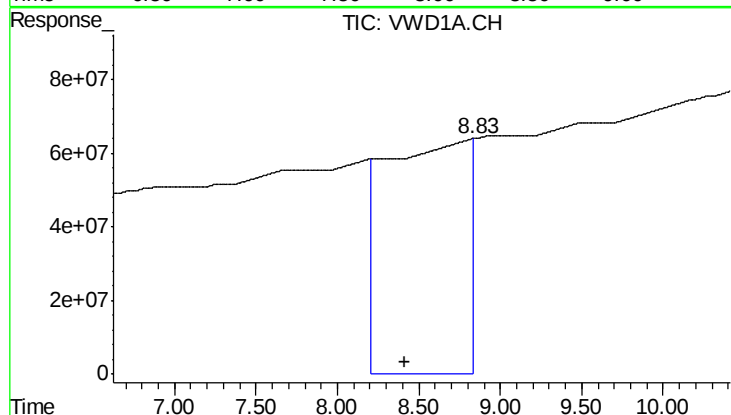


#11 4-Amino-2,6-dinitrotoluene

R.T.: 8.425 min
Delta R.T.: 0.012 min
Response: 5090438
Conc: 923.16 ug/L

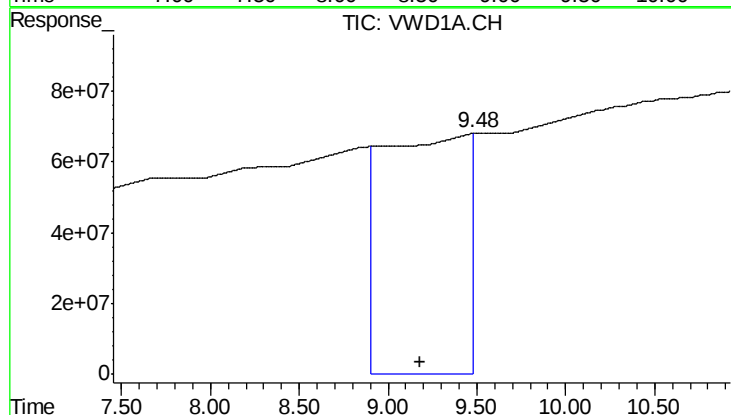

#12 2,4-Dinitrotoluene

R.T.: 9.218 min
Delta R.T.: 0.037 min
Response: 10673085
Conc: 792.32 ug/L

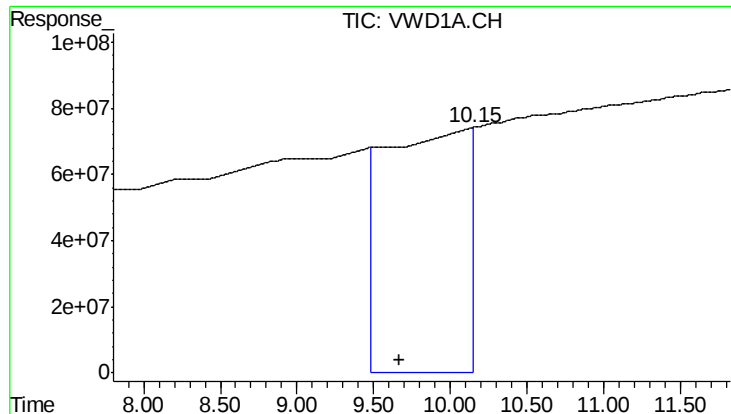


#13 2,6-Dinitrotoluene

R.T.: 9.703 min
 Delta R.T.: 0.037 min
 Response: 5965841
 Conc: 815.86 ug/L

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDICC2000


Manual Integrations
 APPROVED

TEJASKUMAR
 10/13/2014 4:13:55 PM

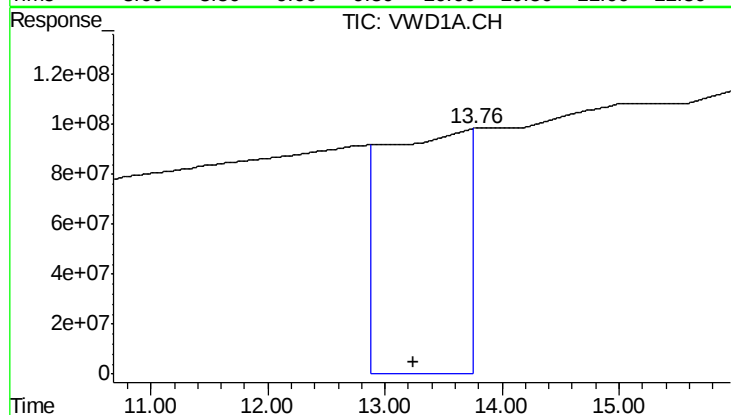


#14 2-Nitrotoluene

R.T.: 13.298 min
 Delta R.T.: 0.057 min
 Response: 5313839
 Conc: 925.40 ug/L

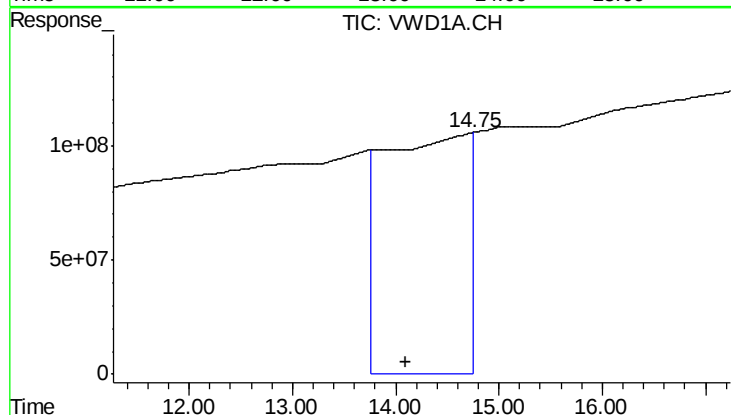


#15 4-Nitrotoluene

R.T.: 14.167 min
 Delta R.T.: 0.066 min
 Response: 4228860
 Conc: 909.29 ug/L

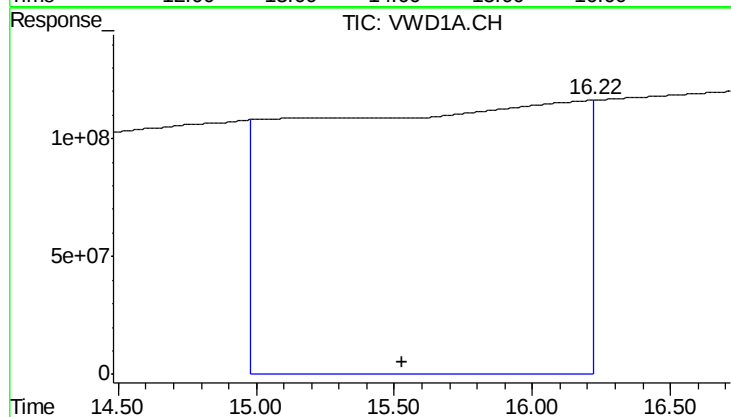

#16 3-Nitrotoluene

R.T.: 15.597 min
 Delta R.T.: 0.070 min
 Response: 5351646
 Conc: 890.50 ug/L

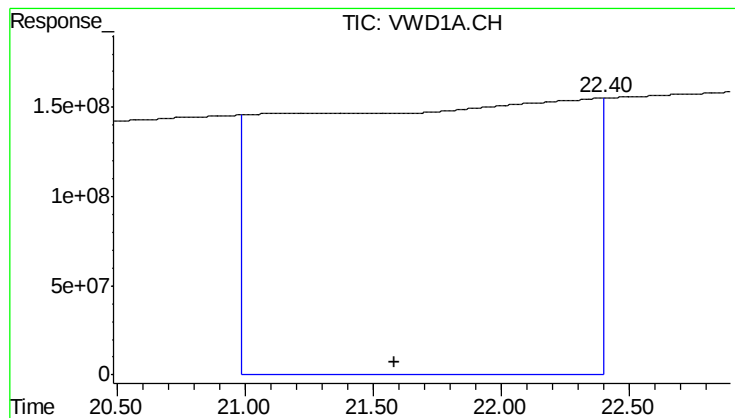

#17 PETN

R.T.: 21.659 min
Delta R.T.: 0.075 min
Response: 2338178
Conc: 349.84 ug/L m

Instrument :
HPLC_N
ClientSampleId :
HSTDICC2000

Manual Integrations
APPROVED

TEJASKUMAR
10/13/2014 4:13:55 PM