

Data File : H:\VOL1\HPLC\HPLC N\120928\HN000509.D Vial: 2
Acq On : 28-Sep-2012, 16:16 Operator: HLM
Sample : NO-CCV Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Sep 28 18:48 2012 Quant Results File: HN092512.RES

Instrument :
HPLC_N
LabSampleId :
NQ-CCV

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN092512.M (Chemstation Integrator)
Title : SW8330 / 8330A confirmation
Last Update : Fri Sep 28 18:45:58 2012
Response via : Initial Calibration
DataAcq Meth : NQ_AGP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

Target Compounds			
1) T Nitroguanidine	4.30	7061779	50.797 ug/L


Quantitation Report


Data File : H:\VOL1\HPLC\HPLC N\120928\HN000509.D Vial: 2
 Acq On : 28-Sep-2012, 16:16 Operator: HLM
 Sample : NQ-CCV Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Sep 28 18:48 2012 Quant Results File: HN092512.RES

Instrument :
 HPLC_N
 LabSampleId :
 NQ-CCV

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN092512.M (Chemstation Integrator)
 Title : SW8330 / 8330A confirmation
 Last Update : Fri Sep 28 18:45:58 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : NQ_AGP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

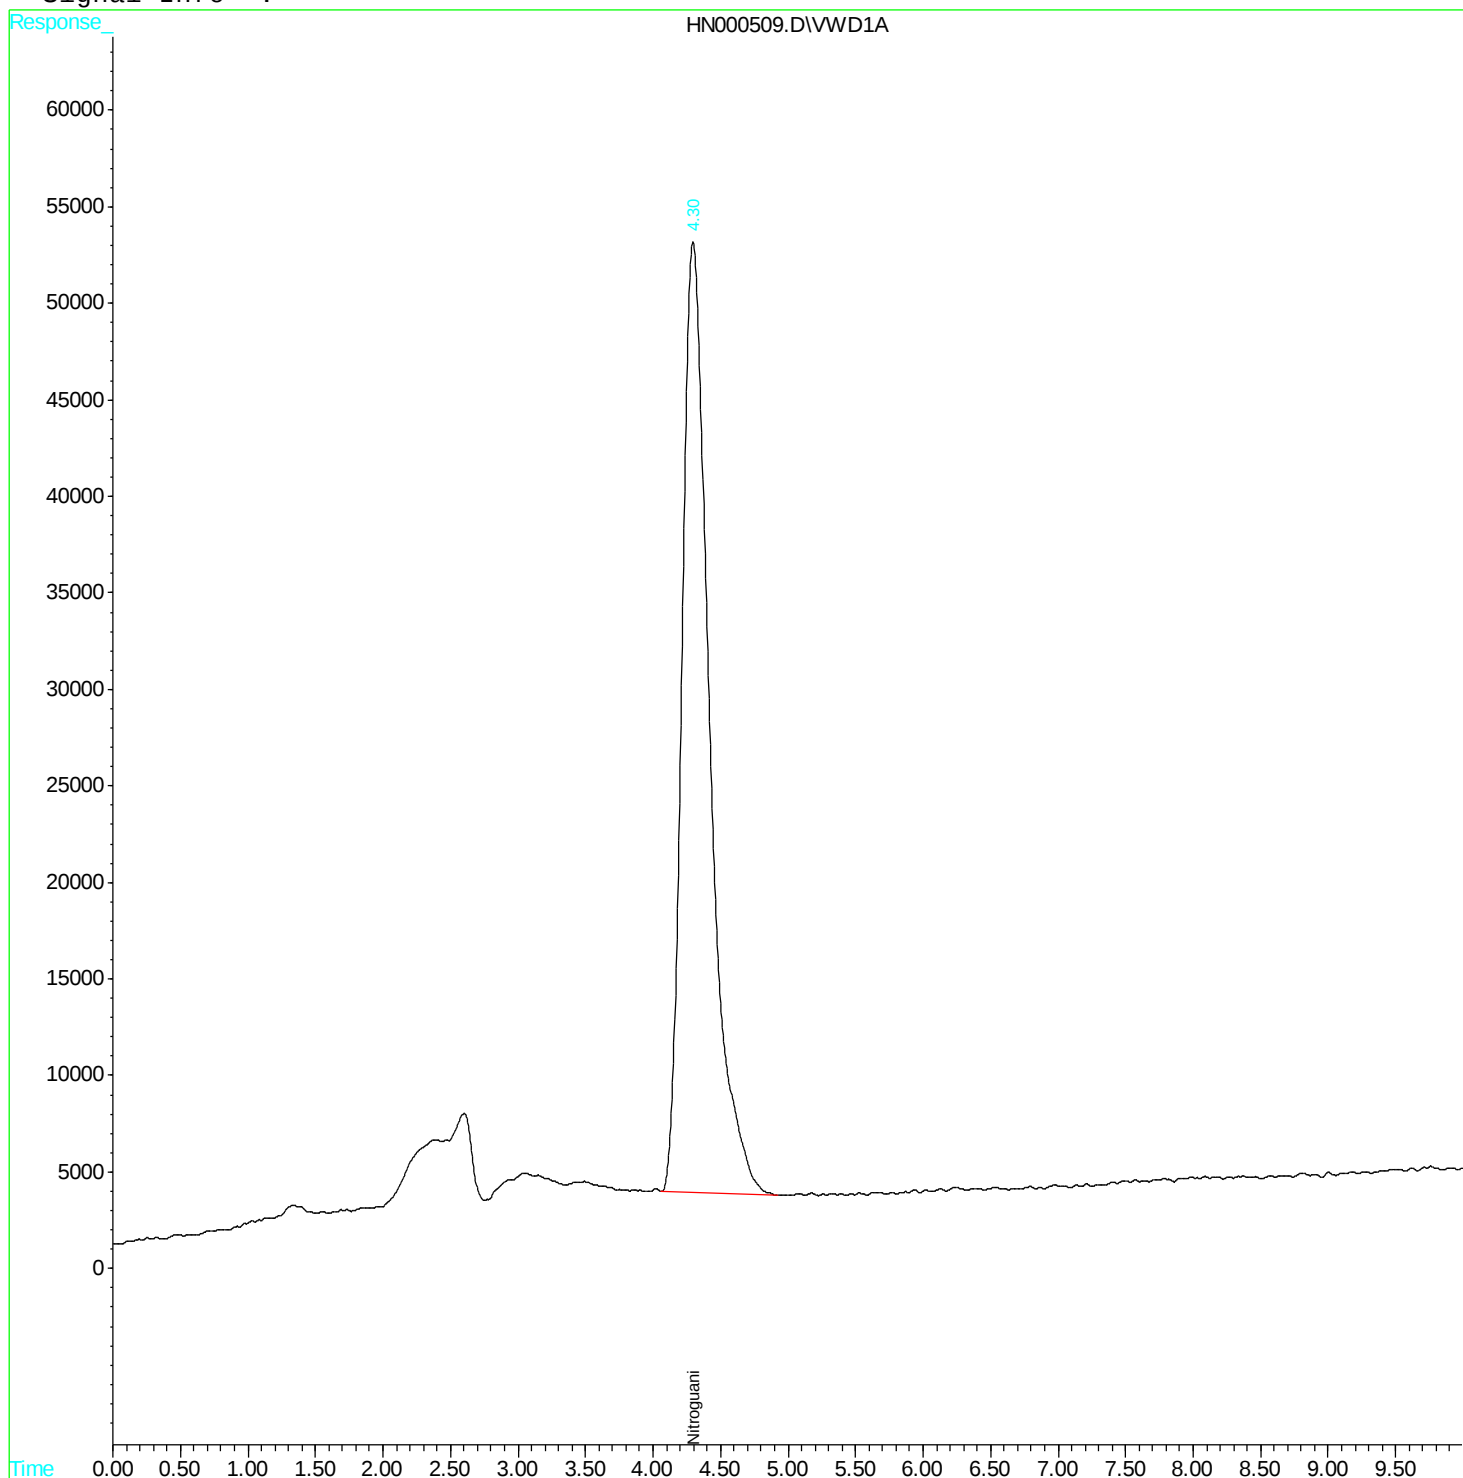

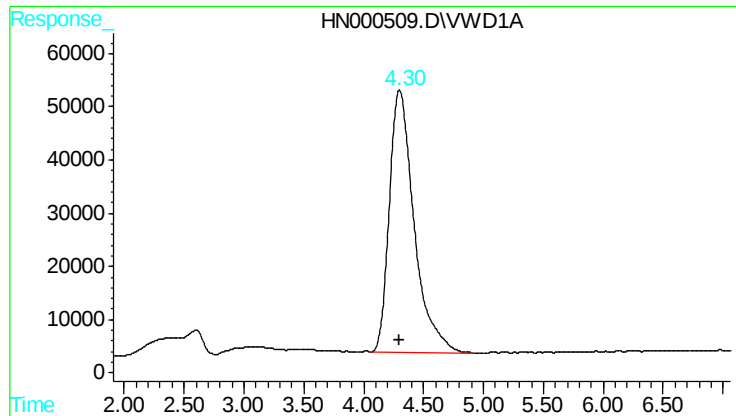

#1 Nitroguanidine

R.T.: 4.299 min
Delta R.T.: 0.000 min
Response: 7061779
Conc: 50.80 ug/L

Instrument :
HPLC_N
LabSampleId :
NQ-CCV