

Data File : H:\VOL1\HPLC\HPLC N\121010\HN000524.D Vial: 42
 Acq On : 10-Oct-2012, 18:28 Operator: HLM
 Sample : 8330-6 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Oct 11 16:01 2012 Quant Results File: HN101012.RES

Instrument :
 HPLC_N
 LabSampleId :
 8330-6

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN101012.M (Chemstation Integrator)
 Title : SW8330 / 8330A confirmation
 Last Update : Thu Oct 11 15:58:27 2012
 Response via : Initial Calibration
 DataAcq Meth : 8330VWDC.M

Volume Inj. :
 Signal Phase :
 Signal Info :

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	7.66	49582453	4758.067 ug/L
Target Compounds				
2) T	HMX	12.98	50964854	4748.094 ug/L
3) T	RDX	10.77	67788558	4834.438 ug/L
4) T	1,3,5-Trinitrobenzene	24.93	70696351	2415.568 ug/L
5) T	Tetryl	35.50	107562917	4905.873 ug/L
6) T	2,4,6-Trinitrotoluene	33.61	66259449	2421.198 ug/L
7) T	2-Amino-4,6-dinitrotoluene	16.31	117589435	2316.475 ug/L
8) T	4-Amino-2,6-dinitrotoluene	16.31	117589435	2316.475 ug/L
9) T	2,4-Dinitrotoluene	21.94	94589813	2431.113 ug/L
10) T	2,6-Dinitrotoluene	20.49	48868970	2421.559 ug/L
11) T	1,3-Dinitrobenzene	15.82	101315725	2465.697 ug/L
12) T	Nitrobenzene	12.29	66364745	2432.714 ug/L
13) T	2-Nitrotoluene	16.86	84855429	4883.845 ug/L
14) T	3-Nitrotoluene	18.11	91510984	4738.114 ug/L
15) T	4-Nitrotoluene	17.39	71529119	4746.061 ug/L
16) T	3,5-Dinitroaniline	13.72	165228808	4673.858 ug/L

Data File : H:\VOL1\HPLC\HPLC N\121010\HN000524.D

Vial: 42

Acq On : 10-Oct-2012, 18:28

Operator: HLM

Sample : 8330-6

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Oct 11 16:01 2012 Quant Results File: HN101012.RES

Instrument :

HPLC_N

LabSampleId :

8330-6

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN101012.M (Chemstation Integrator)

Title : SW8330 / 8330A confirmation

Last Update : Thu Oct 11 15:58:27 2012


Response via : Multiple Level Calibration


DataAcq Meth : 8330VWDC.M

Volume Inj. :

Signal Phase :

Signal Info :

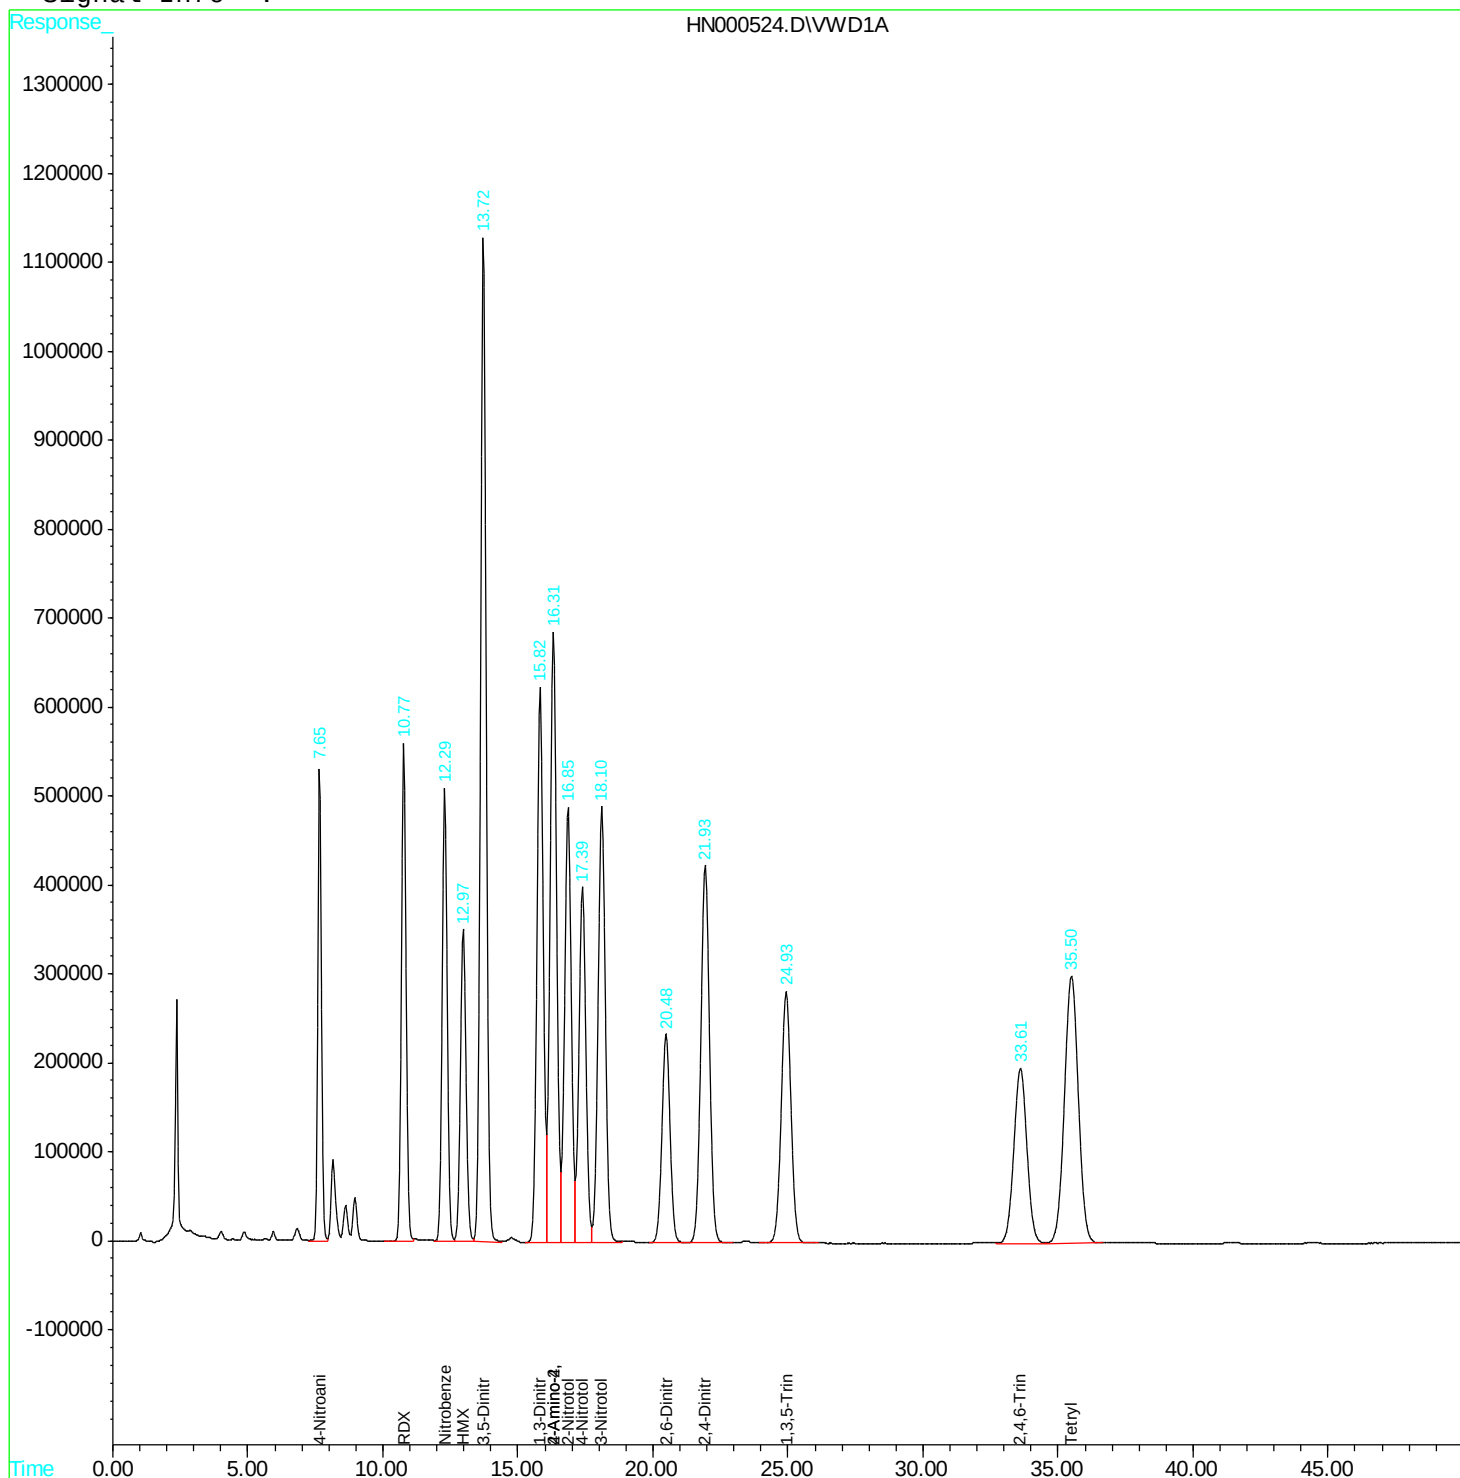


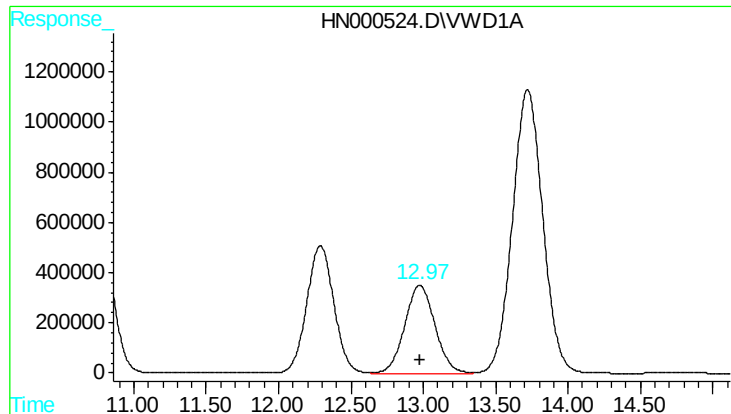

#2 HMX


R.T.: 12.975 min
Delta R.T.: -0.003 min
Response: 50964854
Conc: 4748.09 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-6

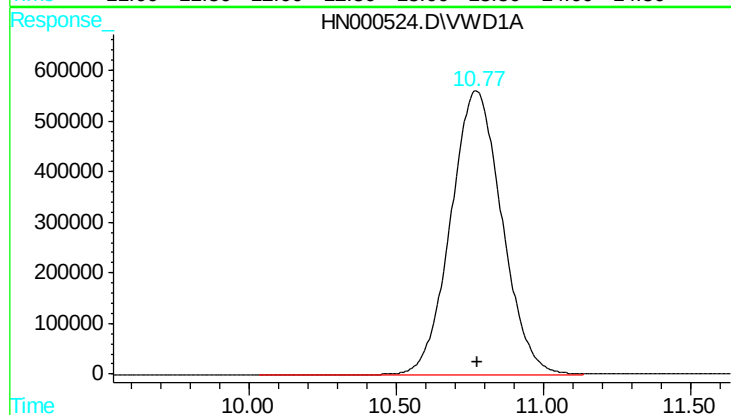


#3 RDX

R.T.: 10.772 min
Delta R.T.: -0.003 min
Response: 67788558
Conc: 4834.44 ug/L

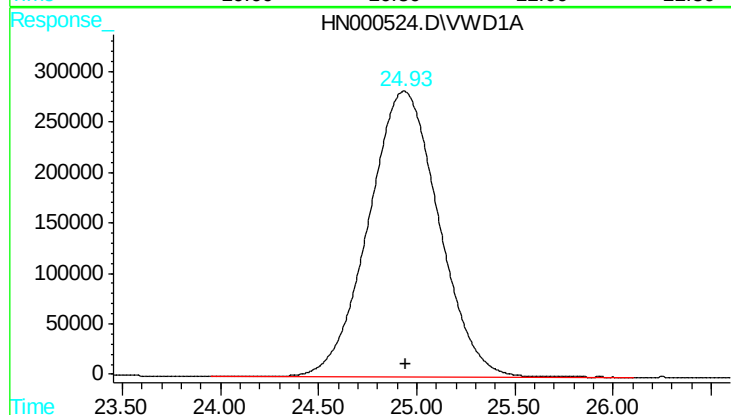


#4 1,3,5-Trinitrobenzene

R.T.: 24.934 min
Delta R.T.: -0.011 min
Response: 70696351
Conc: 2415.57 ug/L

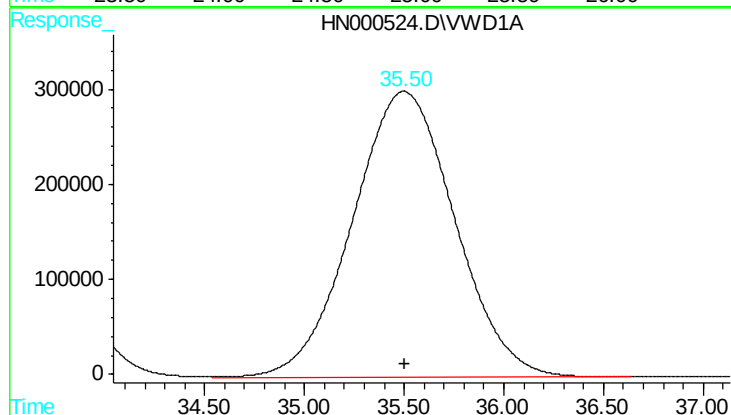

#5 Tetryl


R.T.: 35.499 min
Delta R.T.: 0.000 min
Response: 107562917
Conc: 4905.87 ug/L

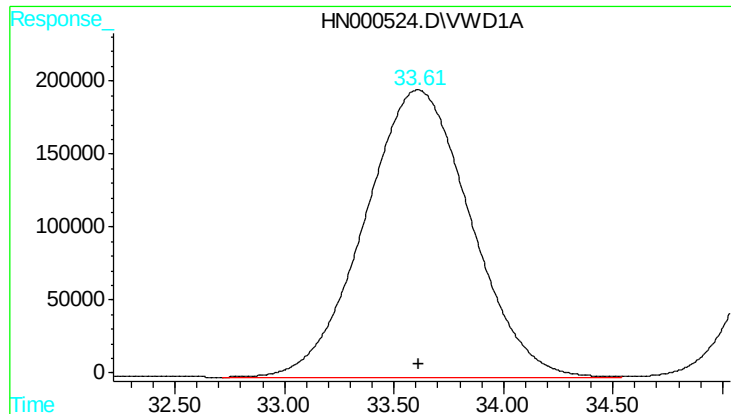

#6 2,4,6-Trinitrotoluene


R.T.: 33.609 min
Delta R.T.: -0.005 min
Response: 66259449
Conc: 2421.20 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-6

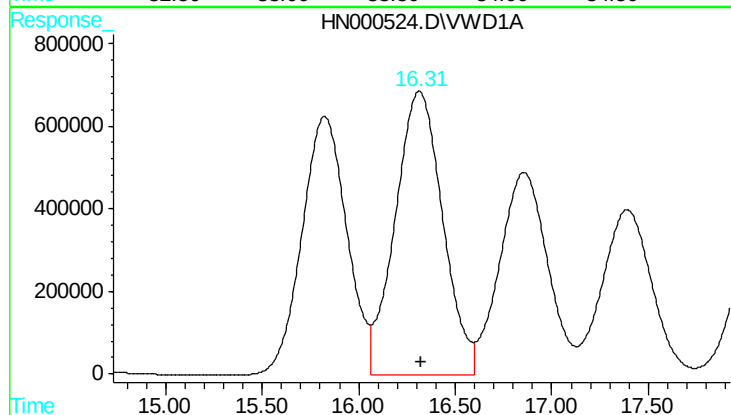


#7 2-Amino-4,6-dinitrotoluene

R.T.: 16.314 min
Delta R.T.: -0.010 min
Response: 117589435
Conc: 2316.48 ug/L

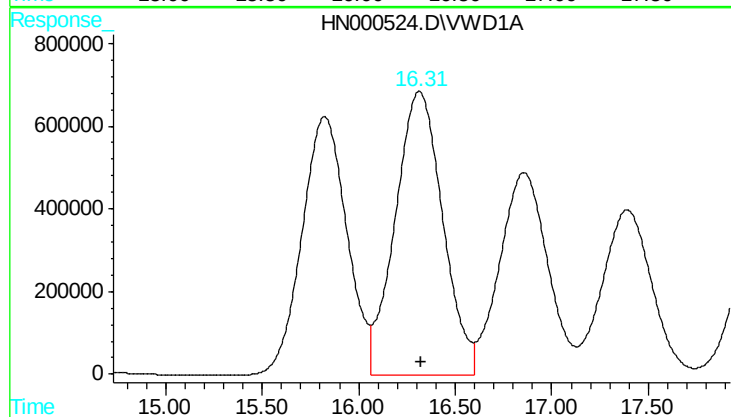


#8 4-Amino-2,6-dinitrotoluene

R.T.: 16.314 min
Delta R.T.: -0.010 min
Response: 117589435
Conc: 2316.48 ug/L

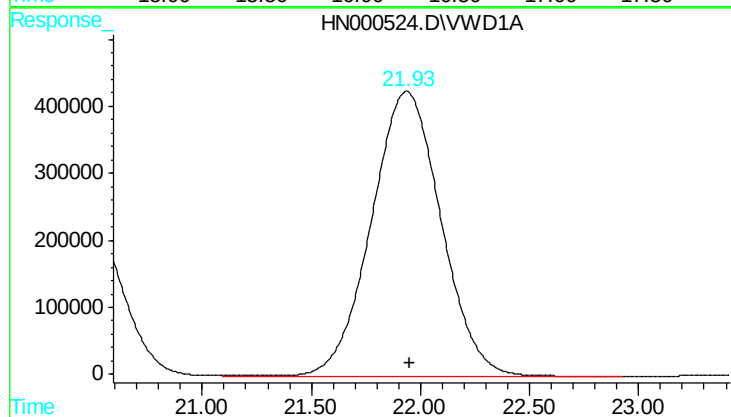

#9 2,4-Dinitrotoluene


R.T.: 21.937 min
Delta R.T.: -0.014 min
Response: 94589813
Conc: 2431.11 ug/L

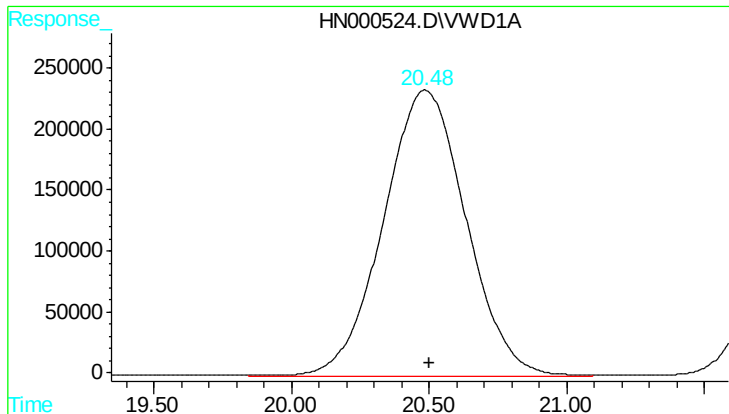

#10 2,6-Dinitrotoluene


R.T.: 20.486 min
Delta R.T.: -0.016 min
Response: 48868970
Conc: 2421.56 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-6

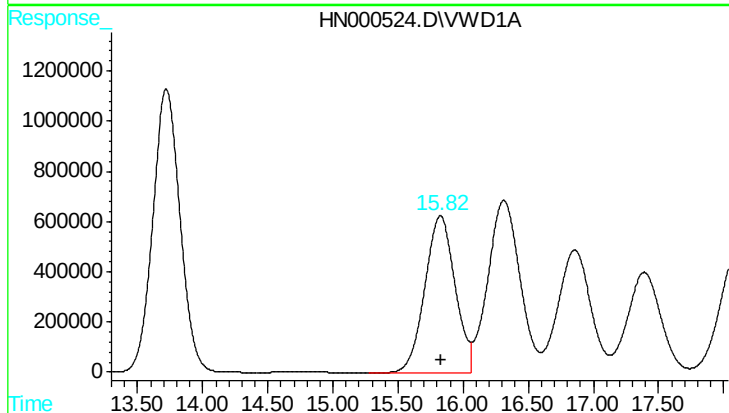


#11 1,3-Dinitrobenzene

R.T.: 15.823 min
Delta R.T.: -0.011 min
Response: 101315725
Conc: 2465.70 ug/L

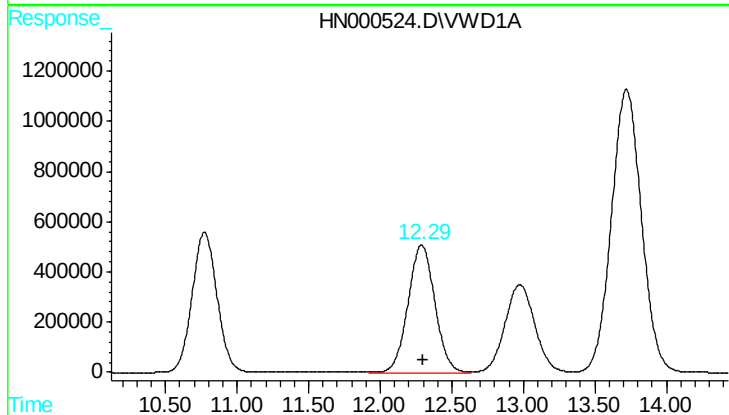


#12 Nitrobenzene

R.T.: 12.289 min
Delta R.T.: -0.010 min
Response: 66364745
Conc: 2432.71 ug/L

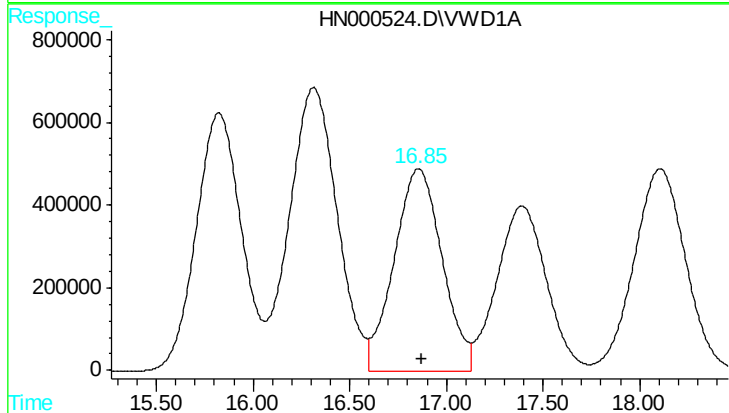

#13 2-Nitrotoluene


R.T.: 16.856 min
Delta R.T.: -0.014 min
Response: 84855429
Conc: 4883.85 ug/L

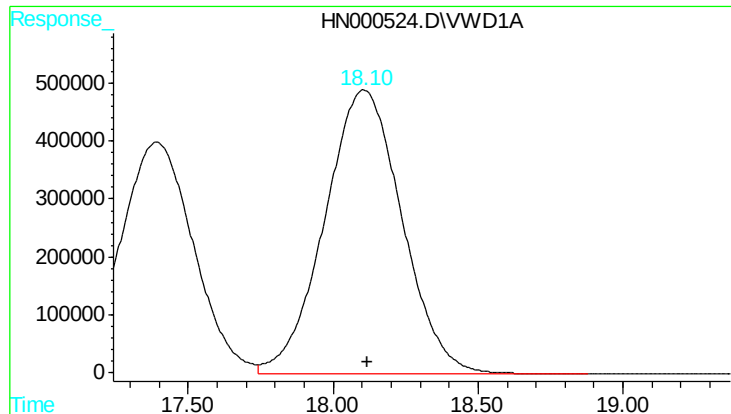

#14 3-Nitrotoluene


R.T.: 18.106 min
Delta R.T.: -0.015 min
Response: 91510984
Conc: 4738.11 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-6

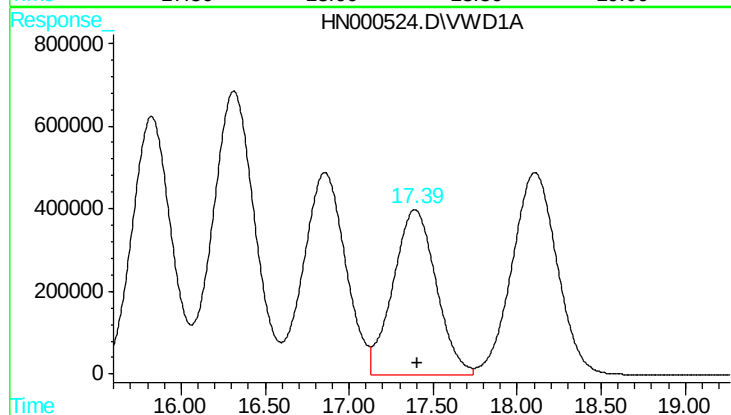

#15 4-Nitrotoluene

R.T.: 17.391 min
Delta R.T.: -0.014 min
Response: 71529119
Conc: 4746.06 ug/L

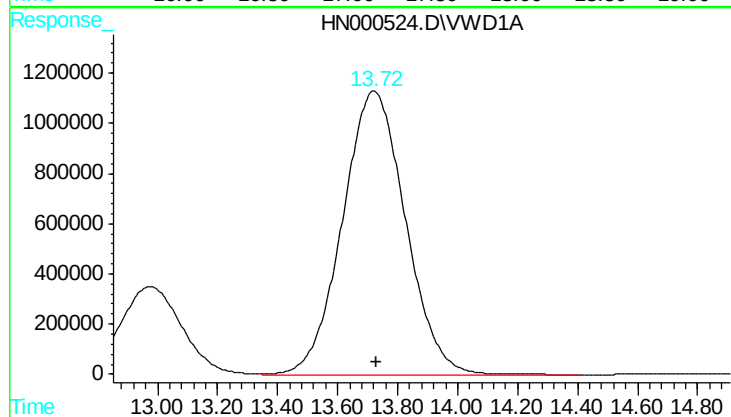

#16 3,5-Dinitroaniline

R.T.: 13.721 min
Delta R.T.: -0.008 min
Response: 165228808
Conc: 4673.86 ug/L