

Data File : H:\VOL1\HPLC\HPLC N\121010\HN000525.D Vial: 43
Acq On : 10-Oct-2012, 19:21 Operator: HLM
Sample : 8330-5 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Oct 11 16:02 2012 Quant Results File: HN101012.RES

Instrument :
HPLC_N
LabSampleId :
8330-5

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN101012.M (Chemstation Integrator)
Title : SW8330 / 8330A confirmation
Last Update : Thu Oct 11 15:58:27 2012
Response via : Initial Calibration
DataAcq Meth : 8330VWDC.M

Volume Inj. :
Signal Phase :
Signal Info :

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	7.66	20794901	1995.535 ug/L
Target Compounds				
2) T	HMX	12.97	20542548	1913.828 ug/L
3) T	RDX	10.77	27293423	1946.470 ug/L
4) T	1,3,5-Trinitrobenzene	24.93	28727277	981.560 ug/L
5) T	Tetryl	35.50	42982996	1960.426 ug/L
6) T	2,4,6-Trinitrotoluene	33.61	26792959	979.046 ug/L
7) T	2-Amino-4,6-dinitrotoluene	16.31	47732778	940.321 ug/L
8) T	4-Amino-2,6-dinitrotoluene	16.31	47732778	940.321 ug/L
9) T	2,4-Dinitrotoluene	21.94	38292635	984.184 ug/L
10) T	2,6-Dinitrotoluene	20.49	19780769	980.178 ug/L
11) T	1,3-Dinitrobenzene	15.82	41013551	998.137 ug/L
12) T	Nitrobenzene	12.29	25470714	933.673 ug/L
13) T	2-Nitrotoluene	16.86	33120072	1906.222 ug/L
14) T	3-Nitrotoluene	18.11	35801906	1853.696 ug/L
15) T	4-Nitrotoluene	17.39	28366061	1882.129 ug/L
16) T	3,5-Dinitroaniline	13.72	66753216	1888.261 ug/L

Data File : H:\VOL1\HPLC\HPLC N\121010\HN000525.D

Vial: 43

Acq On : 10-Oct-2012, 19:21

Operator: HLM

Sample : 8330-5

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Oct 11 16:02 2012 Quant Results File: HN101012.RES

Instrument :

HPLC_N

LabSampleId :

8330-5

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN101012.M (Chemstation Integrator)

Title : SW8330 / 8330A confirmation

Last Update : Thu Oct 11 15:58:27 2012


Response via : Multiple Level Calibration


DataAcq Meth : 8330VWDC.M

Volume Inj. :

Signal Phase :

Signal Info :

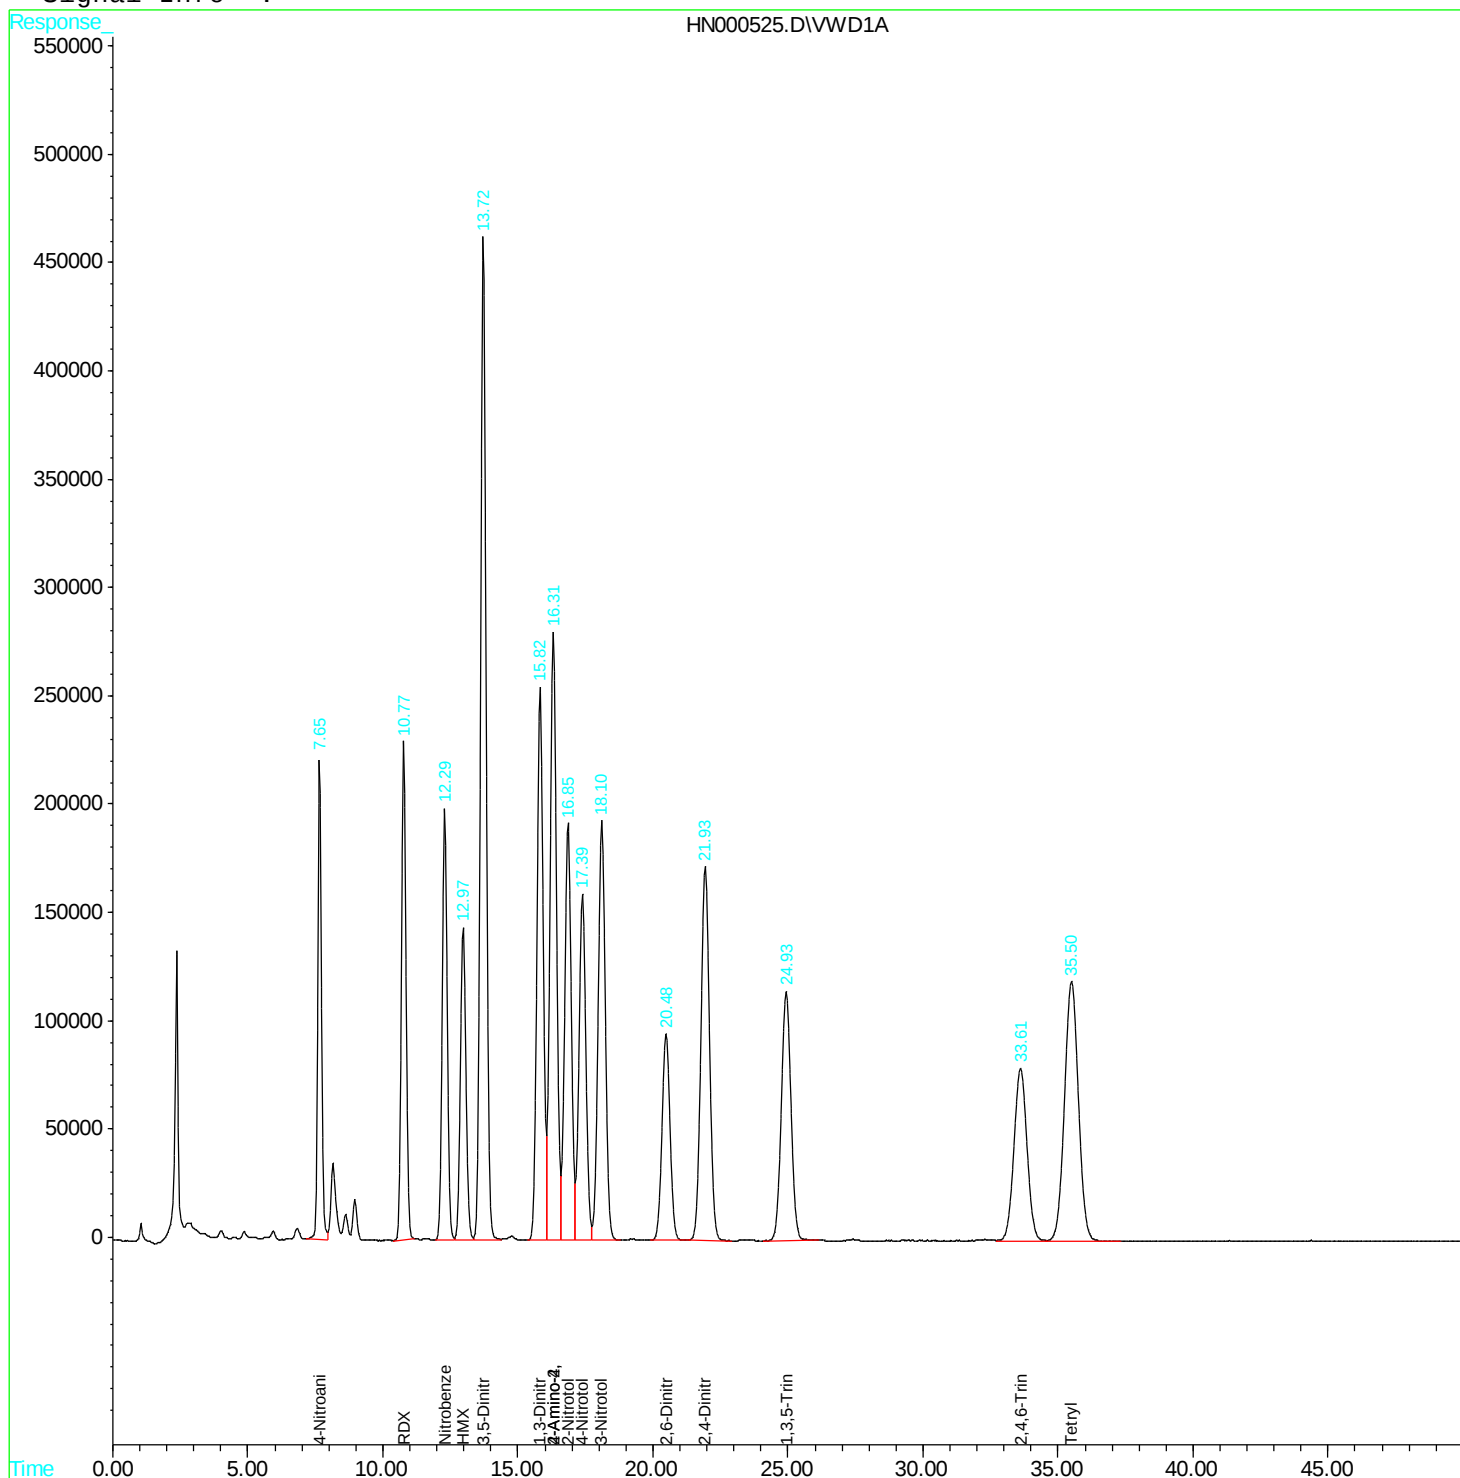


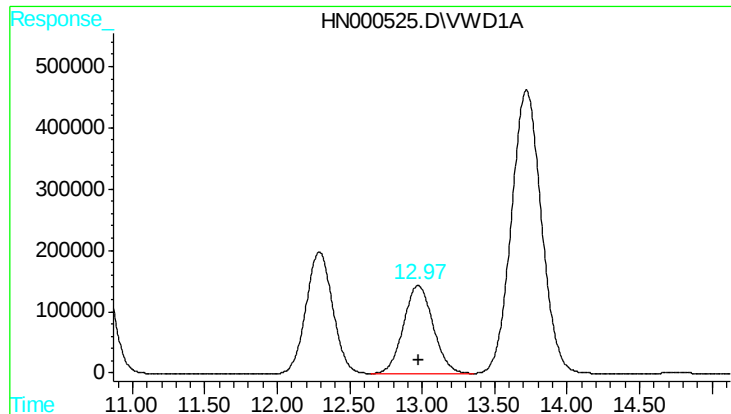

#2 HMX


R.T.: 12.972 min
Delta R.T.: -0.007 min
Response: 20542548
Conc: 1913.83 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-5

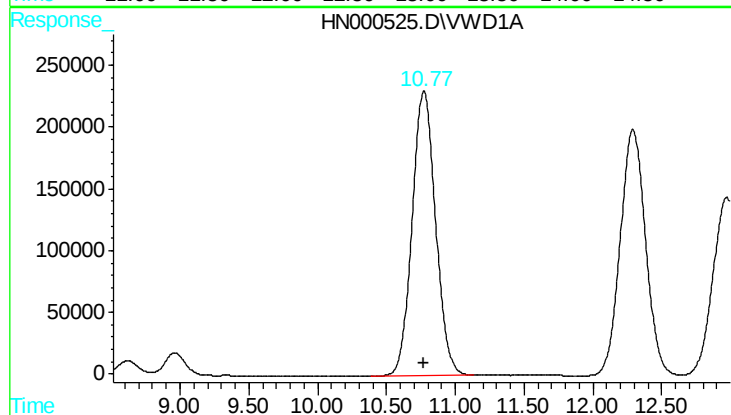


#3 RDX

R.T.: 10.771 min
Delta R.T.: -0.005 min
Response: 27293423
Conc: 1946.47 ug/L

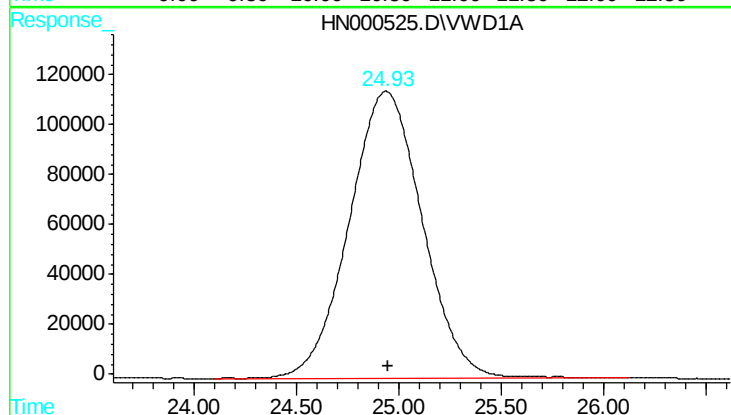


#4 1,3,5-Trinitrobenzene

R.T.: 24.935 min
Delta R.T.: -0.010 min
Response: 28727277
Conc: 981.56 ug/L

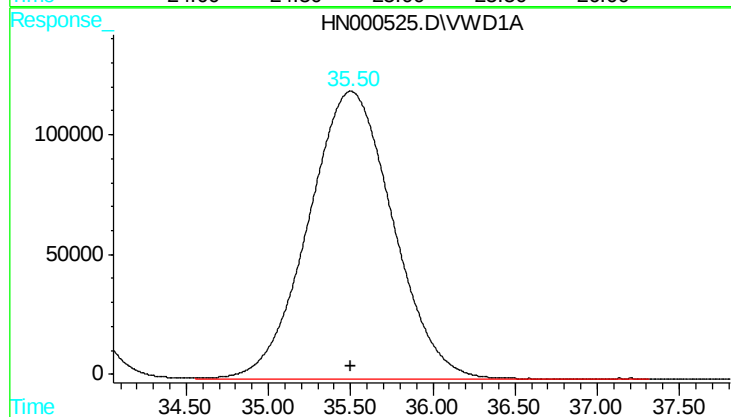

#5 Tetryl


R.T.: 35.501 min
Delta R.T.: 0.000 min
Response: 42982996
Conc: 1960.43 ug/L

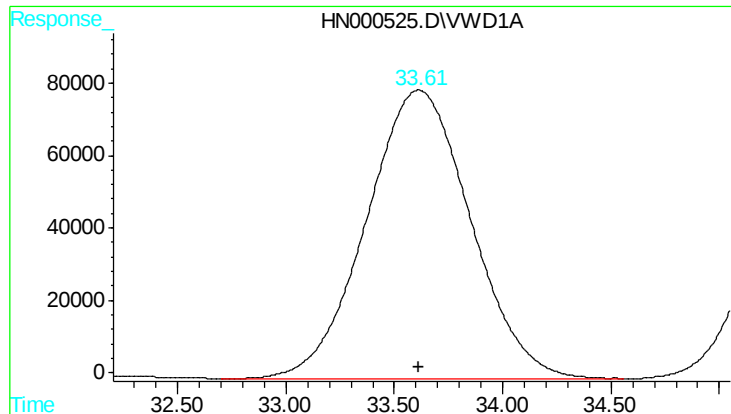

#6 2,4,6-Trinitrotoluene


R.T.: 33.612 min
Delta R.T.: -0.002 min
Response: 26792959
Conc: 979.05 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-5

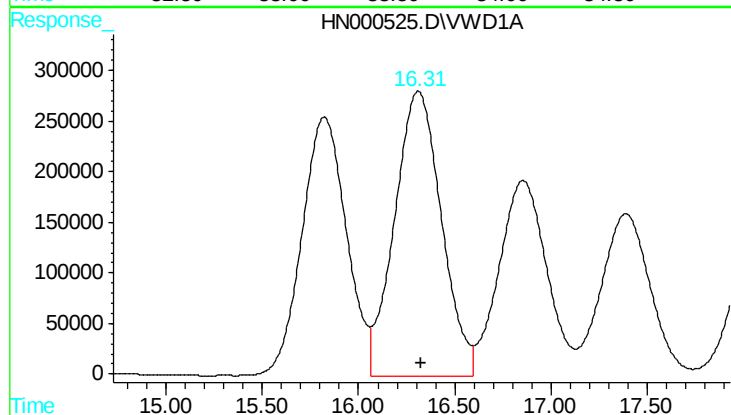


#7 2-Amino-4,6-dinitrotoluene

R.T.: 16.310 min
Delta R.T.: -0.013 min
Response: 47732778
Conc: 940.32 ug/L

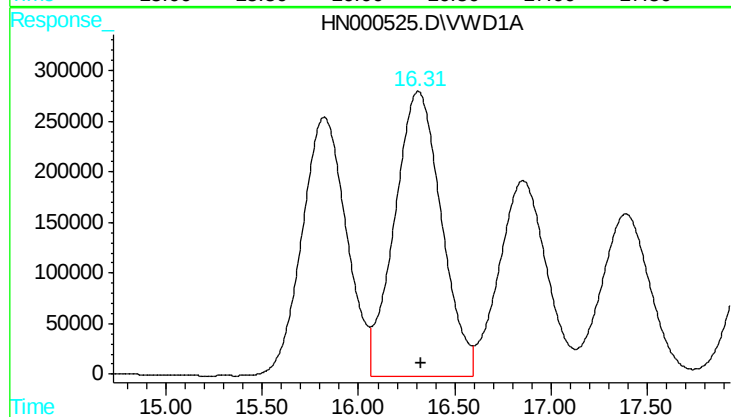


#8 4-Amino-2,6-dinitrotoluene

R.T.: 16.310 min
Delta R.T.: -0.013 min
Response: 47732778
Conc: 940.32 ug/L

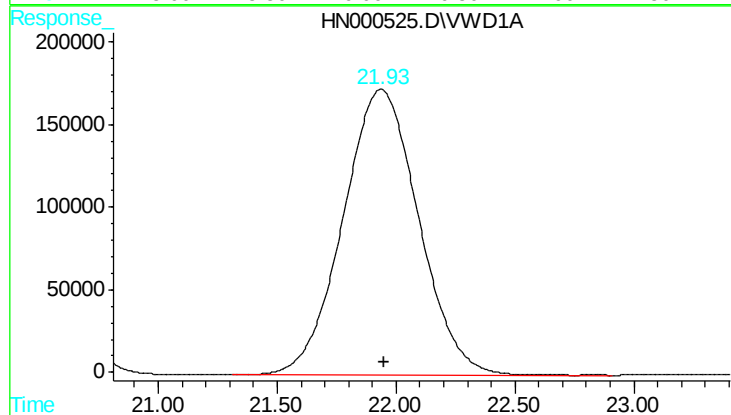

#9 2,4-Dinitrotoluene


R.T.: 21.937 min
Delta R.T.: -0.014 min
Response: 38292635
Conc: 984.18 ug/L

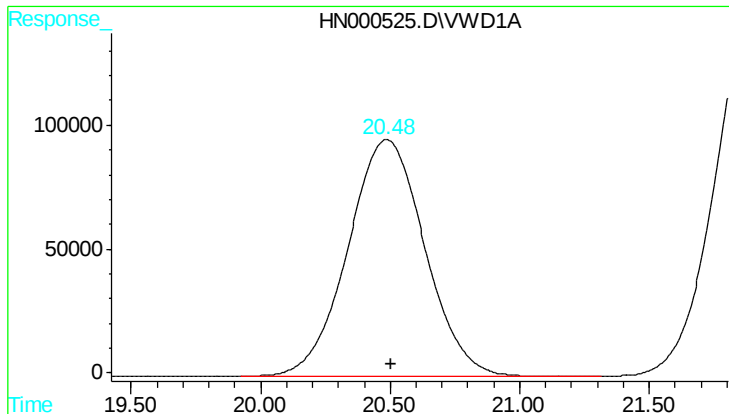

#10 2,6-Dinitrotoluene


R.T.: 20.487 min
Delta R.T.: -0.016 min
Response: 19780769
Conc: 980.18 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-5

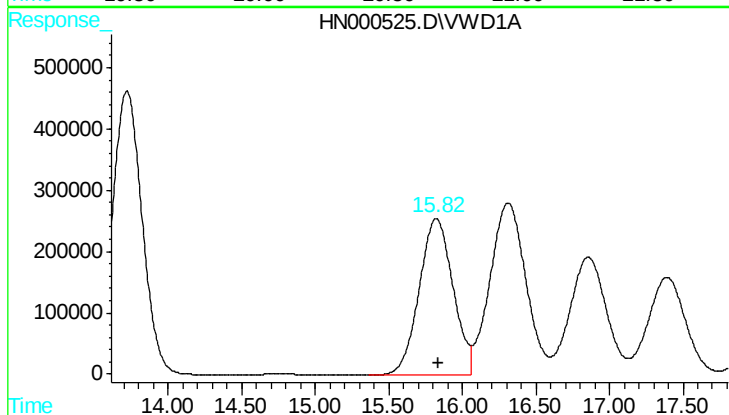


#11 1,3-Dinitrobenzene

R.T.: 15.822 min
Delta R.T.: -0.013 min
Response: 41013551
Conc: 998.14 ug/L

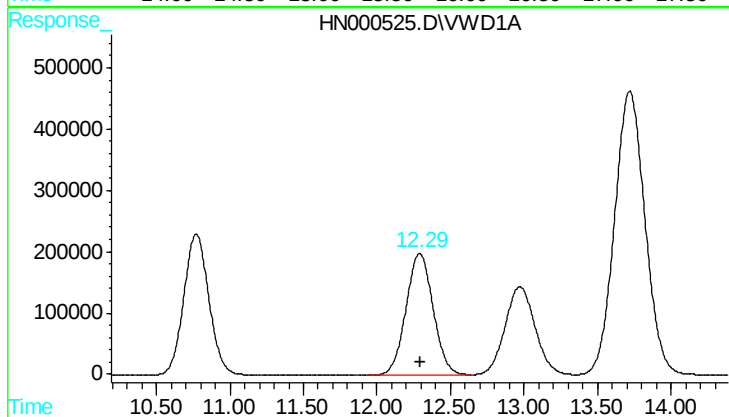


#12 Nitrobenzene

R.T.: 12.290 min
Delta R.T.: -0.009 min
Response: 25470714
Conc: 933.67 ug/L

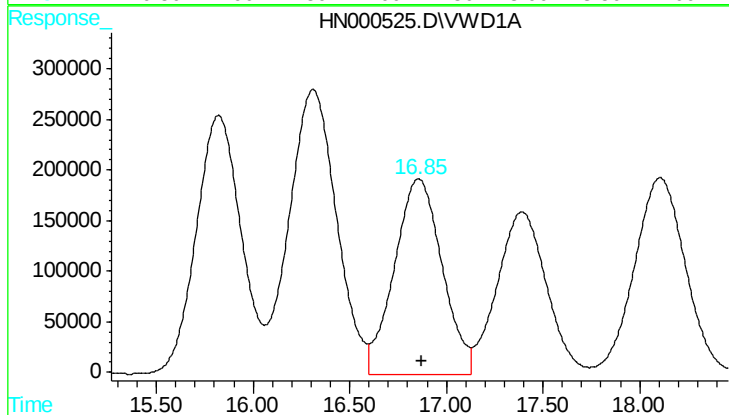

#13 2-Nitrotoluene


R.T.: 16.856 min
Delta R.T.: -0.014 min
Response: 33120072
Conc: 1906.22 ug/L

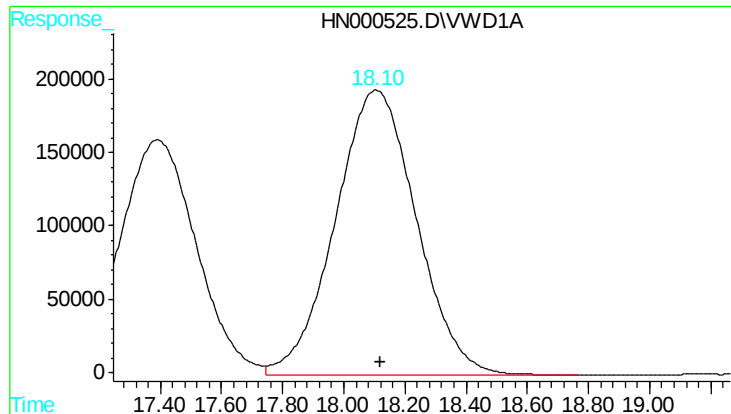

#14 3-Nitrotoluene


R.T.: 18.106 min
 Delta R.T.: -0.015 min
 Response: 35801906
 Conc: 1853.70 ug/L

Instrument :
 HPLC_N
 LabSampleId :
 8330-5

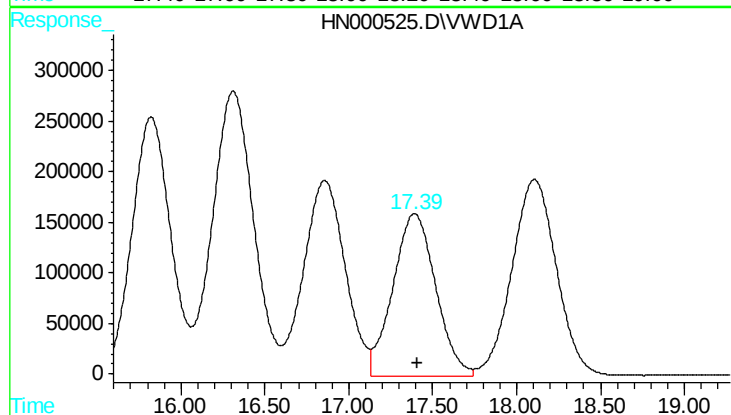

#15 4-Nitrotoluene

R.T.: 17.392 min
 Delta R.T.: -0.014 min
 Response: 28366061
 Conc: 1882.13 ug/L

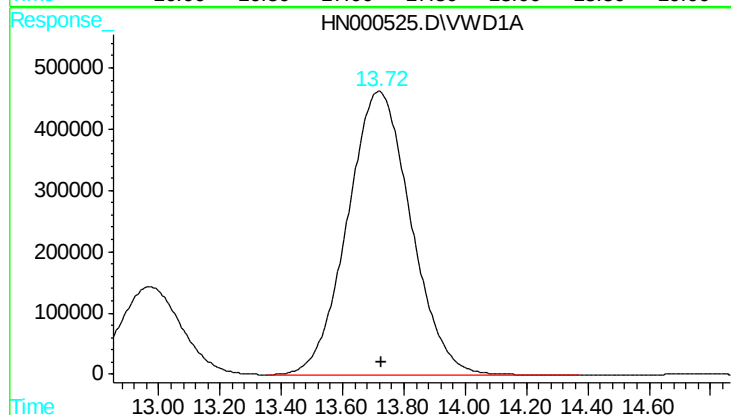

#16 3,5-Dinitroaniline

R.T.: 13.719 min
 Delta R.T.: -0.010 min
 Response: 66753216
 Conc: 1888.26 ug/L