

Data File : H:\VOL1\HPLC\HPLC N\121010\HN000527.D Vial: 45
 Acq On : 10-Oct-2012, 21:06 Operator: HLM
 Sample : 8330-3 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Oct 11 16:02 2012 Quant Results File: HN101012.RES

Instrument :
 HPLC_N
 LabSampleId :
 8330-3

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN101012.M (Chemstation Integrator)
 Title : SW8330 / 8330A confirmation
 Last Update : Thu Oct 11 15:58:27 2012
 Response via : Initial Calibration
 DataAcq Meth : 8330VWDC.M

Volume Inj. :
 Signal Phase :
 Signal Info :

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	7.65	4989060	478.764 ug/L
Target Compounds				
2) T	HMX	12.96	5090986	474.297 ug/L
3) T	RDX	10.76	6707594	478.362 ug/L
4) T	1,3,5-Trinitrobenzene	24.91	6799892	232.340 ug/L
5) T	Tetryl	35.45	10284454	469.067 ug/L
6) T	2,4,6-Trinitrotoluene	33.57	6930862	253.262 ug/L
7) T	2-Amino-4,6-dinitrotoluene	16.30	11703468	230.555 ug/L
8) T	4-Amino-2,6-dinitrotoluene	16.30	11703468	230.555 ug/L
9) T	2,4-Dinitrotoluene	21.92	9389310	241.321 ug/L
10) T	2,6-Dinitrotoluene	20.47	4835304	239.599 ug/L
11) T	1,3-Dinitrobenzene	15.81	10071356	245.104 ug/L
12) T	Nitrobenzene	12.29	6376222	233.731 ug/L
13) T	2-Nitrotoluene	16.85	8146078	468.847 ug/L
14) T	3-Nitrotoluene	18.10	9319100	482.510 ug/L
15) T	4-Nitrotoluene	17.39	7021532	465.889 ug/L
16) T	3,5-Dinitroaniline	13.71	16407529	464.123 ug/L

Quantitation Report

Data File : H:\VOL1\HPLC\HPLC N\121010\HN000527.D

Vial: 45

Acq On : 10-Oct-2012, 21:06

Operator: HLM

Sample : 8330-3

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Oct 11 16:02 2012 Quant Results File: HN101012.RES

Instrument :

HPLC_N

LabSampleId :

8330-3

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN101012.M (Chemstation Integrator)

Title : SW8330 / 8330A confirmation

Last Update : Thu Oct 11 15:58:27 2012


Response via : Multiple Level Calibration


DataAcq Meth : 8330VWDC.M

Volume Inj. :

Signal Phase :

Signal Info :

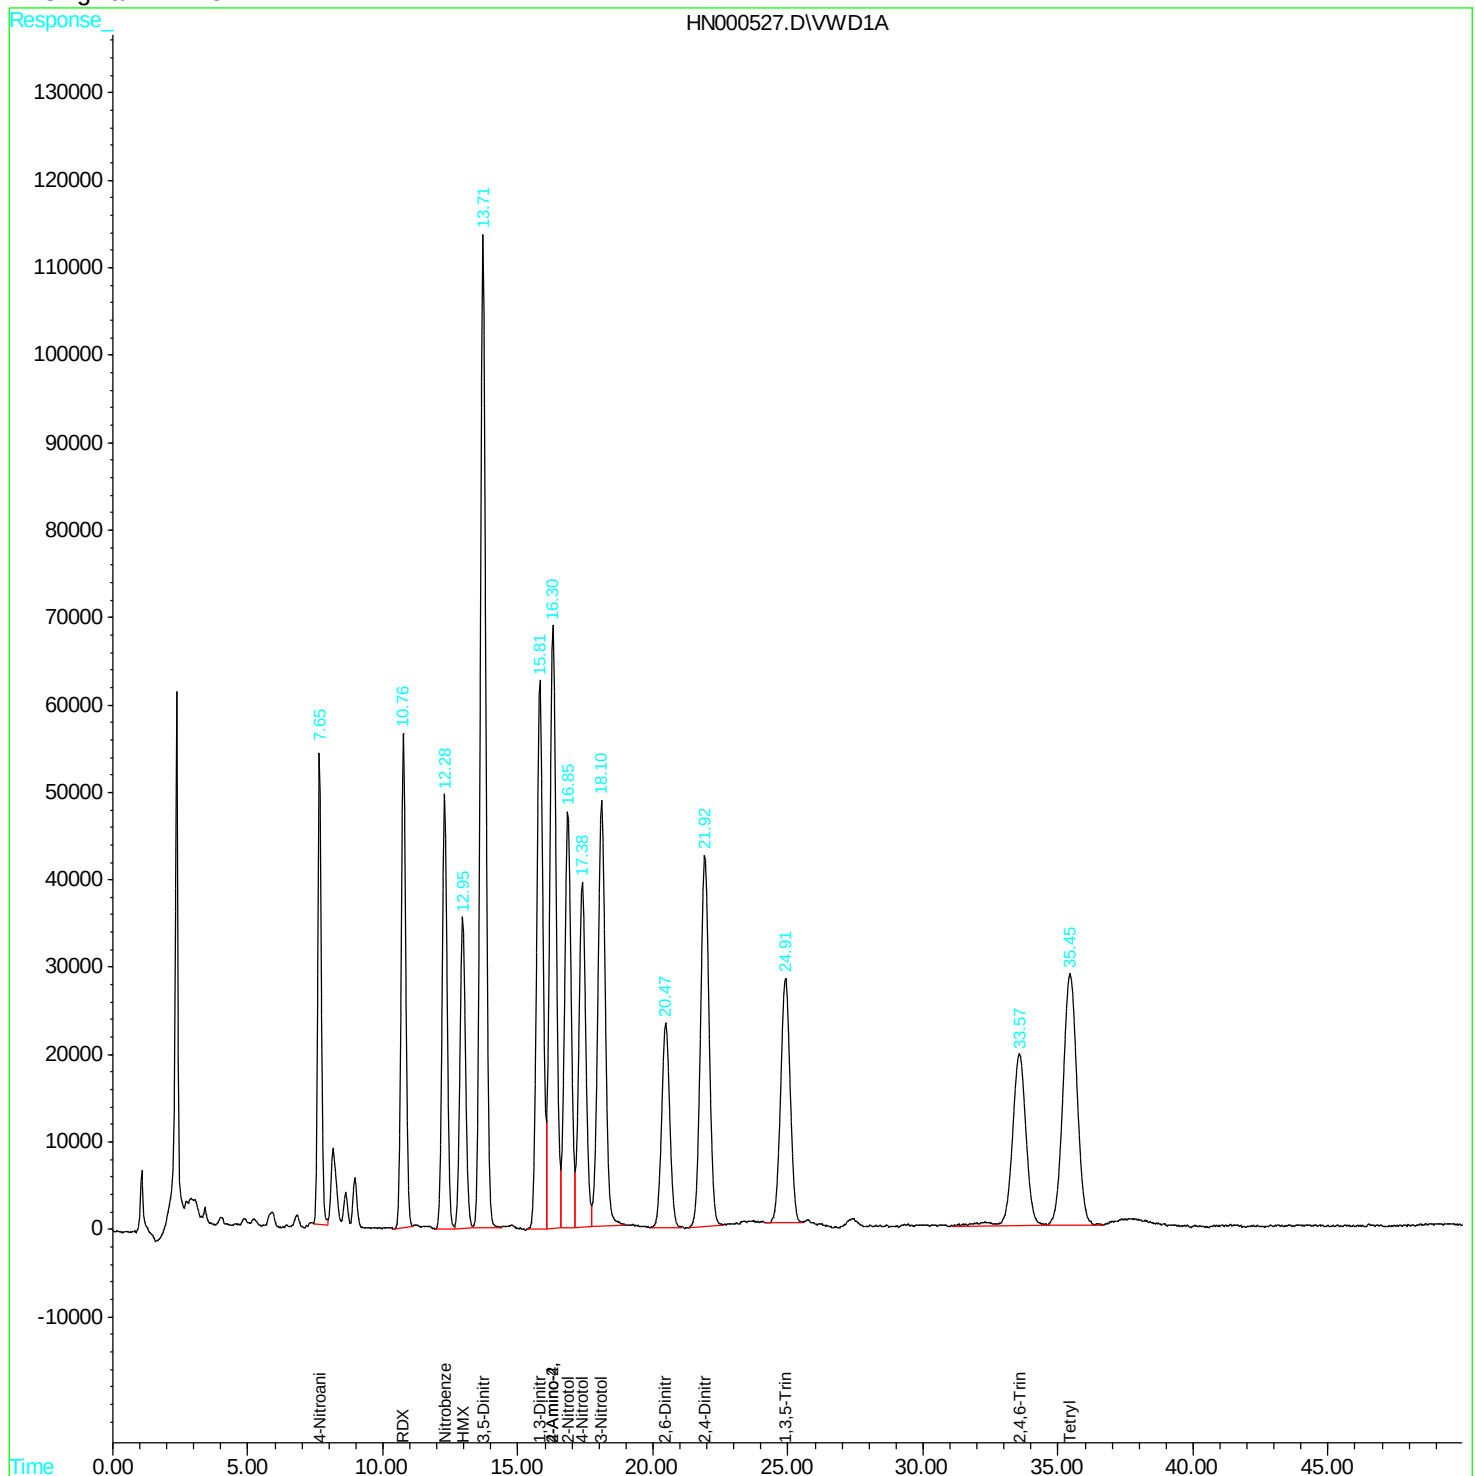


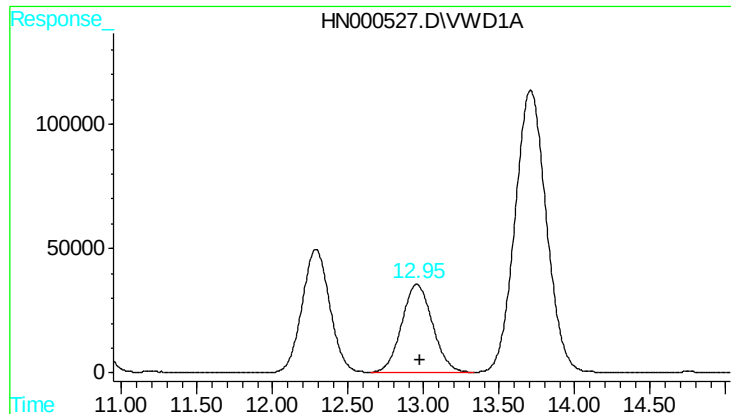

#2 HMX


R.T.: 12.955 min
Delta R.T.: -0.023 min
Response: 5090986
Conc: 474.30 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-3

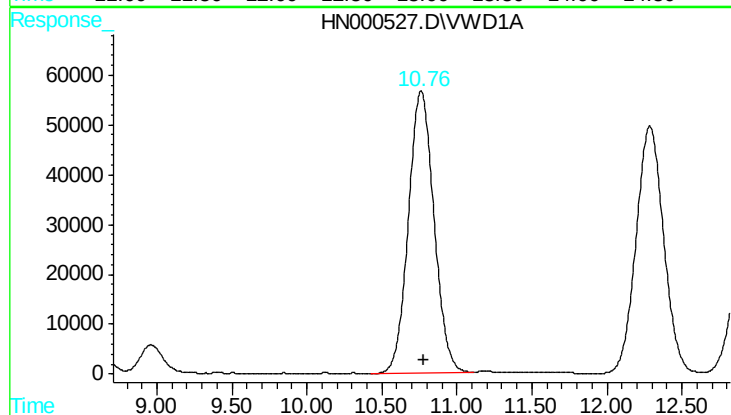


#3 RDX

R.T.: 10.761 min
Delta R.T.: -0.014 min
Response: 6707594
Conc: 478.36 ug/L

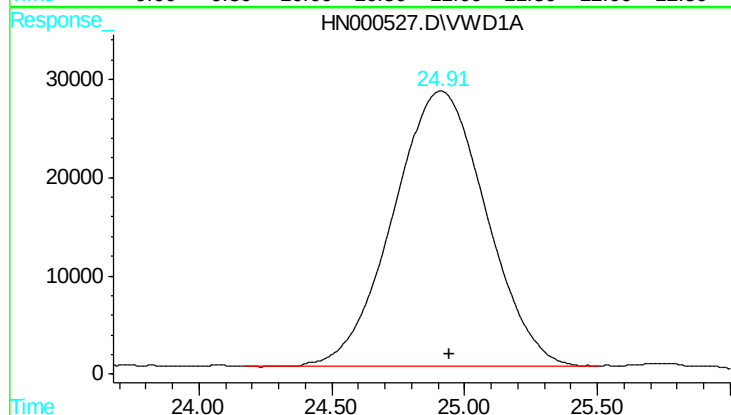


#4 1,3,5-Trinitrobenzene

R.T.: 24.909 min
Delta R.T.: -0.036 min
Response: 6799892
Conc: 232.34 ug/L

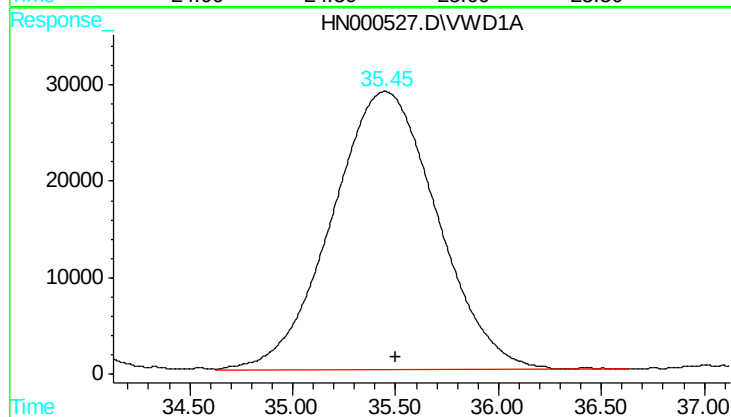

#5 Tetryl


R.T.: 35.449 min
Delta R.T.: -0.051 min
Response: 10284454
Conc: 469.07 ug/L

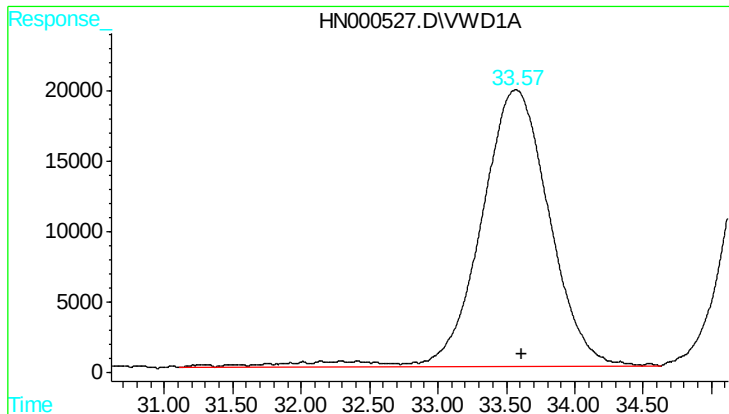

#6 2,4,6-Trinitrotoluene


R.T.: 33.569 min
Delta R.T.: -0.045 min
Response: 6930862
Conc: 253.26 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-3

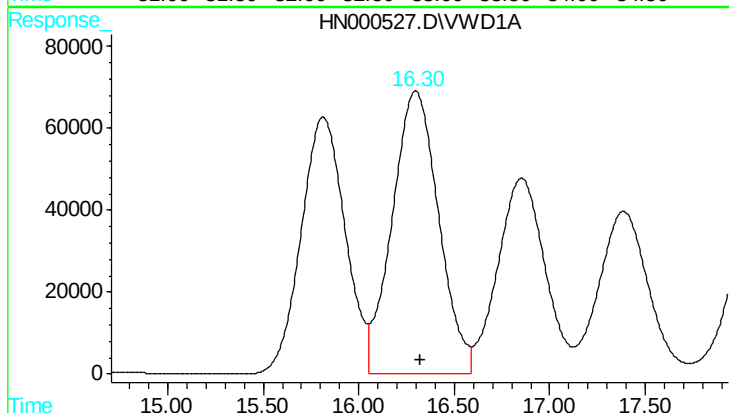


#7 2-Amino-4,6-dinitrotoluene

R.T.: 16.298 min
Delta R.T.: -0.026 min
Response: 11703468
Conc: 230.55 ug/L

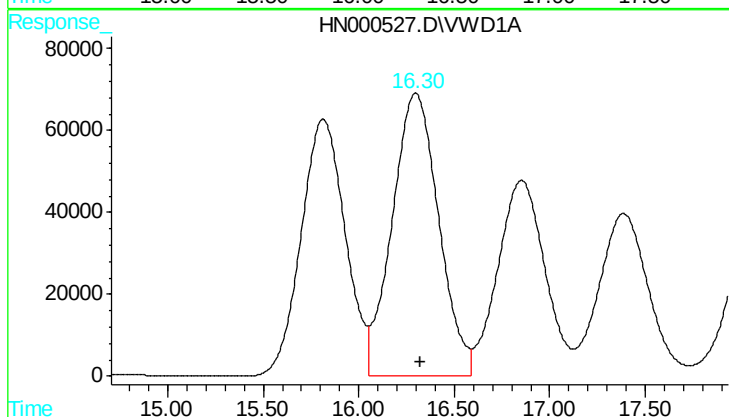


#8 4-Amino-2,6-dinitrotoluene

R.T.: 16.298 min
Delta R.T.: -0.026 min
Response: 11703468
Conc: 230.55 ug/L

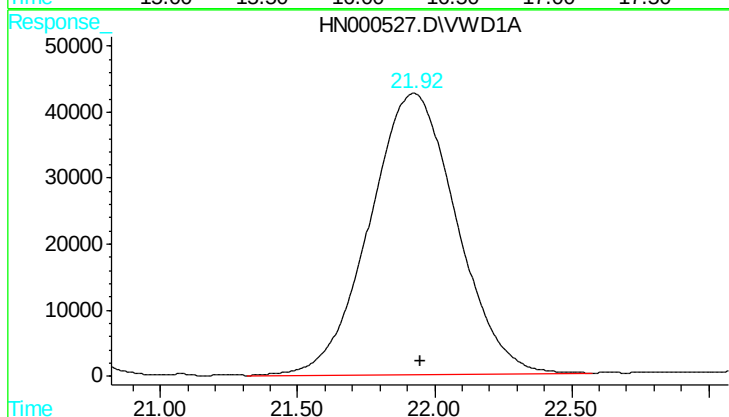

#9 2,4-Dinitrotoluene


R.T.: 21.924 min
Delta R.T.: -0.027 min
Response: 9389310
Conc: 241.32 ug/L

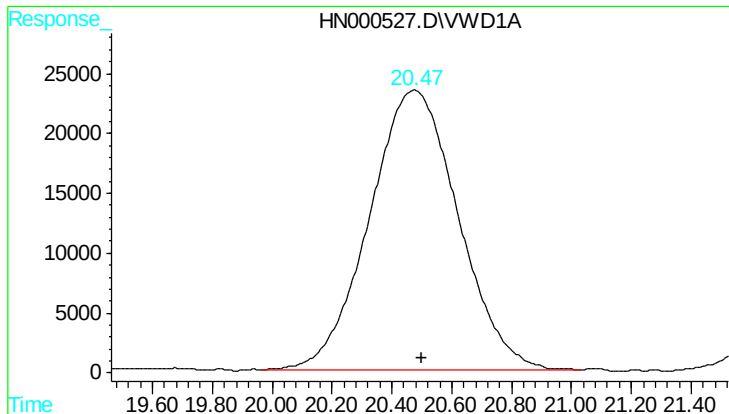

#10 2,6-Dinitrotoluene


R.T.: 20.474 min
Delta R.T.: -0.028 min
Response: 4835304
Conc: 239.60 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-3

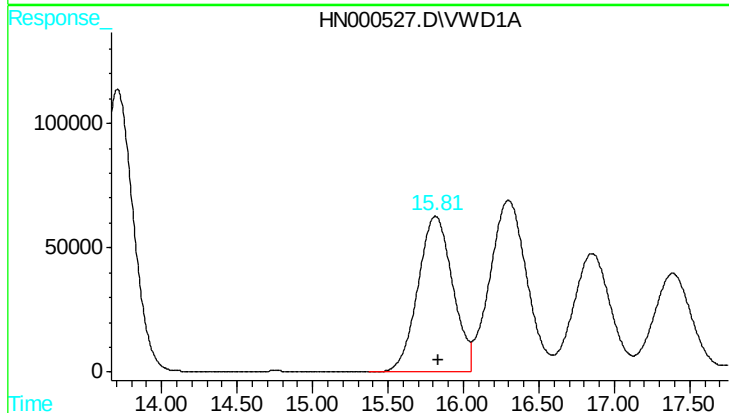


#11 1,3-Dinitrobenzene

R.T.: 15.814 min
Delta R.T.: -0.021 min
Response: 10071356
Conc: 245.10 ug/L

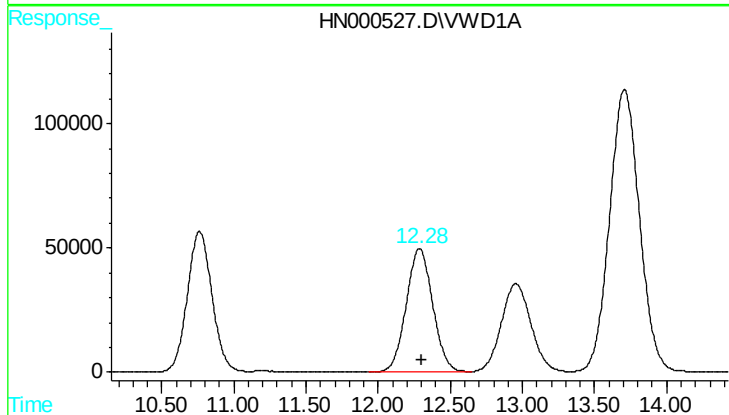


#12 Nitrobenzene

R.T.: 12.286 min
Delta R.T.: -0.013 min
Response: 6376222
Conc: 233.73 ug/L

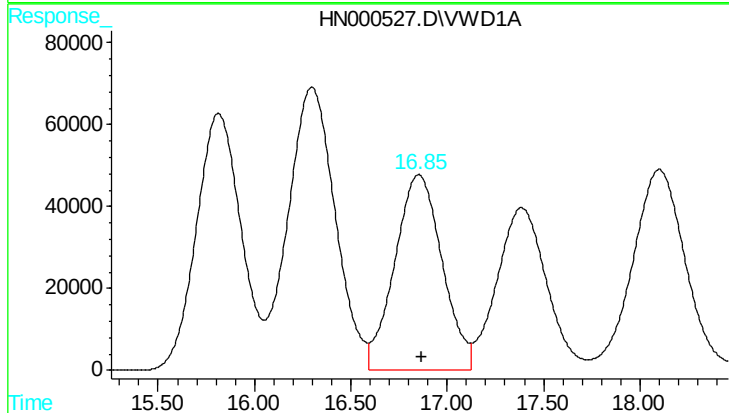

#13 2-Nitrotoluene


R.T.: 16.852 min
Delta R.T.: -0.018 min
Response: 8146078
Conc: 468.85 ug/L

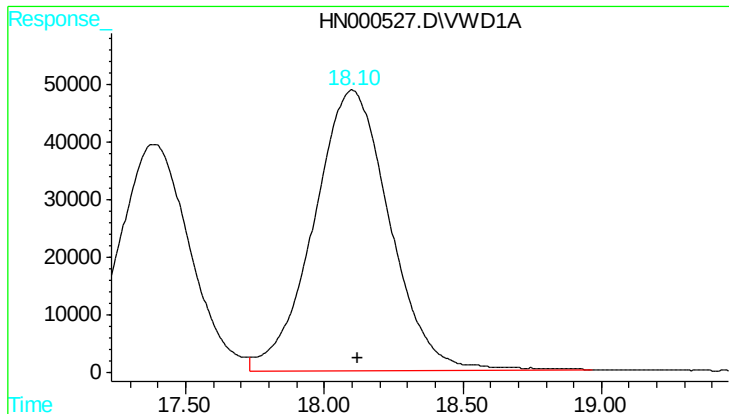

#14 3-Nitrotoluene


R.T.: 18.101 min
Delta R.T.: -0.020 min
Response: 9319100
Conc: 482.51 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-3

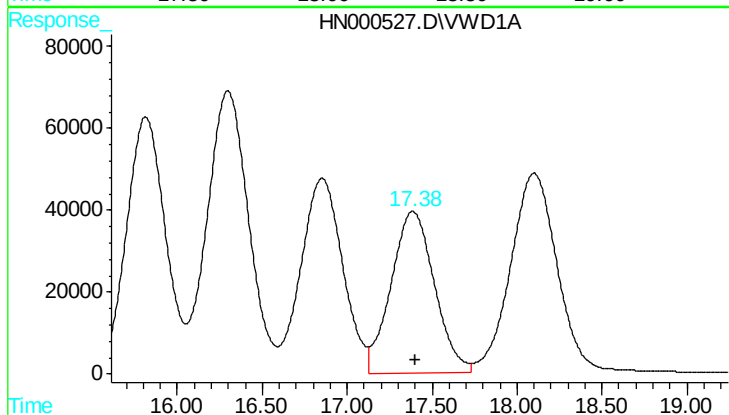

#15 4-Nitrotoluene

R.T.: 17.387 min
Delta R.T.: -0.019 min
Response: 7021532
Conc: 465.89 ug/L

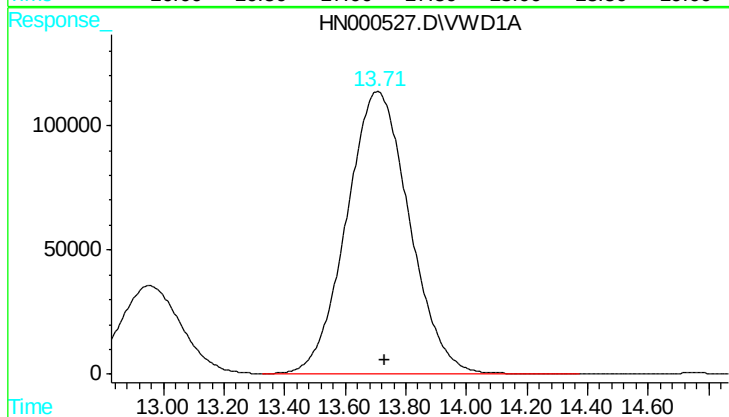

#16 3,5-Dinitroaniline

R.T.: 13.708 min
Delta R.T.: -0.021 min
Response: 16407529
Conc: 464.12 ug/L