

Data File : H:\VOL1\HPLC\HPLC N\121010\HN000528.D Vial: 46
 Acq On : 10-Oct-2012, 21:58 Operator: HLM
 Sample : 8330-2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Oct 11 16:02 2012 Quant Results File: HN101012.RES

Instrument :
 HPLC_N
 LabSampleId :
 8330-2

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN101012.M (Chemstation Integrator)
 Title : SW8330 / 8330A confirmation
 Last Update : Thu Oct 11 15:58:27 2012
 Response via : Initial Calibration
 DataAcq Meth : 8330VWDC.M

Volume Inj. :
 Signal Phase :
 Signal Info :

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	7.65	990474	95.049 ug/L
Target Compounds				
2) T	HMX	12.95	1048414	97.675 ug/L
3) T	RDX	10.76	1325633	94.539 ug/L
4) T	1,3,5-Trinitrobenzene	24.92	1340412	45.799 ug/L
5) T	Tetryl	35.45	2100362	95.796 ug/L
6) T	2,4,6-Trinitrotoluene	33.56	1268810	46.364 ug/L
7) T	2-Amino-4,6-dinitrotoluene	16.30	2336059	46.020 ug/L
8) T	4-Amino-2,6-dinitrotoluene	16.30	2336059	46.020 ug/L
9) T	2,4-Dinitrotoluene	21.93	1846077	47.447 ug/L
10) T	2,6-Dinitrotoluene	20.48	1014420	50.267 ug/L
11) T	1,3-Dinitrobenzene	15.81	2011172	48.945 ug/L
12) T	Nitrobenzene	12.29	1287850	47.208 ug/L
13) T	2-Nitrotoluene	16.85	1549706	89.193 ug/L
14) T	3-Nitrotoluene	18.10	2246985	116.341 ug/L
15) T	4-Nitrotoluene	17.39	1467169	97.349 ug/L
16) T	3,5-Dinitroaniline	13.71	3303791	93.455 ug/L

Data File : H:\VOL1\HPLC\HPLC N\121010\HN000528.D

Vial: 46

Acq On : 10-Oct-2012, 21:58

Operator: HLM

Sample : 8330-2

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Oct 11 16:02 2012 Quant Results File: HN101012.RES

Instrument :

HPLC_N

LabSampleId :

8330-2

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN101012.M (Chemstation Integrator)

Title : SW8330 / 8330A confirmation

Last Update : Thu Oct 11 15:58:27 2012


Response via : Multiple Level Calibration


DataAcq Meth : 8330VWDC.M

Volume Inj. :

Signal Phase :

Signal Info :

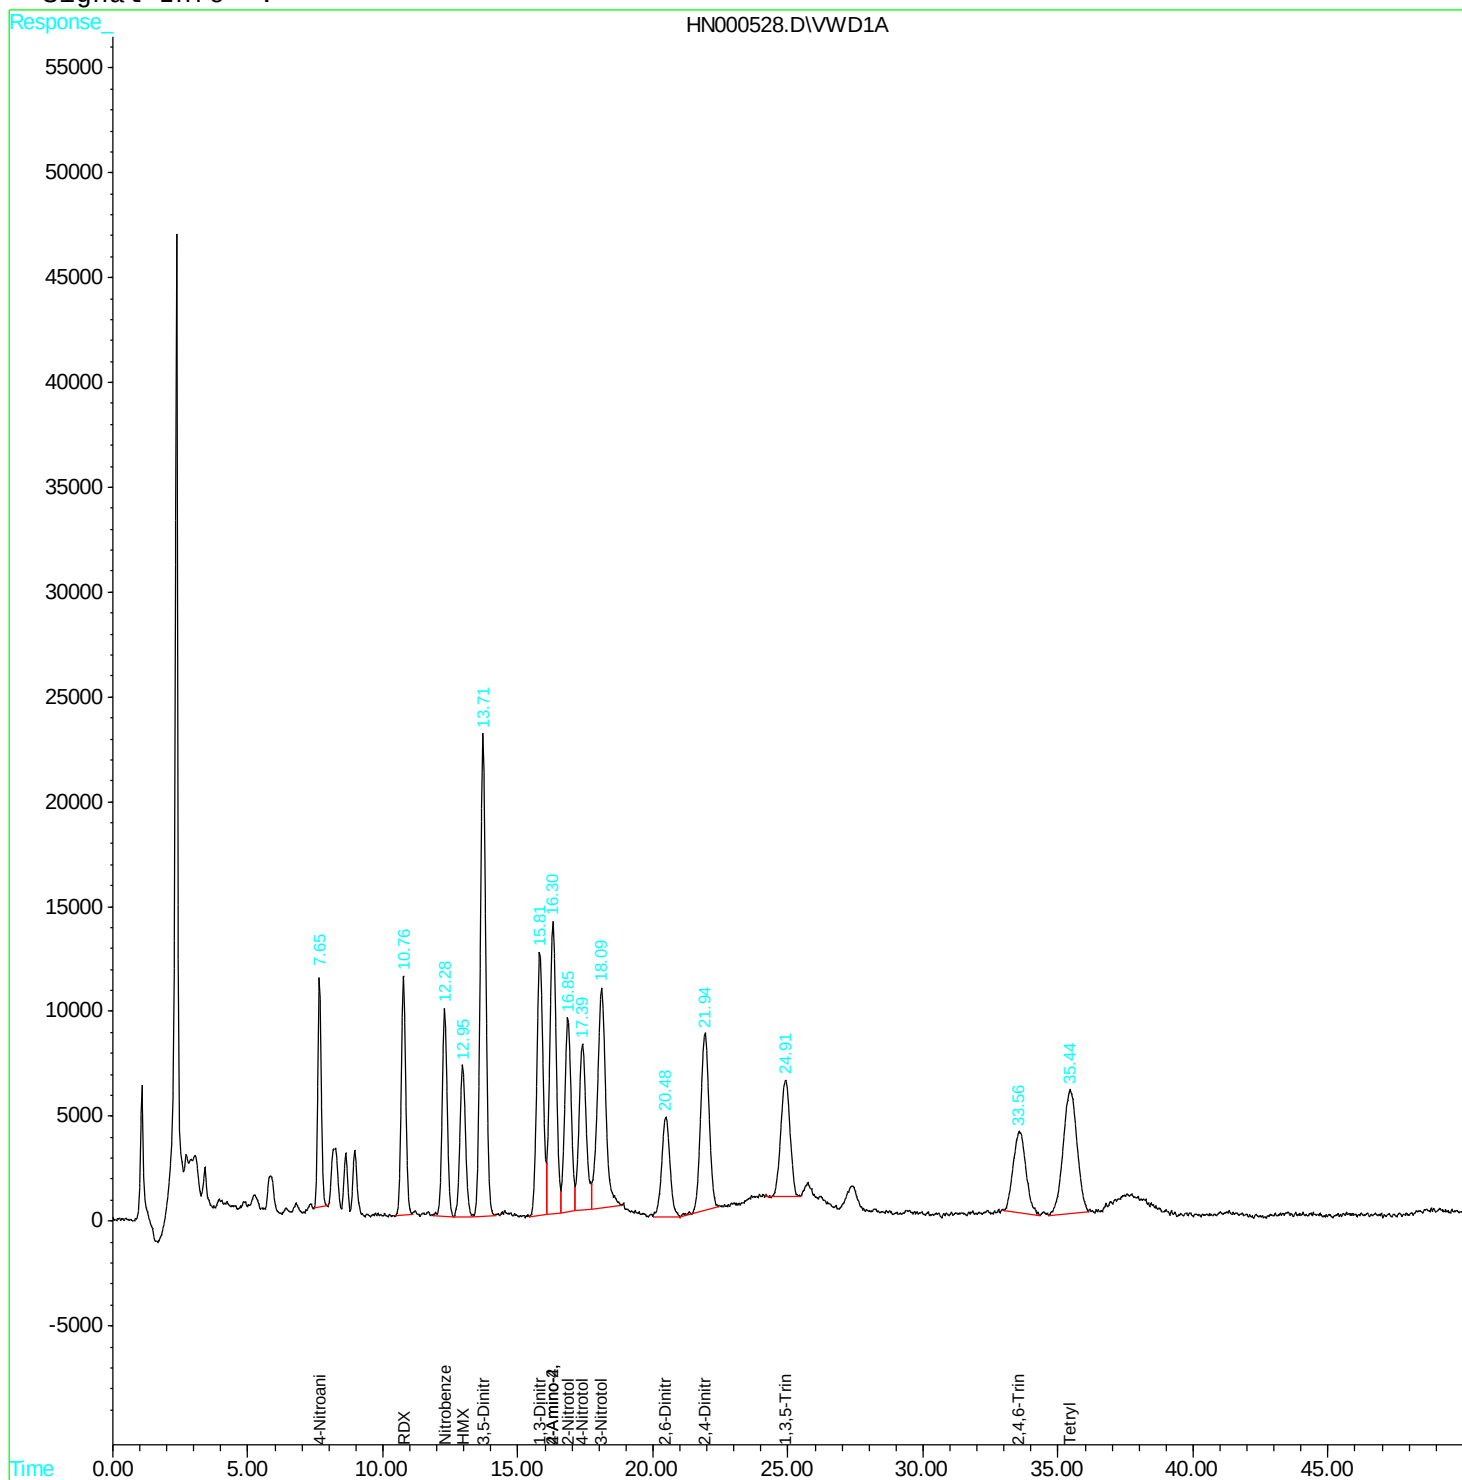


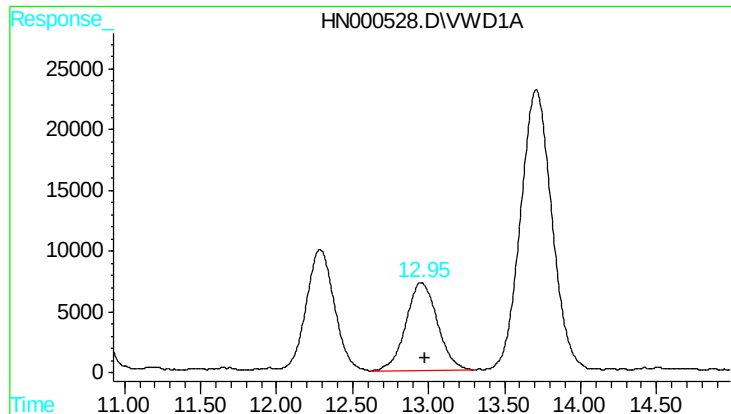

#2 HMX


R.T.: 12.951 min
Delta R.T.: -0.027 min
Response: 1048414
Conc: 97.67 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-2

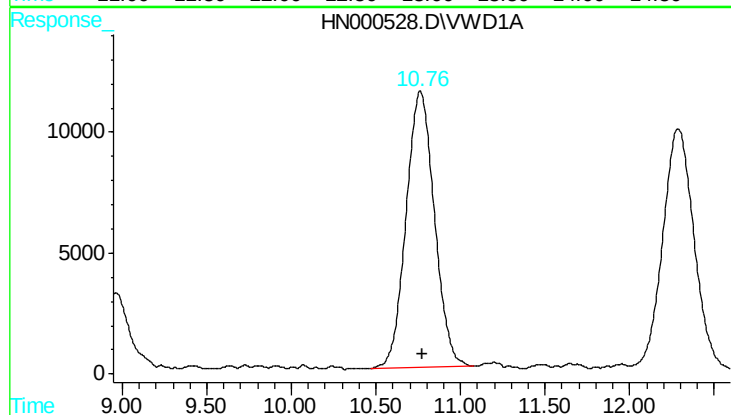


#3 RDX

R.T.: 10.763 min
Delta R.T.: -0.013 min
Response: 1325633
Conc: 94.54 ug/L

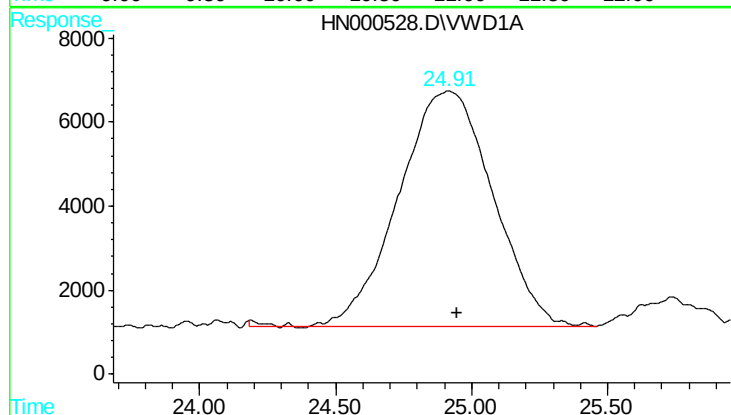


#4 1,3,5-Trinitrobenzene

R.T.: 24.916 min
Delta R.T.: -0.029 min
Response: 1340412
Conc: 45.80 ug/L

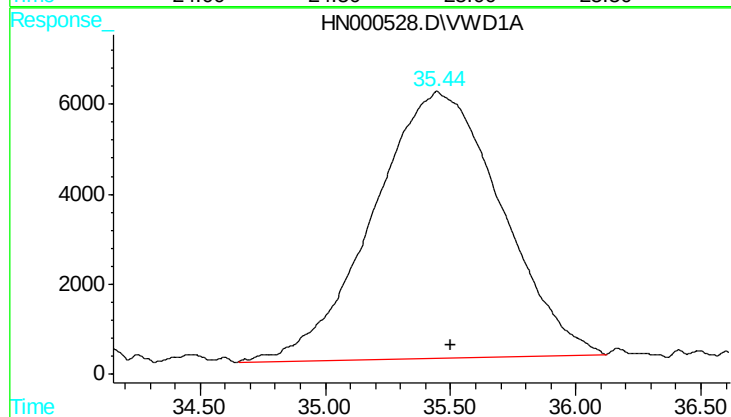

#5 Tetryl


R.T.: 35.448 min
Delta R.T.: -0.052 min
Response: 2100362
Conc: 95.80 ug/L

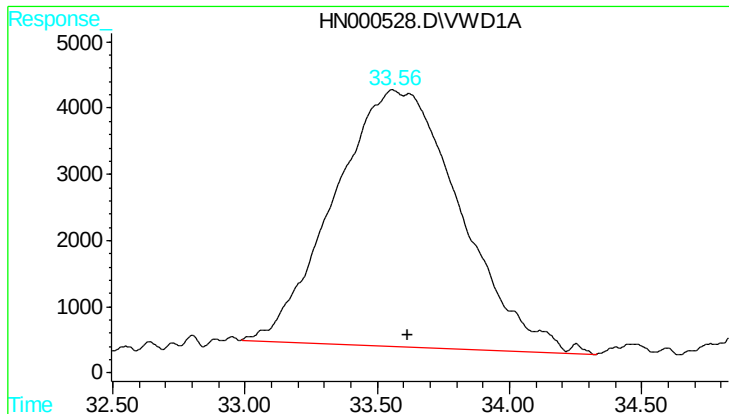

#6 2,4,6-Trinitrotoluene


R.T.: 33.562 min
Delta R.T.: -0.052 min
Response: 1268810
Conc: 46.36 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-2

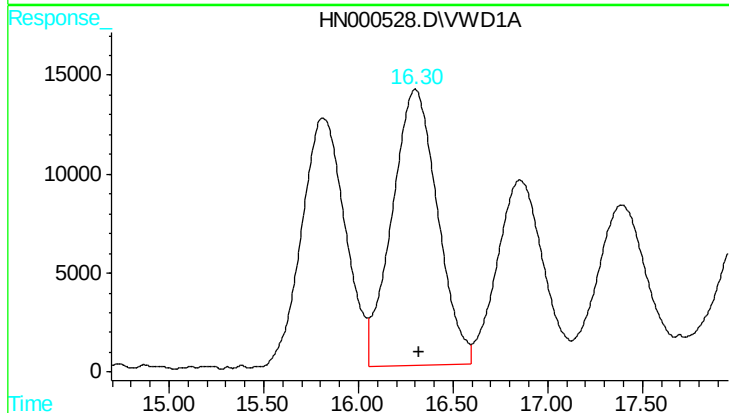


#7 2-Amino-4,6-dinitrotoluene

R.T.: 16.300 min
Delta R.T.: -0.024 min
Response: 2336059
Conc: 46.02 ug/L

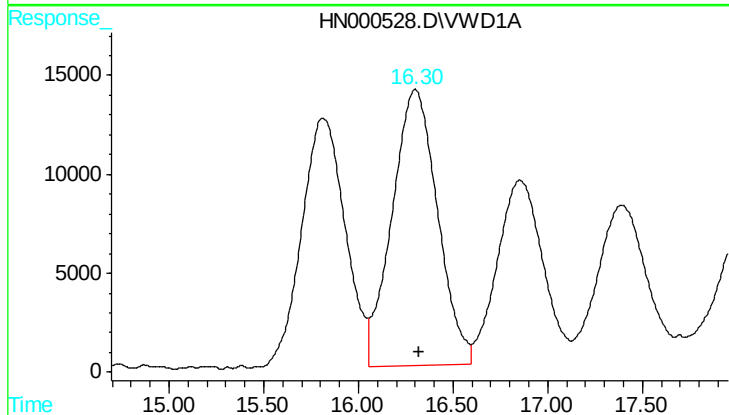


#8 4-Amino-2,6-dinitrotoluene

R.T.: 16.300 min
Delta R.T.: -0.024 min
Response: 2336059
Conc: 46.02 ug/L

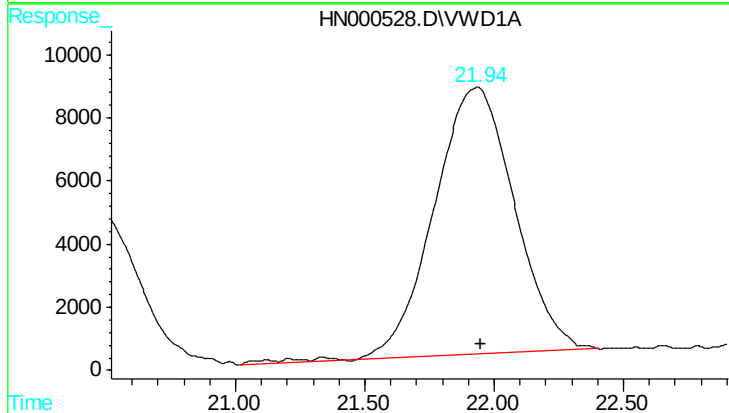

#9 2,4-Dinitrotoluene


R.T.: 21.934 min
Delta R.T.: -0.017 min
Response: 1846077
Conc: 47.45 ug/L

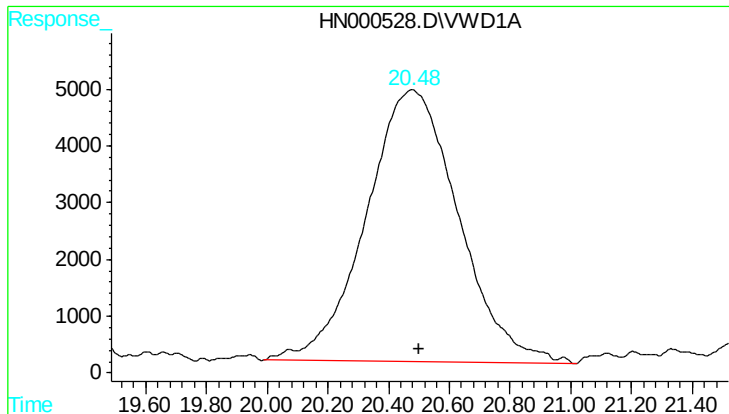

#10 2,6-Dinitrotoluene


R.T.: 20.478 min
Delta R.T.: -0.024 min
Response: 1014420
Conc: 50.27 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-2

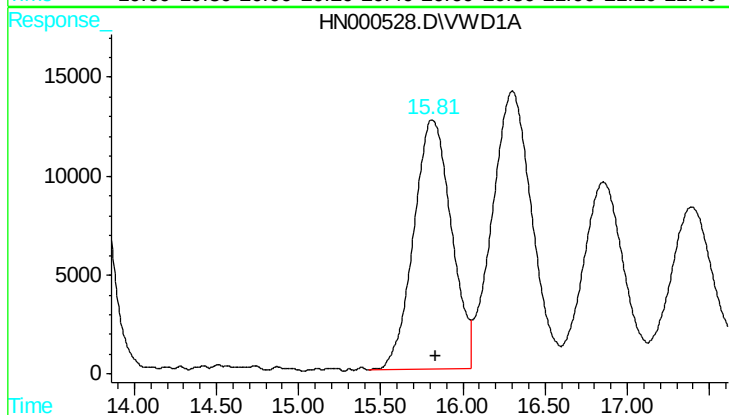


#11 1,3-Dinitrobenzene

R.T.: 15.814 min
Delta R.T.: -0.021 min
Response: 2011172
Conc: 48.95 ug/L

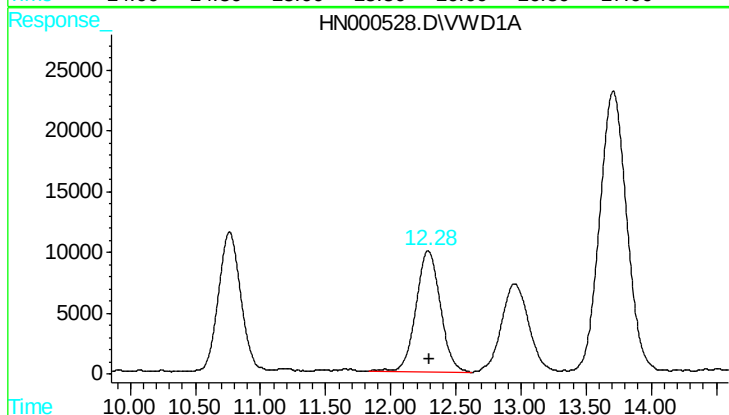


#12 Nitrobenzene

R.T.: 12.286 min
Delta R.T.: -0.013 min
Response: 1287850
Conc: 47.21 ug/L

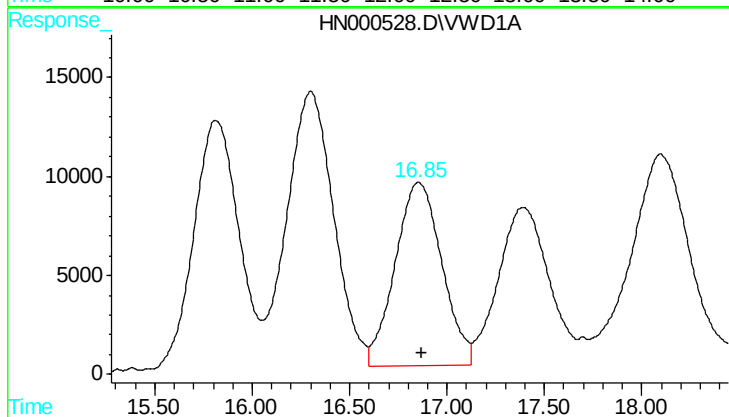

#13 2-Nitrotoluene


R.T.: 16.854 min
Delta R.T.: -0.016 min
Response: 1549706
Conc: 89.19 ug/L

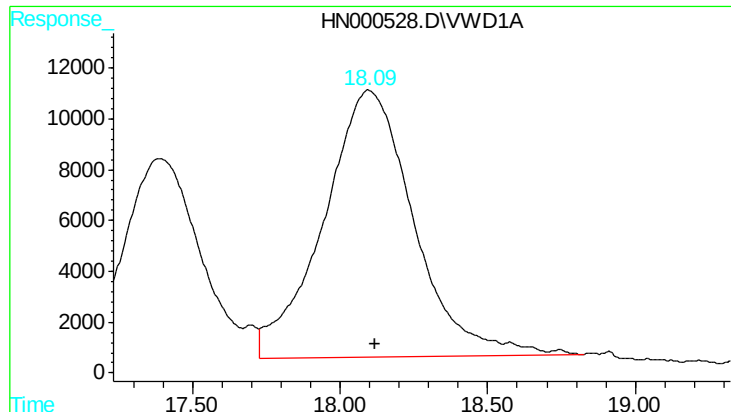

#14 3-Nitrotoluene


R.T.: 18.097 min
Delta R.T.: -0.024 min
Response: 2246985
Conc: 116.34 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-2

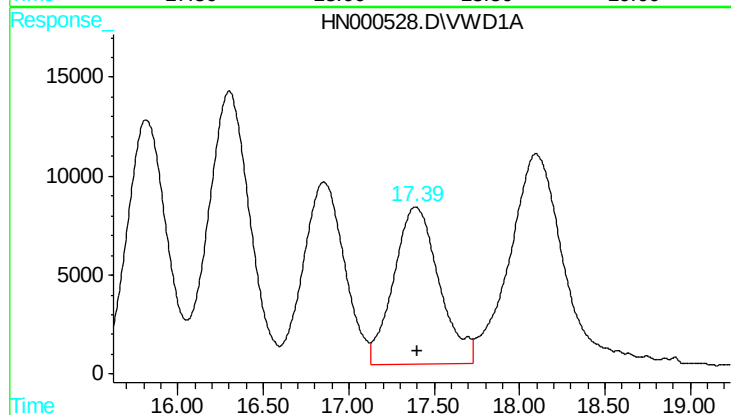

#15 4-Nitrotoluene

R.T.: 17.391 min
Delta R.T.: -0.015 min
Response: 1467169
Conc: 97.35 ug/L

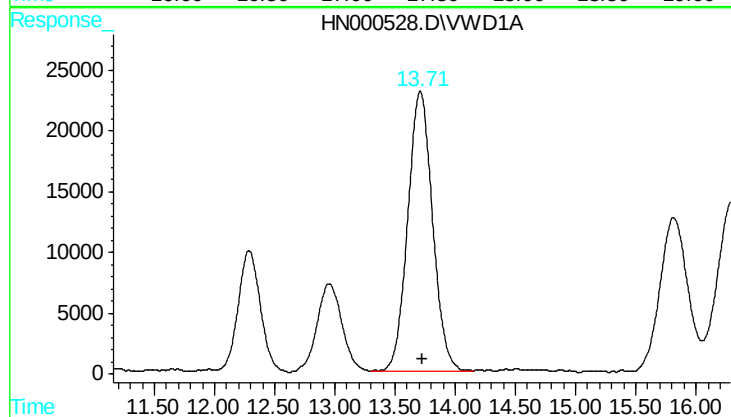

#16 3,5-Dinitroaniline

R.T.: 13.709 min
Delta R.T.: -0.020 min
Response: 3303791
Conc: 93.45 ug/L