

Data File : H:\VOL1\HPLC\HPLC N\121010\HN000530.D Vial: 48  
 Acq On : 10-Oct-2012, 23:44 Operator: HLM  
 Sample : 8330-ICV Inst : G1314A  
 Misc : Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 11 16:10 2012 Quant Results File: HN101012.RES

Instrument :  
 HPLC\_N  
 ClientSampleId :  
 ICVHN101012

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN101012.M (Chemstation Integrator)  
 Title : SW8330 / 8330A confirmation  
 Last Update : Thu Oct 11 16:07:34 2012  
 Response via : Initial Calibration  
 DataAcq Meth : 8330VWDC.M

Volume Inj. :  
 Signal Phase :  
 Signal Info :

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

#### System Monitoring Compounds

##### Target Compounds

|       |                            |       |          |          |      |
|-------|----------------------------|-------|----------|----------|------|
| 2) T  | HMX                        | 12.96 | 10189536 | 986.701  | ug/L |
| 3) T  | RDX                        | 10.76 | 14060234 | 1009.095 | ug/L |
| 4) T  | 1,3,5-Trinitrobenzene      | 24.92 | 28990645 | 1040.304 | ug/L |
| 5) T  | Tetryl                     | 35.48 | 21928005 | 1014.618 | ug/L |
| 6) T  | 2,4,6-Trinitrotoluene      | 33.60 | 28269593 | 1052.780 | ug/L |
| 7) T  | 2-Amino-4,6-dinitrotoluene | 16.31 | 47611197 | 1019.819 | ug/L |
| 8) T  | 4-Amino-2,6-dinitrotoluene | 16.31 | 47611197 | 1019.819 | ug/L |
| 9) T  | 2,4-Dinitrotoluene         | 21.93 | 36830679 | 972.344  | ug/L |
| 10) T | 2,6-Dinitrotoluene         | 20.49 | 19586893 | 998.642  | ug/L |
| 11) T | 1,3-Dinitrobenzene         | 15.82 | 40525384 | 1001.663 | ug/L |
| 12) T | Nitrobenzene               | 12.29 | 25963058 | 993.965  | ug/L |
| 13) T | 2-Nitrotoluene             | 16.86 | 16794110 | 1050.739 | ug/L |
| 14) T | 3-Nitrotoluene             | 18.11 | 18442161 | 1002.090 | ug/L |
| 15) T | 4-Nitrotoluene             | 17.40 | 14289685 | 1047.064 | ug/L |
| 16) T | 3,5-Dinitroaniline         | 13.71 | 32275313 | 965.172  | ug/L |

Data File : H:\VOL1\HPLC\HPLC N\121010\HN000530.D

Vial: 48

Acq On : 10-Oct-2012, 23:44

Operator: HLM

Sample : 8330-ICV

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Oct 11 16:10 2012 Quant Results File: HN101012.RES

Instrument :

HPLC\_N

ClientSampleId :

ICVHN101012

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN101012.M (Chemstation Integrator)

Title : SW8330 / 8330A confirmation

Last Update : Thu Oct 11 16:07:34 2012


Response via : Multiple Level Calibration


DataAcq Meth : 8330VWDC.M

Volume Inj. :

Signal Phase :

Signal Info :

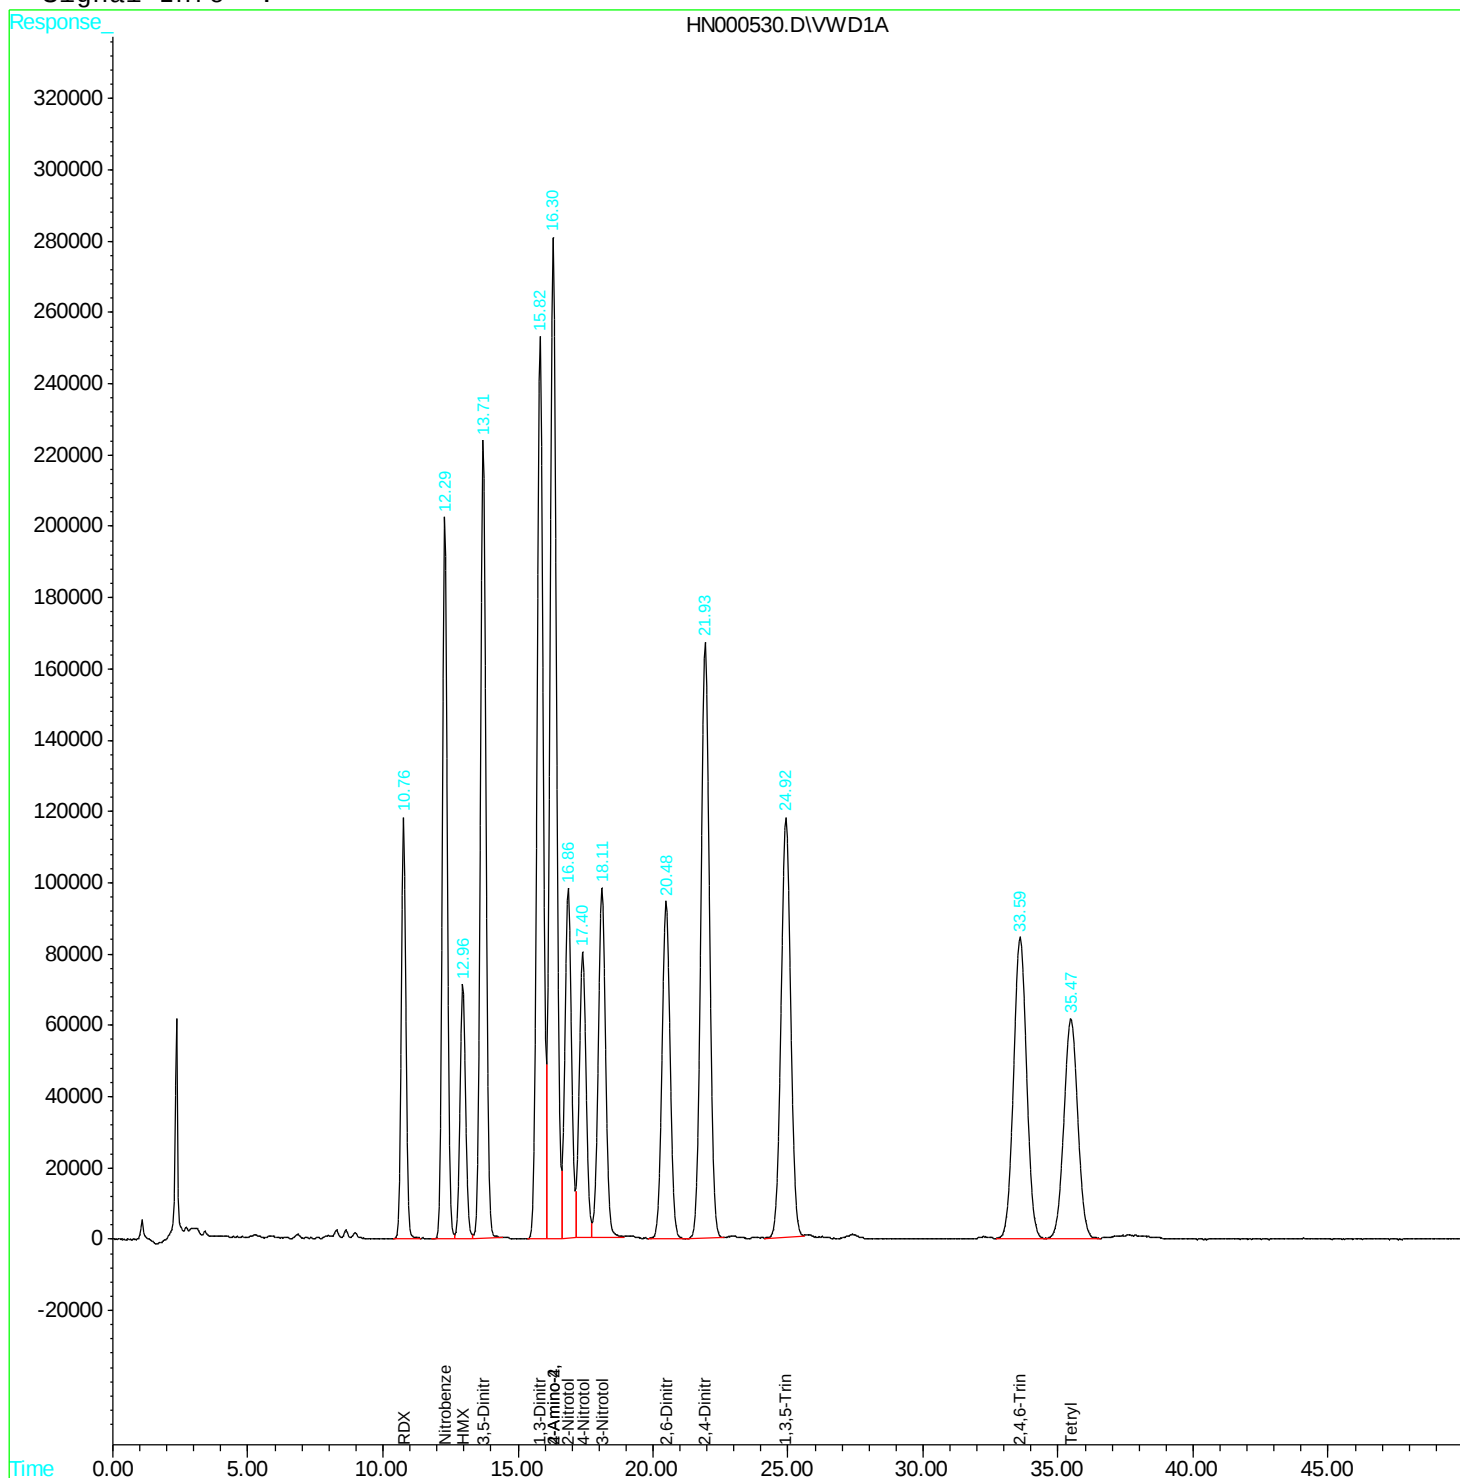


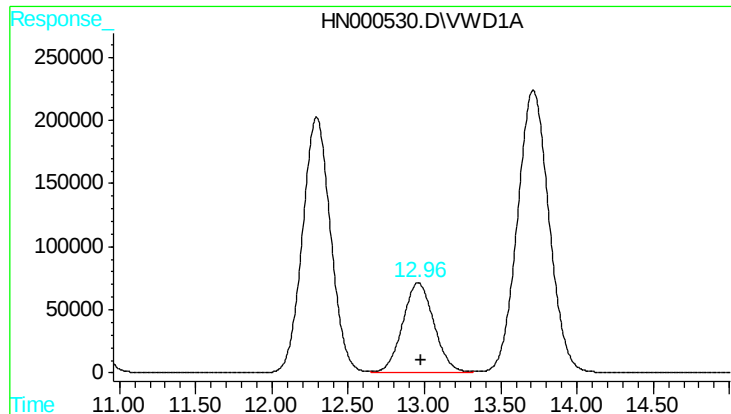

#2 HMX


R.T.: 12.959 min  
Delta R.T.: -0.023 min  
Response: 10189536  
Conc: 986.70 ug/L

Instrument :  
HPLC\_N  
ClientSampleId :  
ICVHN101012

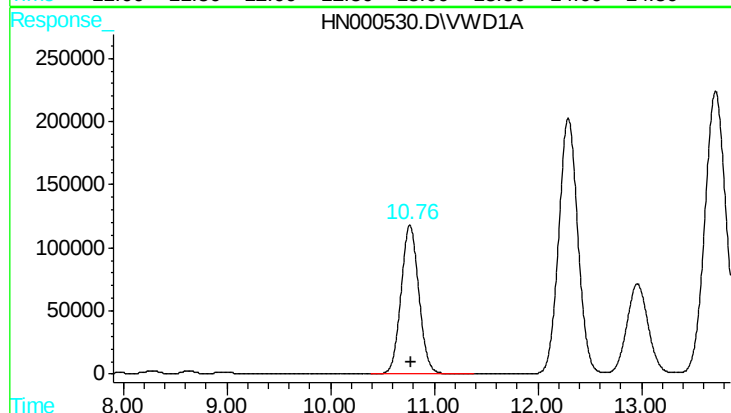


#3 RDX

R.T.: 10.765 min  
Delta R.T.: -0.013 min  
Response: 14060234  
Conc: 1009.10 ug/L

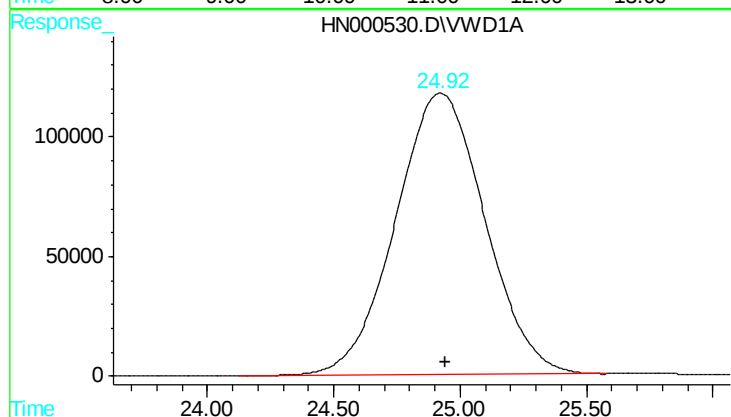


#4 1,3,5-Trinitrobenzene

R.T.: 24.922 min  
Delta R.T.: -0.022 min  
Response: 28990645  
Conc: 1040.30 ug/L

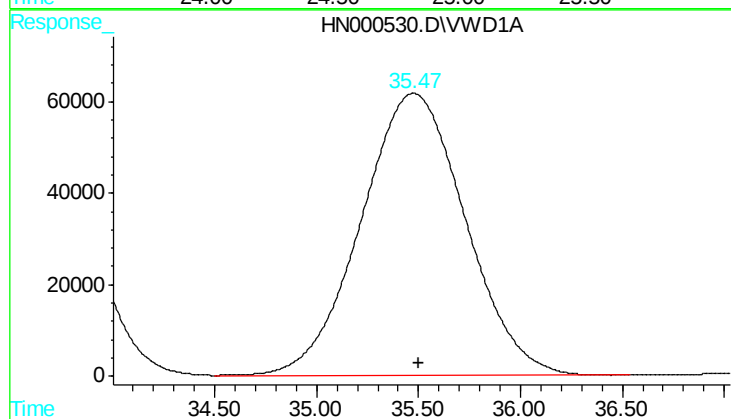

#5 Tetryl


R.T.: 35.475 min  
Delta R.T.: -0.024 min  
Response: 21928005  
Conc: 1014.62 ug/L

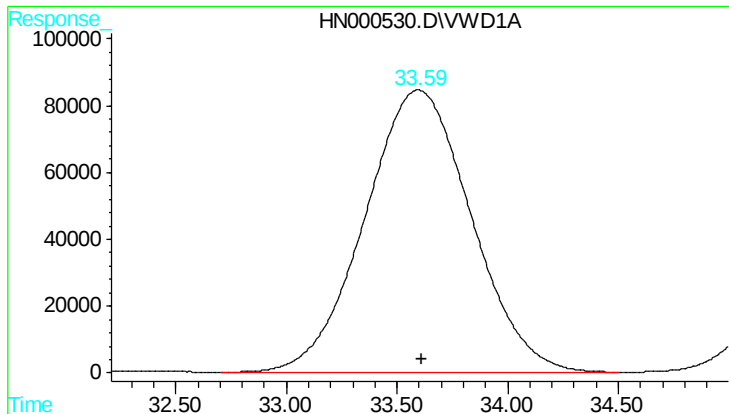

#6 2,4,6-Trinitrotoluene


R.T.: 33.595 min  
Delta R.T.: -0.019 min  
Response: 28269593  
Conc: 1052.78 ug/L

Instrument :  
HPLC\_N  
ClientSampleId :  
ICVHN101012

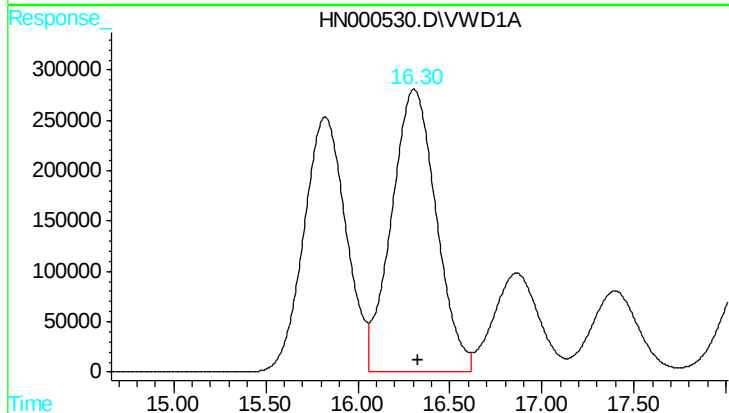


#7 2-Amino-4,6-dinitrotoluene

R.T.: 16.305 min  
Delta R.T.: -0.018 min  
Response: 47611197  
Conc: 1019.82 ug/L

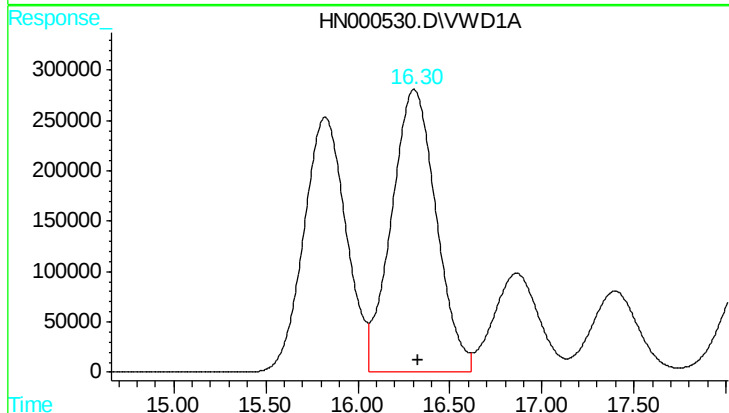


#8 4-Amino-2,6-dinitrotoluene

R.T.: 16.305 min  
Delta R.T.: -0.018 min  
Response: 47611197  
Conc: 1019.82 ug/L

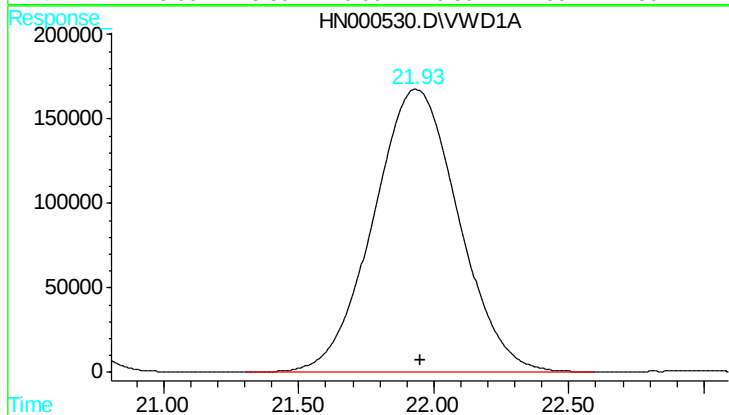

#9 2,4-Dinitrotoluene


R.T.: 21.935 min  
Delta R.T.: -0.016 min  
Response: 36830679  
Conc: 972.34 ug/L

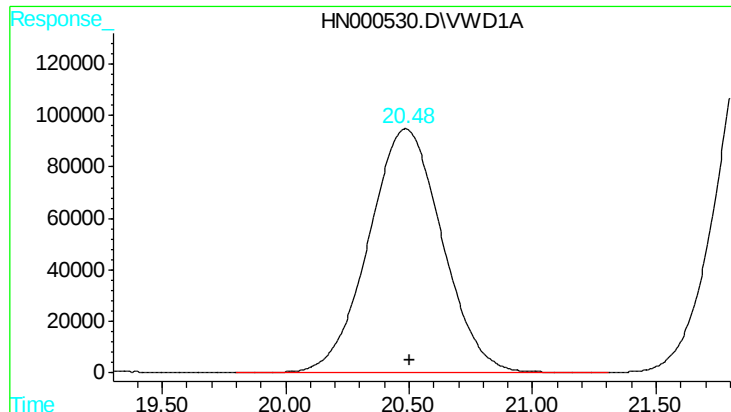

#10 2,6-Dinitrotoluene


R.T.: 20.486 min  
Delta R.T.: -0.016 min  
Response: 19586893  
Conc: 998.64 ug/L

Instrument :  
HPLC\_N  
ClientSampleId :  
ICVHN101012

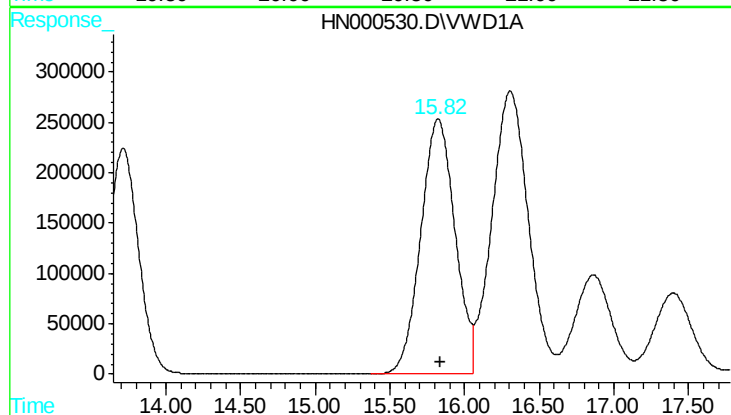


#11 1,3-Dinitrobenzene

R.T.: 15.822 min  
Delta R.T.: -0.013 min  
Response: 40525384  
Conc: 1001.66 ug/L

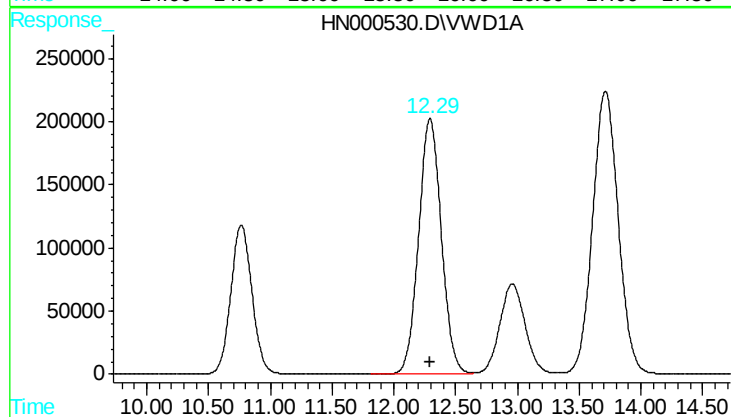


#12 Nitrobenzene

R.T.: 12.293 min  
Delta R.T.: -0.007 min  
Response: 25963058  
Conc: 993.97 ug/L

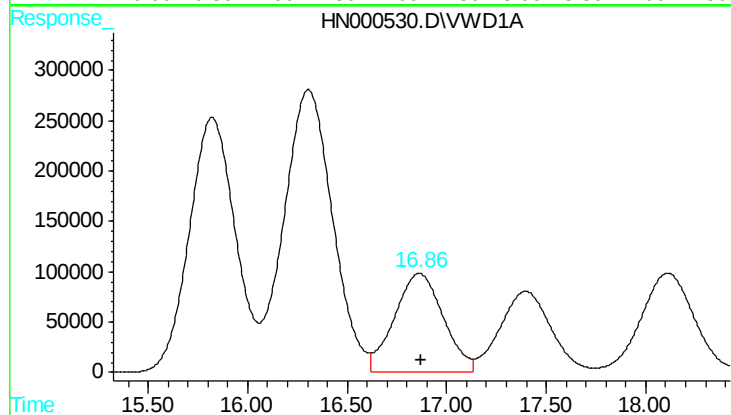

#13 2-Nitrotoluene


R.T.: 16.862 min  
Delta R.T.: -0.009 min  
Response: 16794110  
Conc: 1050.74 ug/L

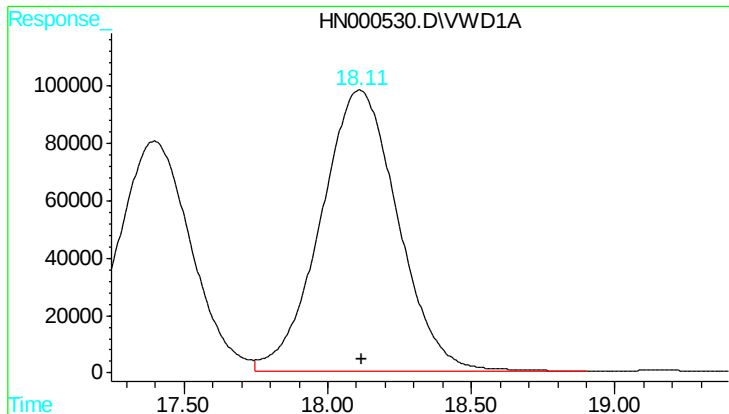

#14 3-Nitrotoluene


R.T.: 18.111 min  
 Delta R.T.: -0.009 min  
 Response: 18442161  
 Conc: 1002.09 ug/L

Instrument :  
 HPLC\_N  
 ClientSampleId :  
 ICVHN101012

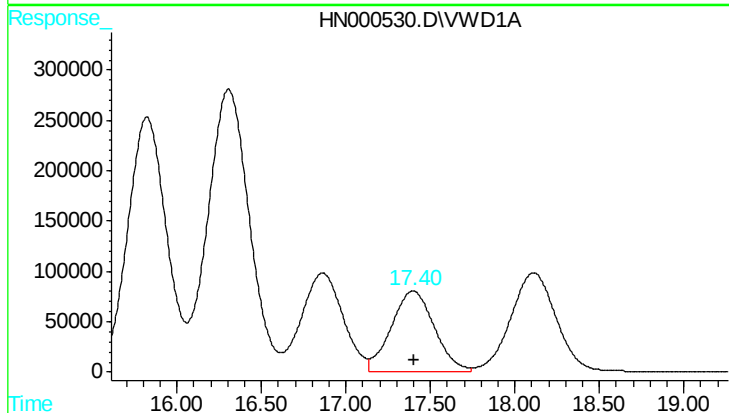

#15 4-Nitrotoluene

R.T.: 17.397 min  
 Delta R.T.: -0.009 min  
 Response: 14289685  
 Conc: 1047.06 ug/L

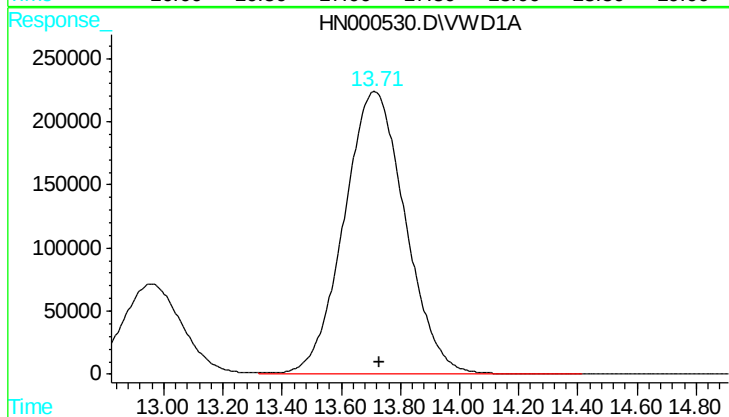

#16 3,5-Dinitroaniline

R.T.: 13.713 min  
 Delta R.T.: -0.016 min  
 Response: 32275313  
 Conc: 965.17 ug/L