

Data File : H:\VOL1\HPLC\HPLC N\121010\HN000537.D Vial: 47
 Acq On : 11-Oct-2012, 05:52 Operator: HLM
 Sample : 8330-MRL Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Oct 11 16:11 2012 Quant Results File: HN101012.RES

Instrument :
 HPLC_N
 ClientSampleId :
 8330-MRL

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN101012.M (Chemstation Integrator)
 Title : SW8330 / 8330A confirmation
 Last Update : Thu Oct 11 16:04:33 2012
 Response via : Initial Calibration
 DataAcq Meth : 8330VWDC.M

Volume Inj. :
 Signal Phase :
 Signal Info :

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	7.67	211240	20.417 ug/L
Target Compounds				
3) T	RDX	10.79	286315	20.549 ug/L
7) T	2-Amino-4,6-dinitrotoluene	16.35	450663	9.653 ug/L
8) T	4-Amino-2,6-dinitrotoluene	16.35	450663	9.653 ug/L
11) T	1,3-Dinitrobenzene	15.87	412626	10.199 ug/L
12) T	Nitrobenzene	12.32	314458	12.039 ug/L
13) T	2-Nitrotoluene	16.90	249289	15.597 ug/L
14) T	3-Nitrotoluene	18.14	713050	28.645 ug/L
16) T	3,5-Dinitroaniline	13.75	700390	20.945 ug/L

Data File : H:\VOL1\HPLC\HPLC N\121010\HN000537.D

Vial: 47

Acq On : 11-Oct-2012, 05:52

Operator: HLM

Sample : 8330-MRL

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Oct 11 16:11 2012 Quant Results File: HN101012.RES

Instrument :

HPLC_N

ClientSampleId :

8330-MRL

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN101012.M (Chemstation Integrator)

Title : SW8330 / 8330A confirmation

Last Update : Thu Oct 11 16:04:33 2012


Response via : Multiple Level Calibration


DataAcq Meth : 8330VWDC.M

Volume Inj. :

Signal Phase :

Signal Info :

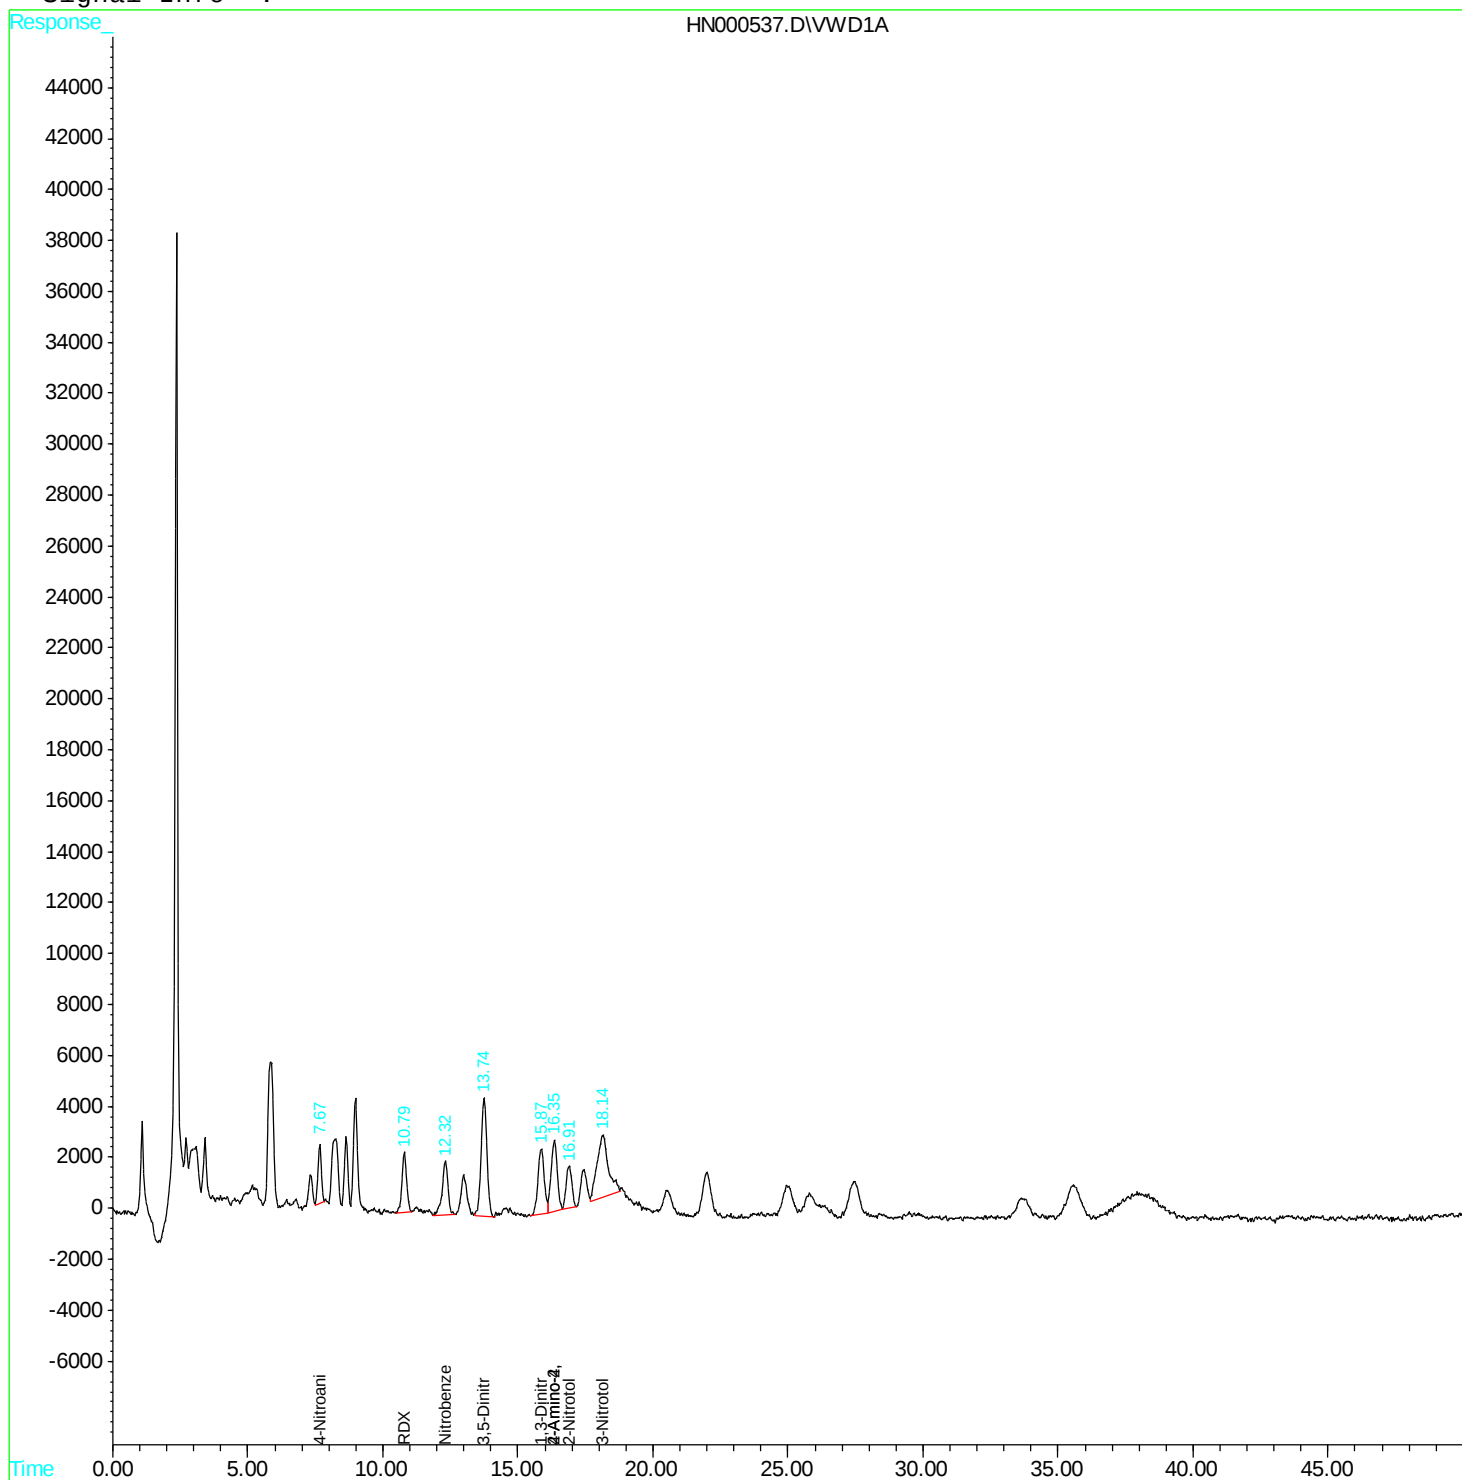


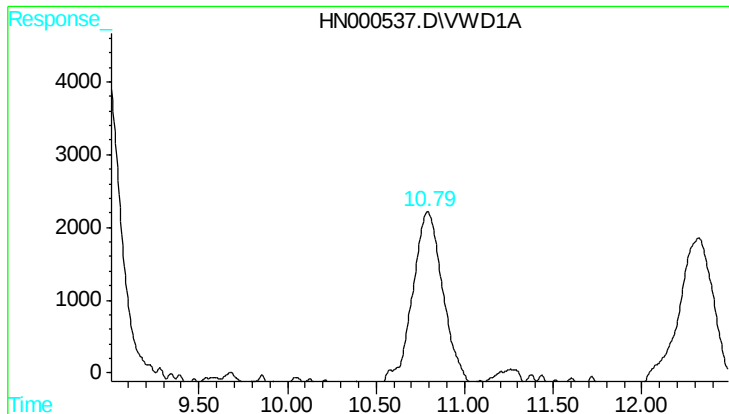

#3 RDX


R.T.: 10.792 min
Delta R.T.: 0.014 min
Response: 286315
Conc: 20.55 ug/L

Instrument :
HPLC_N
ClientSampleId :
8330-MRL

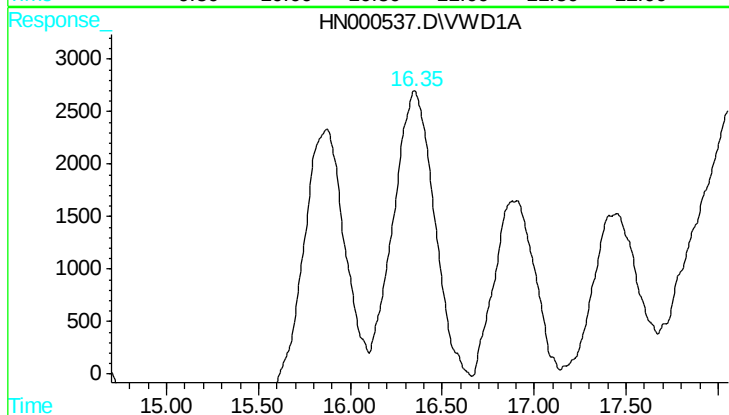


#7 2-Amino-4,6-dinitrotoluene

R.T.: 16.350 min
Delta R.T.: 0.027 min
Response: 450663
Conc: 9.65 ug/L

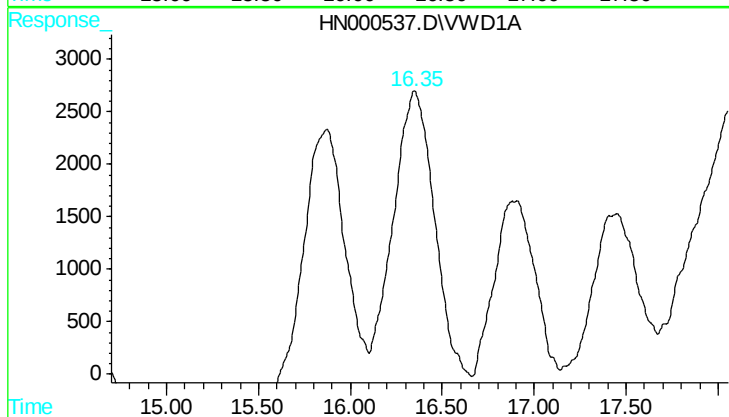


#8 4-Amino-2,6-dinitrotoluene

R.T.: 16.350 min
Delta R.T.: 0.027 min
Response: 450663
Conc: 9.65 ug/L

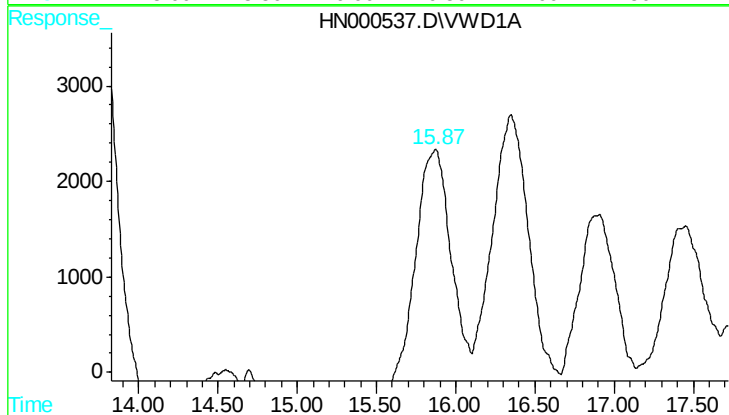

#11 1,3-Dinitrobenzene


R.T.: 15.869 min
Delta R.T.: 0.034 min
Response: 412626
Conc: 10.20 ug/L

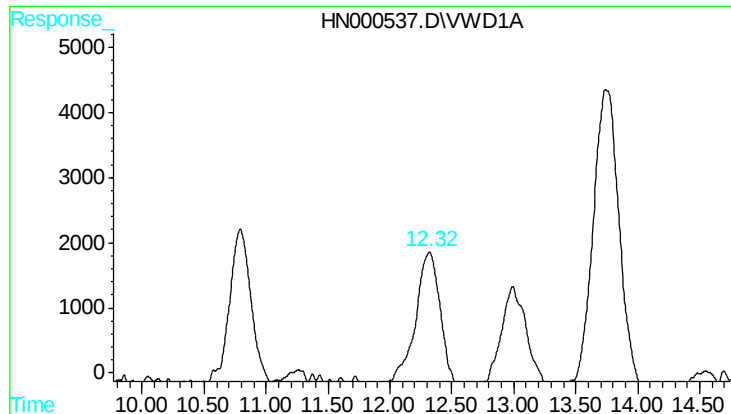

#12 Nitrobenzene


R.T.: 12.318 min
Delta R.T.: 0.018 min
Response: 314458
Conc: 12.04 ug/L

Instrument :
HPLC_N
ClientSampleId :
8330-MRL

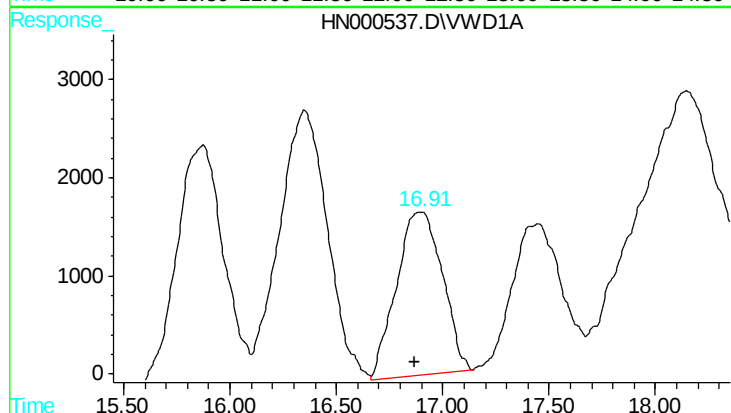


#13 2-Nitrotoluene

R.T.: 16.896 min
Delta R.T.: 0.026 min
Response: 249289
Conc: 15.60 ug/L

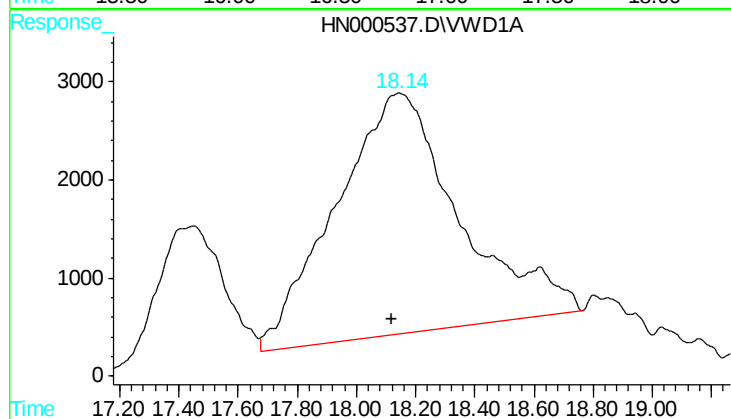

#14 3-Nitrotoluene

R.T.: 18.144 min
Delta R.T.: 0.024 min
Response: 713050
Conc: 28.65 ug/L

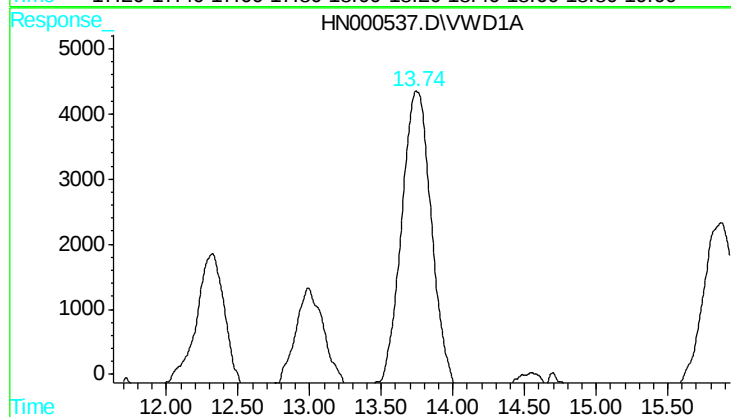

#16 3,5-Dinitroaniline

R.T.: 13.750 min
Delta R.T.: 0.020 min
Response: 700390
Conc: 20.94 ug/L