

Data Path : S:\HPCHEM1\HPLC_N\Data\HN101012\
 Data File : HN000526.D
 Signal(s) : VWD1A.CH
 Acq On : 10-Oct-2012, 20:13
 Operator : HLM
 Sample : 8330-4
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 HPLC_N
 LabSampleId :
 8330-4

Integration File: events.e
 Quant Time: Nov 17 04:27:07 2012
 Quant Method : H:\VOL1\HPLC\HPLC_N\METHODS\HN101012.M
 Quant Title : SW8330 / 8330A confirmation
 QLast Update : Thu Oct 11 15:58:27 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	7.661	10416799	999.624 ug/L
Target Compounds				
2) T	HMX	12.982	10334730	962.826 ug/L
3) T	RDX	10.778	13732710	979.368 ug/L
4) T	1,3,5-Trinitrobenzene	24.945	14497493	495.353 ug/L
5) T	Tetryl	35.500	21531180	982.023 ug/L
6) T	2,4,6-Trinitrotoluene	33.614	13423085	490.495 ug/L
7) T	2-Amino-4,6-dinitroto...	16.323	24050428	473.786 ug/L
8) T	4-Amino-2,6-dinitroto...	16.323	24050428	473.786 ug/L
9) T	2,4-Dinitrotoluene	21.951	19220055	493.987 ug/L
10) T	2,6-Dinitrotoluene	20.502	9955455	493.314 ug/L
11) T	1,3-Dinitrobenzene	15.835	20702882	503.841 ug/L
12) T	Nitrobenzene	12.299	13055872	478.585 ug/L
13) T	2-Nitrotoluene	16.870	16967522	976.564 ug/L
14) T	3-Nitrotoluene	18.121	18720552	969.284 ug/L
15) T	4-Nitrotoluene	17.406	14553743	965.662 ug/L
16) T	3,5-Dinitroaniline	13.729	33586251	950.061 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_N\Data\HN101012\
Data File : HN000526.D
Signal(s) : VWD1A.CH
Acq On : 10-Oct-2012, 20:13
Operator : HLM
Sample : 8330-4
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
HPLC_N
LabSampleId :
8330-4

Integration File: events.e
Quant Time: Nov 17 04:27:07 2012
Quant Method : H:\VOL1\HPLC\HPLC_N\METHODS\HN101012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Thu Oct 11 15:58:27 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

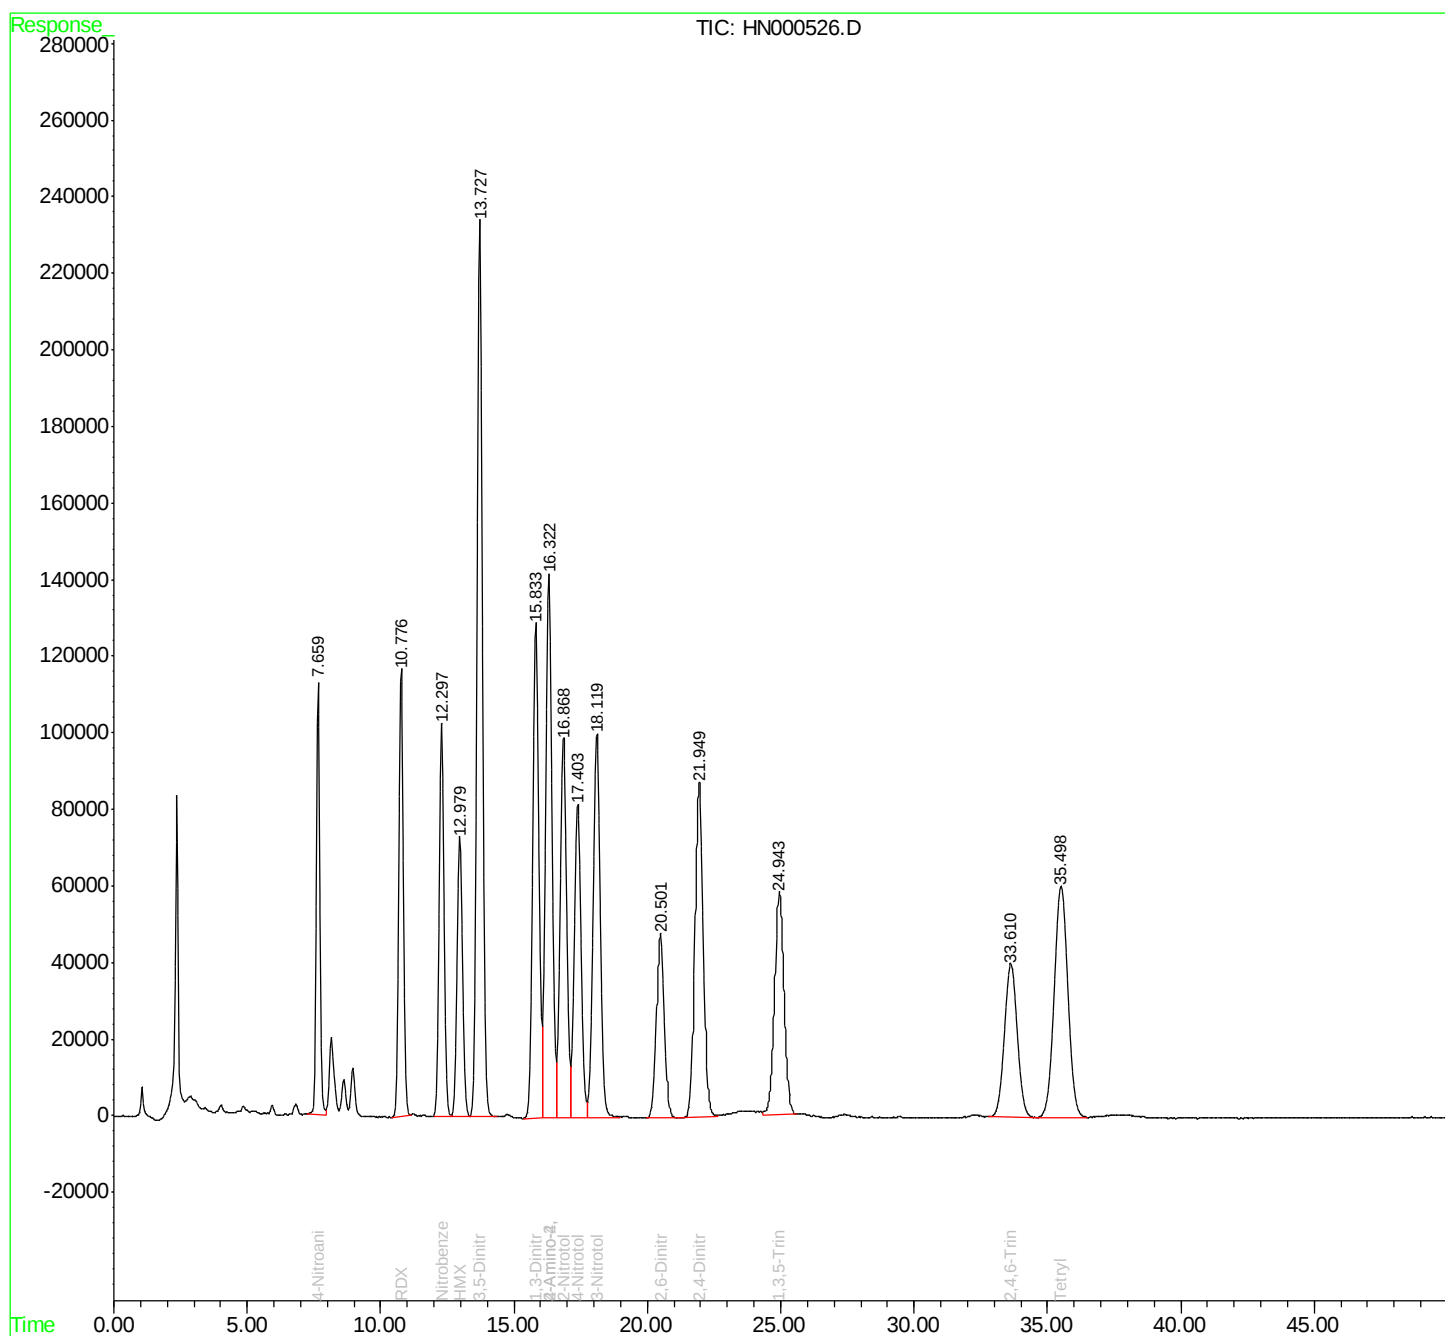


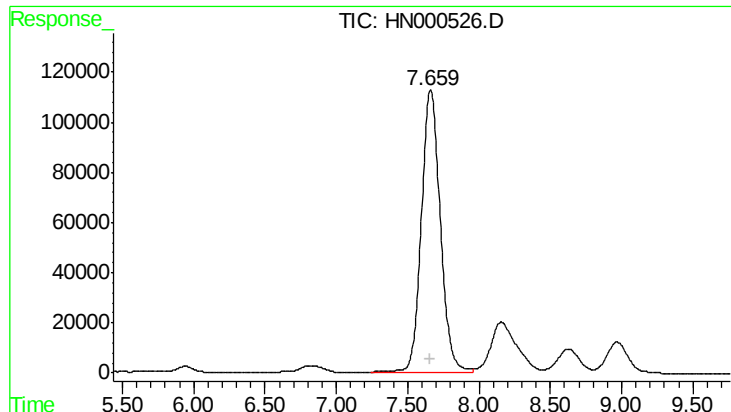

#1 4-Nitroaniline


R.T.: 7.661 min
Delta R.T.: 0.002 min
Response: 10416799
Conc: 999.62 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-4

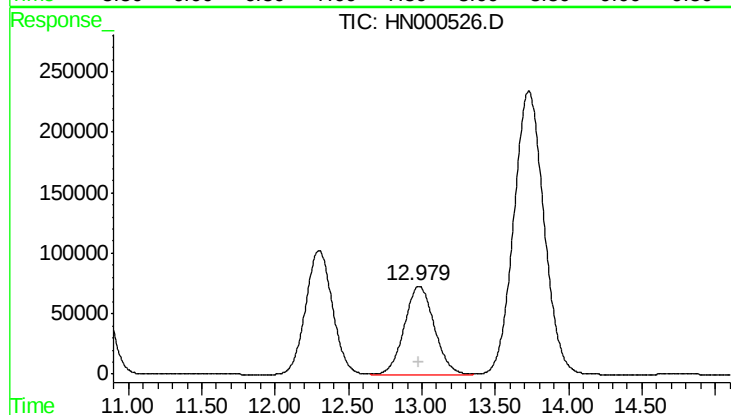


#2 HMX

R.T.: 12.982 min
Delta R.T.: 0.003 min
Response: 10334730
Conc: 962.83 ug/L

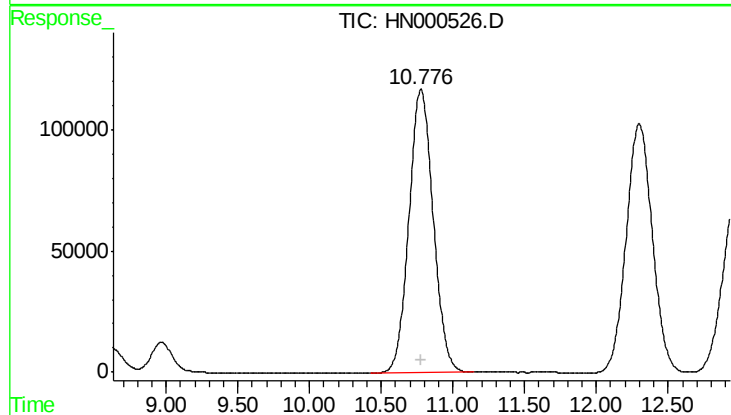


#3 RDX

R.T.: 10.778 min
Delta R.T.: 0.002 min
Response: 13732710
Conc: 979.37 ug/L

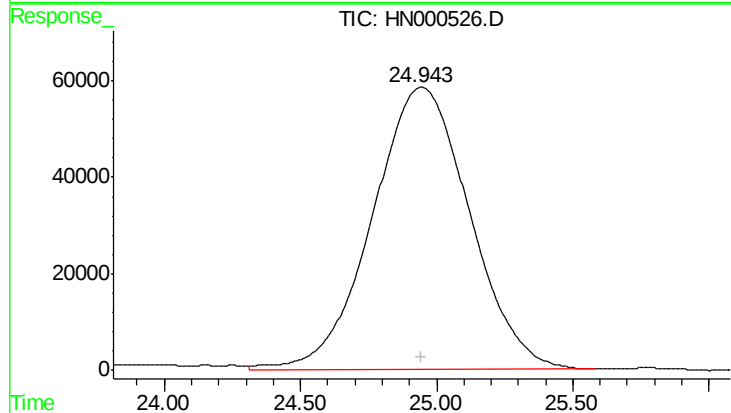

#4 1,3,5-Trinitrobenzene


R.T.: 24.945 min
Delta R.T.: 0.000 min
Response: 14497493
Conc: 495.35 ug/L

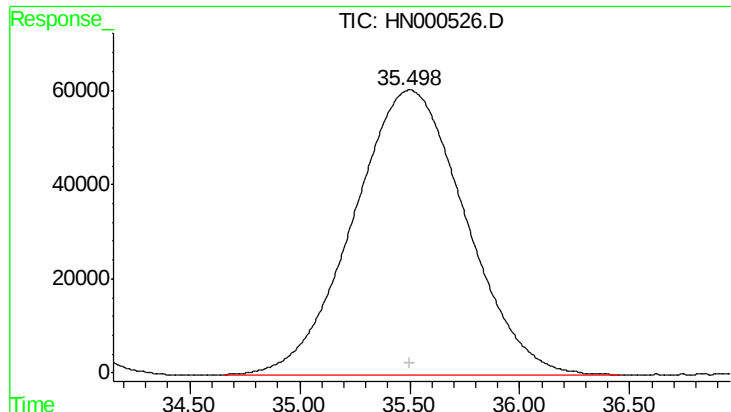

#5 Tetraol


R.T.: 35.500 min
Delta R.T.: 0.000 min
Response: 21531180
Conc: 982.02 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-4

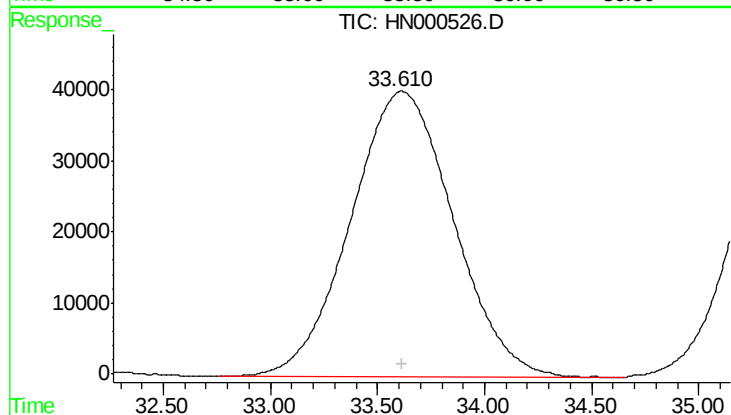


#6 2,4,6-Trinitrotoluene

R.T.: 33.614 min
Delta R.T.: 0.000 min
Response: 13423085
Conc: 490.50 ug/L

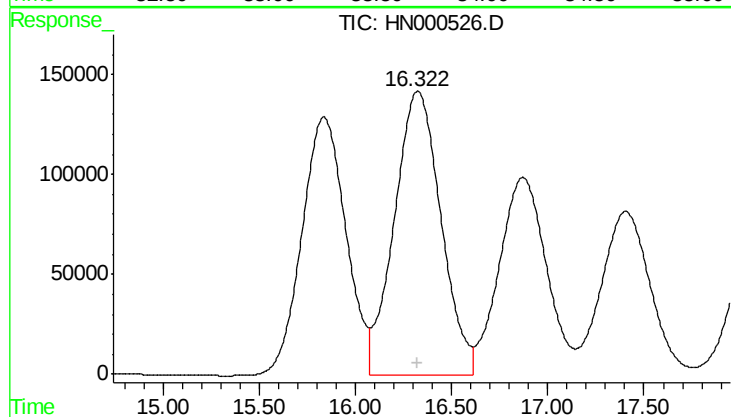


#7 2-Amino-4,6-dinitrotoluene

R.T.: 16.323 min
Delta R.T.: 0.000 min
Response: 24050428
Conc: 473.79 ug/L

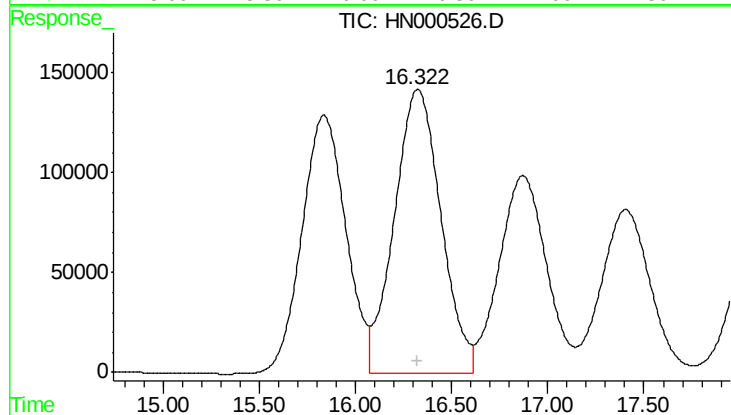

#8 4-Amino-2,6-dinitrotoluene


R.T.: 16.323 min
Delta R.T.: 0.000 min
Response: 24050428
Conc: 473.79 ug/L

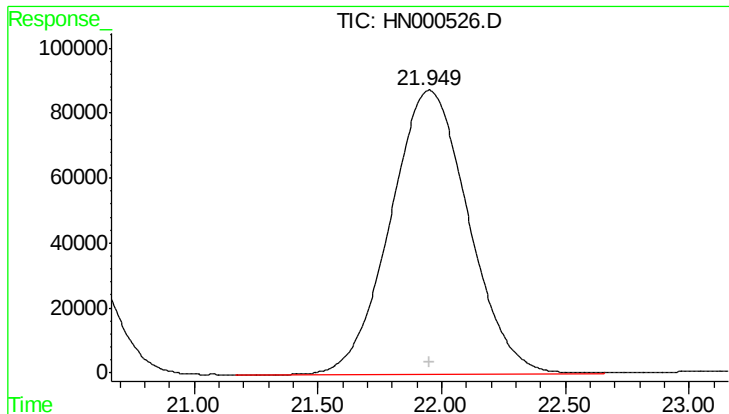

#9 2,4-Dinitrotoluene


R.T.: 21.951 min
Delta R.T.: 0.000 min
Response: 19220055
Conc: 493.99 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-4

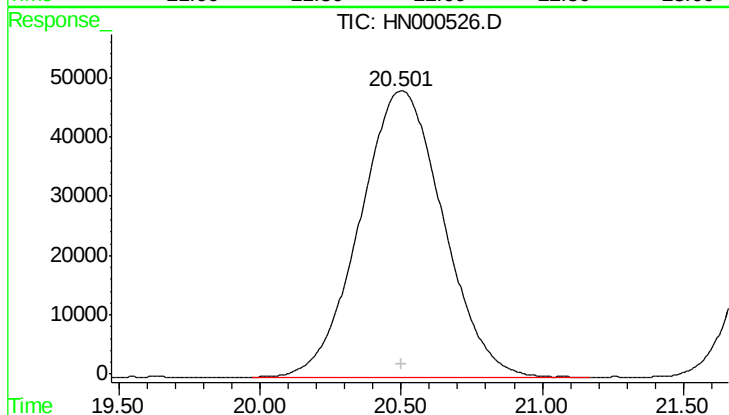


#10 2,6-Dinitrotoluene

R.T.: 20.502 min
Delta R.T.: 0.000 min
Response: 9955455
Conc: 493.31 ug/L

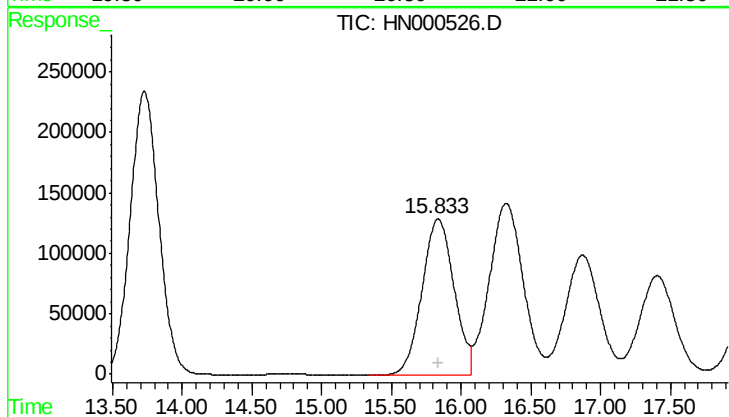


#11 1,3-Dinitrobenzene

R.T.: 15.835 min
Delta R.T.: 0.000 min
Response: 20702882
Conc: 503.84 ug/L

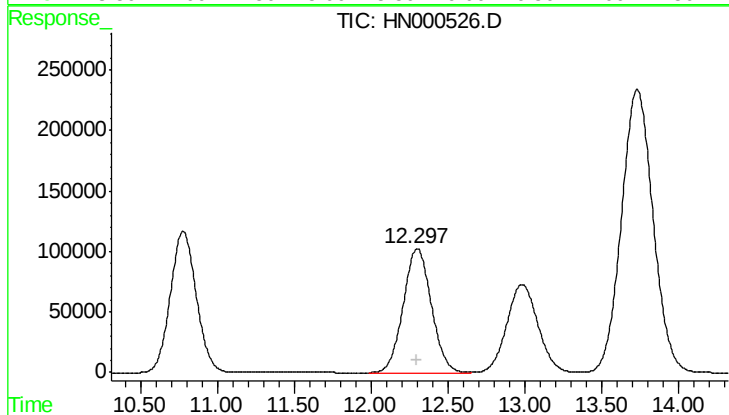

#12 Nitrobenzene


R.T.: 12.299 min
Delta R.T.: 0.000 min
Response: 13055872
Conc: 478.59 ug/L

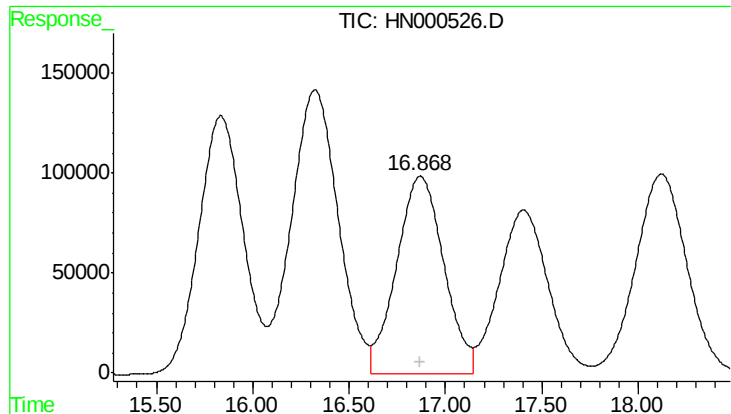

#13 2-Nitrotoluene


R.T.: 16.870 min
Delta R.T.: 0.000 min
Response: 16967522
Conc: 976.56 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-4

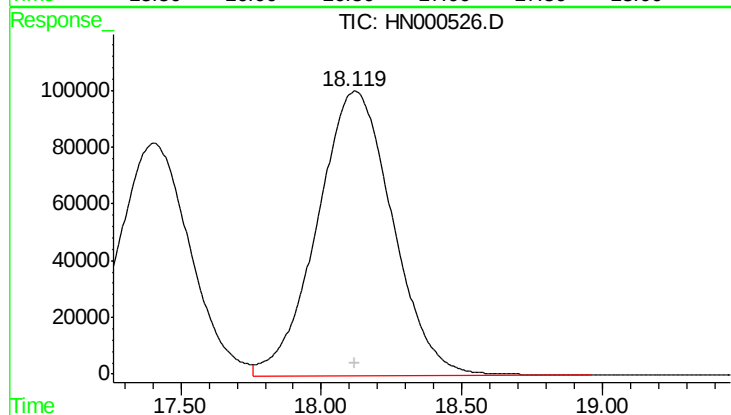


#14 3-Nitrotoluene

R.T.: 18.121 min
Delta R.T.: 0.000 min
Response: 18720552
Conc: 969.28 ug/L

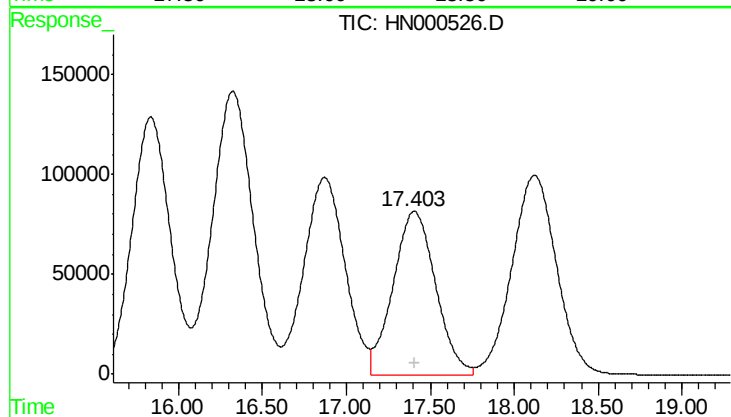

#15 4-Nitrotoluene

R.T.: 17.406 min
Delta R.T.: 0.000 min
Response: 14553743
Conc: 965.66 ug/L

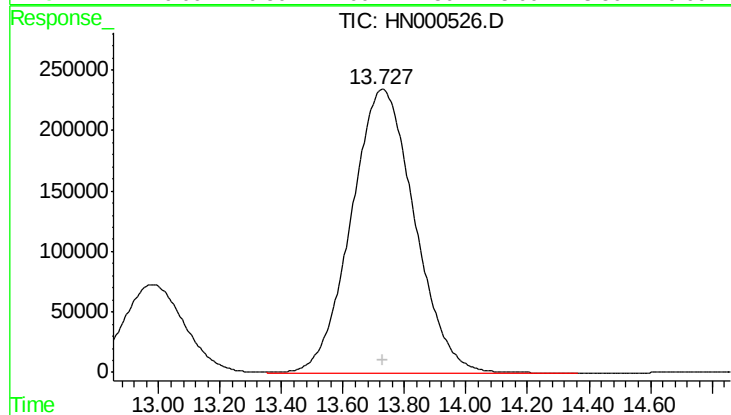

#16 3,5-Dinitroaniline

R.T.: 13.729 min
Delta R.T.: 0.000 min
Response: 33586251
Conc: 950.06 ug/L