

Data Path : S:\HPCHEM1\HPLC_N\Data\HN101012\
 Data File : HN000527.D
 Signal(s) : VWD1A.CH
 Acq On : 10-Oct-2012, 21:06
 Operator : HLM
 Sample : 8330-3
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 HPLC_N
 LabSampleId :
 8330-3

Integration File: events.e
 Quant Time: Nov 17 04:23:27 2012
 Quant Method : H:\VOL1\HPLC\HPLC_N\METHODS\HN101012.M
 Quant Title : SW8330 / 8330A confirmation
 QLast Update : Thu Oct 11 15:58:27 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	7.653	4989060	478.764 ug/L
Target Compounds				
2) T	HMX	12.955	5090986	474.297 ug/L
3) T	RDX	10.761	6707594	478.362 ug/L
4) T	1,3,5-Trinitrobenzene	24.909	6799892	232.340 ug/L
5) T	Tetryl	35.449	10284454	469.067 ug/L
6) T	2,4,6-Trinitrotoluene	33.569	6930862	253.262 ug/L
7) T	2-Amino-4,6-dinitroto...	16.298	11703468	230.555 ug/L
8) T	4-Amino-2,6-dinitroto...	16.298	11703468	230.555 ug/L
9) T	2,4-Dinitrotoluene	21.924	9389310	241.321 ug/L
10) T	2,6-Dinitrotoluene	20.474	4835304	239.599 ug/L
11) T	1,3-Dinitrobenzene	15.814	10071356	245.104 ug/L
12) T	Nitrobenzene	12.286	6376222	233.731 ug/L
13) T	2-Nitrotoluene	16.852	8146078	468.847 ug/L
14) T	3-Nitrotoluene	18.101	9319100	482.510 ug/L
15) T	4-Nitrotoluene	17.387	7021532	465.889 ug/L
16) T	3,5-Dinitroaniline	13.708	16407529	464.123 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_N\Data\HN101012\
Data File : HN000527.D
Signal(s) : VWD1A.CH
Acq On : 10-Oct-2012, 21:06
Operator : HLM
Sample : 8330-3
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
HPLC_N
LabSampleId :
8330-3

Integration File: events.e
Quant Time: Nov 17 04:23:27 2012
Quant Method : H:\VOL1\HPLC\HPLC_N\METHODS\HN101012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Thu Oct 11 15:58:27 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

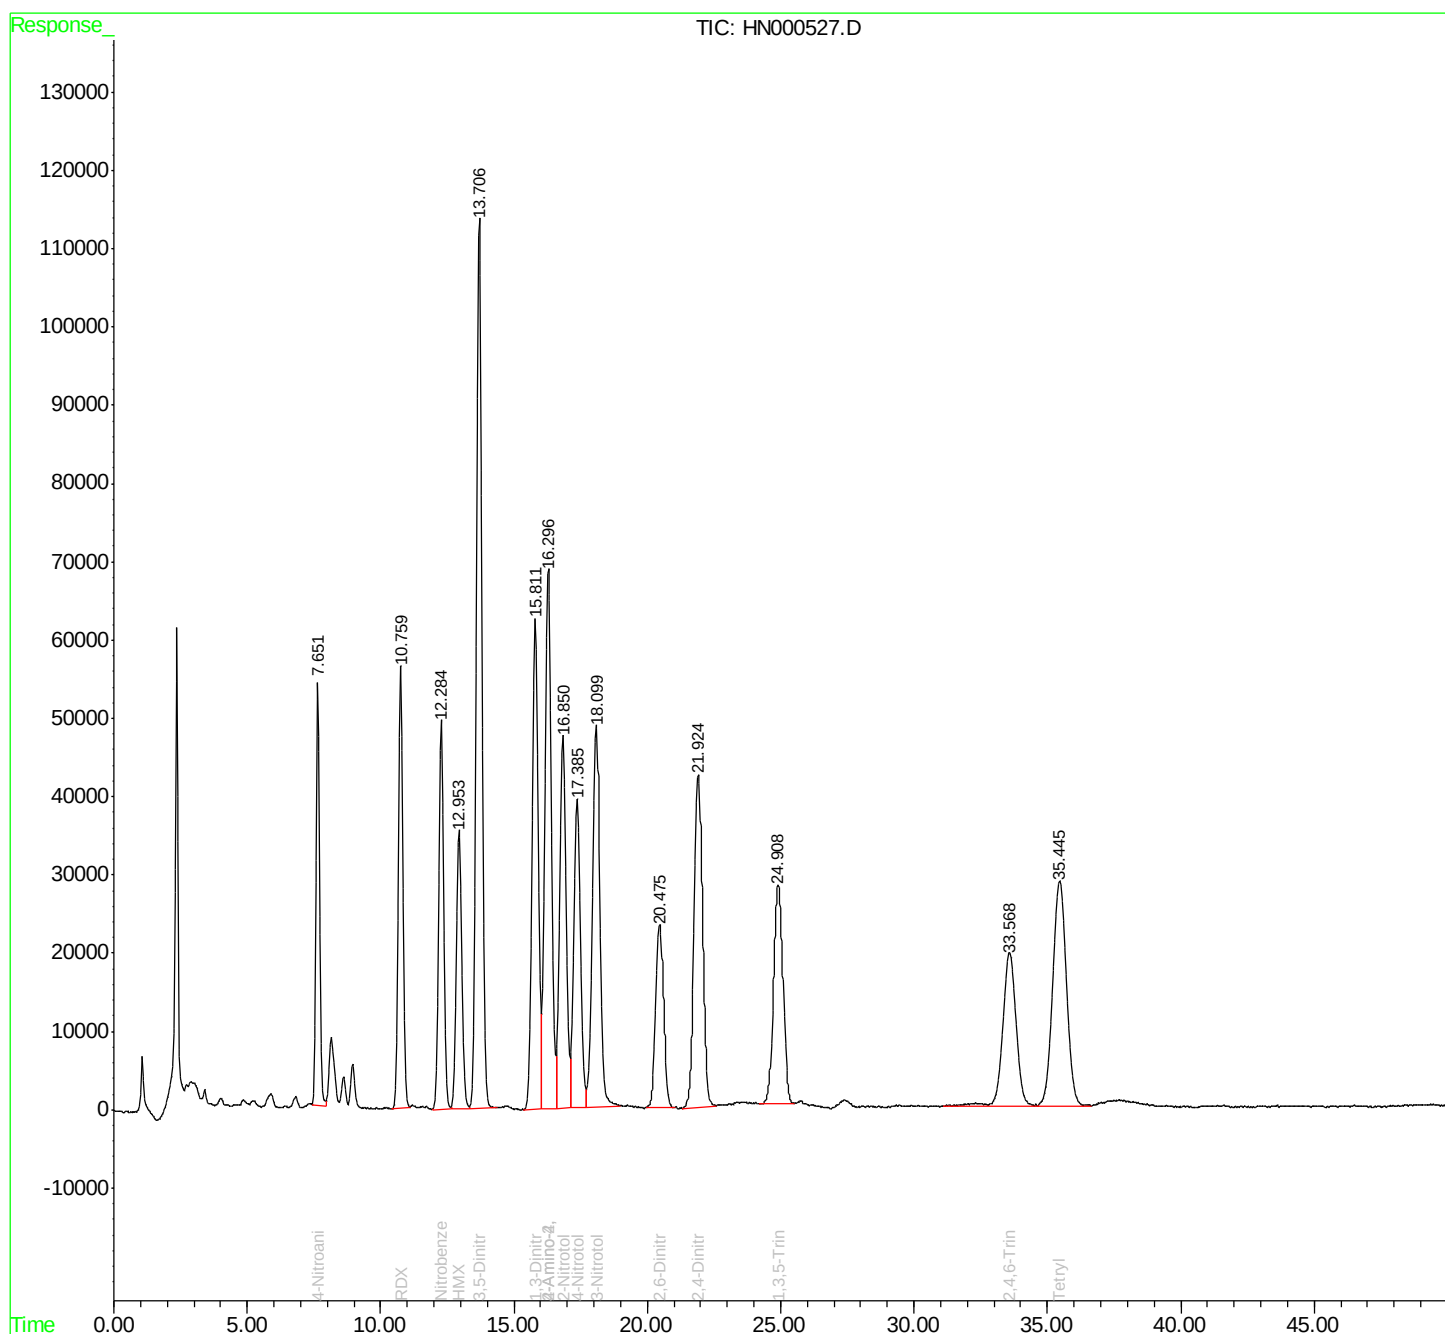


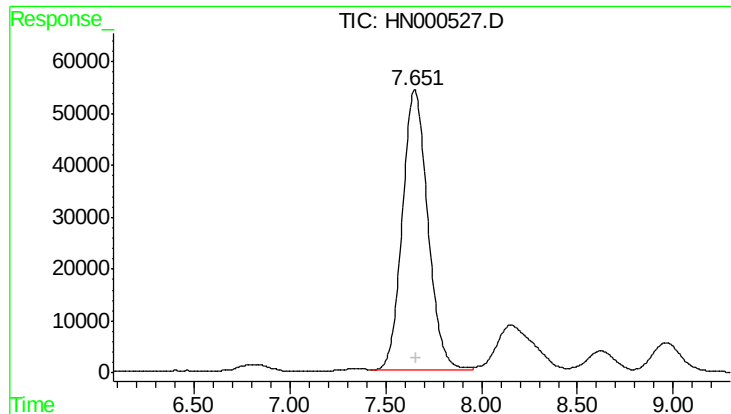

#1 4-Nitroaniline


R.T.: 7.653 min
Delta R.T.: -0.007 min
Response: 4989060
Conc: 478.76 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-3

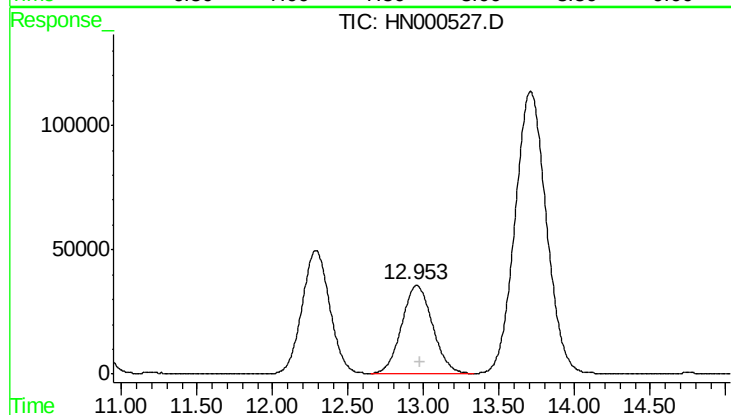


#2 HMX

R.T.: 12.955 min
Delta R.T.: -0.023 min
Response: 5090986
Conc: 474.30 ug/L

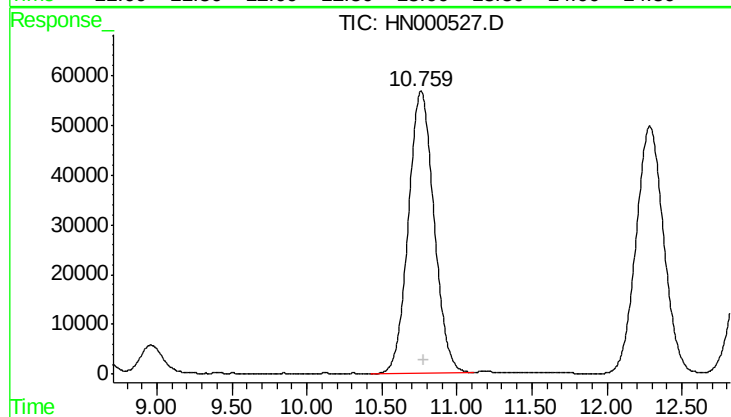


#3 RDX

R.T.: 10.761 min
Delta R.T.: -0.014 min
Response: 6707594
Conc: 478.36 ug/L

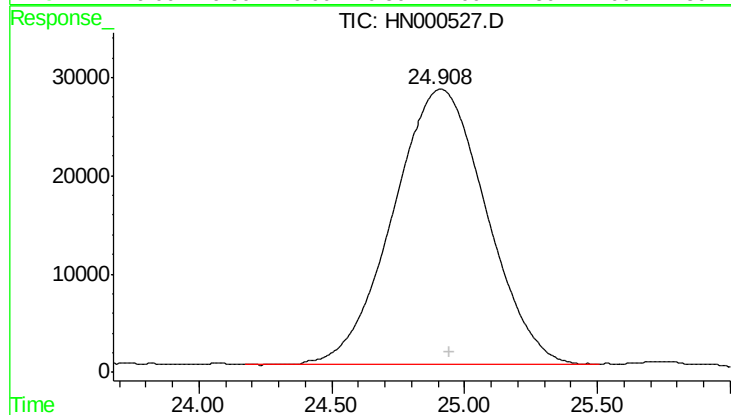

#4 1,3,5-Trinitrobenzene


R.T.: 24.909 min
Delta R.T.: -0.036 min
Response: 6799892
Conc: 232.34 ug/L

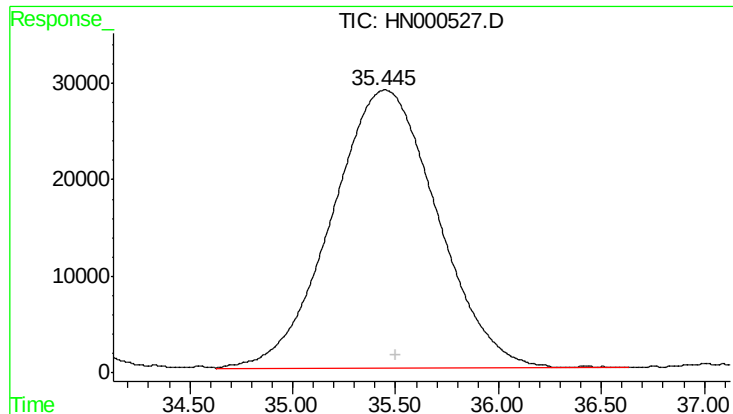

#5 Tetryl


R.T.: 35.449 min
Delta R.T.: -0.051 min
Response: 10284454
Conc: 469.07 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-3

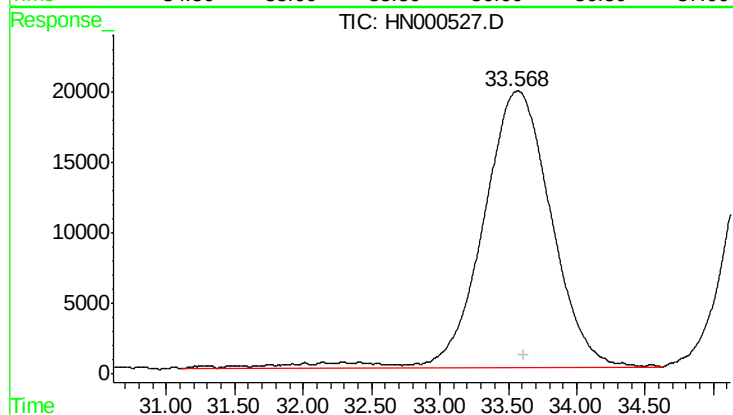


#6 2,4,6-Trinitrotoluene

R.T.: 33.569 min
Delta R.T.: -0.045 min
Response: 6930862
Conc: 253.26 ug/L

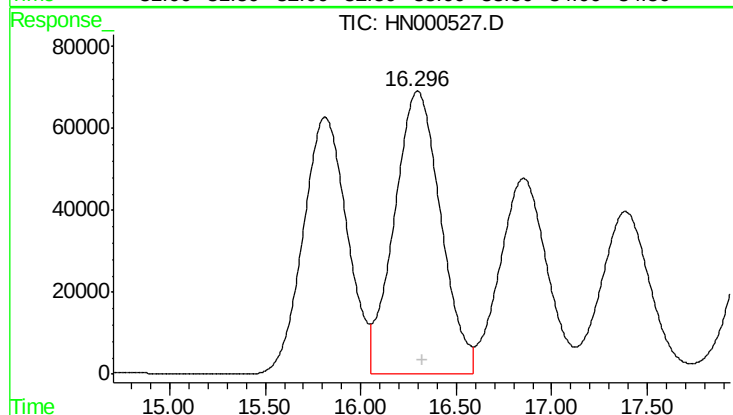


#7 2-Amino-4,6-dinitrotoluene

R.T.: 16.298 min
Delta R.T.: -0.026 min
Response: 11703468
Conc: 230.55 ug/L

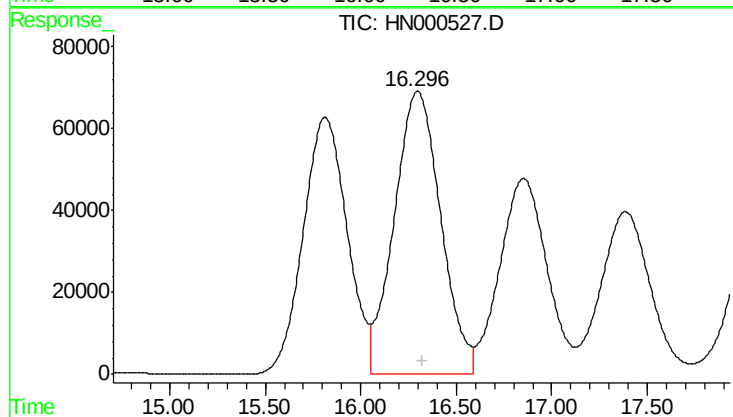

#8 4-Amino-2,6-dinitrotoluene


R.T.: 16.298 min
Delta R.T.: -0.026 min
Response: 11703468
Conc: 230.55 ug/L

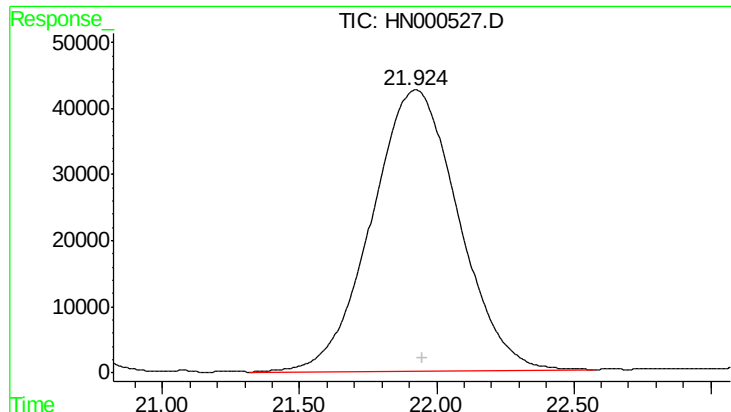

#9 2,4-Dinitrotoluene


R.T.: 21.924 min
Delta R.T.: -0.027 min
Response: 9389310
Conc: 241.32 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-3

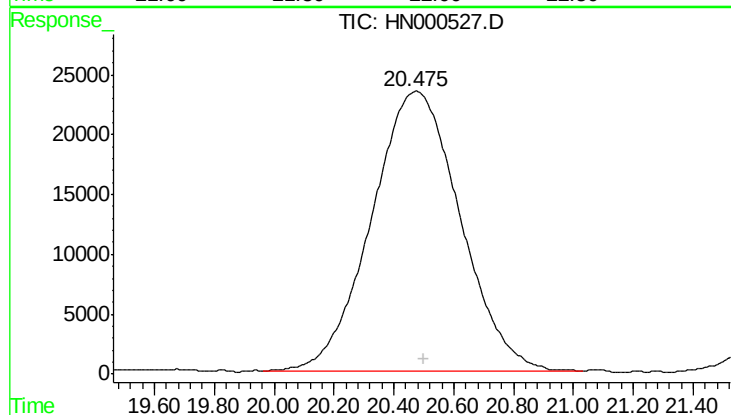


#10 2,6-Dinitrotoluene

R.T.: 20.474 min
Delta R.T.: -0.028 min
Response: 4835304
Conc: 239.60 ug/L

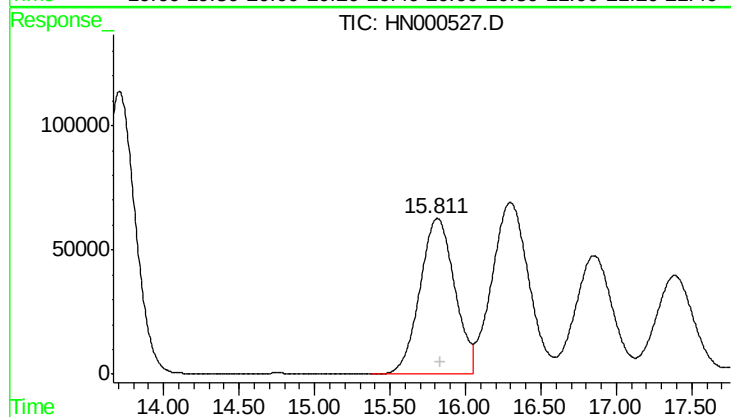


#11 1,3-Dinitrobenzene

R.T.: 15.814 min
Delta R.T.: -0.021 min
Response: 10071356
Conc: 245.10 ug/L

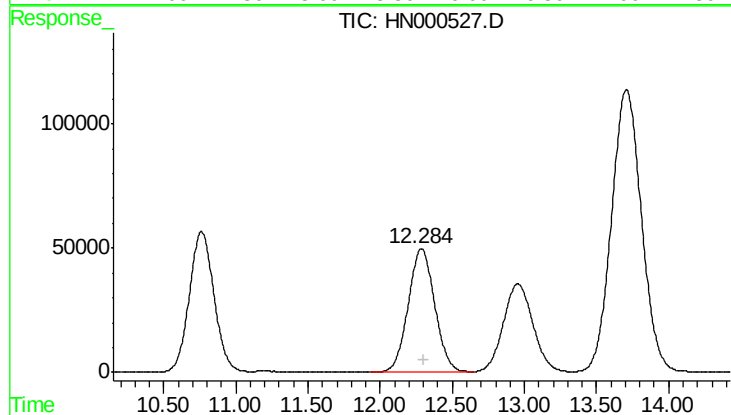

#12 Nitrobenzene


R.T.: 12.286 min
Delta R.T.: -0.013 min
Response: 6376222
Conc: 233.73 ug/L

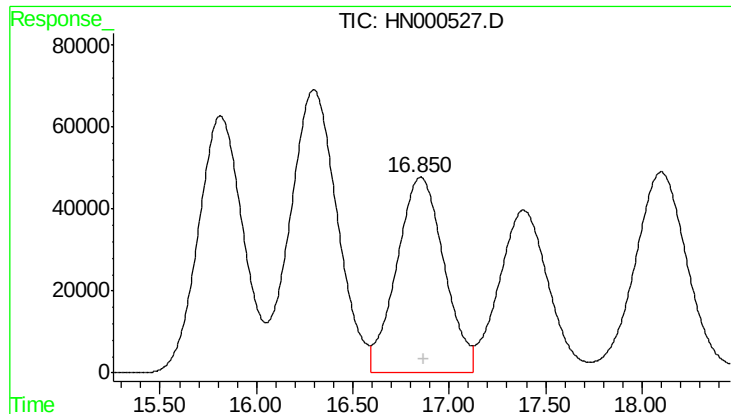

#13 2-Nitrotoluene


R.T.: 16.852 min
Delta R.T.: -0.018 min
Response: 8146078
Conc: 468.85 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-3

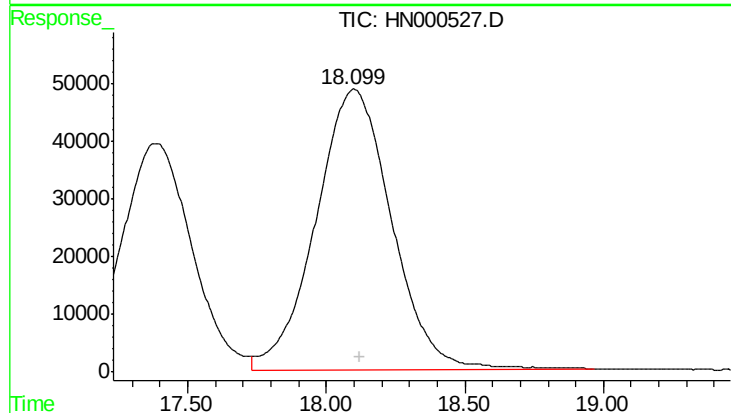


#14 3-Nitrotoluene

R.T.: 18.101 min
Delta R.T.: -0.020 min
Response: 9319100
Conc: 482.51 ug/L

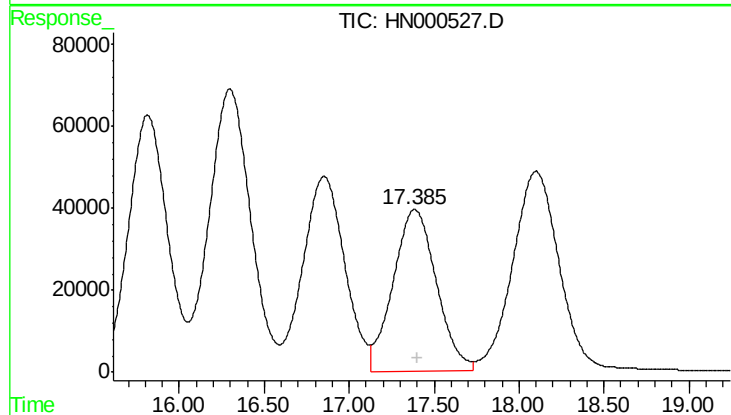

#15 4-Nitrotoluene

R.T.: 17.387 min
Delta R.T.: -0.019 min
Response: 7021532
Conc: 465.89 ug/L

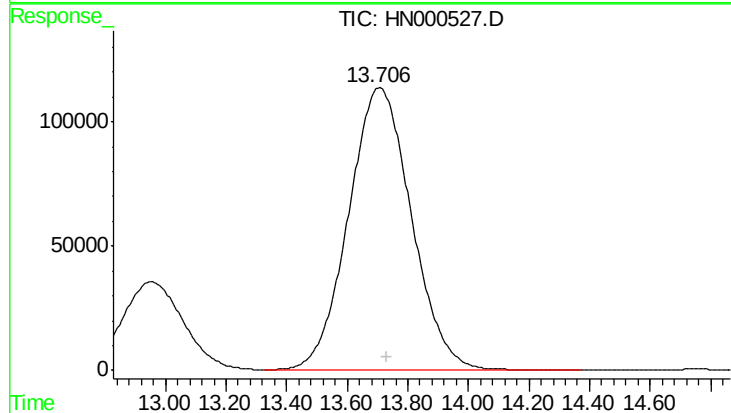

#16 3,5-Dinitroaniline

R.T.: 13.708 min
Delta R.T.: -0.021 min
Response: 16407529
Conc: 464.12 ug/L