

Data Path : S:\HPCHEM1\HPLC_N\Data\HN101012\
 Data File : HN000528.D
 Signal(s) : VWD1A.CH
 Acq On : 10-Oct-2012, 21:58
 Operator : HLM
 Sample : 8330-2
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 HPLC_N
 LabSampleId :
 8330-2

Integration File: events.e
 Quant Time: Nov 17 04:27:19 2012
 Quant Method : H:\VOL1\HPLC\HPLC_N\METHODS\HN101012.M
 Quant Title : SW8330 / 8330A confirmation
 QLast Update : Thu Oct 11 15:58:27 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	7.652	990474	95.049 ug/L
Target Compounds			
2) T HMX	12.951	1048414	97.675 ug/L
3) T RDX	10.763	1325633	94.539 ug/L
4) T 1,3,5-Trinitrobenzene	24.916	1340412	45.799 ug/L
5) T Tetryl	35.448	2100362	95.796 ug/L
6) T 2,4,6-Trinitrotoluene	33.562	1268810	46.364 ug/L
7) T 2-Amino-4,6-dinitroto...	16.300	2336059	46.020 ug/L
8) T 4-Amino-2,6-dinitroto...	16.300	2336059	46.020 ug/L
9) T 2,4-Dinitrotoluene	21.934	1846077	47.447 ug/L
10) T 2,6-Dinitrotoluene	20.478	1014420	50.267 ug/L
11) T 1,3-Dinitrobenzene	15.813	2011172	48.945 ug/L
12) T Nitrobenzene	12.286	1287850	47.208 ug/L
13) T 2-Nitrotoluene	16.854	1549706	89.193 ug/L
14) T 3-Nitrotoluene	18.097	2246985	116.341 ug/L
15) T 4-Nitrotoluene	17.391	1467169	97.349 ug/L
16) T 3,5-Dinitroaniline	13.709	3303791	93.455 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_N\Data\HN101012\
Data File : HN000528.D
Signal(s) : VWD1A.CH
Acq On : 10-Oct-2012, 21:58
Operator : HLM
Sample : 8330-2
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
HPLC_N
LabSampleId :
8330-2

Integration File: events.e
Quant Time: Nov 17 04:27:19 2012
Quant Method : H:\VOL1\HPLC\HPLC_N\METHODS\HN101012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Thu Oct 11 15:58:27 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

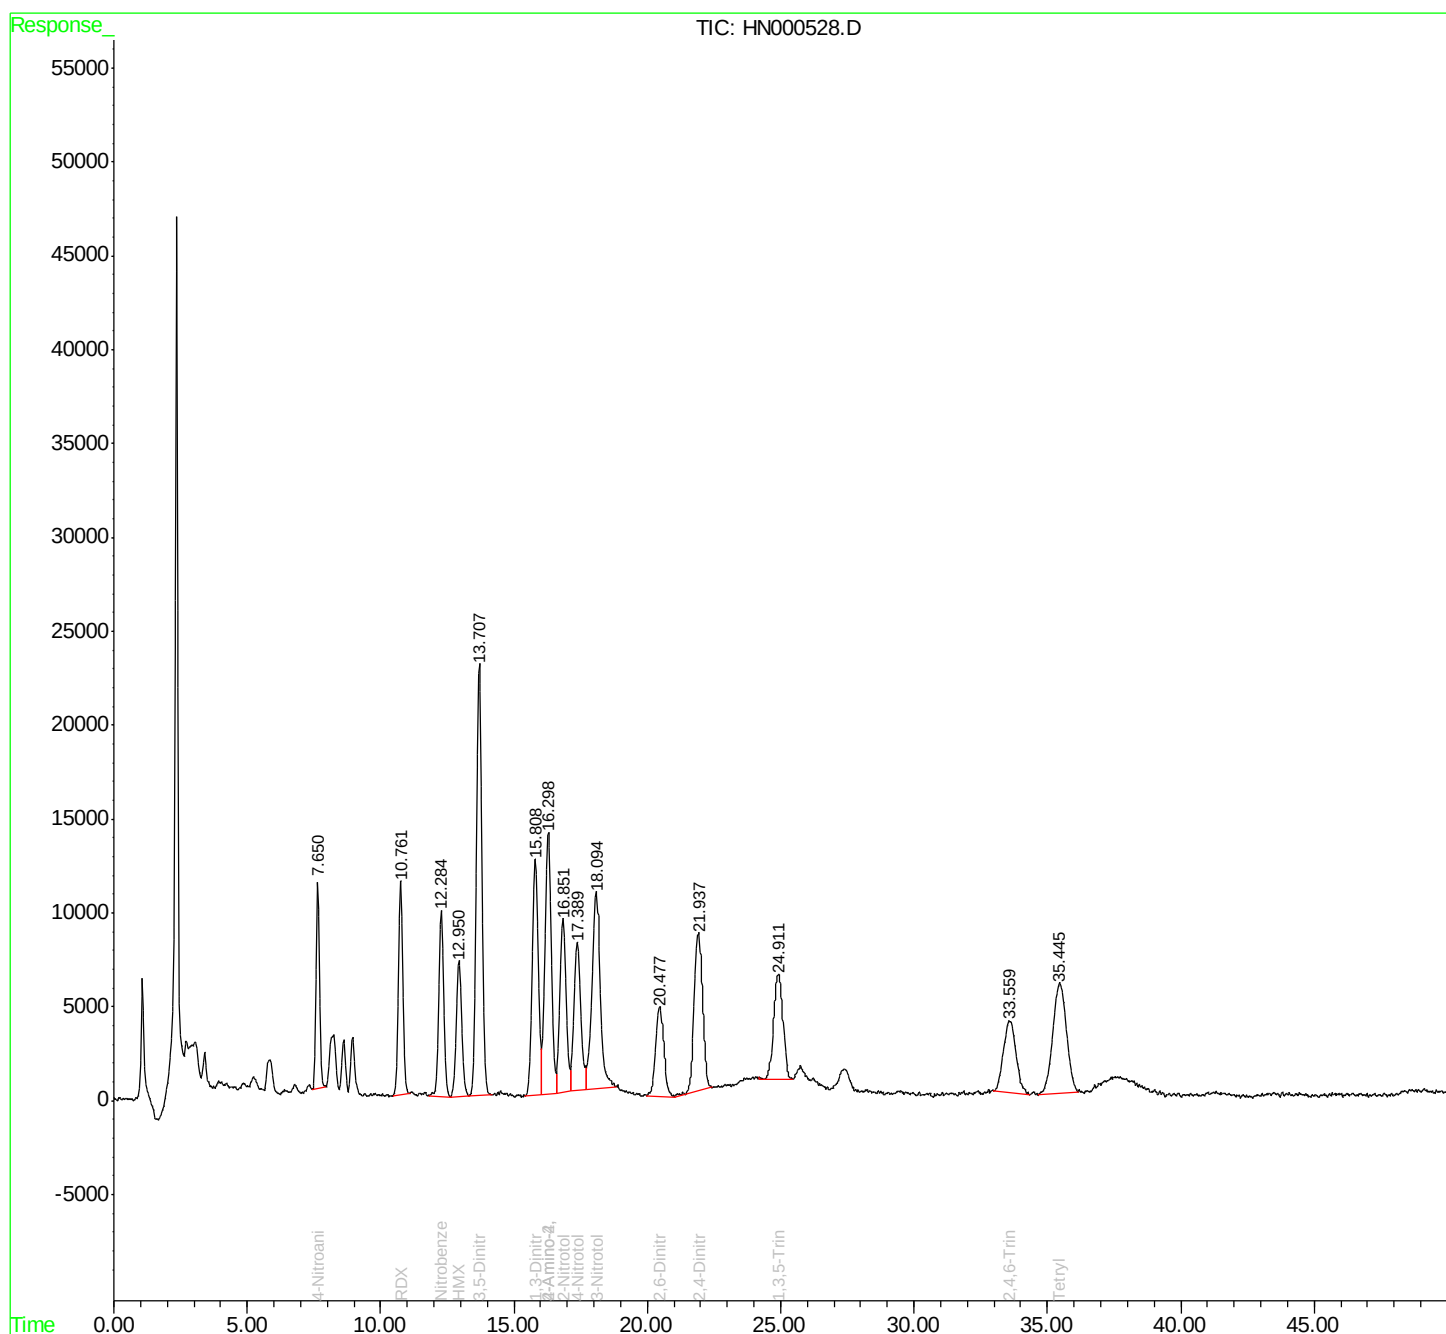


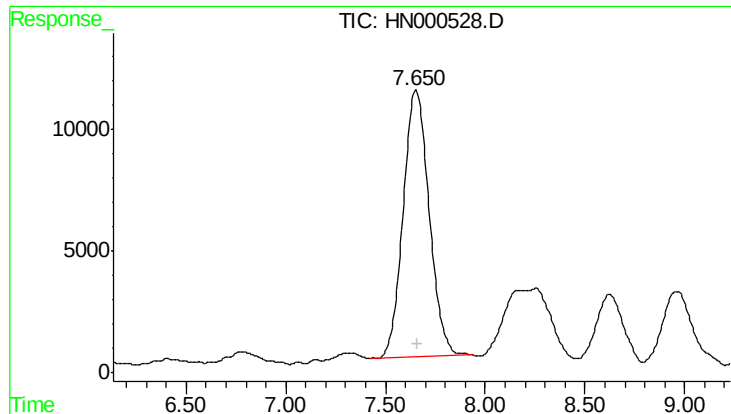

#1 4-Nitroaniline


R.T.: 7.652 min
Delta R.T.: -0.007 min
Response: 990474
Conc: 95.05 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-2

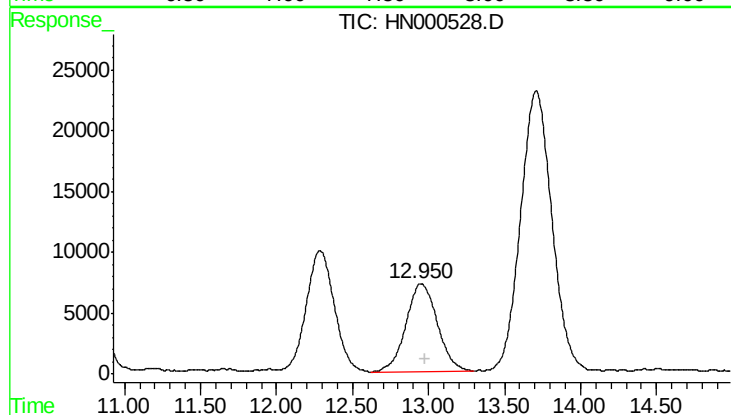


#2 HMX

R.T.: 12.951 min
Delta R.T.: -0.027 min
Response: 1048414
Conc: 97.67 ug/L

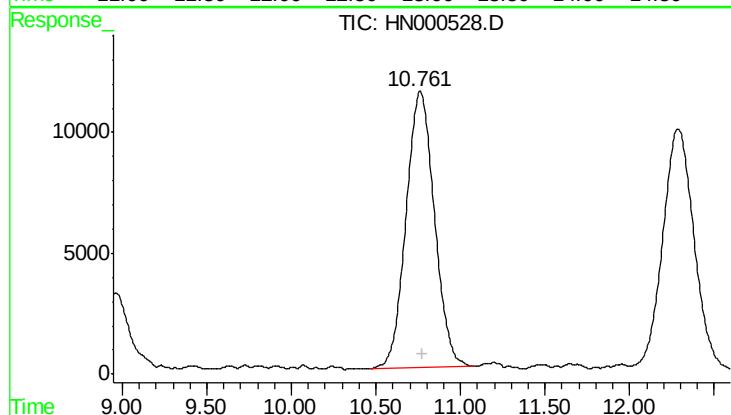


#3 RDX

R.T.: 10.763 min
Delta R.T.: -0.013 min
Response: 1325633
Conc: 94.54 ug/L

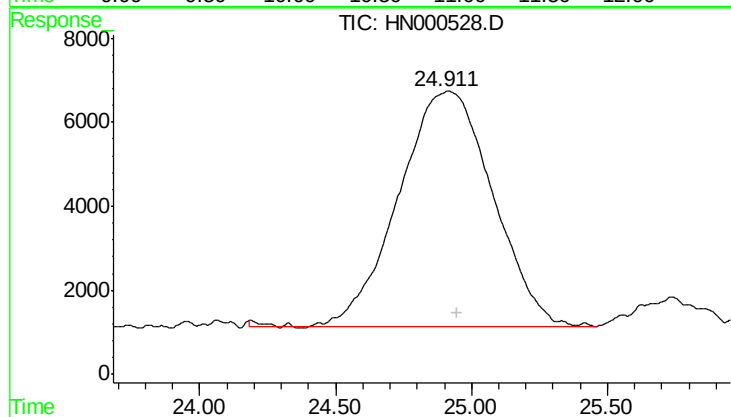

#4 1,3,5-Trinitrobenzene


R.T.: 24.916 min
Delta R.T.: -0.029 min
Response: 1340412
Conc: 45.80 ug/L

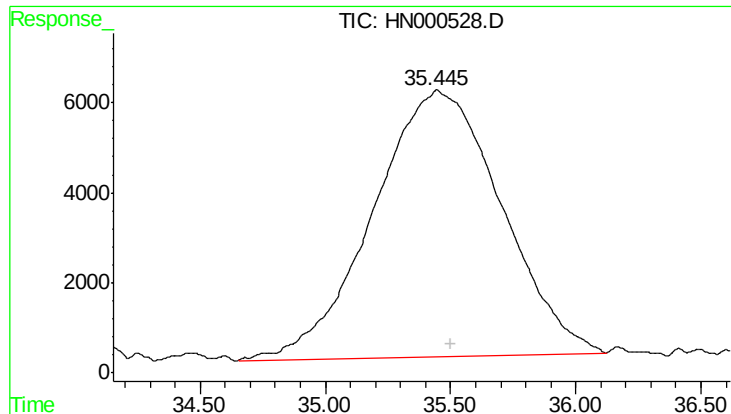

#5 Tetryl


R.T.: 35.448 min
 Delta R.T.: -0.052 min
 Response: 2100362
 Conc: 95.80 ug/L

Instrument :
 HPLC_N
 LabSampleId :
 8330-2

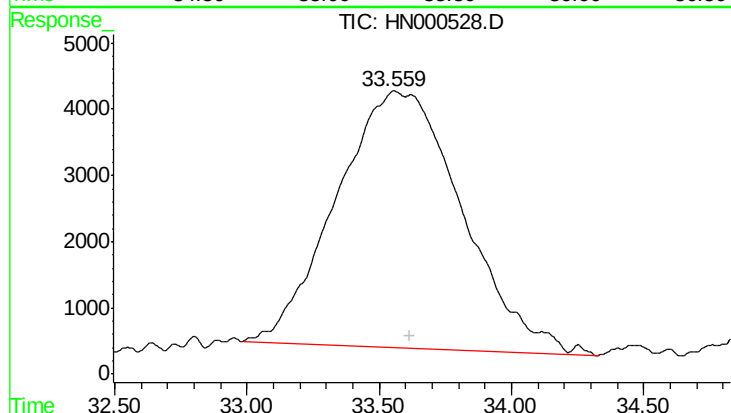


#6 2,4,6-Trinitrotoluene

R.T.: 33.562 min
 Delta R.T.: -0.052 min
 Response: 1268810
 Conc: 46.36 ug/L

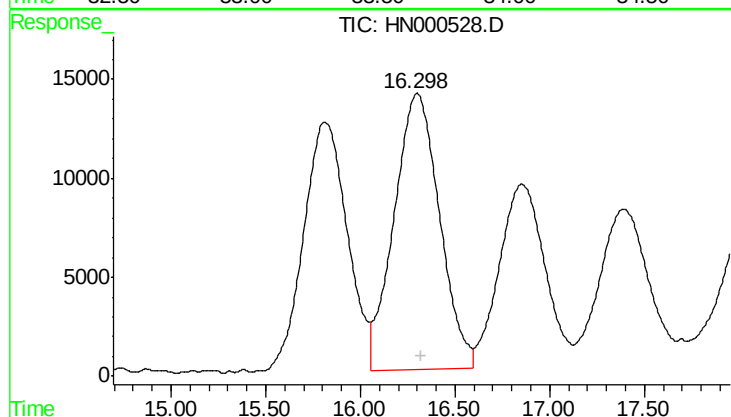


#7 2-Amino-4,6-dinitrotoluene

R.T.: 16.300 min
 Delta R.T.: -0.024 min
 Response: 2336059
 Conc: 46.02 ug/L

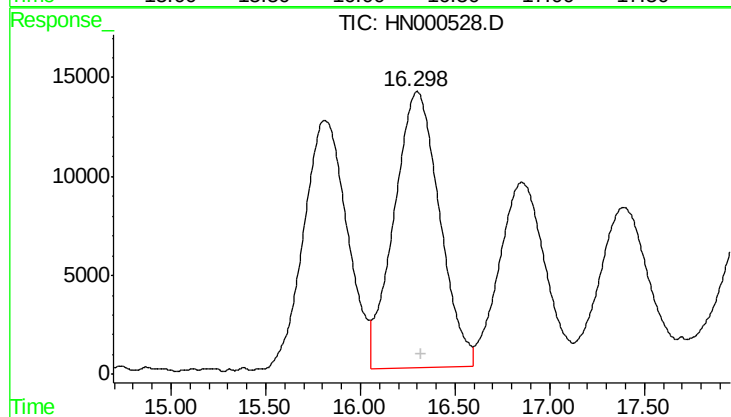

#8 4-Amino-2,6-dinitrotoluene


R.T.: 16.300 min
 Delta R.T.: -0.024 min
 Response: 2336059
 Conc: 46.02 ug/L

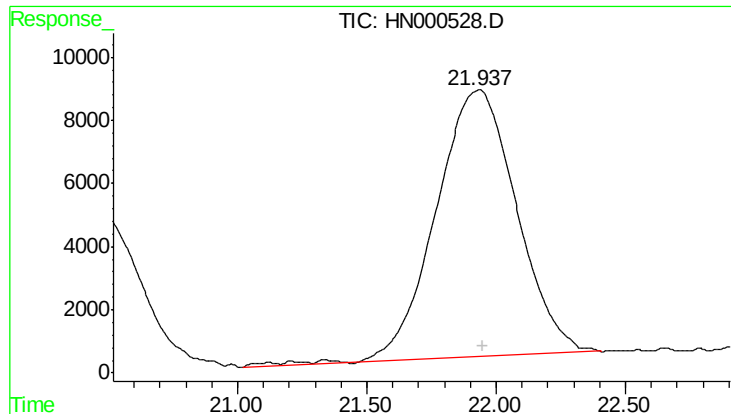

#9 2,4-Dinitrotoluene


R.T.: 21.934 min
Delta R.T.: -0.017 min
Response: 1846077
Conc: 47.45 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-2

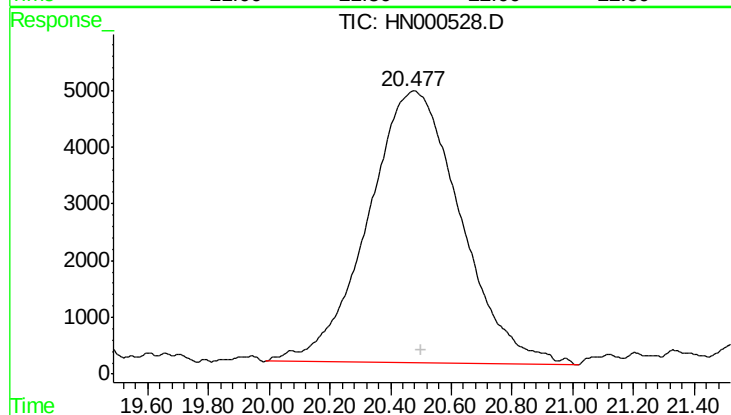


#10 2,6-Dinitrotoluene

R.T.: 20.478 min
Delta R.T.: -0.024 min
Response: 1014420
Conc: 50.27 ug/L

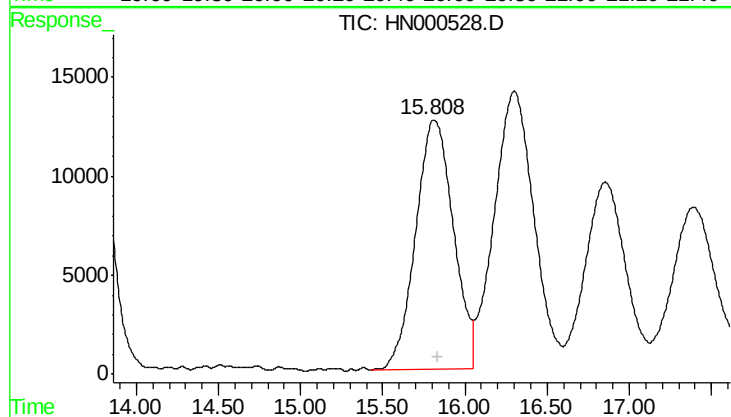


#11 1,3-Dinitrobenzene

R.T.: 15.813 min
Delta R.T.: -0.021 min
Response: 2011172
Conc: 48.95 ug/L

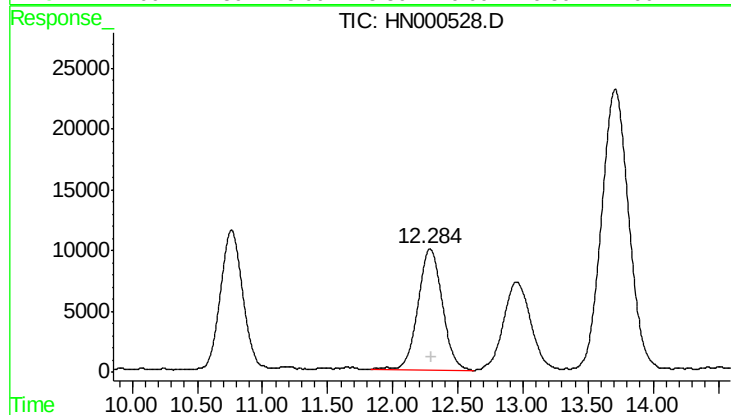

#12 Nitrobenzene


R.T.: 12.286 min
Delta R.T.: -0.013 min
Response: 1287850
Conc: 47.21 ug/L

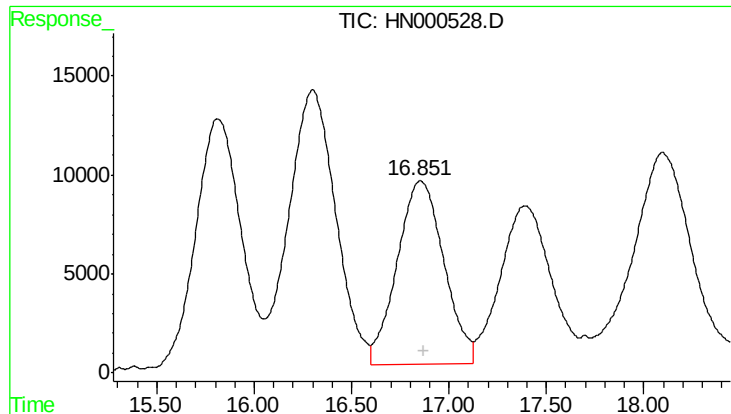

#13 2-Nitrotoluene


R.T.: 16.854 min
Delta R.T.: -0.016 min
Response: 1549706
Conc: 89.19 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-2

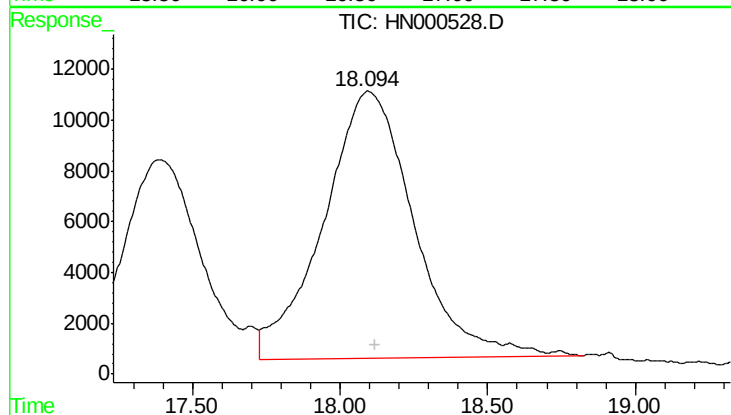


#14 3-Nitrotoluene

R.T.: 18.097 min
Delta R.T.: -0.024 min
Response: 2246985
Conc: 116.34 ug/L

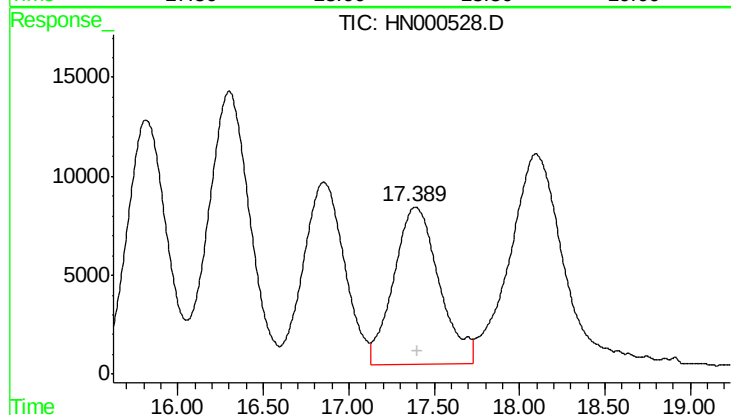

#15 4-Nitrotoluene

R.T.: 17.391 min
Delta R.T.: -0.015 min
Response: 1467169
Conc: 97.35 ug/L

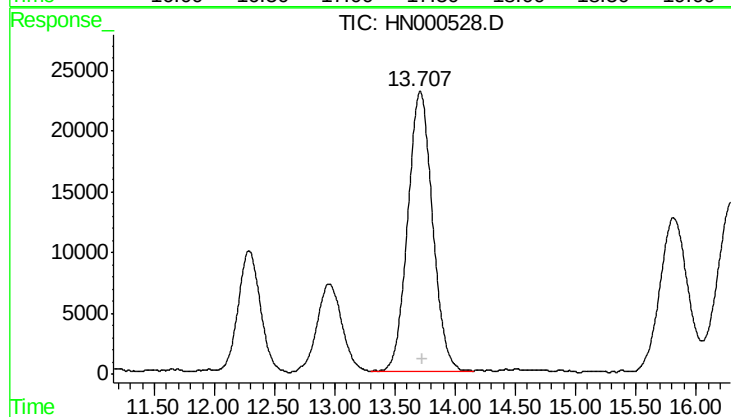

#16 3,5-Dinitroaniline

R.T.: 13.709 min
Delta R.T.: -0.020 min
Response: 3303791
Conc: 93.45 ug/L