

Data Path : S:\HPCHEM1\HPLC_N\Data\HN101012\
 Data File : HN000529.D
 Signal(s) : VWD1A.CH
 Acq On : 10-Oct-2012, 22:51
 Operator : HLM
 Sample : 8330-1
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 HPLC_N
 LabSampleId :
 8330-1

Integration File: events.e
 Quant Time: Nov 17 04:27:25 2012
 Quant Method : H:\VOL1\HPLC\HPLC_N\METHODS\HN101012.M
 Quant Title : SW8330 / 8330A confirmation
 QLast Update : Thu Oct 11 15:58:27 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

	Compound	R.T.	Response	Conc	Units

System Monitoring Compounds					
1) S	4-Nitroaniline	7.652	229267	22.001	ug/L m
Target Compounds					
2) T	HMX	12.935	209924	19.557	ug/L m
3) T	RDX	10.769	319848	22.810	ug/L
4) T	1,3,5-Trinitrobenzene	24.911	271962	9.292	ug/L m
5) T	Tetryl	35.441	471294	21.495	ug/L m
6) T	2,4,6-Trinitrotoluene	33.516	278714	10.185	ug/L m
7) T	2-Amino-4,6-dinitroto...	16.301	437112	8.611	ug/L
8) T	4-Amino-2,6-dinitroto...	16.301	437112	8.611	ug/L
9) T	2,4-Dinitrotoluene	21.939	382220	9.824	ug/L
10) T	2,6-Dinitrotoluene	20.472	188122	9.322	ug/L m
11) T	1,3-Dinitrobenzene	15.823	392941	9.563	ug/L
12) T	Nitrobenzene	12.291	273339	10.020	ug/L
13) T	2-Nitrotoluene	16.880	272220	15.668	ug/L
14) T	3-Nitrotoluene	18.119	542412	28.084	ug/L m
15) T	4-Nitrotoluene	17.390	202539	13.439	ug/L m
16) T	3,5-Dinitroaniline	13.720	695564	19.676	ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_N\Data\HN101012\
Data File : HN000529.D
Signal(s) : VWD1A.CH
Acq On : 10-Oct-2012, 22:51
Operator : HLM
Sample : 8330-1
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
HPLC_N
LabSampleId :
8330-1

Integration File: events.e
Quant Time: Nov 17 04:27:25 2012
Quant Method : H:\VOL1\HPLC\HPLC_N\METHODS\HN101012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Thu Oct 11 15:58:27 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

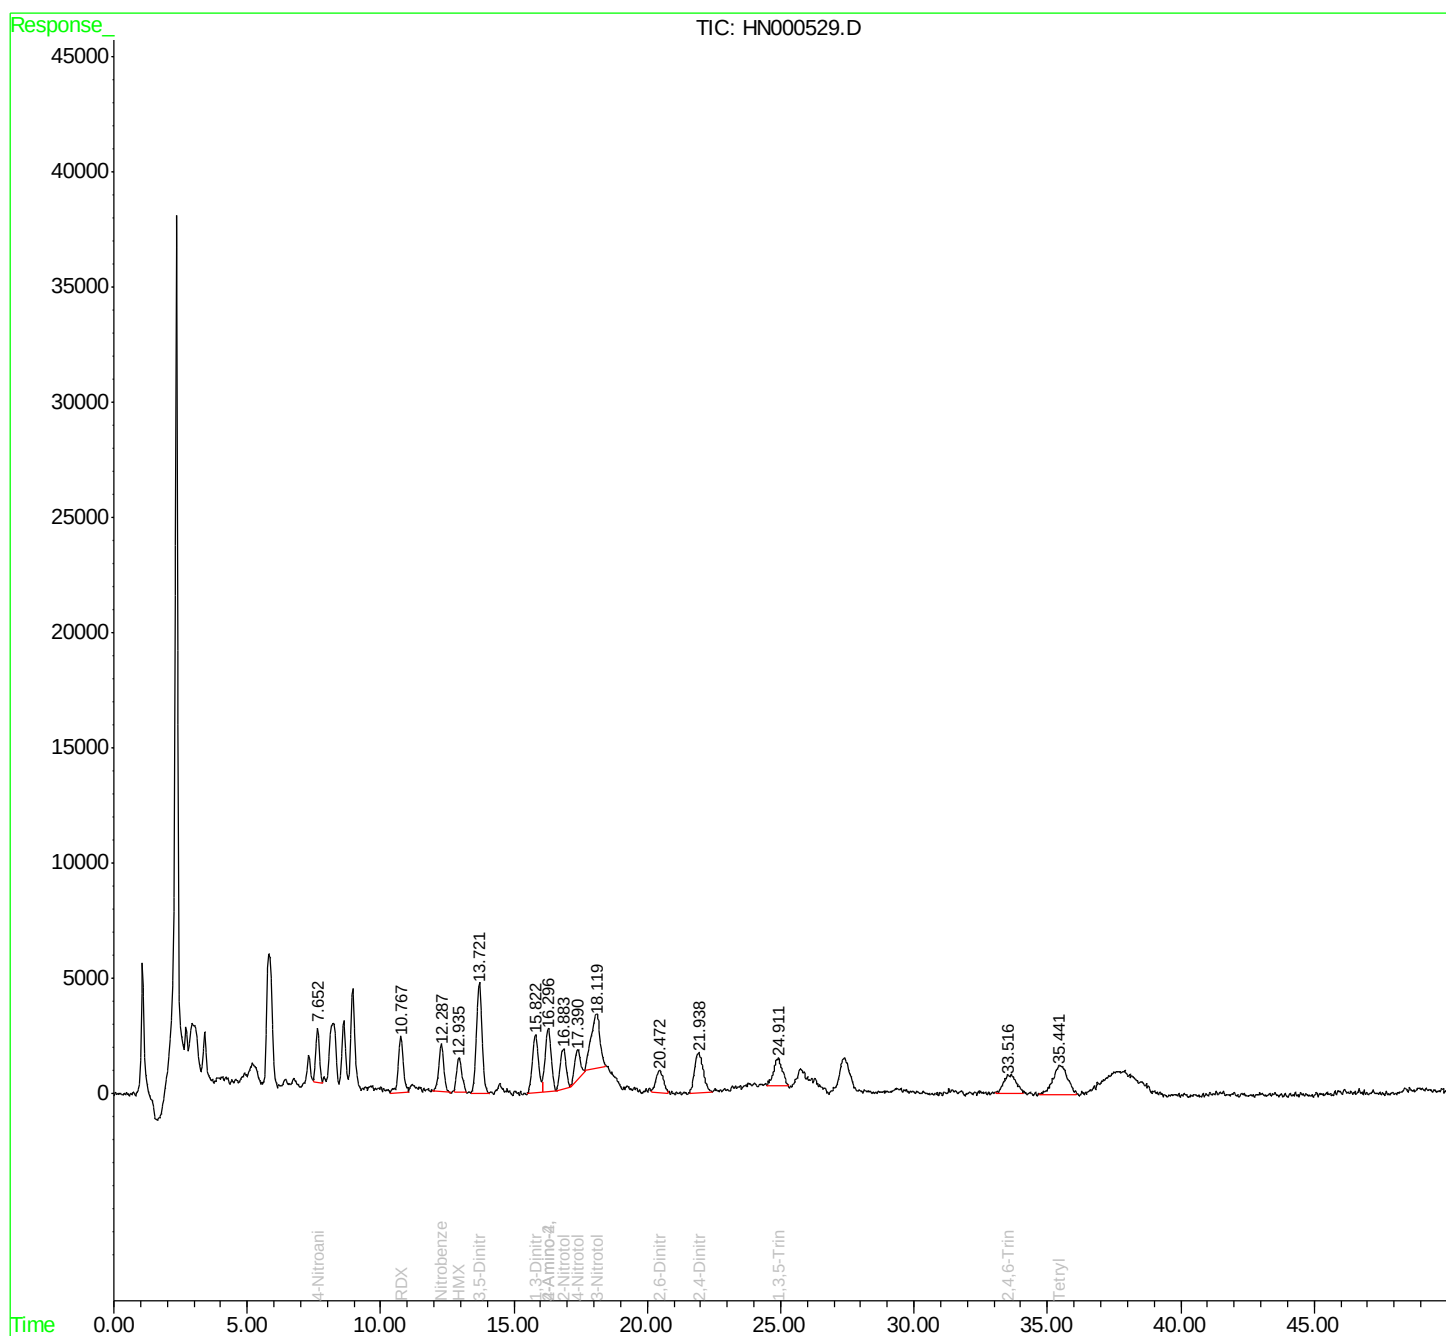


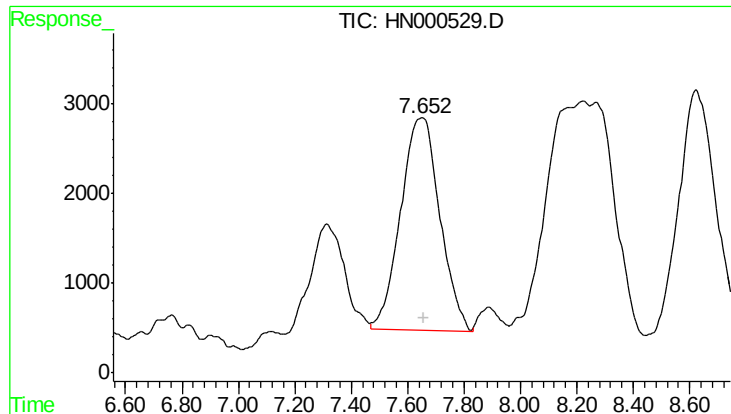

#1 4-Nitroaniline


R.T.: 7.652 min
Delta R.T.: -0.007 min
Response: 229267
Conc: 22.00 ug/L m

Instrument :
HPLC_N
LabSampleId :
8330-1

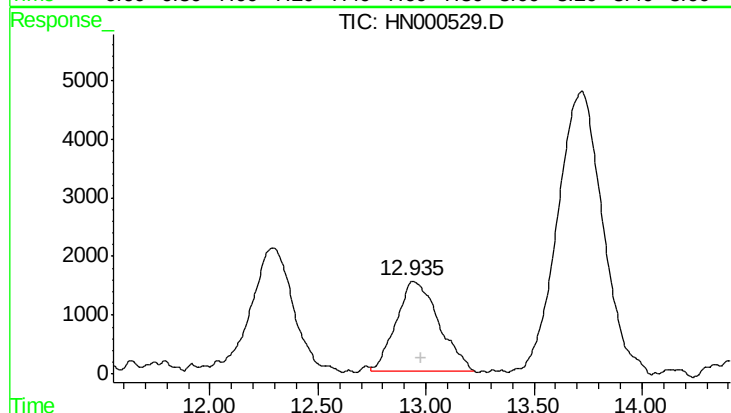


#2 HMX

R.T.: 12.935 min
Delta R.T.: -0.043 min
Response: 209924
Conc: 19.56 ug/L m

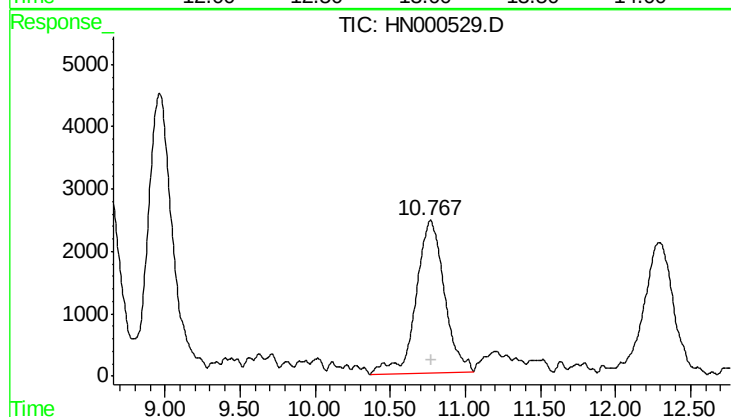


#3 RDX

R.T.: 10.769 min
Delta R.T.: -0.006 min
Response: 319848
Conc: 22.81 ug/L

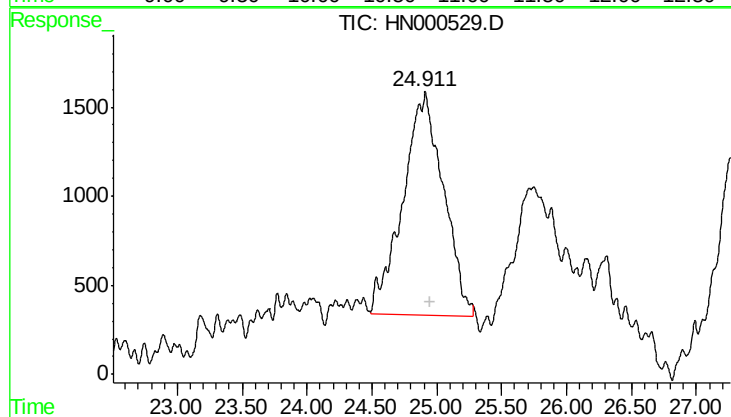

#4 1,3,5-Trinitrobenzene


R.T.: 24.911 min
Delta R.T.: -0.034 min
Response: 271962
Conc: 9.29 ug/L m

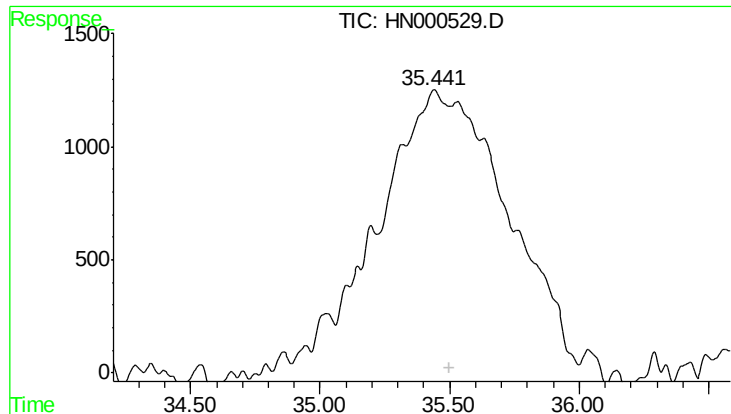

#5 Tetryl


R.T.: 35.441 min
Delta R.T.: -0.059 min
Response: 471294
Conc: 21.50 ug/L m

Instrument :
HPLC_N
LabSampleId :
8330-1

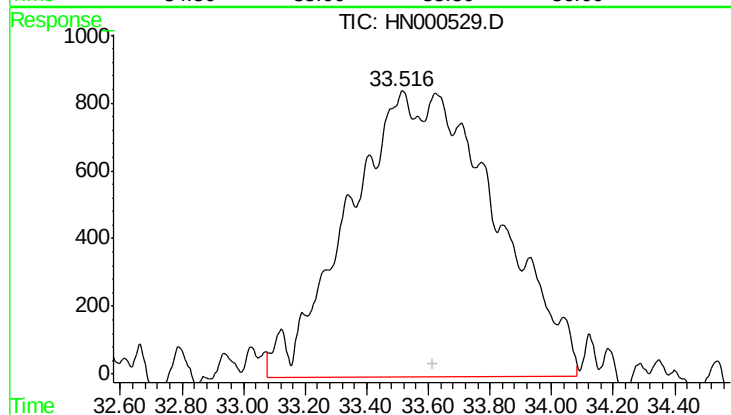


#6 2,4,6-Trinitrotoluene

R.T.: 33.516 min
Delta R.T.: -0.098 min
Response: 278714
Conc: 10.18 ug/L m

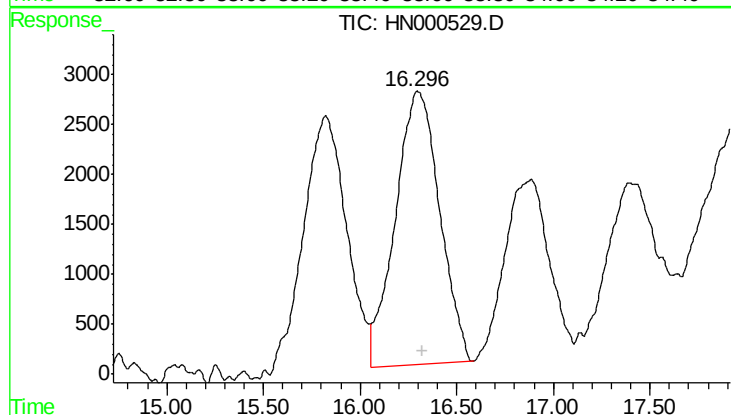


#7 2-Amino-4,6-dinitrotoluene

R.T.: 16.301 min
Delta R.T.: -0.023 min
Response: 437112
Conc: 8.61 ug/L

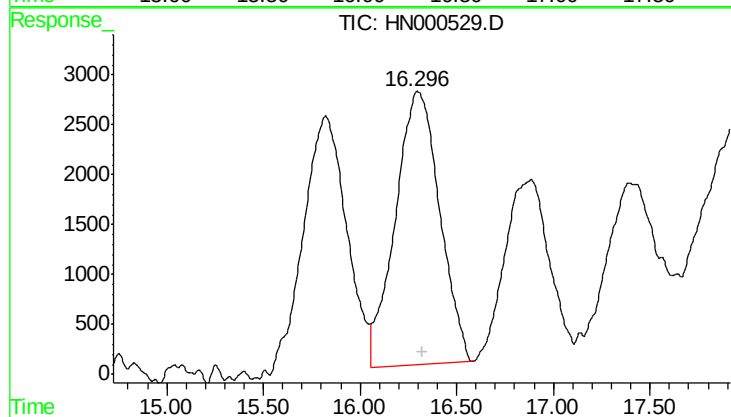

#8 4-Amino-2,6-dinitrotoluene


R.T.: 16.301 min
Delta R.T.: -0.023 min
Response: 437112
Conc: 8.61 ug/L

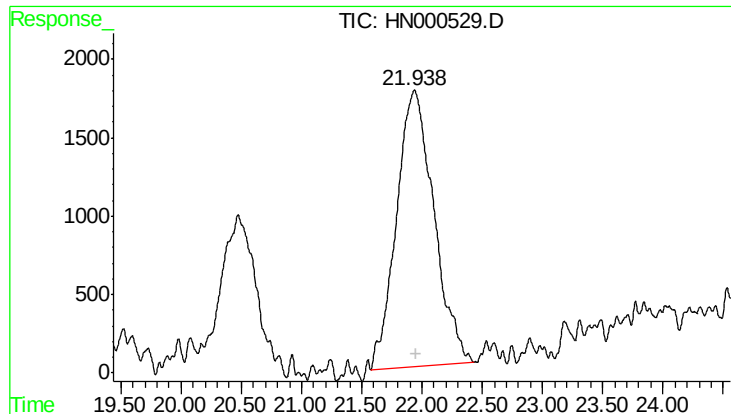

#9 2,4-Dinitrotoluene


R.T.: 21.939 min
Delta R.T.: -0.012 min
Response: 382220
Conc: 9.82 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-1

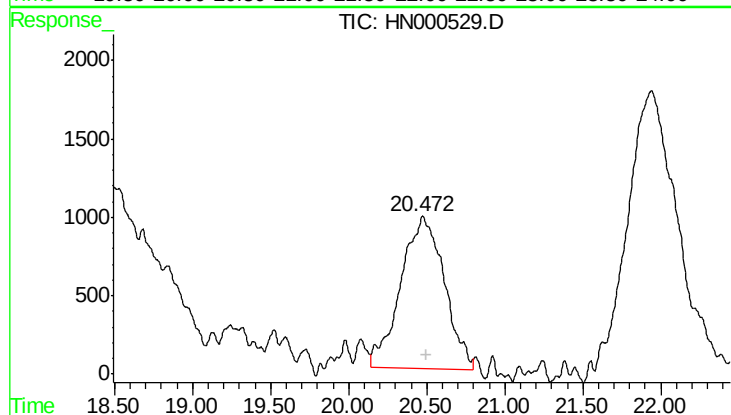


#10 2,6-Dinitrotoluene

R.T.: 20.472 min
Delta R.T.: -0.030 min
Response: 188122
Conc: 9.32 ug/L m

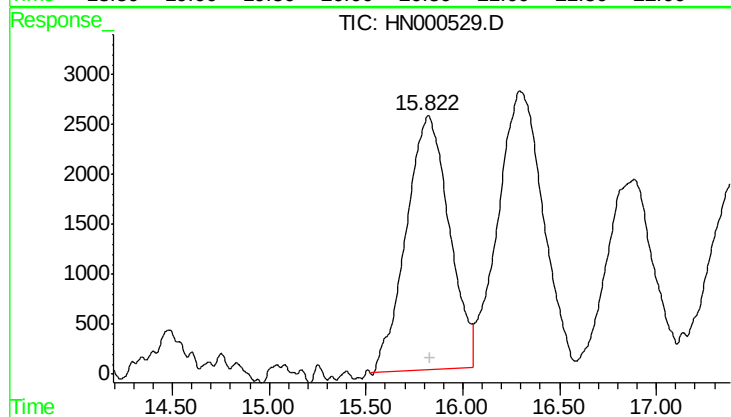


#11 1,3-Dinitrobenzene

R.T.: 15.823 min
Delta R.T.: -0.012 min
Response: 392941
Conc: 9.56 ug/L

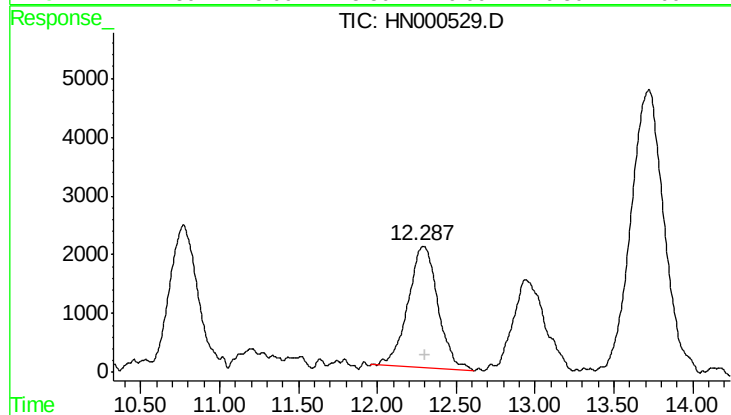

#12 Nitrobenzene


R.T.: 12.291 min
Delta R.T.: -0.009 min
Response: 273339
Conc: 10.02 ug/L

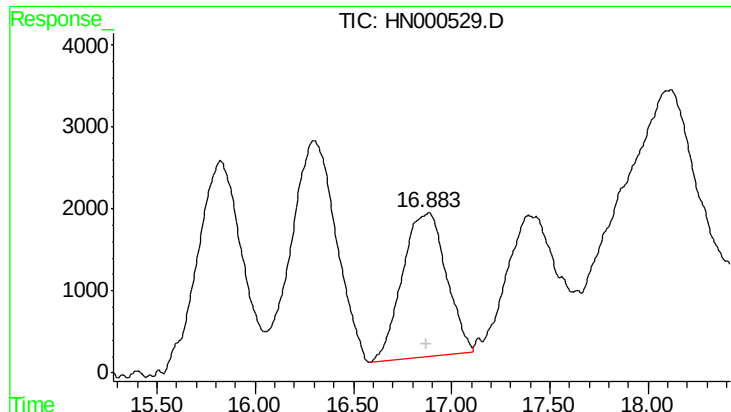

#13 2-Nitrotoluene


R.T.: 16.880 min
Delta R.T.: 0.010 min
Response: 272220
Conc: 15.67 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-1

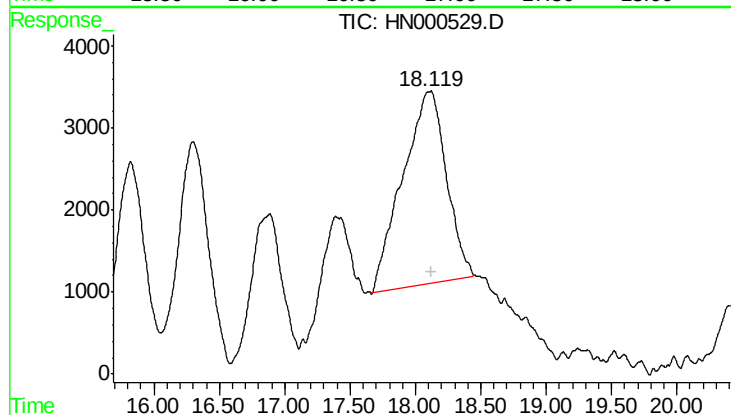


#14 3-Nitrotoluene

R.T.: 18.119 min
Delta R.T.: -0.002 min
Response: 542412
Conc: 28.08 ug/L m

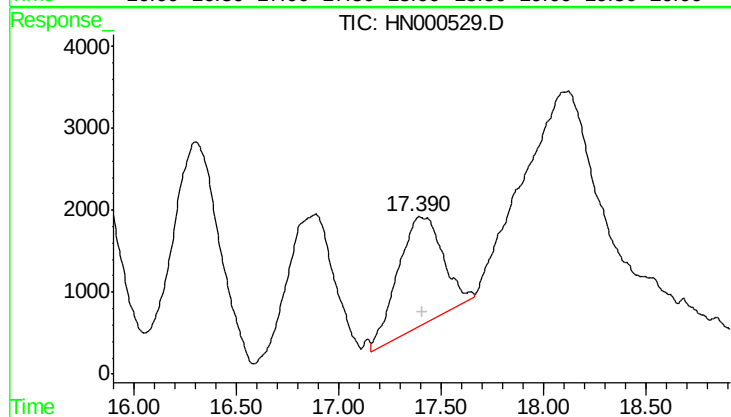

#15 4-Nitrotoluene

R.T.: 17.390 min
Delta R.T.: -0.015 min
Response: 202539
Conc: 13.44 ug/L m

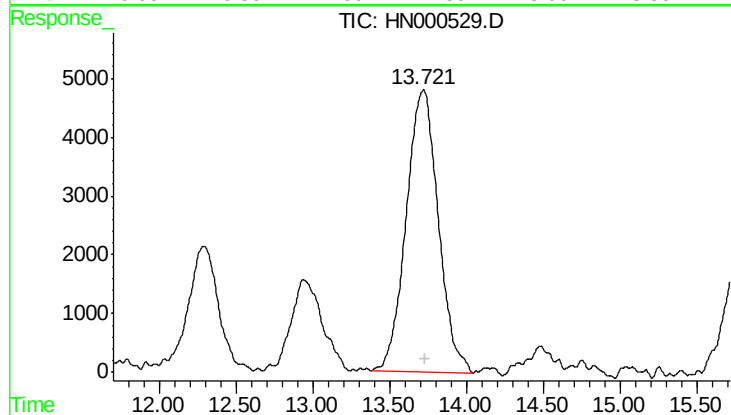

#16 3,5-Dinitroaniline

R.T.: 13.720 min
Delta R.T.: -0.009 min
Response: 695564
Conc: 19.68 ug/L