

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN120315\
 Data File : HN007614.D
 Signal(s) : vwd1A.ch
 Acq On : 03-Dec-2015, 18:33
 Operator : UM/MA
 Sample : G4254-01DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 03 19:08:47 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN120315.M
 Quant Title :
 QLast Update : Thu Dec 03 17:29:35 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	1.325	182188	49.566 ug/L
Target Compounds				
2) T	HMX	0.890	857024	197.155 ug/L
3) T	RDX	1.698	2063681	379.834 ug/L
4) T	1,3,5-Trinitrobenzene	2.624	5815181	508.657 ug/L
5) T	1,3-Dinitrobenzene	3.491	2208349	132.179 ng/ml
7) T	Nitrobenzene	4.661	3354175	336.337 ug/L
9) T	2,4,6-Trinitrotoluene	6.399	3429232	299.691 ug/L
10) T	2-Amino-4,6-dinitroto...	6.963	1468148	133.226 ug/L
11) T	4-Amino-2,6-dinitroto...	7.314	4818913	655.660 ug/L
13) T	2,6-Dinitrotoluene	8.411	2294416	258.327 ug/L
14) T	2-Nitrotoluene	11.535	1082831	163.317 ug/L
15) T	4-Nitrotoluene	12.247	1481342	280.132 ug/L
16) T	3-Nitrotoluene	13.502	3707423	540.314 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN120315\
Data File : HN007614.D
Signal(s) : vwd1A.ch
Acq On : 03-Dec-2015, 18:33
Operator : UM/MA
Sample : G4254-01DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 03 19:08:47 2015
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN120315.M
Quant Title :
QLast Update : Thu Dec 03 17:29:35 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

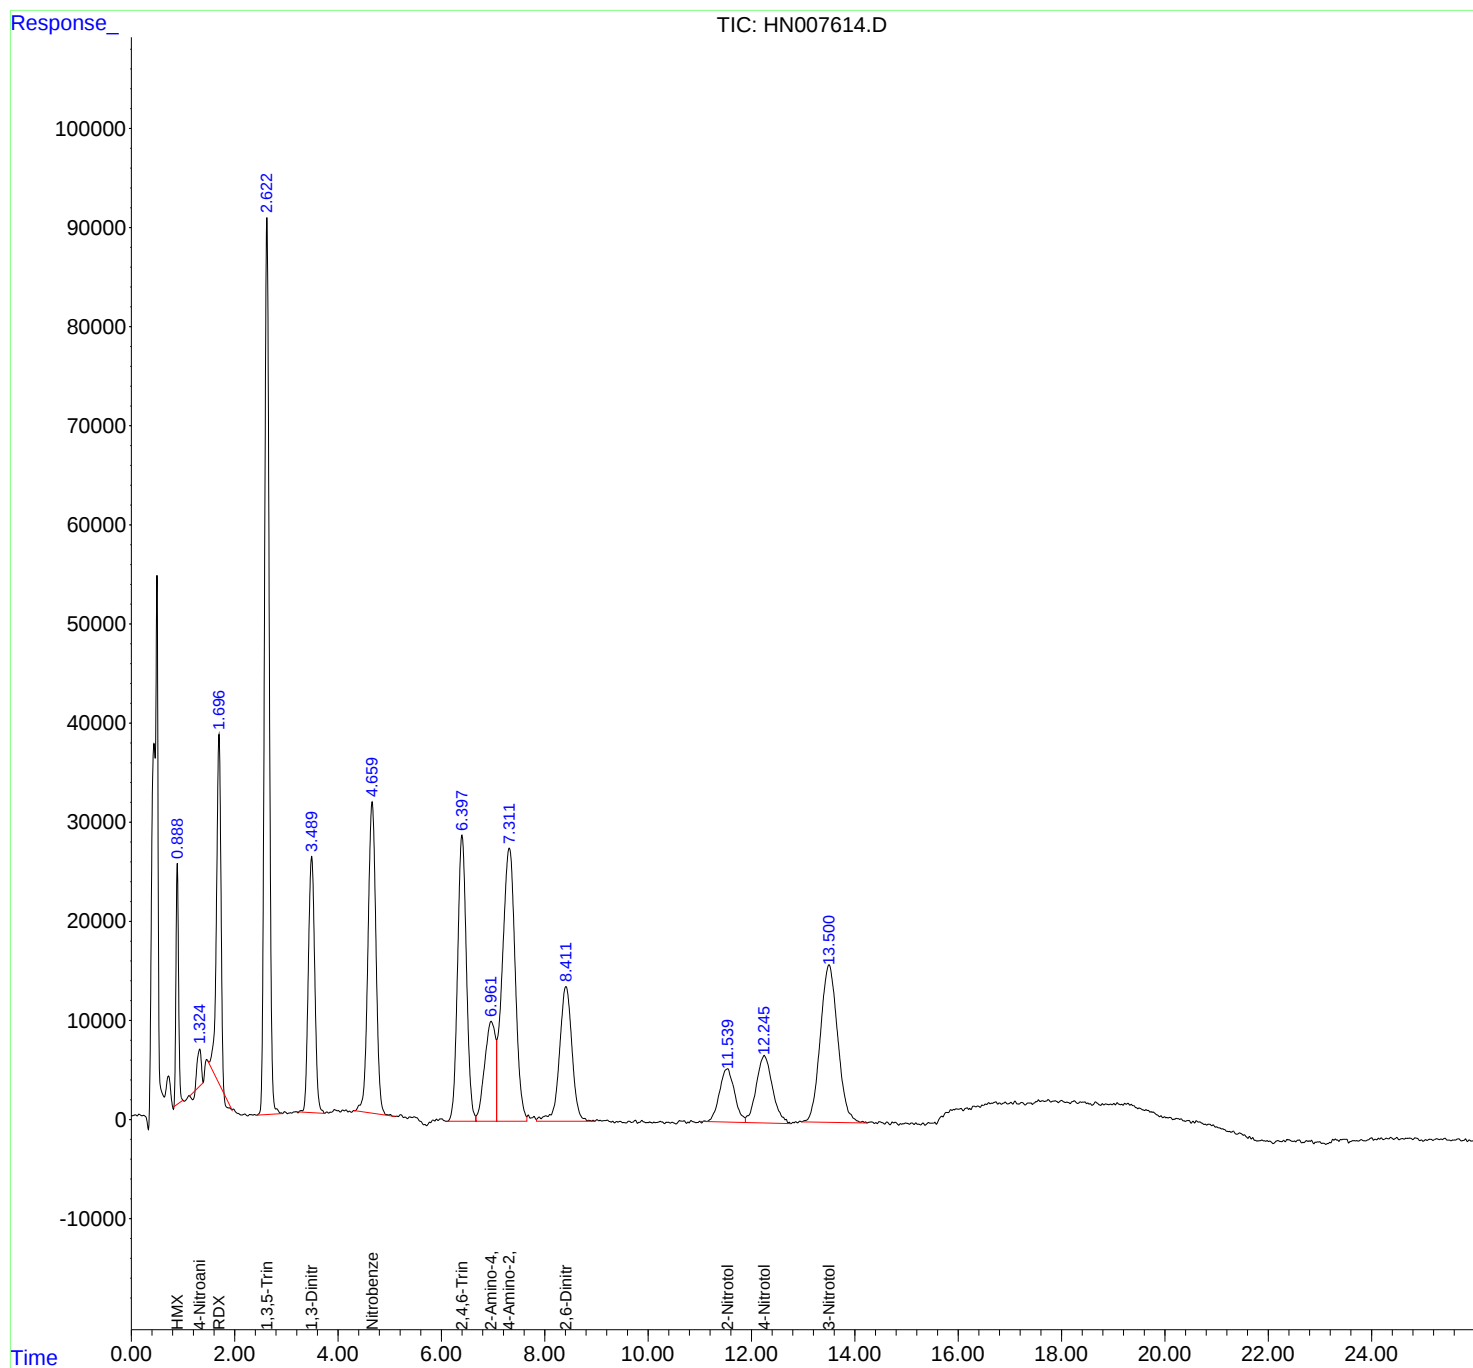


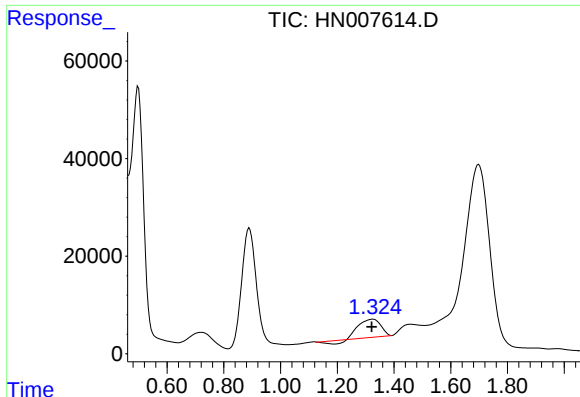

#1 4-Nitroaniline


R.T.: 1.325 min
Delta R.T.: 0.003 min
Response: 182188
Conc: 49.57 ug/L

Instrument :
HPLC_N
ClientSampleId :

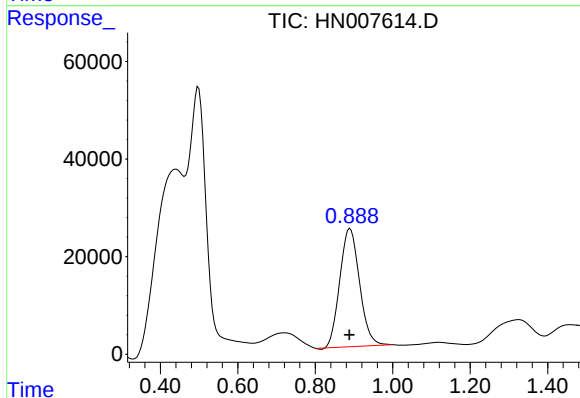


#2 HMX

R.T.: 0.890 min
Delta R.T.: 0.002 min
Response: 857024
Conc: 197.15 ug/L

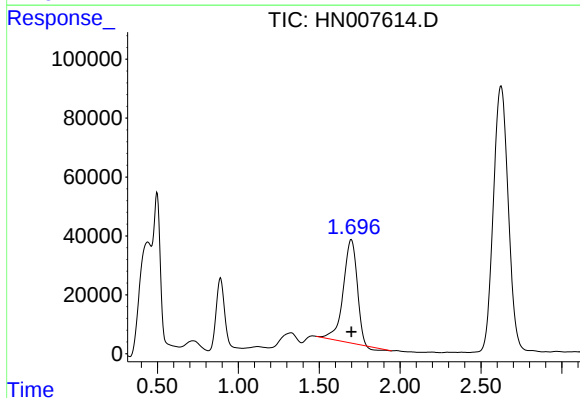


#3 RDX

R.T.: 1.698 min
Delta R.T.: 0.000 min
Response: 2063681
Conc: 379.83 ug/L

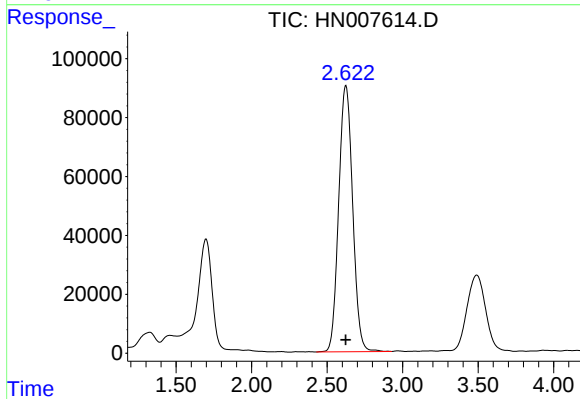

#4 1,3,5-Trinitrobenzene


R.T.: 2.624 min
Delta R.T.: 0.001 min
Response: 5815181
Conc: 508.66 ug/L

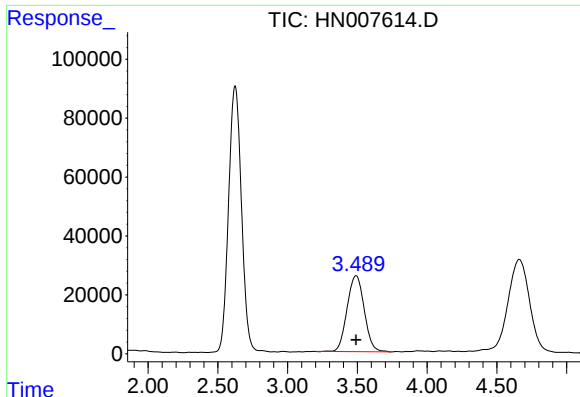

#5 1,3-Dinitrobenzene


R.T.: 3.491 min
Delta R.T.: 0.000 min
Response: 2208349
Conc: 132.18 ng/ml

Instrument :
HPLC_N
ClientSampleId :

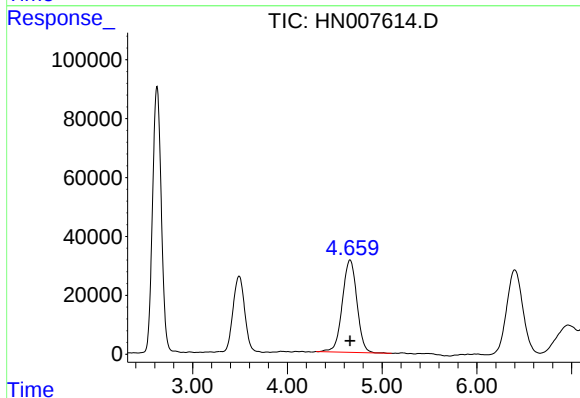


#7 Nitrobenzene

R.T.: 4.661 min
Delta R.T.: -0.002 min
Response: 3354175
Conc: 336.34 ug/L

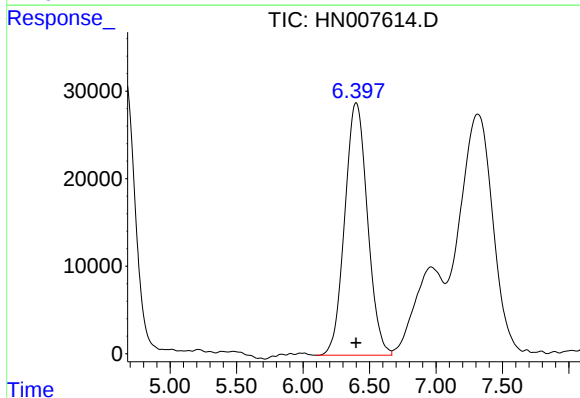


#9 2,4,6-Trinitrotoluene

R.T.: 6.399 min
Delta R.T.: 0.000 min
Response: 3429232
Conc: 299.69 ug/L

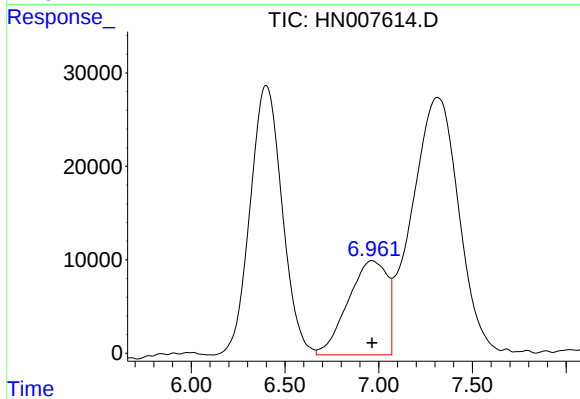

#10 2-Amino-4,6-dinitrotoluene


R.T.: 6.963 min
Delta R.T.: -0.001 min
Response: 1468148
Conc: 133.23 ug/L

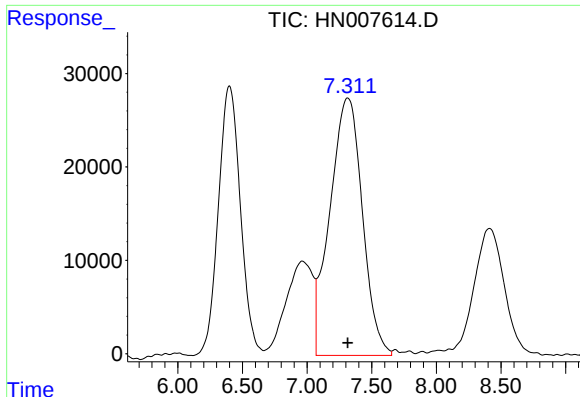

#11 4-Amino-2,6-dinitrotoluene


R.T.: 7.314 min
Delta R.T.: 0.000 min
Response: 4818913
Conc: 655.66 ug/L

Instrument :
HPLC_N
ClientSampleId :

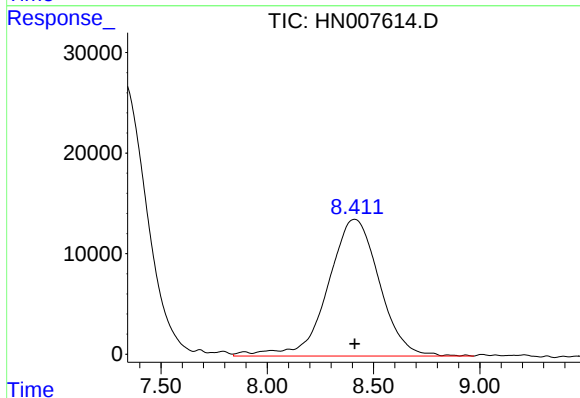


#13 2,6-Dinitrotoluene

R.T.: 8.411 min
Delta R.T.: 0.000 min
Response: 2294416
Conc: 258.33 ug/L

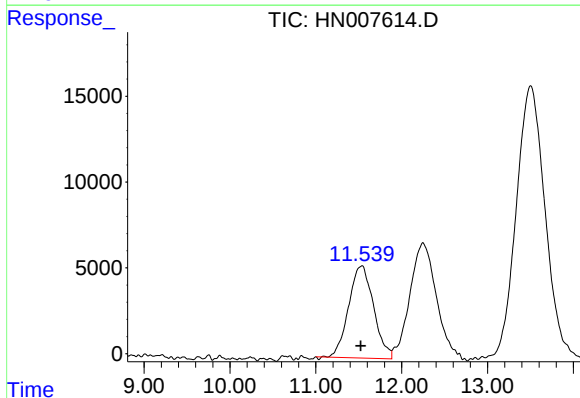


#14 2-Nitrotoluene

R.T.: 11.535 min
Delta R.T.: 0.011 min
Response: 1082831
Conc: 163.32 ug/L

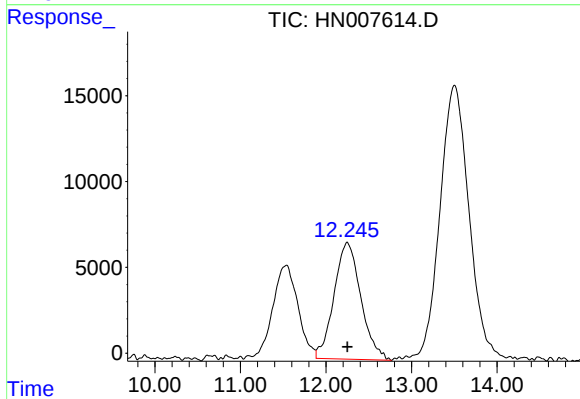

#15 4-Nitrotoluene

R.T.: 12.247 min
Delta R.T.: -0.002 min
Response: 1481342
Conc: 280.13 ug/L

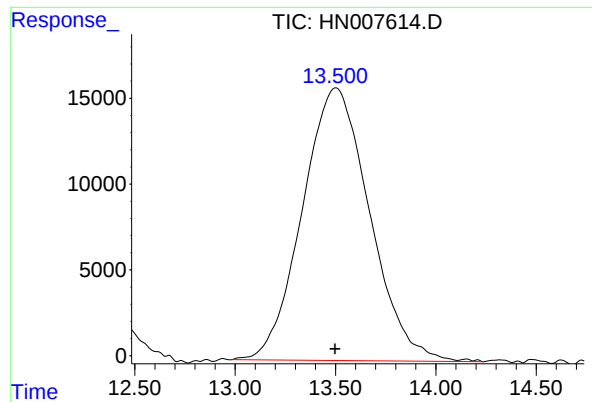

#16 3-Nitrotoluene

R.T.: 13.502 min
Delta R.T.: 0.003 min
Response: 3707423
Conc: 540.31 ug/L

Instrument :
HPLC_N
ClientSampleId :