

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN120315\
 Data File : HN007604.D
 Signal(s) : vwd1A.ch
 Acq On : 03-Dec-2015, 13:53
 Operator : UM/MA
 Sample : SSTDICC2000
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 SSTDICC2000

Integration File: autoint1.e
 Quant Time: Dec 03 16:11:14 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN120315.M
 Quant Title :
 QLast Update : Thu Dec 03 15:18:43 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.322	7235991	1883.745 ug/L
Target Compounds			
2) T HMX	0.888	8983969	1826.464 ug/L
3) T RDX	1.699	11324516	1996.203 ug/L
4) T 1,3,5-Trinitrobenzene	2.623	23657918	2012.526 ug/L
5) T 1,3-Dinitrobenzene	3.490	34579747	2041.651 ng/ml
6) T 3,5-Dinitroaniline	3.871	25175952	2045.980 ug/L
7) T Nitrobenzene	4.663	20319644	2003.711 ug/L
8) T Tetryl	6.158	13850072	1871.599 ug/L
9) T 2,4,6-Trinitrotoluene	6.400	24369049	2023.990 ug/L
10) T 2-Amino-4,6-dinitroto...	6.966	23216794	2058.340 ug/L
11) T 4-Amino-2,6-dinitroto...	7.315	14594861	2050.077 ug/L
12) T 2,4-Dinitrotoluene	8.015	31346504	2049.064 ug/L
13) T 2,6-Dinitrotoluene	8.413	17583918	2024.701 ug/L
14) T 2-Nitrotoluene	11.526	13196618	2064.177 ug/L
15) T 4-Nitrotoluene	12.250	10806413	2008.871 ug/L
16) T 3-Nitrotoluene	13.501	13725360	2006.820 ug/L
17) T PETN	18.467	20458863	2621.249 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN120315\
Data File : HN007604.D
Signal(s) : vwd1A.ch
Acq On : 03-Dec-2015, 13:53
Operator : UM/MA
Sample : SSTDICC2000
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
SSTDICC2000

Integration File: autoint1.e
Quant Time: Dec 03 16:11:14 2015
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN120315.M
Quant Title :
QLast Update : Thu Dec 03 15:18:43 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

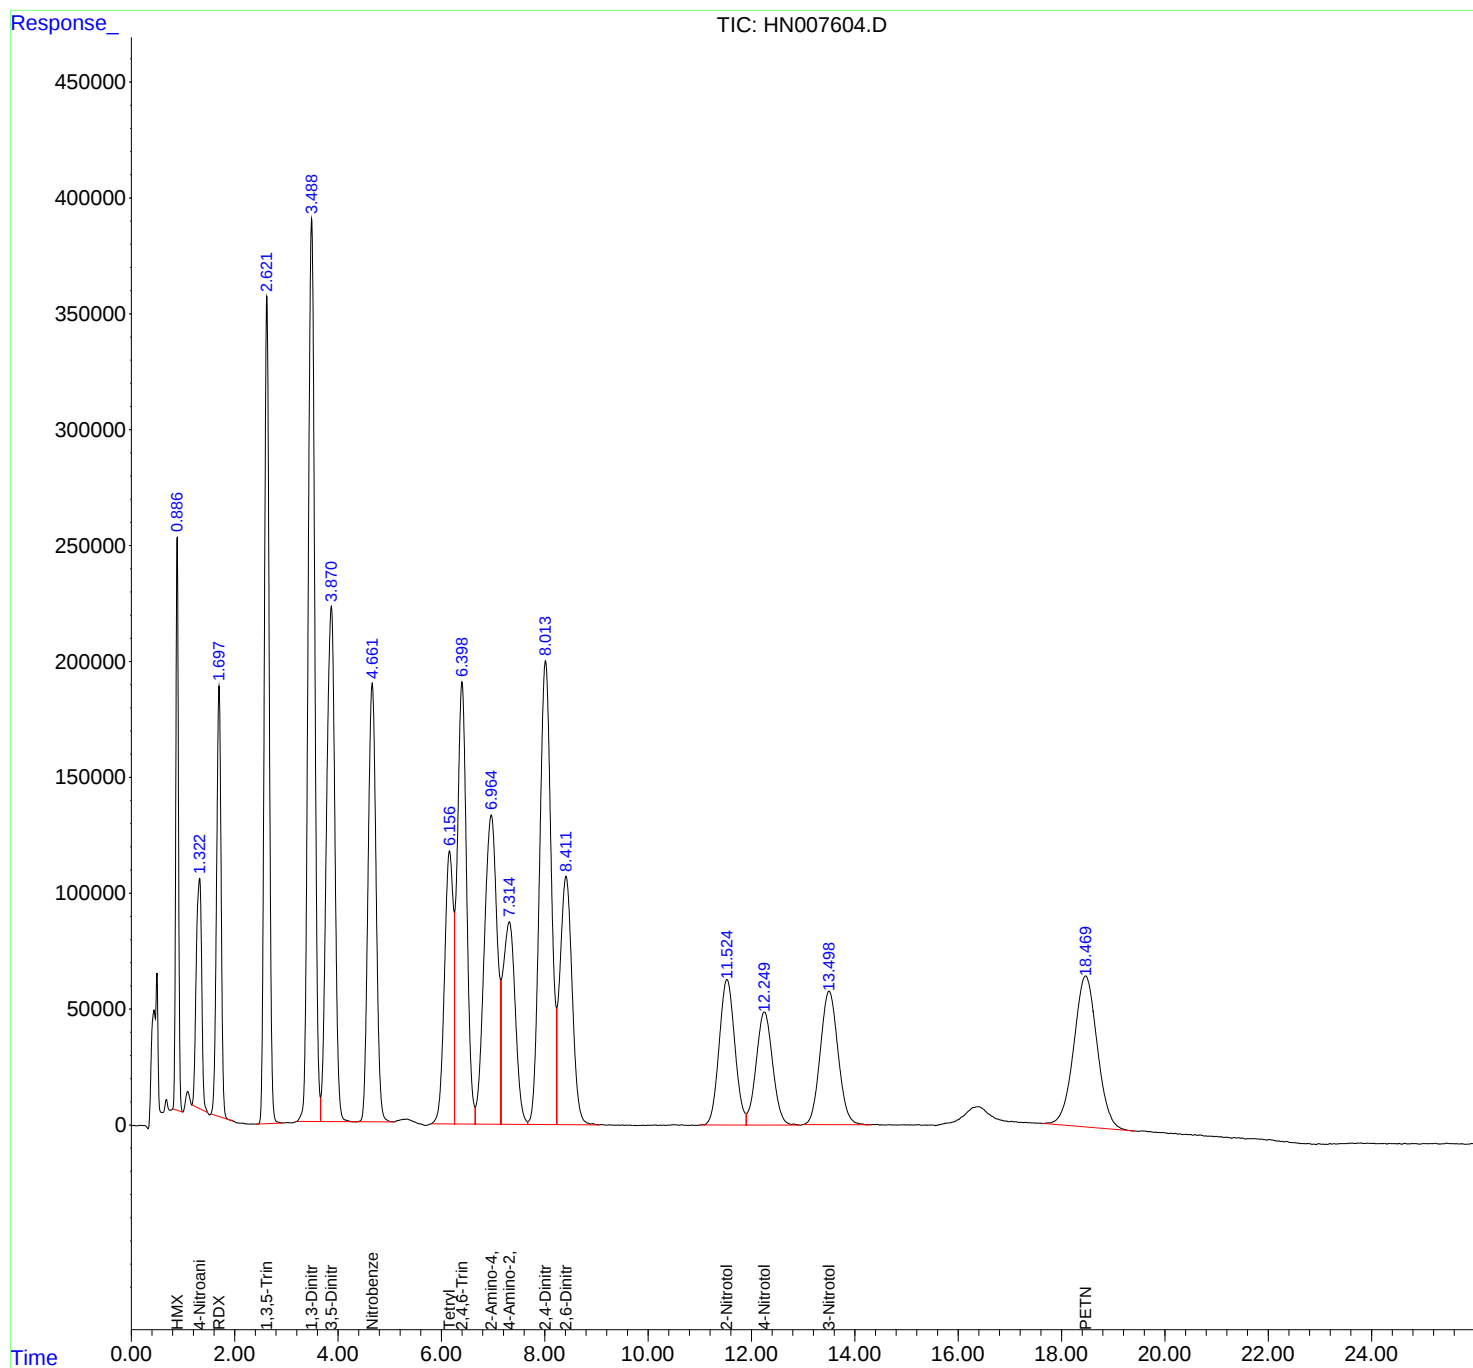


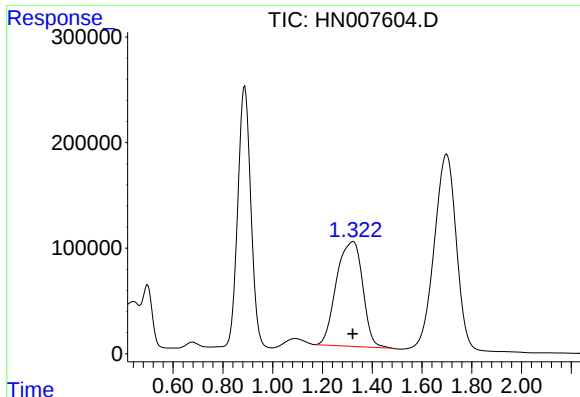

#1 4-Nitroaniline


R.T.: 1.322 min
Delta R.T.: 0.000 min
Response: 7235991
Conc: 1883.74 ug/L

Instrument :
HPLC_N
ClientSampleId :
SSTDICC2000

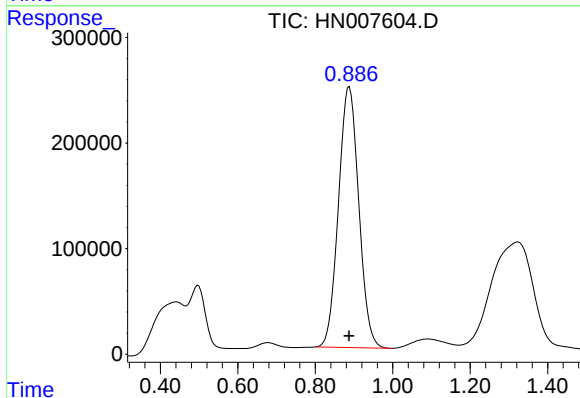


#2 HMX

R.T.: 0.888 min
Delta R.T.: 0.000 min
Response: 8983969
Conc: 1826.46 ug/L

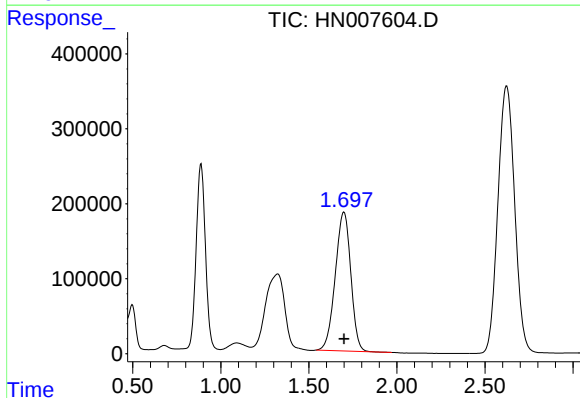


#3 RDX

R.T.: 1.699 min
Delta R.T.: 0.000 min
Response: 11324516
Conc: 1996.20 ug/L

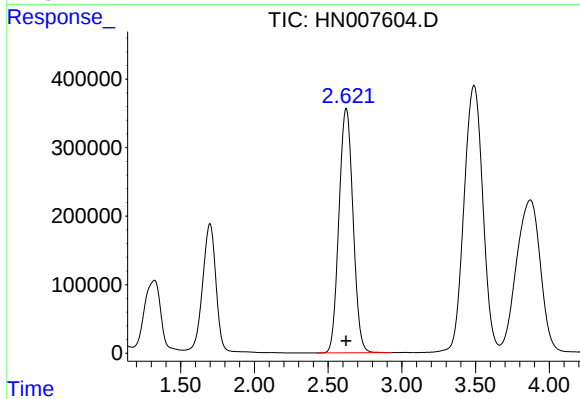

#4 1,3,5-Trinitrobenzene


R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 23657918
Conc: 2012.53 ug/L

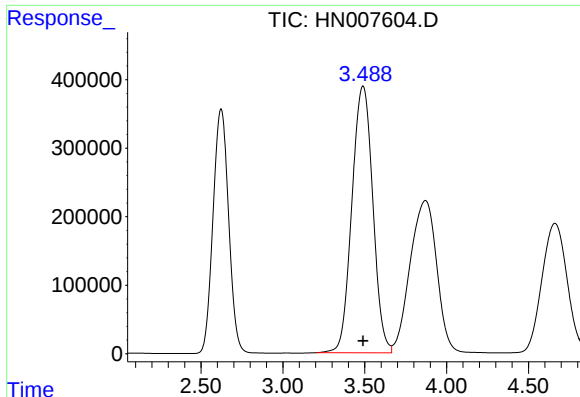

#5 1,3-Dinitrobenzene


R.T.: 3.490 min
Delta R.T.: 0.000 min
Response: 34579747
Conc: 2041.65 ng/ml

Instrument :
HPLC_N
ClientSampleId :
SSTDICC2000

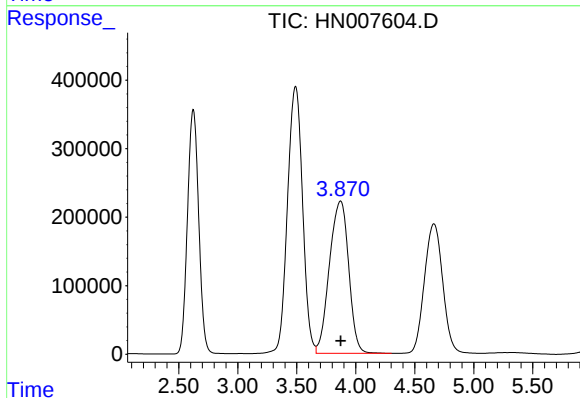


#6 3,5-Dinitroaniline

R.T.: 3.871 min
Delta R.T.: 0.000 min
Response: 25175952
Conc: 2045.98 ug/L

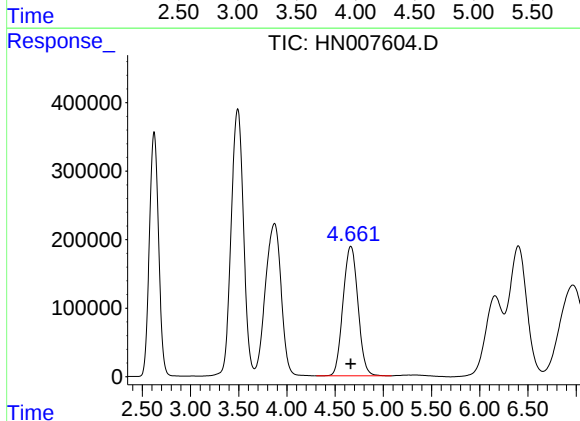


#7 Nitrobenzene

R.T.: 4.663 min
Delta R.T.: 0.000 min
Response: 20319644
Conc: 2003.71 ug/L

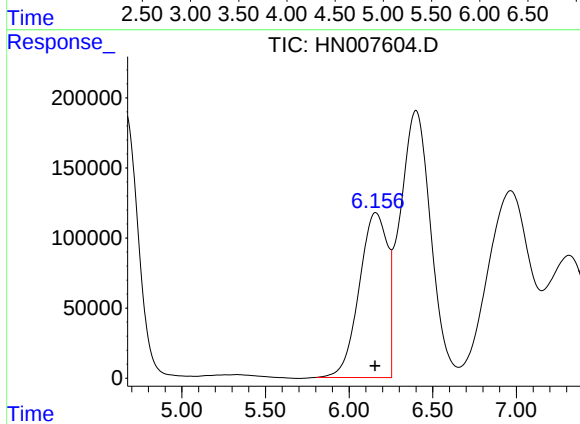

#8 Tetryl


R.T.: 6.158 min
Delta R.T.: 0.002 min
Response: 13850072
Conc: 1871.60 ug/L

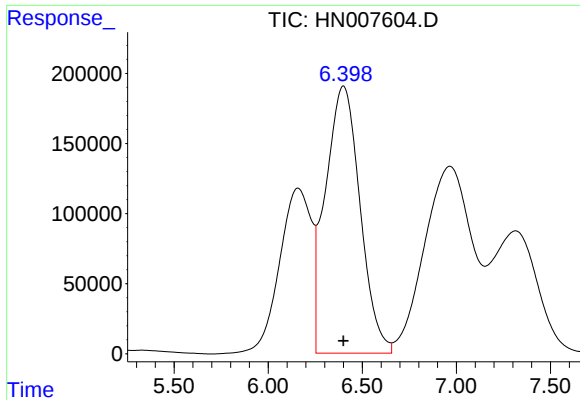

#9 2,4,6-Trinitrotoluene


R.T.: 6.400 min
Delta R.T.: 0.000 min
Response: 24369049
Conc: 2023.99 ug/L

Instrument :
HPLC_N
ClientSampleId :
SSTDICC2000

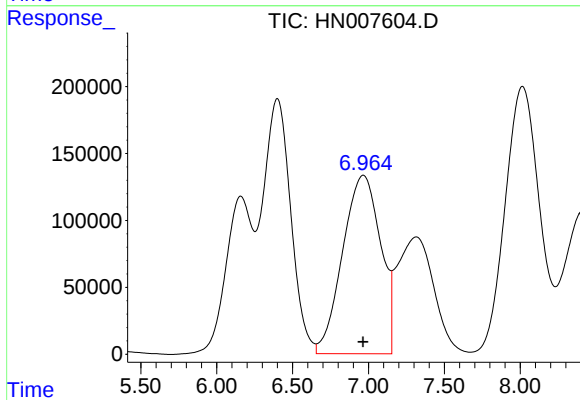


#10 2-Amino-4,6-dinitrotoluene

R.T.: 6.966 min
Delta R.T.: 0.001 min
Response: 23216794
Conc: 2058.34 ug/L

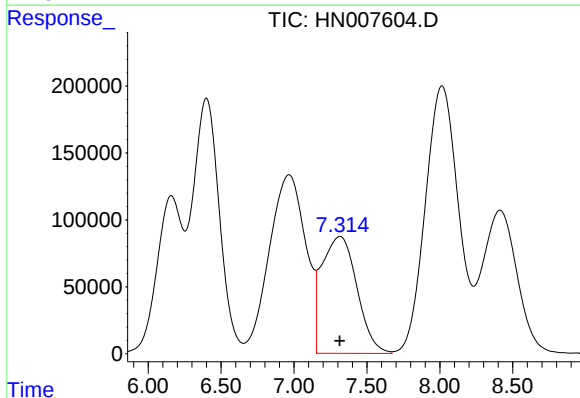


#11 4-Amino-2,6-dinitrotoluene

R.T.: 7.315 min
Delta R.T.: 0.000 min
Response: 14594861
Conc: 2050.08 ug/L

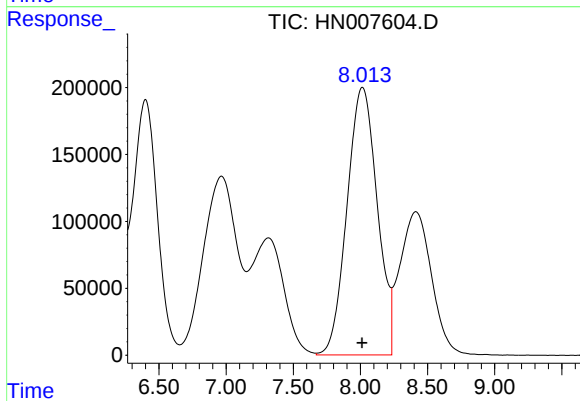

#12 2,4-Dinitrotoluene

R.T.: 8.015 min
Delta R.T.: 0.002 min
Response: 31346504
Conc: 2049.06 ug/L

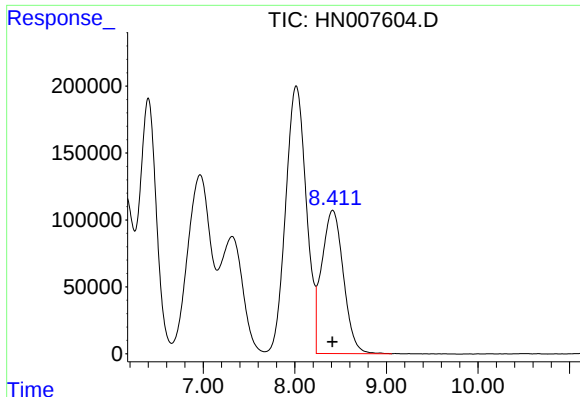

#13 2,6-Dinitrotoluene


R.T.: 8.413 min

Delta R.T.: 0.002 min

Response: 17583918

Conc: 2024.70 ug/L

Instrument :
HPLC_N
ClientSampleId :
SSTDICC2000

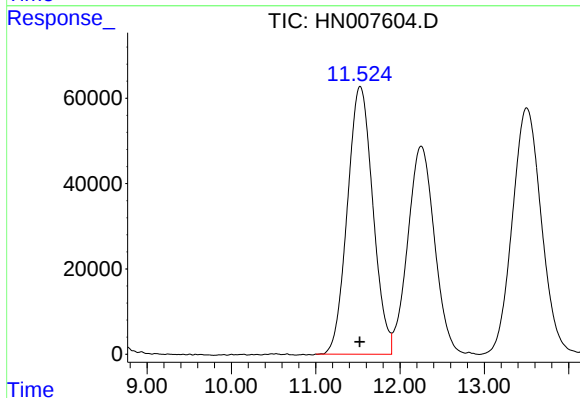


#14 2-Nitrotoluene

R.T.: 11.526 min

Delta R.T.: 0.002 min

Response: 13196618

Conc: 2064.18 ug/L

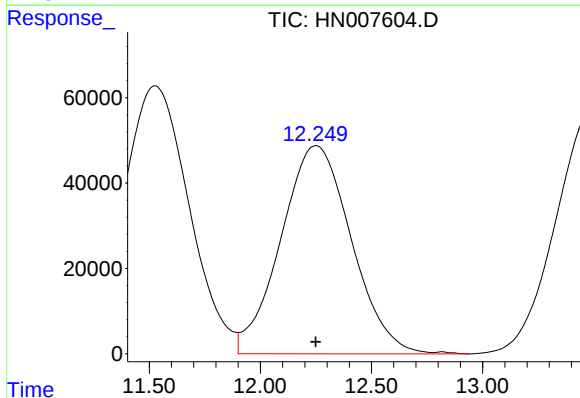


#15 4-Nitrotoluene

R.T.: 12.250 min

Delta R.T.: 0.001 min

Response: 10806413

Conc: 2008.87 ug/L

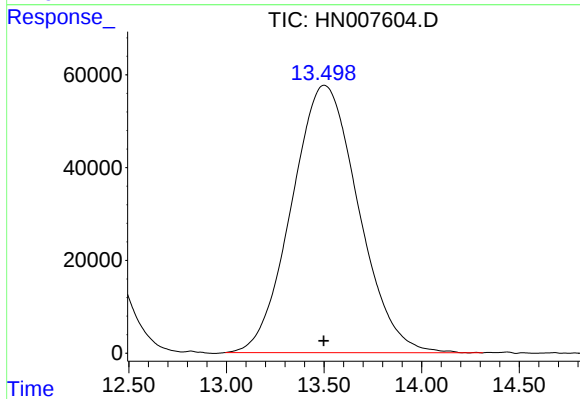


#16 3-Nitrotoluene

R.T.: 13.501 min

Delta R.T.: 0.003 min

Response: 13725360

Conc: 2006.82 ug/L

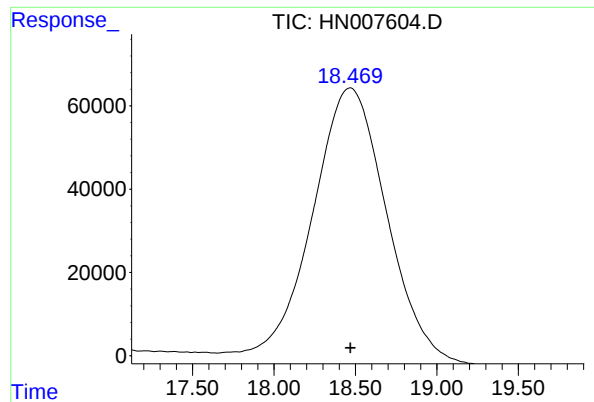

#17 PETN

R.T.: 18.467 min
Delta R.T.: -0.002 min
Response: 20458863
Conc: 2621.25 ug/L

Instrument :
HPLC_N
ClientSampleId :
SSTDICC2000