

Data Path : S:\HPCHEM1\HPLC_N\Data\HN112012\
 Data File : HN000589.D
 Signal(s) : VWD1A.CH
 Acq On : 20-Nov-2012, 11:55
 Operator : HLM
 Sample : 8330-6
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 HPLC_N
 LabSampleId :
 8330-6

Integration File: events.e
 Quant Time: Nov 22 03:08:58 2012
 Quant Method : S:\HPCHEM1\HPLC_N\Method\HN112012.M
 Quant Title : SW8330 / 8330A confirmation
 QLast Update : Wed Nov 21 16:37:45 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc	Units

System Monitoring Compounds				
1) S 4-Nitroaniline	7.561	49904766	4949.606	ug/L
Target Compounds				
2) T HMX	12.714	50945190	5051.469	ug/L
3) T RDX	10.589	68339279	4956.098	ug/L
4) T 1,3,5-Trinitrobenzene	24.341	70369486	2519.155	ug/L
5) T Tetryl	34.338	106470646	4936.248	ug/L
6) T 2,4,6-Trinitrotoluene	32.613	66381970	2449.944	ug/L
7) T 2-Amino-4,6-dinitroto...	15.915	117492608	2463.657	ug/L
8) T 4-Amino-2,6-dinitroto...	15.915	117492608	2449.319	ug/L
9) T 2,4-Dinitrotoluene	21.376	94578149	2461.925	ug/L
10) T 2,6-Dinitrotoluene	19.975	49109225	2416.939	ug/L
11) T 1,3-Dinitrobenzene	15.506	101165944	2394.425	ug/L
12) T Nitrobenzene	12.086	66027504	2519.257	ug/L
13) T 2-Nitrotoluene	16.490	84502409	4999.695	ug/L
14) T 3-Nitrotoluene	17.697	90043063	4968.562	ug/L
15) T 4-Nitrotoluene	17.010	70948909	5088.822	ug/L
16) T 3,5-Dinitroaniline	13.436	165023590	4943.850	ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_N\Data\HN112012\
Data File : HN000589.D
Signal(s) : VWD1A.CH
Acq On : 20-Nov-2012, 11:55
Operator : HLM
Sample : 8330-6
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_N
LabSampleId :
8330-6

Integration File: events.e
Quant Time: Nov 22 03:08:58 2012
Quant Method : S:\HPCHEM1\HPLC_N\Method\HN112012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Wed Nov 21 16:37:45 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

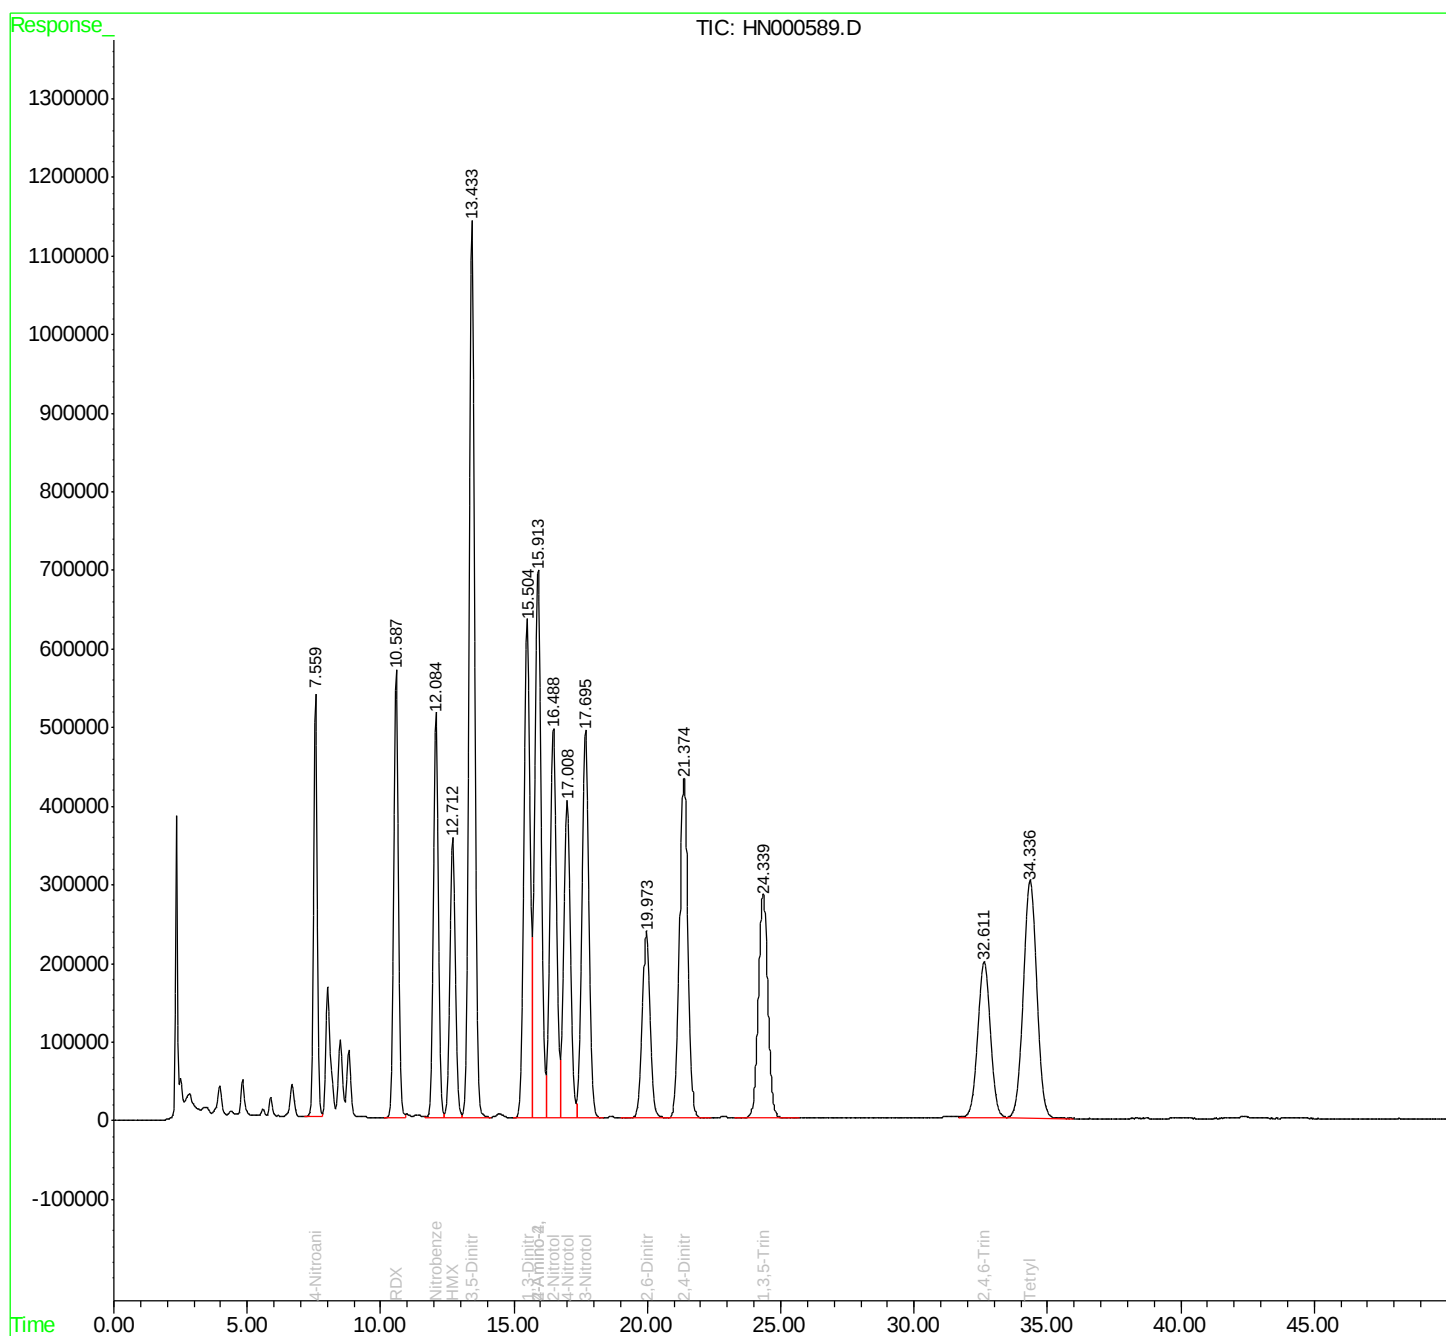


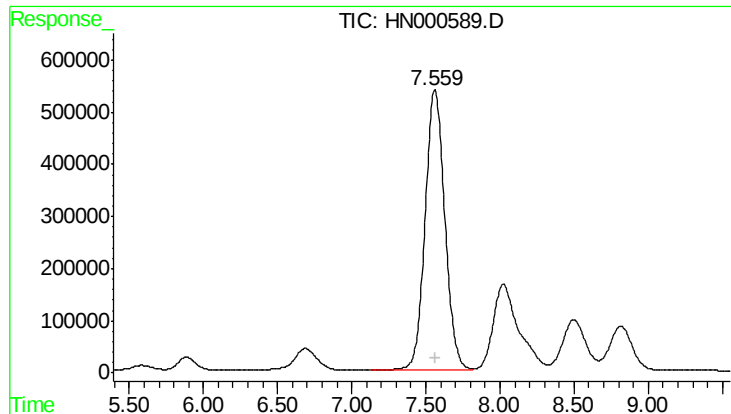

#1 4-Nitroaniline


R.T.: 7.561 min
Delta R.T.: -0.004 min
Response: 49904766
Conc: 4949.61 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-6

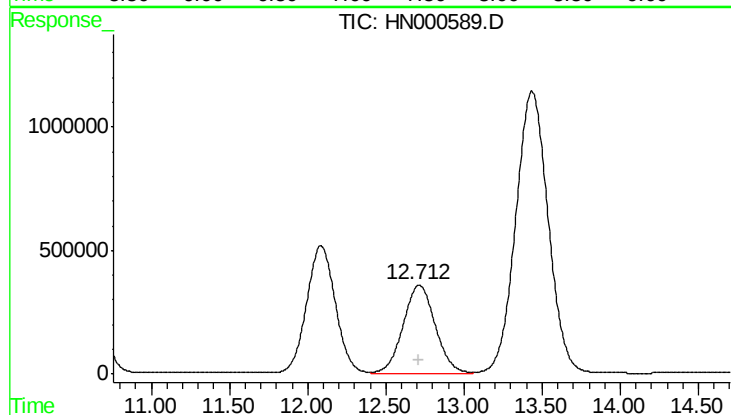


#2 HMX

R.T.: 12.714 min
Delta R.T.: 0.000 min
Response: 50945190
Conc: 5051.47 ug/L

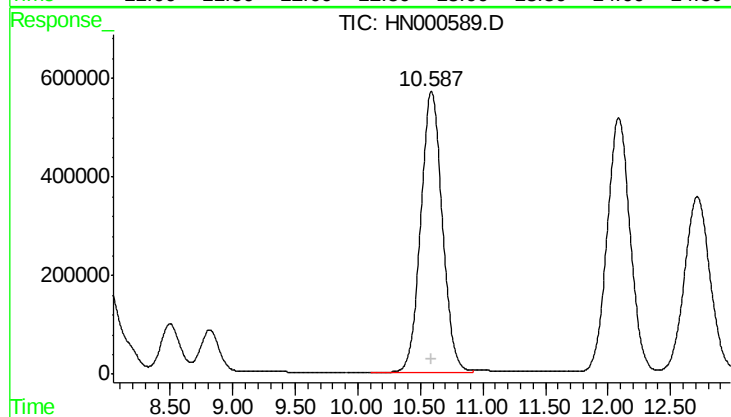


#3 RDX

R.T.: 10.589 min
Delta R.T.: -0.004 min
Response: 68339279
Conc: 4956.10 ug/L

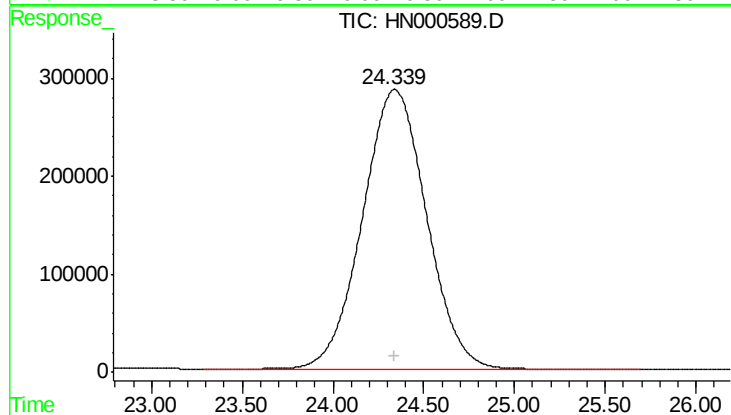

#4 1,3,5-Trinitrobenzene


R.T.: 24.341 min
Delta R.T.: 0.000 min
Response: 70369486
Conc: 2519.15 ug/L

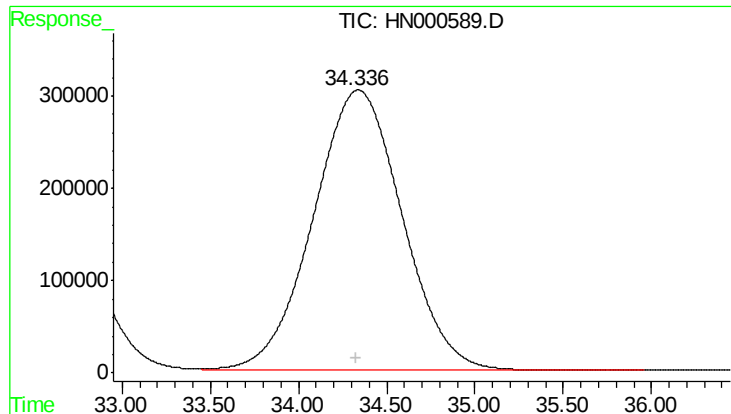

#5 Tetryl


R.T.: 34.338 min
Delta R.T.: 0.016 min
Response: 106470646
Conc: 4936.25 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-6

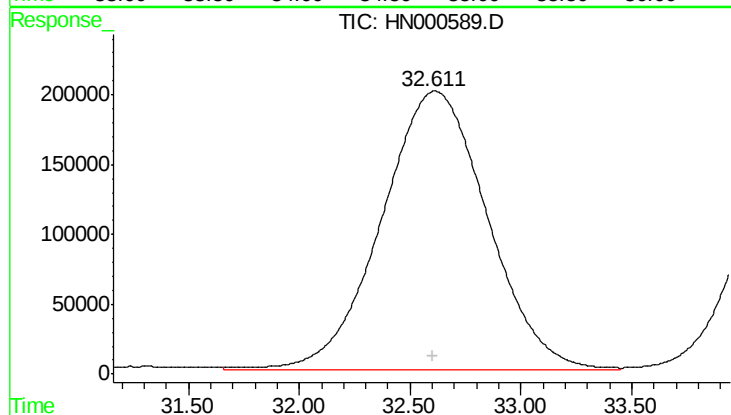


#6 2,4,6-Trinitrotoluene

R.T.: 32.613 min
Delta R.T.: 0.010 min
Response: 66381970
Conc: 2449.94 ug/L

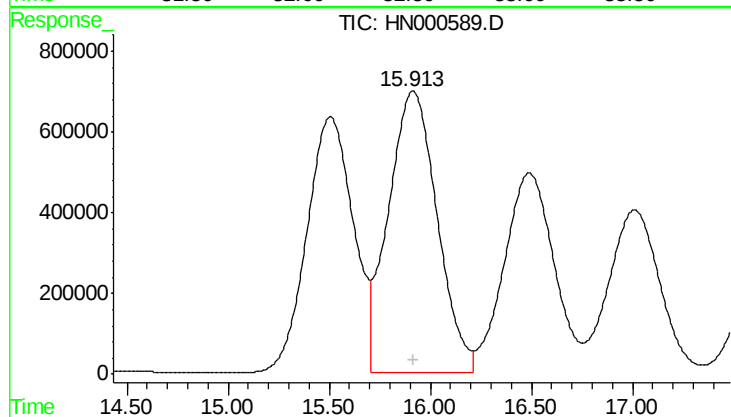


#7 2-Amino-4,6-dinitrotoluene

R.T.: 15.915 min
Delta R.T.: -0.006 min
Response: 117492608
Conc: 2463.66 ug/L

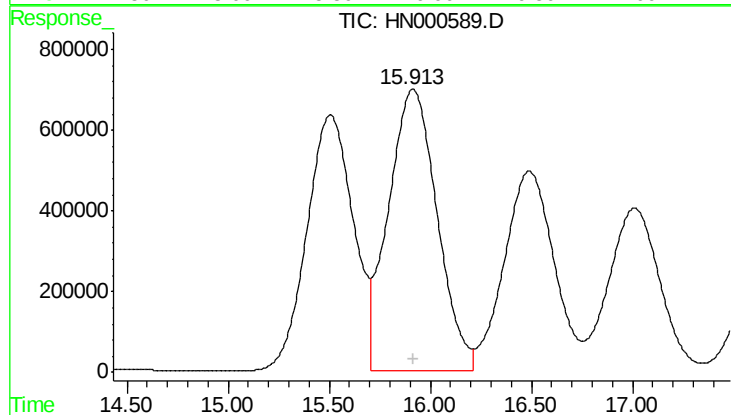

#8 4-Amino-2,6-dinitrotoluene


R.T.: 15.915 min
Delta R.T.: -0.006 min
Response: 117492608
Conc: 2449.32 ug/L

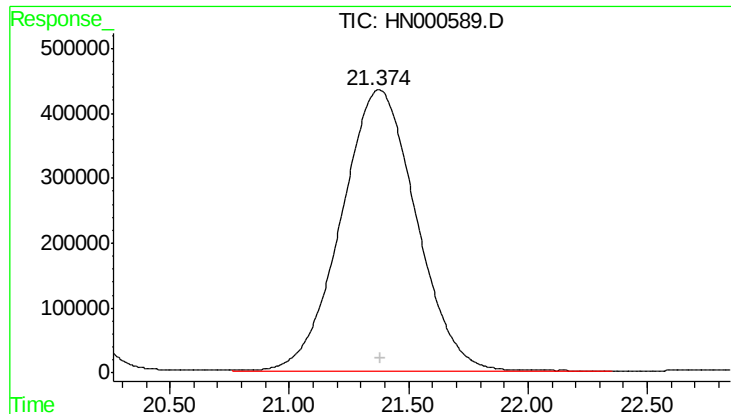

#9 2,4-Dinitrotoluene


R.T.: 21.376 min
Delta R.T.: -0.007 min
Response: 94578149
Conc: 2461.92 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-6

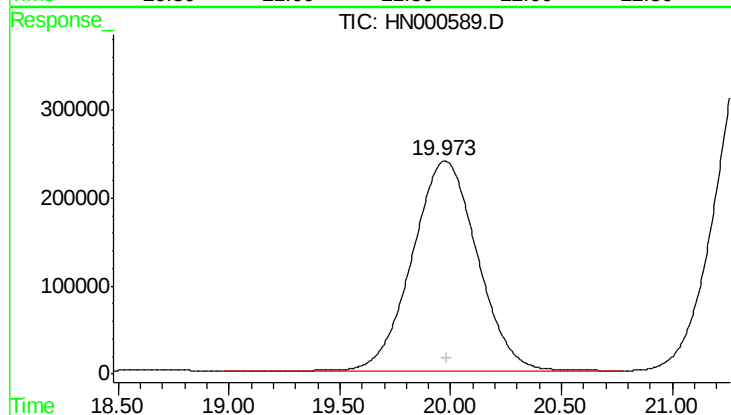


#10 2,6-Dinitrotoluene

R.T.: 19.975 min
Delta R.T.: -0.006 min
Response: 49109225
Conc: 2416.94 ug/L

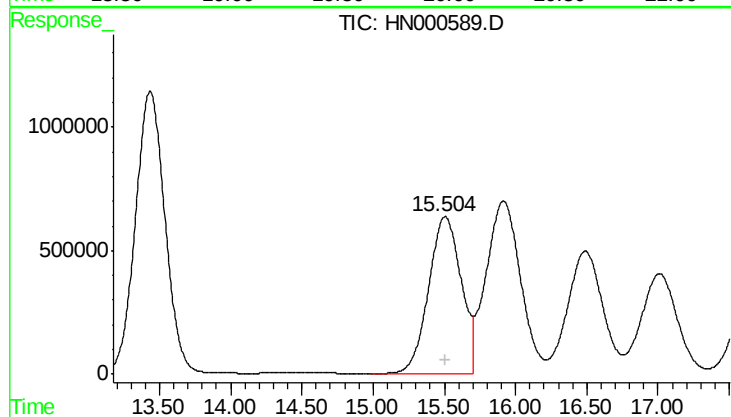


#11 1,3-Dinitrobenzene

R.T.: 15.506 min
Delta R.T.: -0.006 min
Response: 101165944
Conc: 2394.43 ug/L

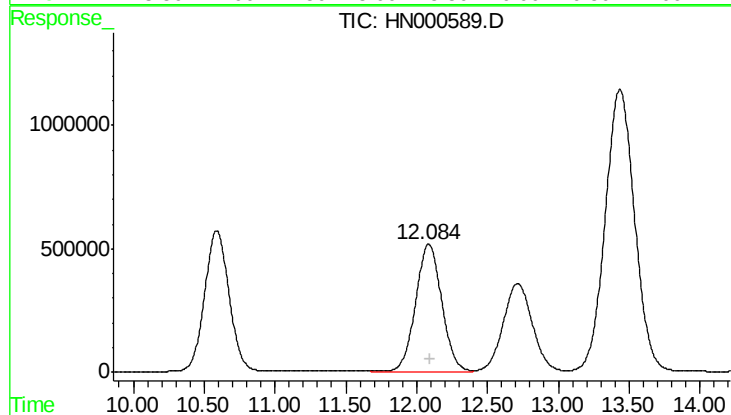

#12 Nitrobenzene


R.T.: 12.086 min
Delta R.T.: -0.006 min
Response: 66027504
Conc: 2519.26 ug/L

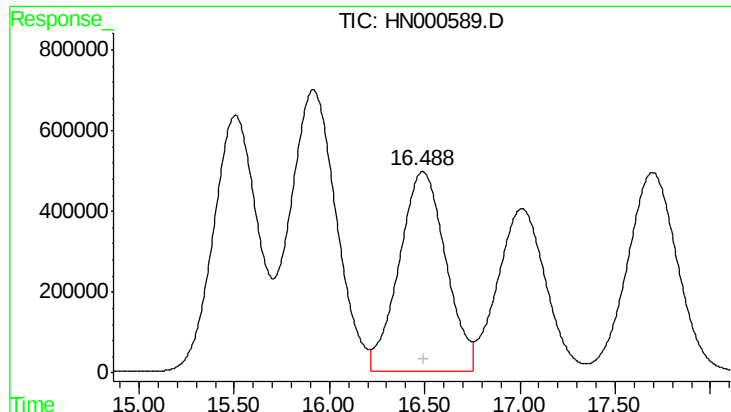

#13 2-Nitrotoluene


R.T.: 16.490 min
 Delta R.T.: -0.007 min
 Response: 84502409
 Conc: 4999.69 ug/L

Instrument :
 HPLC_N
 LabSampleId :
 8330-6

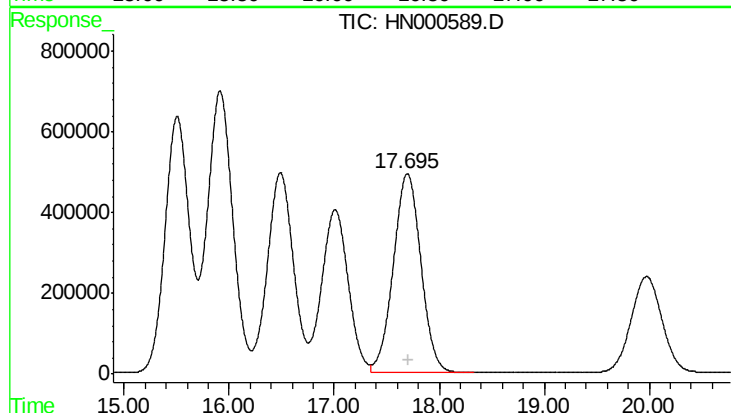


#14 3-Nitrotoluene

R.T.: 17.697 min
 Delta R.T.: -0.008 min
 Response: 90043063
 Conc: 4968.56 ug/L

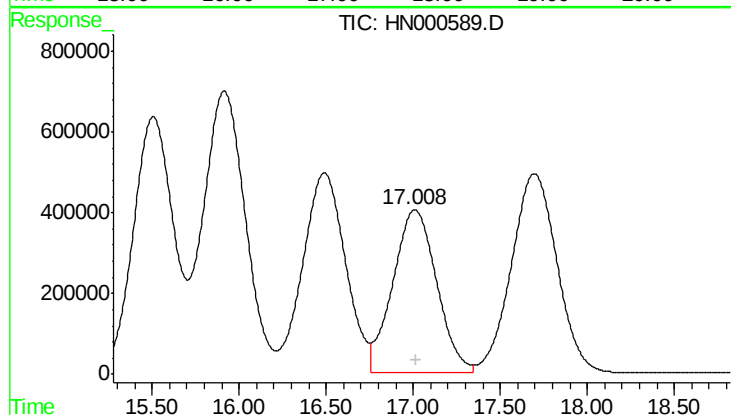

#15 4-Nitrotoluene

R.T.: 17.010 min
 Delta R.T.: -0.008 min
 Response: 70948909
 Conc: 5088.82 ug/L

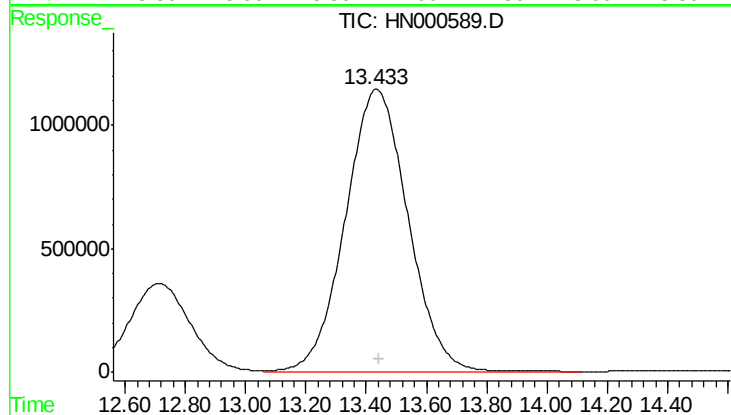

#16 3,5-Dinitroaniline

R.T.: 13.436 min
 Delta R.T.: -0.005 min
 Response: 165023590
 Conc: 4943.85 ug/L