

Data Path : S:\HPCHEM1\HPLC_N\Data\HN112012\
 Data File : HN000592.D
 Signal(s) : VWD1A.CH
 Acq On : 20-Nov-2012, 14:33
 Operator : HLM
 Sample : 8330-4
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 HPLC_N
 LabSampleId :
 8330-4

Integration File: events.e
 Quant Time: Nov 22 03:09:19 2012
 Quant Method : S:\HPCHEM1\HPLC_N\Method\HN112012.M
 Quant Title : SW8330 / 8330A confirmation
 QLast Update : Wed Nov 21 16:37:45 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	7.566	10025294	994.319 ug/L
Target Compounds			
2) T HMX	12.714	10269095	1018.232 ug/L
3) T RDX	10.594	13642351	989.370 ug/L
4) T 1,3,5-Trinitrobenzene	24.341	14131801	505.904 ug/L
5) T Tetryl	34.322	21570366	1000.057 ug/L
6) T 2,4,6-Trinitrotoluene	32.603	13208764	487.493 ug/L
7) T 2-Amino-4,6-dinitroto...	15.920	23815804	499.384 ug/L
8) T 4-Amino-2,6-dinitroto...	15.920	23815804	496.478 ug/L
9) T 2,4-Dinitrotoluene	21.383	19080054	496.665 ug/L
10) T 2,6-Dinitrotoluene	19.981	9820071	483.301 ug/L
11) T 1,3-Dinitrobenzene	15.512	20381715	482.400 ug/L
12) T Nitrobenzene	12.092	13267040	506.199 ug/L
13) T 2-Nitrotoluene	16.497	17077568	1010.416 ug/L
14) T 3-Nitrotoluene	17.705	18254137	1007.260 ug/L
15) T 4-Nitrotoluene	17.018	14387892	1031.974 ug/L
16) T 3,5-Dinitroaniline	13.441	33319338	998.195 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_N\Data\HN112012\
Data File : HN000592.D
Signal(s) : VWD1A.CH
Acq On : 20-Nov-2012, 14:33
Operator : HLM
Sample : 8330-4
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
HPLC_N
LabSampleId :
8330-4

Integration File: events.e
Quant Time: Nov 22 03:09:19 2012
Quant Method : S:\HPCHEM1\HPLC_N\Method\HN112012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Wed Nov 21 16:37:45 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

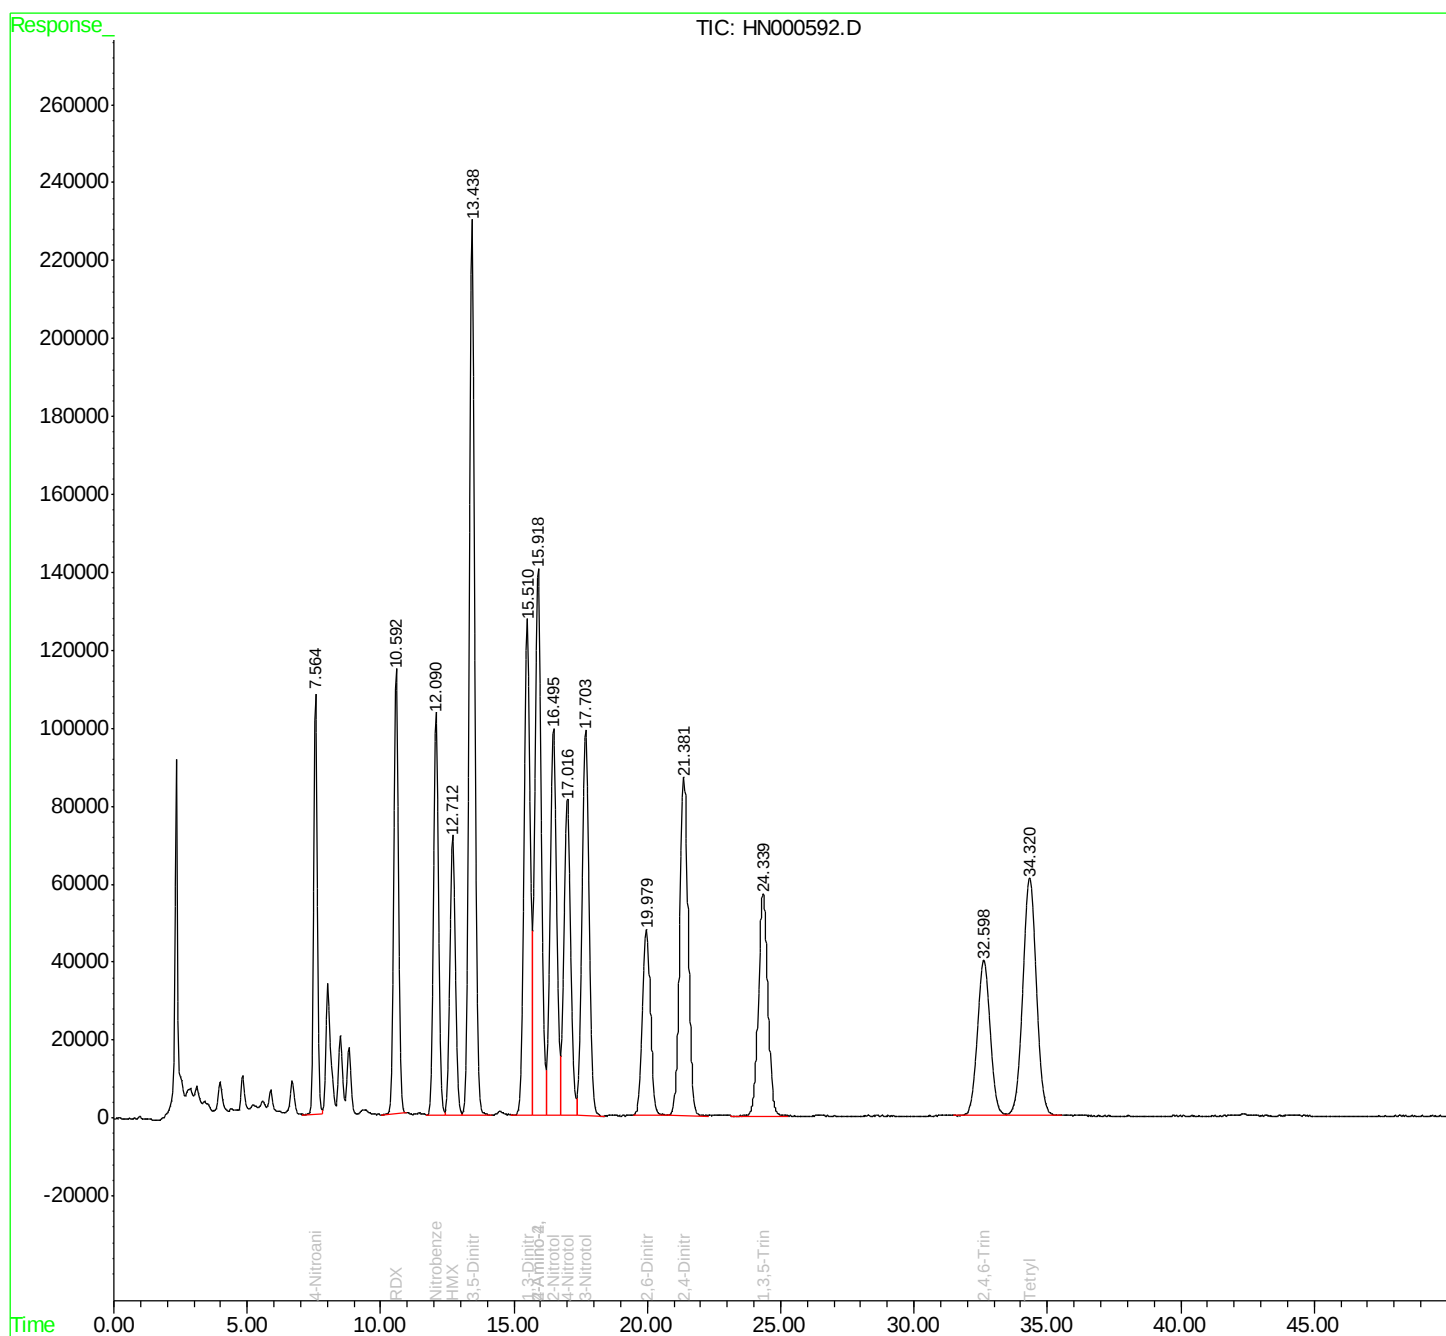


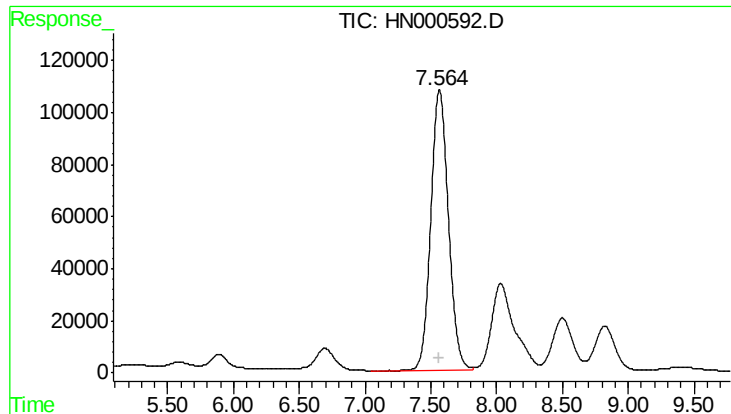

#1 4-Nitroaniline


R.T.: 7.566 min
Delta R.T.: 0.000 min
Response: 10025294
Conc: 994.32 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-4

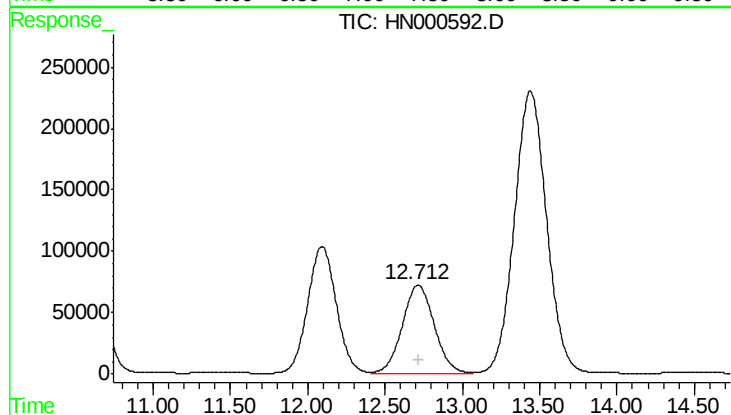


#2 HMX

R.T.: 12.714 min
Delta R.T.: 0.000 min
Response: 10269095
Conc: 1018.23 ug/L

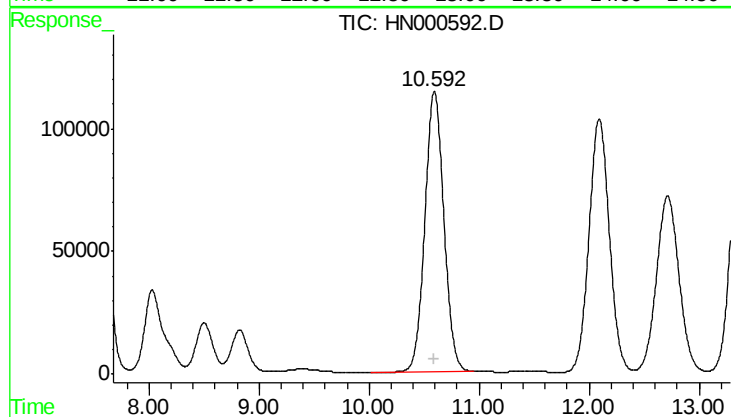


#3 RDX

R.T.: 10.594 min
Delta R.T.: 0.000 min
Response: 13642351
Conc: 989.37 ug/L

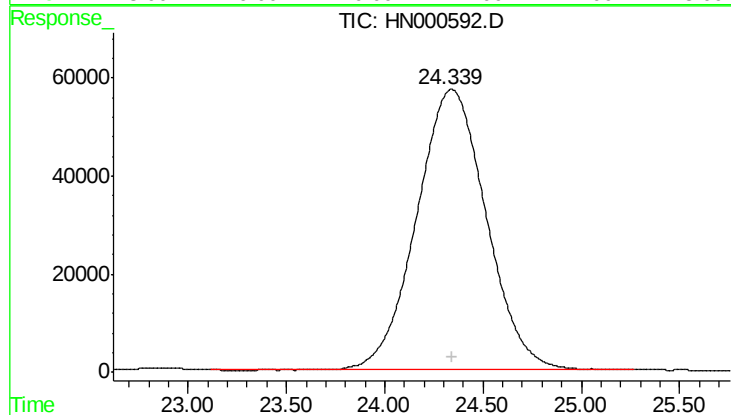

#4 1,3,5-Trinitrobenzene


R.T.: 24.341 min
Delta R.T.: 0.000 min
Response: 14131801
Conc: 505.90 ug/L

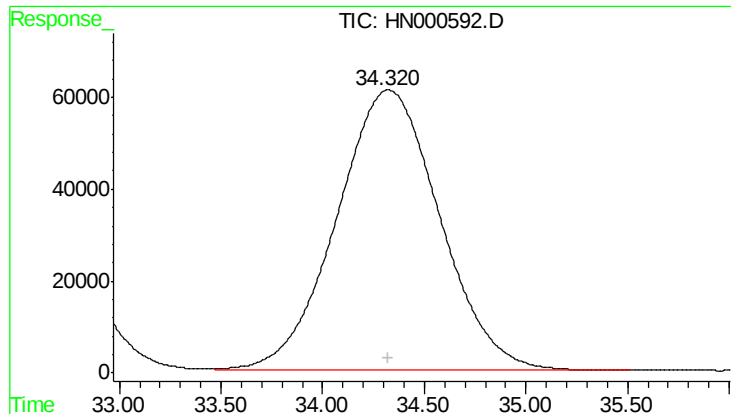

#5 Tetryl


R.T.: 34.322 min
Delta R.T.: 0.000 min
Response: 21570366
Conc: 1000.06 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-4

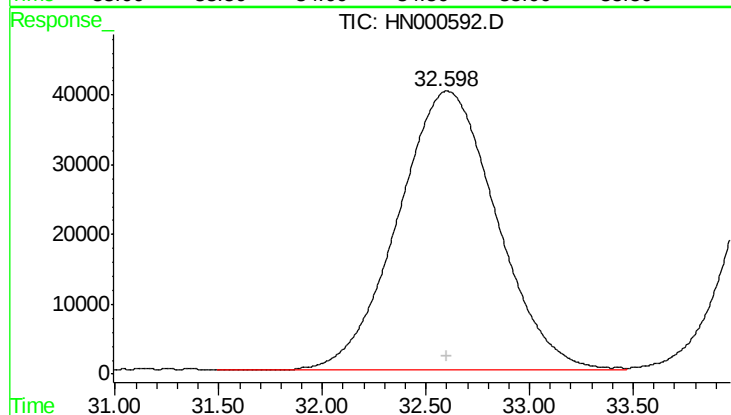


#6 2,4,6-Trinitrotoluene

R.T.: 32.603 min
Delta R.T.: 0.000 min
Response: 13208764
Conc: 487.49 ug/L

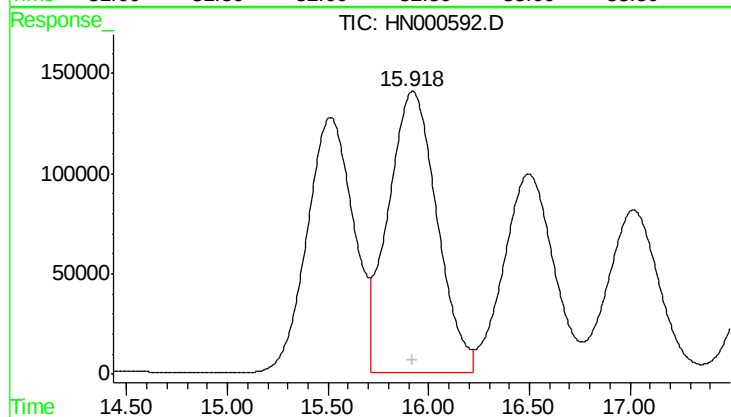


#7 2-Amino-4,6-dinitrotoluene

R.T.: 15.920 min
Delta R.T.: 0.000 min
Response: 23815804
Conc: 499.38 ug/L

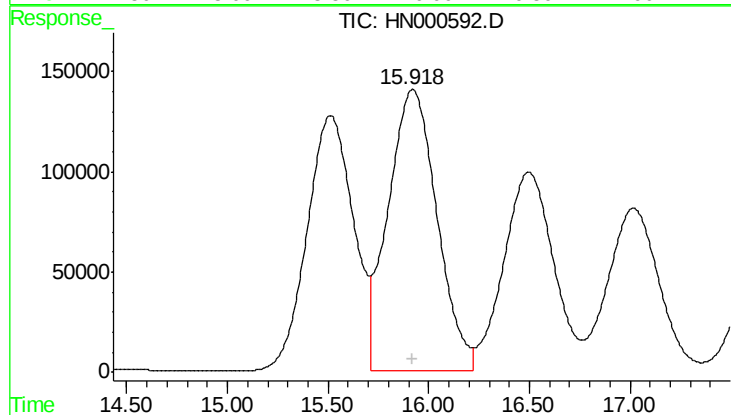

#8 4-Amino-2,6-dinitrotoluene


R.T.: 15.920 min
Delta R.T.: 0.000 min
Response: 23815804
Conc: 496.48 ug/L

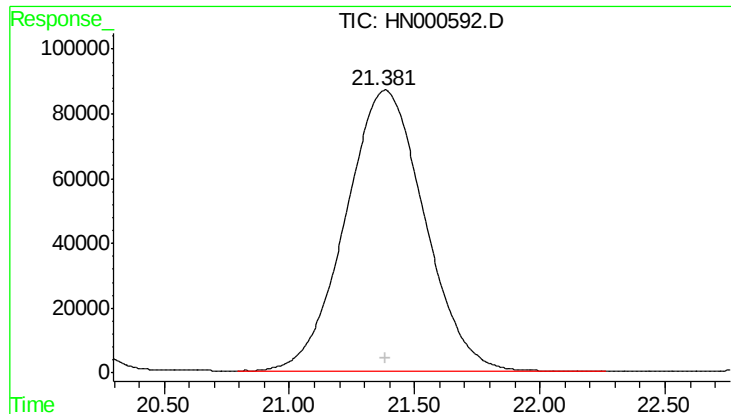

#9 2,4-Dinitrotoluene


R.T.: 21.383 min
Delta R.T.: 0.000 min
Response: 19080054
Conc: 496.66 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-4

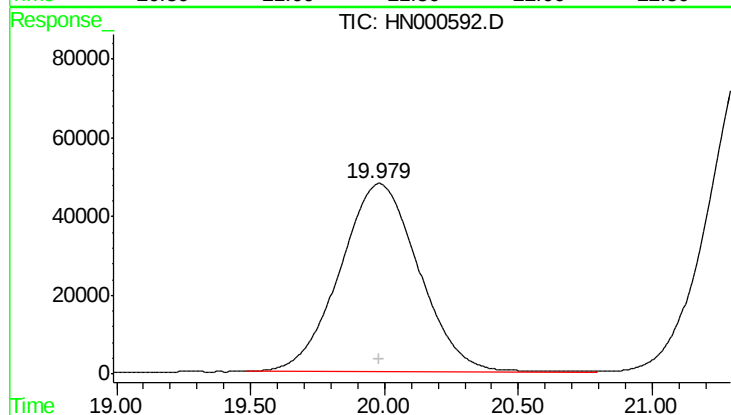


#10 2,6-Dinitrotoluene

R.T.: 19.981 min
Delta R.T.: 0.000 min
Response: 9820071
Conc: 483.30 ug/L

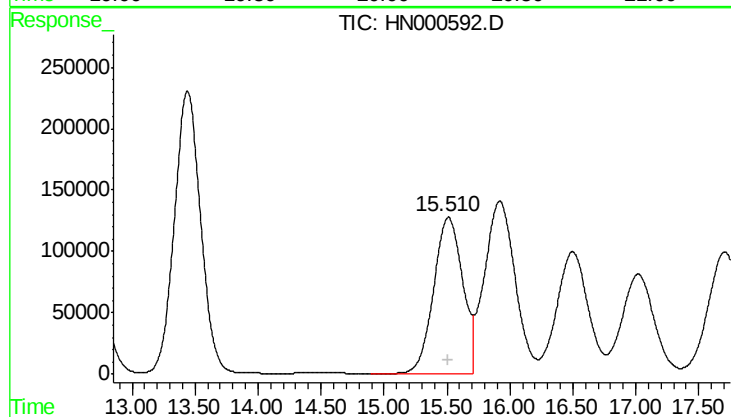


#11 1,3-Dinitrobenzene

R.T.: 15.512 min
Delta R.T.: 0.000 min
Response: 20381715
Conc: 482.40 ug/L

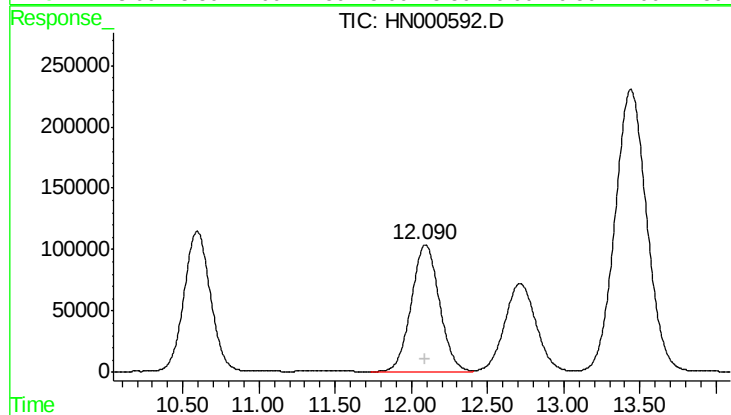

#12 Nitrobenzene


R.T.: 12.092 min
Delta R.T.: 0.000 min
Response: 13267040
Conc: 506.20 ug/L

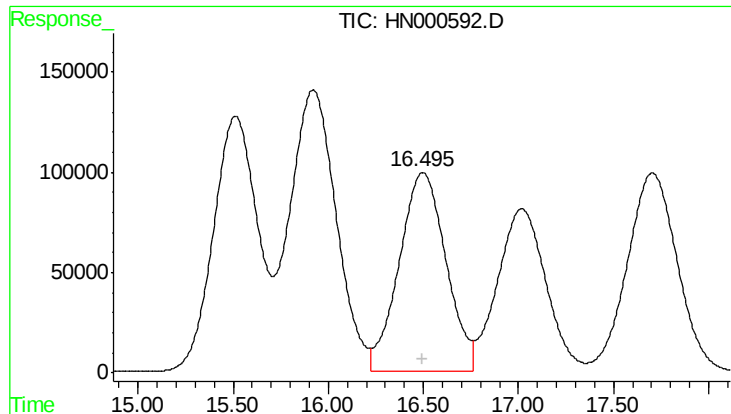

#13 2-Nitrotoluene


R.T.: 16.497 min
Delta R.T.: 0.000 min
Response: 17077568
Conc: 1010.42 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-4

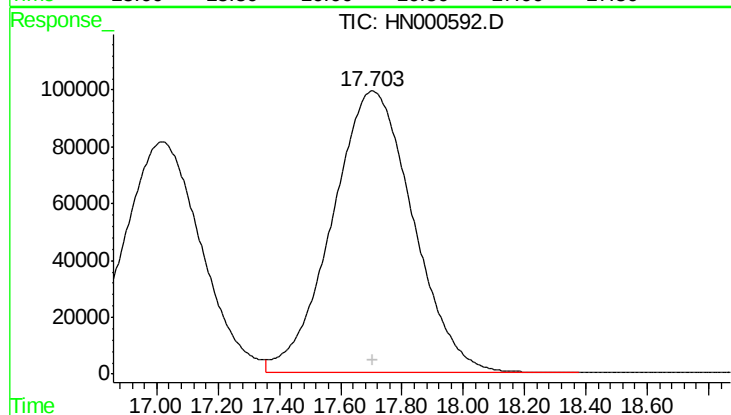


#14 3-Nitrotoluene

R.T.: 17.705 min
Delta R.T.: 0.000 min
Response: 18254137
Conc: 1007.26 ug/L

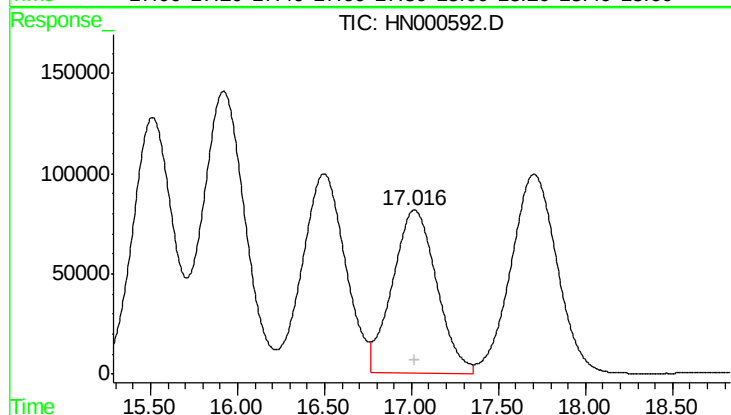

#15 4-Nitrotoluene

R.T.: 17.018 min
Delta R.T.: 0.000 min
Response: 14387892
Conc: 1031.97 ug/L

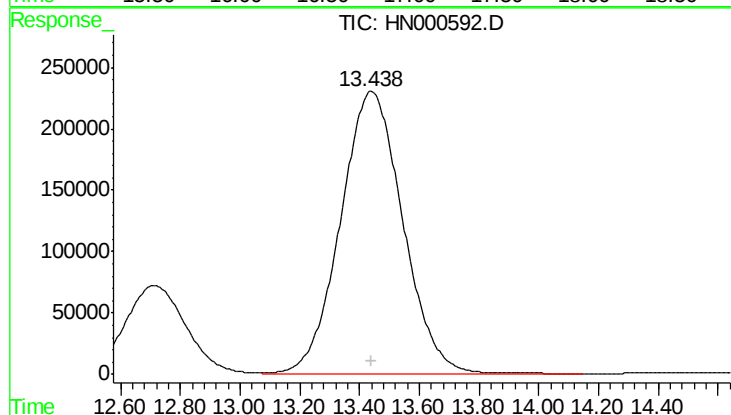

#16 3,5-Dinitroaniline

R.T.: 13.441 min
Delta R.T.: 0.000 min
Response: 33319338
Conc: 998.20 ug/L