

Data Path : S:\HPCHEM1\HPLC_N\Data\HN112012\
 Data File : HN000593.D
 Signal(s) : VWD1A.CH
 Acq On : 20-Nov-2012, 15:25
 Operator : HLM
 Sample : 8330-3
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 HPLC_N
 LabSampleId :
 8330-3

Integration File: events.e
 Quant Time: Nov 22 03:09:29 2012
 Quant Method : S:\HPCHEM1\HPLC_N\Method\HN112012.M
 Quant Title : SW8330 / 8330A confirmation
 QLast Update : Wed Nov 21 16:37:45 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	7.568	4972104	493.138 ug/L
Target Compounds				
2) T	HMX	12.714	5043140	500.052 ug/L
3) T	RDX	10.595	6873305	498.466 ug/L
4) T	1,3,5-Trinitrobenzene	24.342	7018228	251.245 ug/L
5) T	Tetryl	34.329	10739526	497.912 ug/L
6) T	2,4,6-Trinitrotoluene	32.609	6669982	246.167 ug/L
7) T	2-Amino-4,6-dinitroto...	15.922	11981964	251.245 ug/L
8) T	4-Amino-2,6-dinitroto...	15.922	11981964	249.783 ug/L
9) T	2,4-Dinitrotoluene	21.385	9482262	246.829 ug/L
10) T	2,6-Dinitrotoluene	19.983	4885137	240.425 ug/L
11) T	1,3-Dinitrobenzene	15.514	10241028	242.388 ug/L
12) T	Nitrobenzene	12.094	6500196	248.013 ug/L
13) T	2-Nitrotoluene	16.500	8618358	509.916 ug/L
14) T	3-Nitrotoluene	17.709	9133243	503.971 ug/L
15) T	4-Nitrotoluene	17.021	7276982	521.943 ug/L
16) T	3,5-Dinitroaniline	13.442	16471612	493.464 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_N\Data\HN112012\
Data File : HN000593.D
Signal(s) : VWD1A.CH
Acq On : 20-Nov-2012, 15:25
Operator : HLM
Sample : 8330-3
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
HPLC_N
LabSampleId :
8330-3

Integration File: events.e
Quant Time: Nov 22 03:09:29 2012
Quant Method : S:\HPCHEM1\HPLC_N\Method\HN112012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Wed Nov 21 16:37:45 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

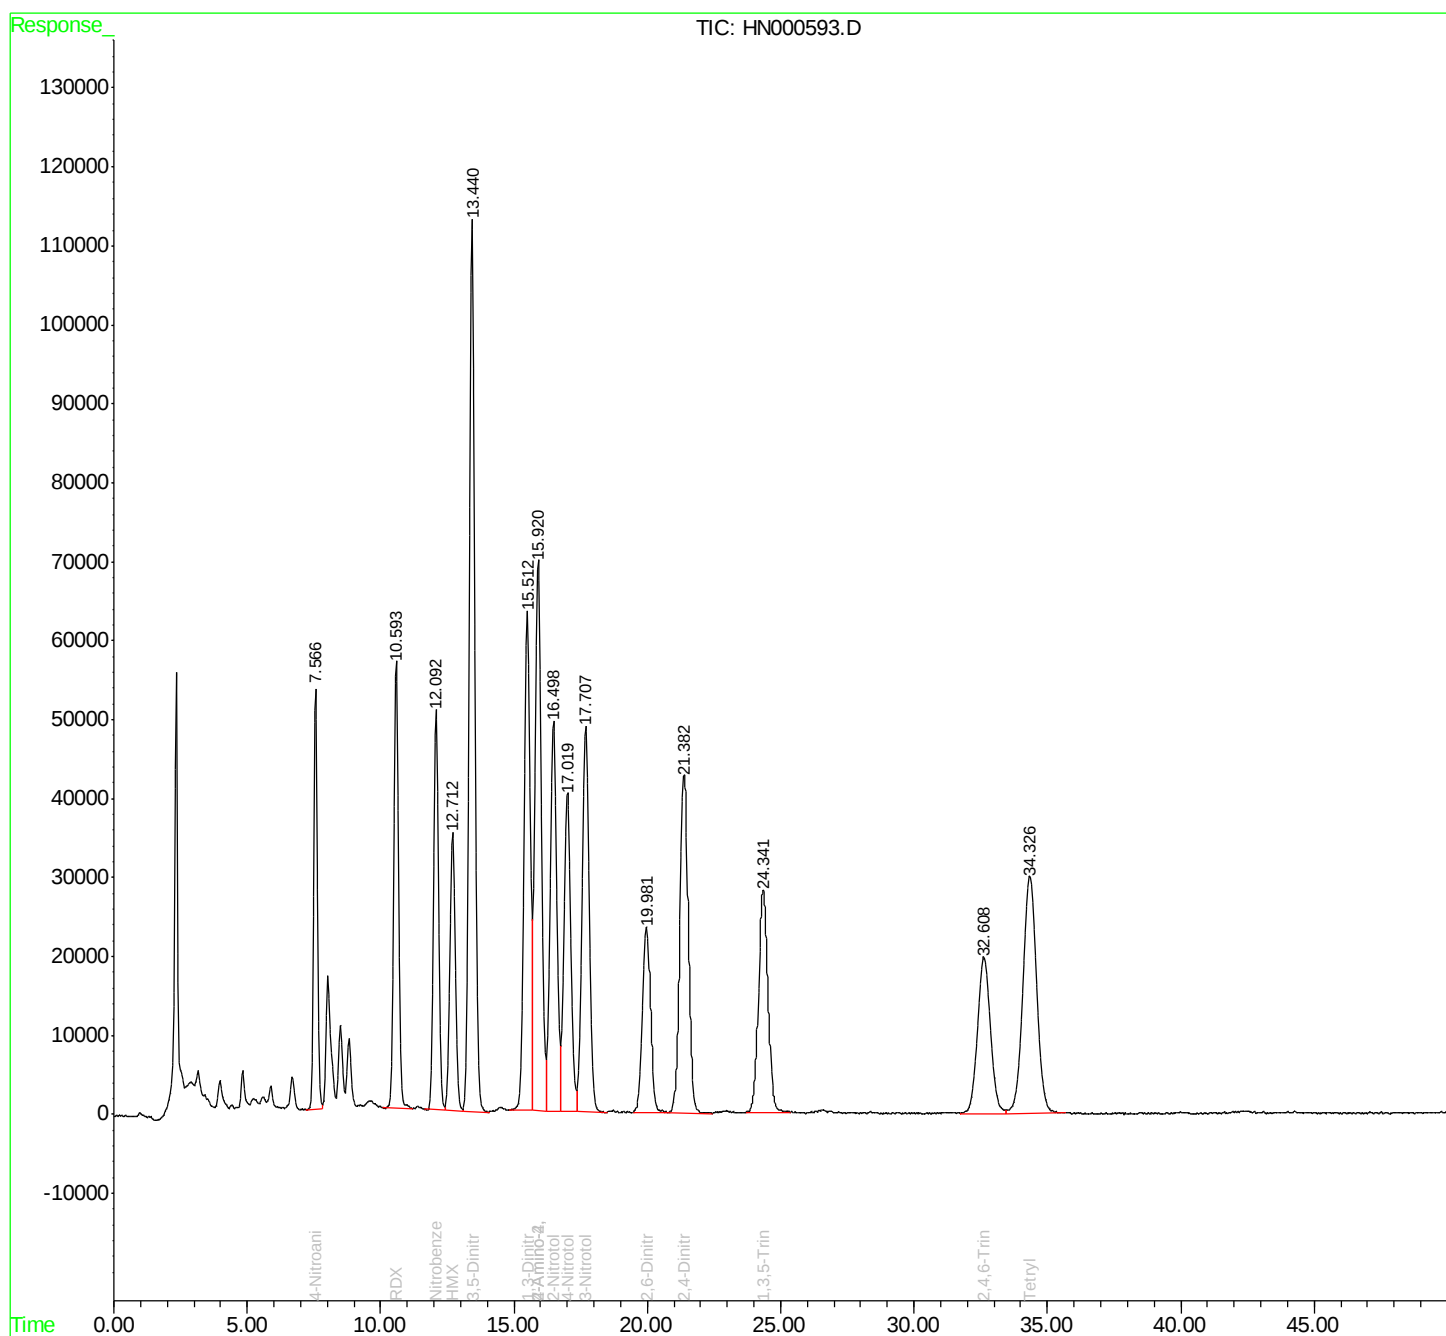


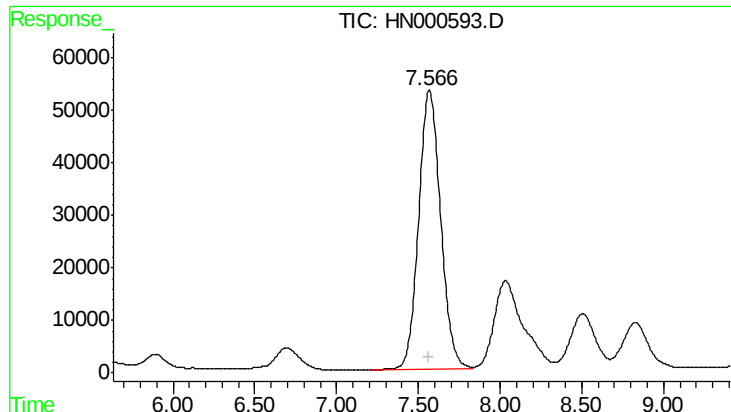

#1 4-Nitroaniline


R.T.: 7.568 min
Delta R.T.: 0.002 min
Response: 4972104
Conc: 493.14 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-3

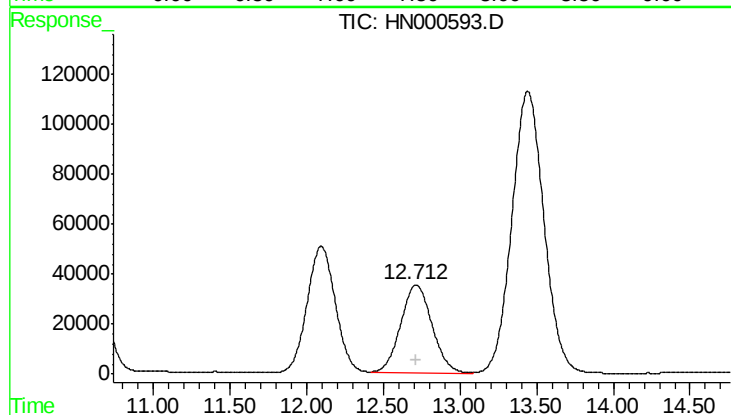


#2 HMX

R.T.: 12.714 min
Delta R.T.: 0.000 min
Response: 5043140
Conc: 500.05 ug/L

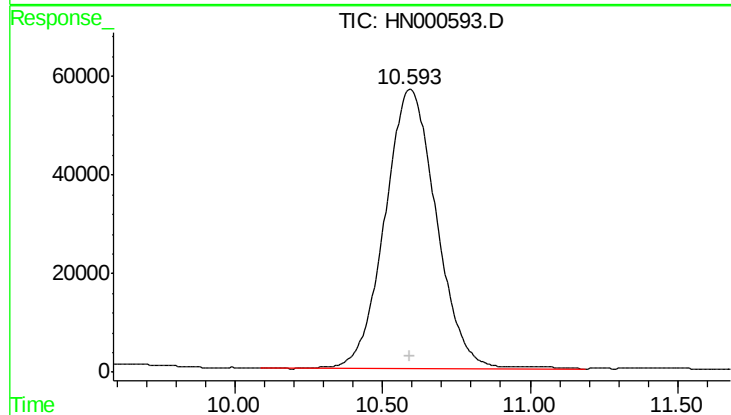


#3 RDX

R.T.: 10.595 min
Delta R.T.: 0.001 min
Response: 6873305
Conc: 498.47 ug/L

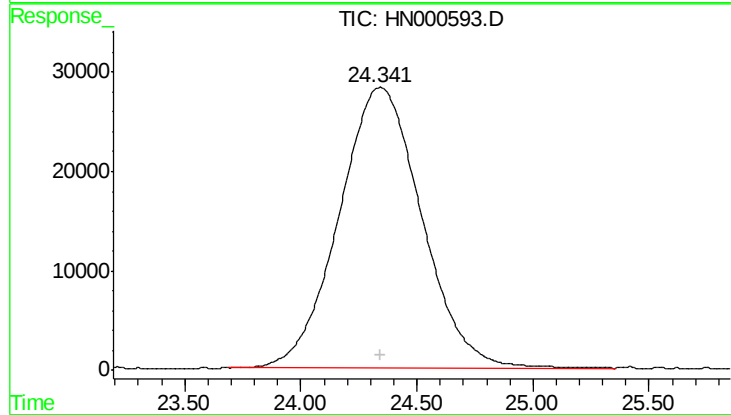

#4 1,3,5-Trinitrobenzene


R.T.: 24.342 min
Delta R.T.: 0.001 min
Response: 7018228
Conc: 251.25 ug/L

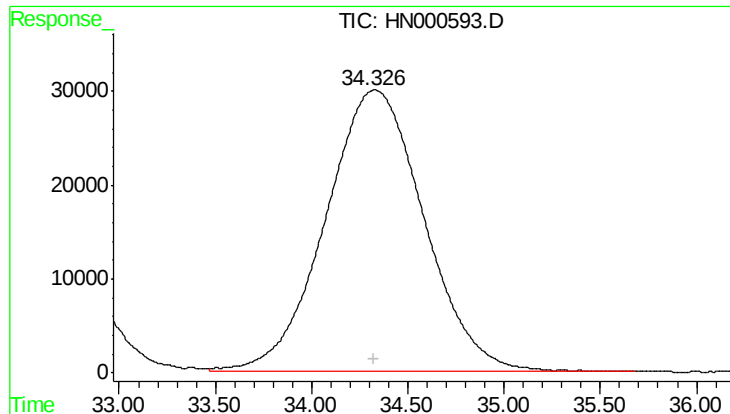

#5 Tetryl


R.T.: 34.329 min
Delta R.T.: 0.007 min
Response: 10739526
Conc: 497.91 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-3

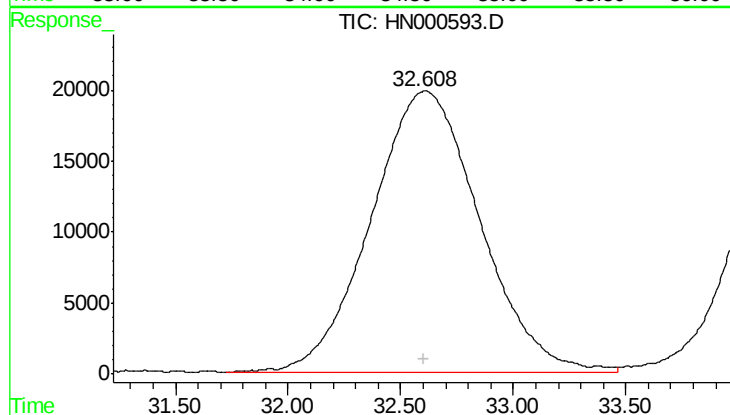


#6 2,4,6-Trinitrotoluene

R.T.: 32.609 min
Delta R.T.: 0.006 min
Response: 6669982
Conc: 246.17 ug/L

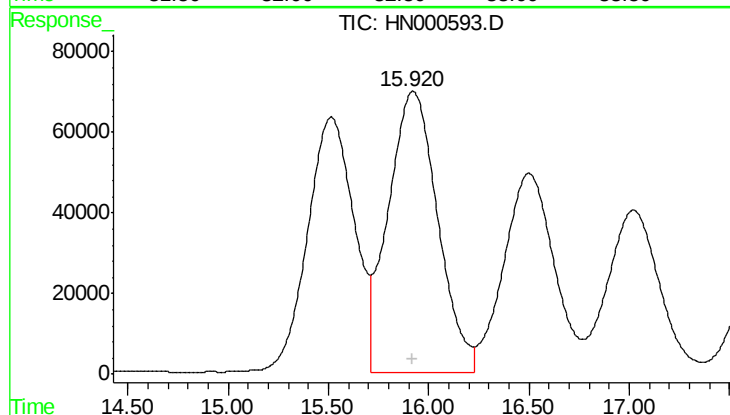


#7 2-Amino-4,6-dinitrotoluene

R.T.: 15.922 min
Delta R.T.: 0.002 min
Response: 11981964
Conc: 251.25 ug/L

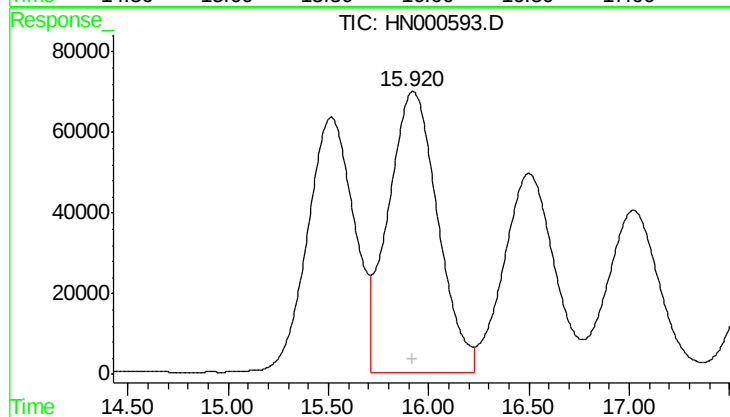

#8 4-Amino-2,6-dinitrotoluene


R.T.: 15.922 min
Delta R.T.: 0.002 min
Response: 11981964
Conc: 249.78 ug/L

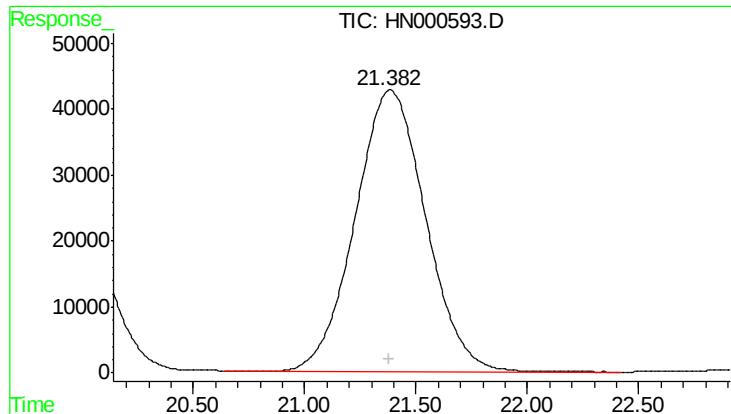

#9 2,4-Dinitrotoluene


R.T.: 21.385 min
Delta R.T.: 0.002 min
Response: 9482262
Conc: 246.83 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-3

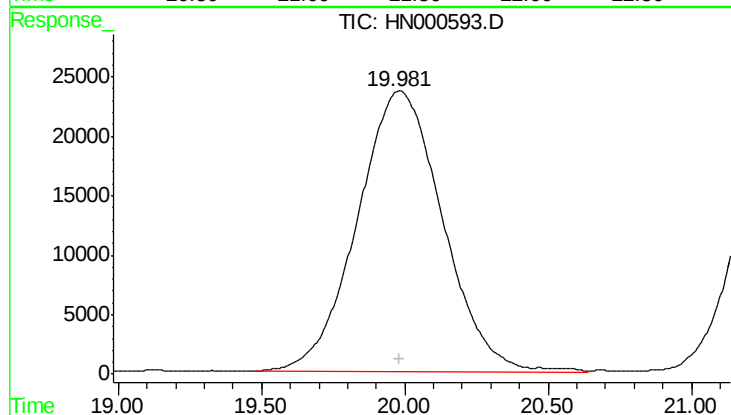


#10 2,6-Dinitrotoluene

R.T.: 19.983 min
Delta R.T.: 0.001 min
Response: 4885137
Conc: 240.42 ug/L

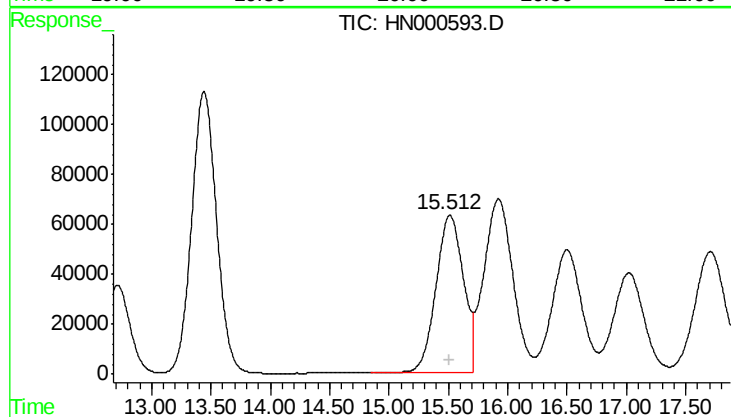


#11 1,3-Dinitrobenzene

R.T.: 15.514 min
Delta R.T.: 0.002 min
Response: 10241028
Conc: 242.39 ug/L

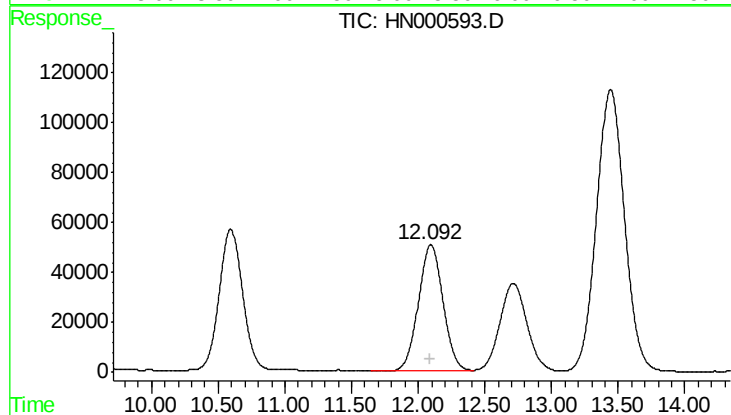

#12 Nitrobenzene


R.T.: 12.094 min
Delta R.T.: 0.002 min
Response: 6500196
Conc: 248.01 ug/L

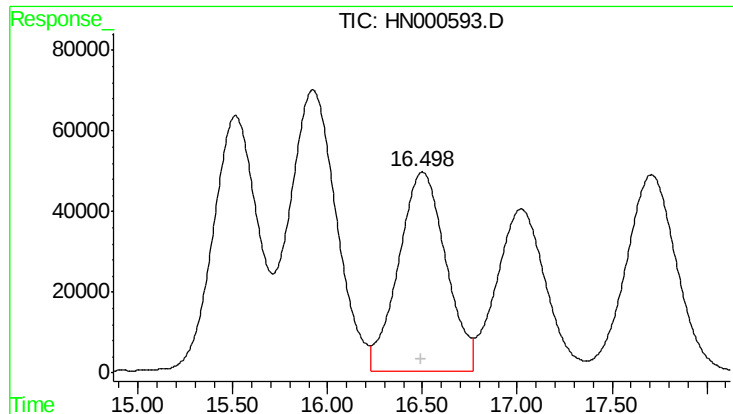

#13 2-Nitrotoluene


R.T.: 16.500 min
Delta R.T.: 0.003 min
Response: 8618358
Conc: 509.92 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-3

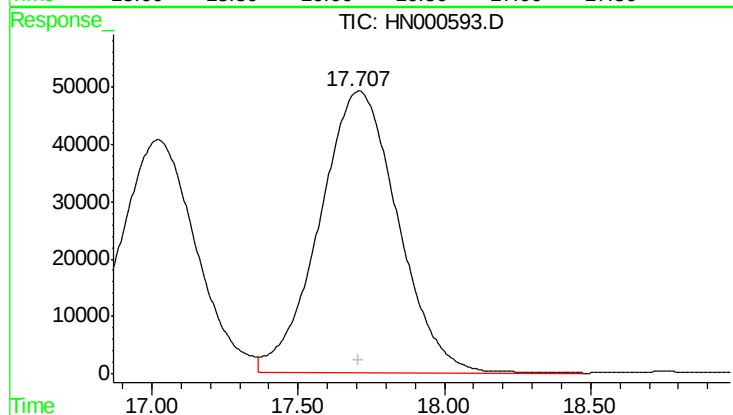


#14 3-Nitrotoluene

R.T.: 17.709 min
Delta R.T.: 0.004 min
Response: 9133243
Conc: 503.97 ug/L

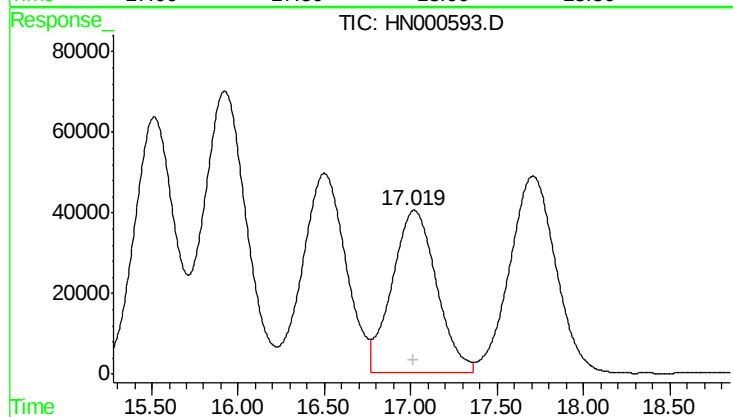

#15 4-Nitrotoluene

R.T.: 17.021 min
Delta R.T.: 0.003 min
Response: 7276982
Conc: 521.94 ug/L

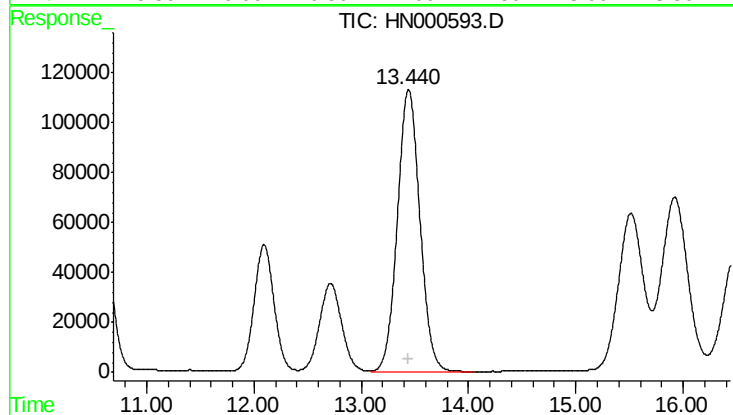

#16 3,5-Dinitroaniline

R.T.: 13.442 min
Delta R.T.: 0.000 min
Response: 16471612
Conc: 493.46 ug/L