

Data Path : S:\HPCHEM1\HPLC_N\Data\HN112012\
 Data File : HN000594.D
 Signal(s) : VWD1A.CH
 Acq On : 20-Nov-2012, 16:18
 Operator : HLM
 Sample : 8330-2
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 HPLC_N
 LabSampleId :
 8330-2

Integration File: events.e
 Quant Time: Nov 22 03:09:40 2012
 Quant Method : S:\HPCHEM1\HPLC_N\Method\HN112012.M
 Quant Title : SW8330 / 8330A confirmation
 QLast Update : Wed Nov 21 16:37:45 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	7.573	981429	97.339 ug/L
Target Compounds			
2) T HMX	12.725	989837	98.147 ug/L
3) T RDX	10.602	1340231	97.196 ug/L
4) T 1,3,5-Trinitrobenzene	24.356	1390182	49.767 ug/L
5) T Tetryl	34.341	2209828	102.453 ug/L
6) T 2,4,6-Trinitrotoluene	32.645	1414071	52.189 ug/L
7) T 2-Amino-4,6-dinitroto...	15.929	2457806	51.537 ug/L
8) T 4-Amino-2,6-dinitroto...	15.929	2457806	51.237 ug/L
9) T 2,4-Dinitrotoluene	21.397	1935250	50.376 ug/L
10) T 2,6-Dinitrotoluene	19.984	1033673	50.873 ug/L
11) T 1,3-Dinitrobenzene	15.522	2185182	51.720 ug/L
12) T Nitrobenzene	12.100	1273310	48.583 ug/L
13) T 2-Nitrotoluene	16.505	1771545	104.816 ug/L
14) T 3-Nitrotoluene	17.716	1917621	105.814 ug/L
15) T 4-Nitrotoluene	17.023	1493292	107.107 ug/L
16) T 3,5-Dinitroaniline	13.448	3265030	97.815 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_N\Data\HN112012\
Data File : HN000594.D
Signal(s) : VWD1A.CH
Acq On : 20-Nov-2012, 16:18
Operator : HLM
Sample : 8330-2
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
HPLC_N
LabSampleId :
8330-2

Integration File: events.e
Quant Time: Nov 22 03:09:40 2012
Quant Method : S:\HPCHEM1\HPLC_N\Method\HN112012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Wed Nov 21 16:37:45 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

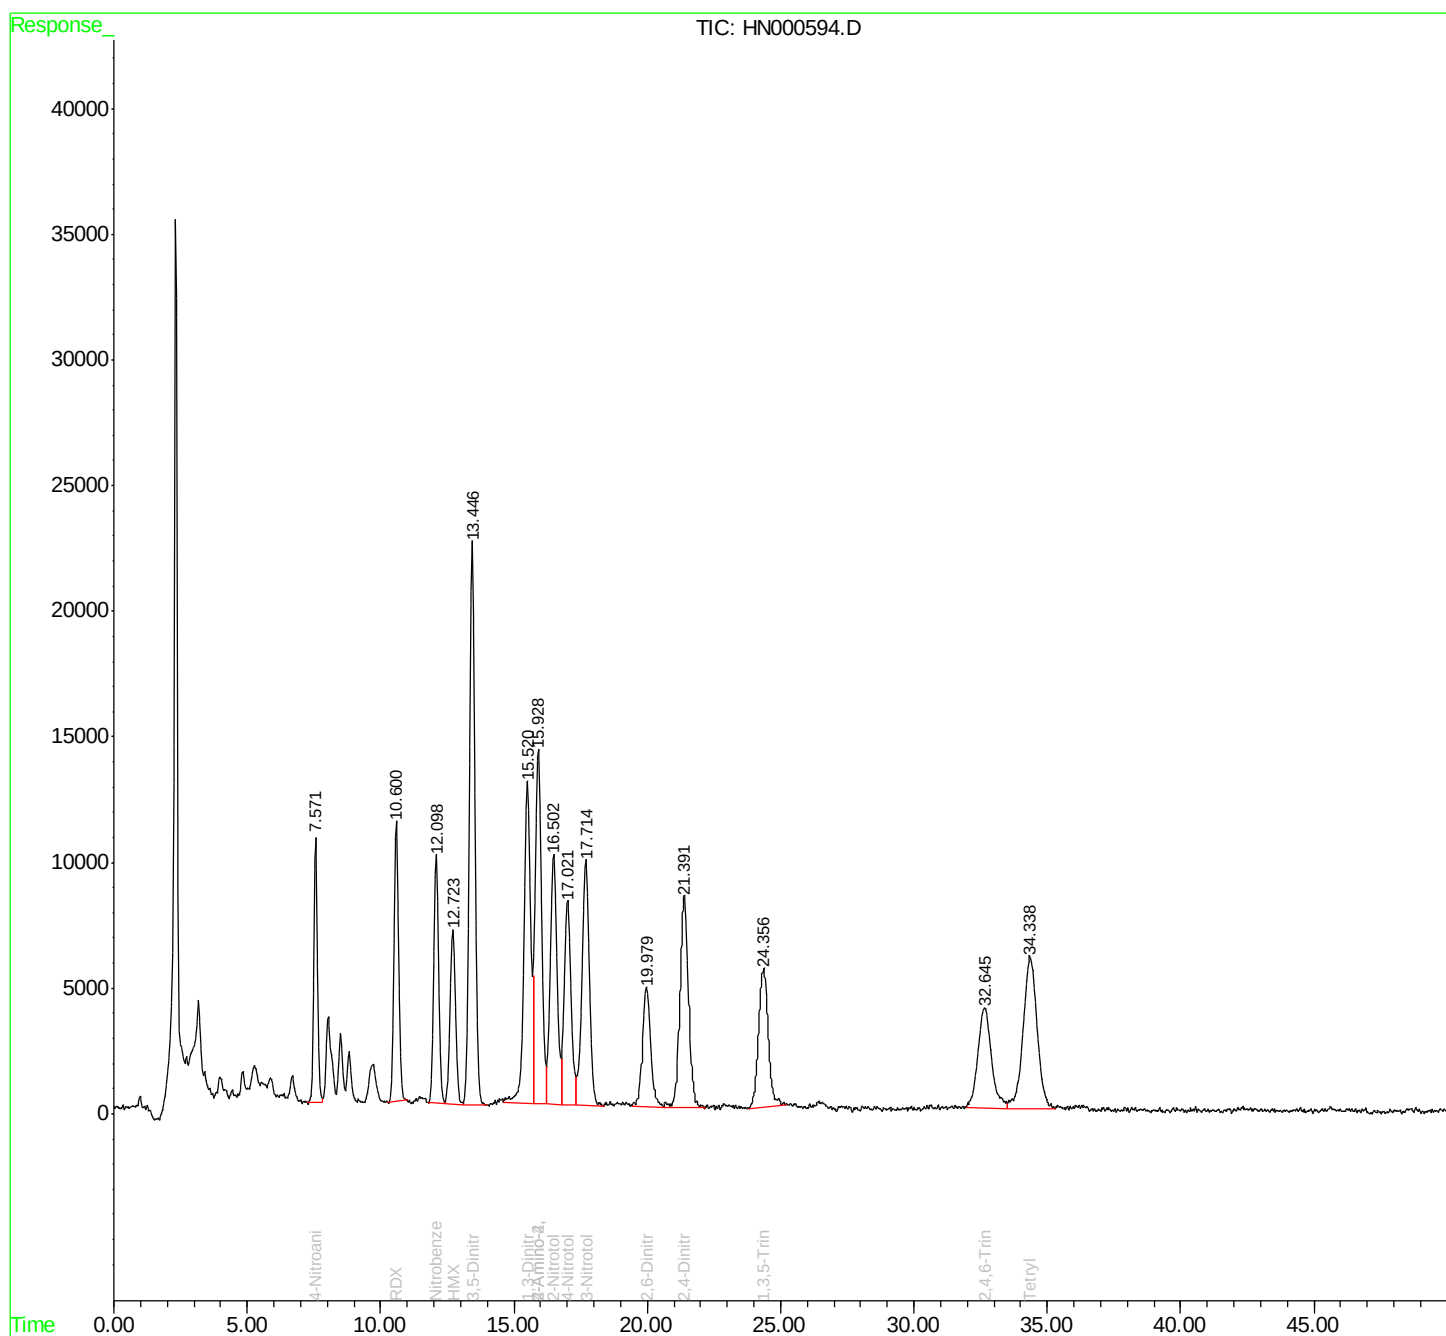


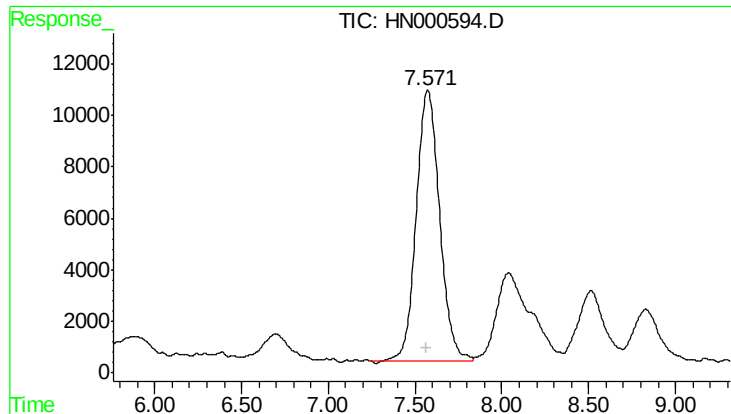

#1 4-Nitroaniline


R.T.: 7.573 min
Delta R.T.: 0.007 min
Response: 981429
Conc: 97.34 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-2

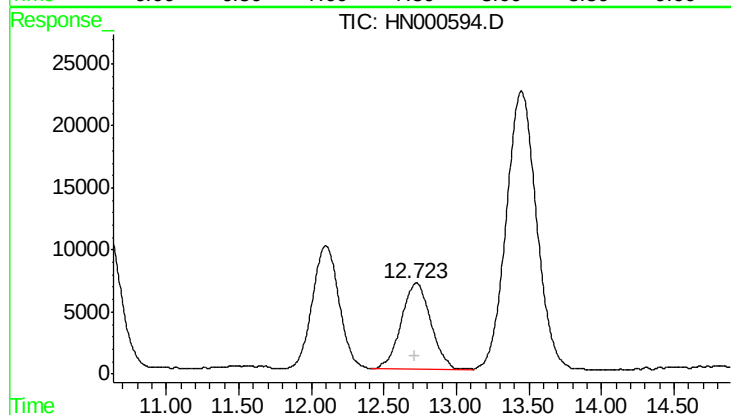


#2 HMX

R.T.: 12.725 min
Delta R.T.: 0.011 min
Response: 989837
Conc: 98.15 ug/L

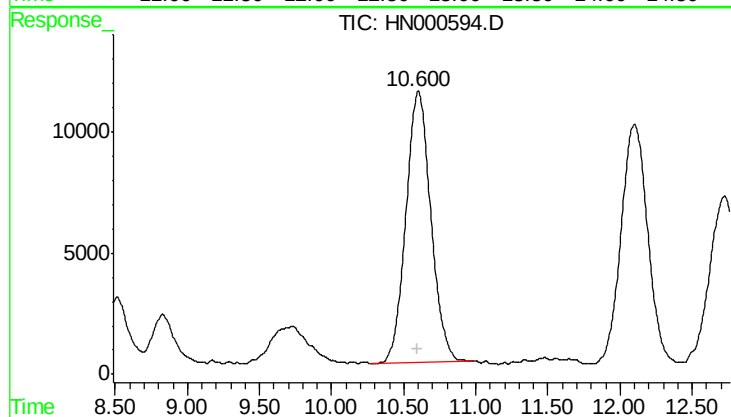


#3 RDX

R.T.: 10.602 min
Delta R.T.: 0.009 min
Response: 1340231
Conc: 97.20 ug/L

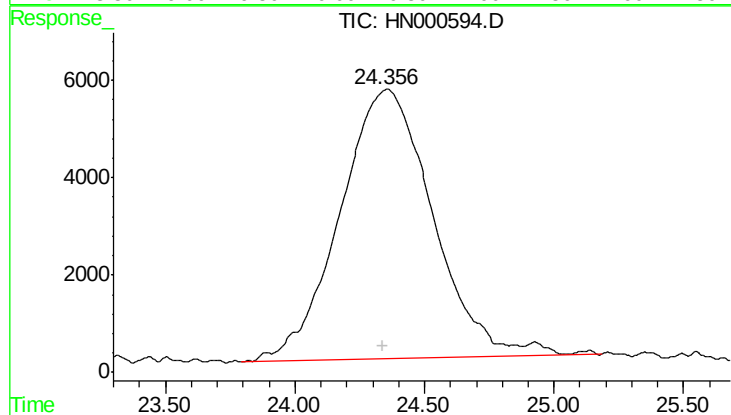

#4 1,3,5-Trinitrobenzene


R.T.: 24.356 min
Delta R.T.: 0.015 min
Response: 1390182
Conc: 49.77 ug/L

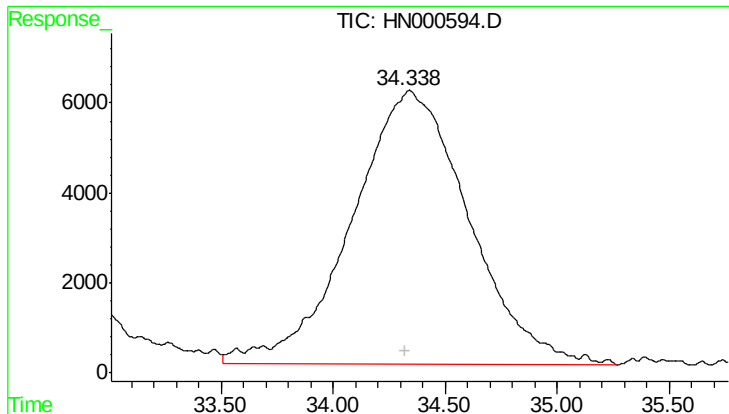

#5 Tetryl


R.T.: 34.341 min
Delta R.T.: 0.019 min
Response: 2209828
Conc: 102.45 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-2

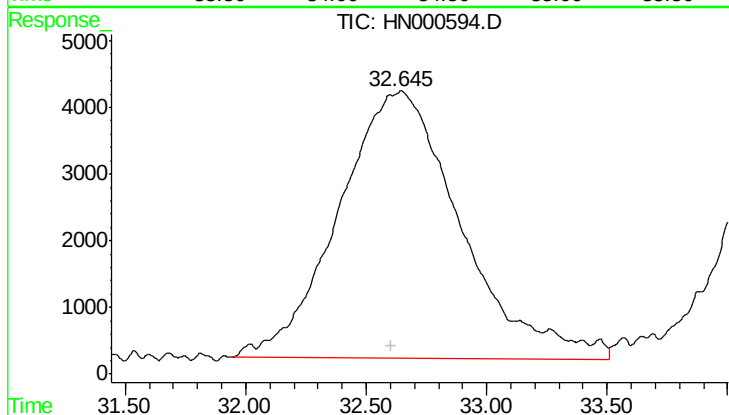


#6 2,4,6-Trinitrotoluene

R.T.: 32.645 min
Delta R.T.: 0.042 min
Response: 1414071
Conc: 52.19 ug/L

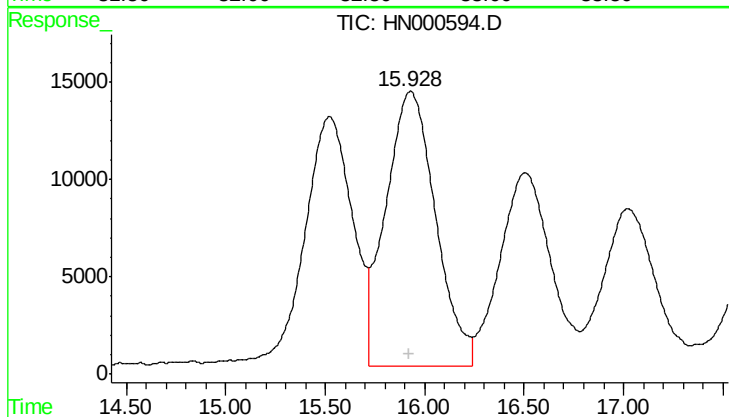


#7 2-Amino-4,6-dinitrotoluene

R.T.: 15.929 min
Delta R.T.: 0.009 min
Response: 2457806
Conc: 51.54 ug/L

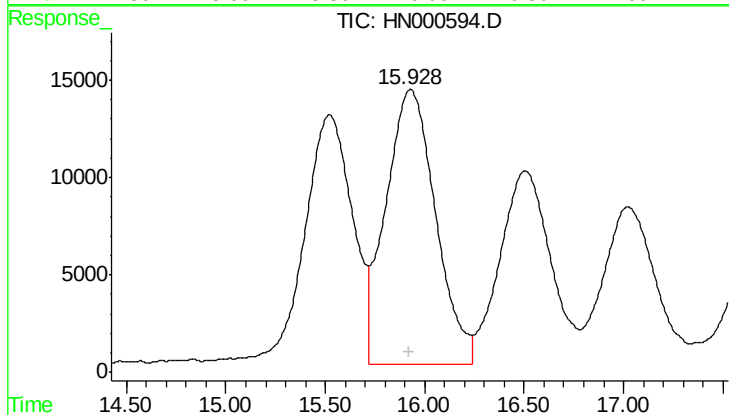

#8 4-Amino-2,6-dinitrotoluene


R.T.: 15.929 min
Delta R.T.: 0.009 min
Response: 2457806
Conc: 51.24 ug/L

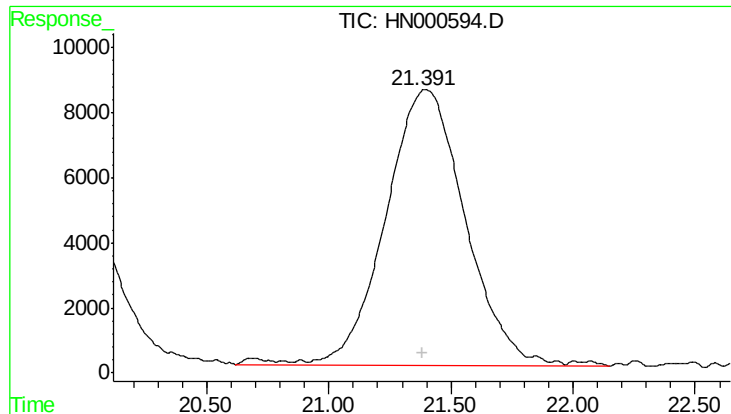

#9 2,4-Dinitrotoluene


R.T.: 21.397 min
Delta R.T.: 0.014 min
Response: 1935250
Conc: 50.38 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-2

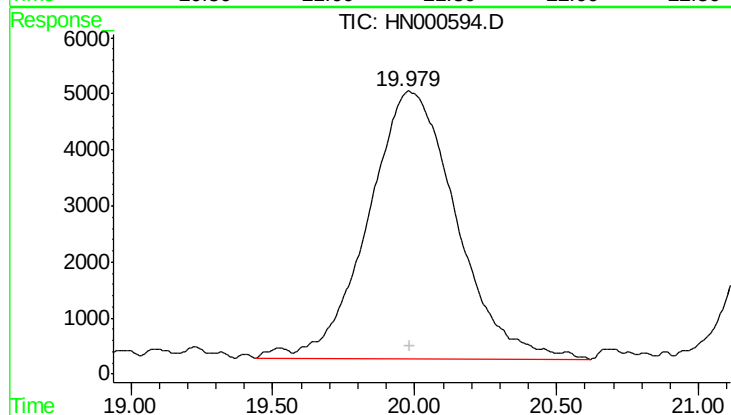


#10 2,6-Dinitrotoluene

R.T.: 19.984 min
Delta R.T.: 0.003 min
Response: 1033673
Conc: 50.87 ug/L

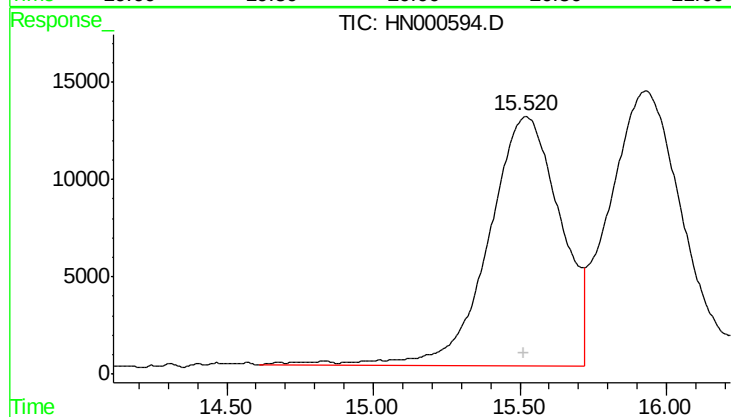


#11 1,3-Dinitrobenzene

R.T.: 15.522 min
Delta R.T.: 0.009 min
Response: 2185182
Conc: 51.72 ug/L

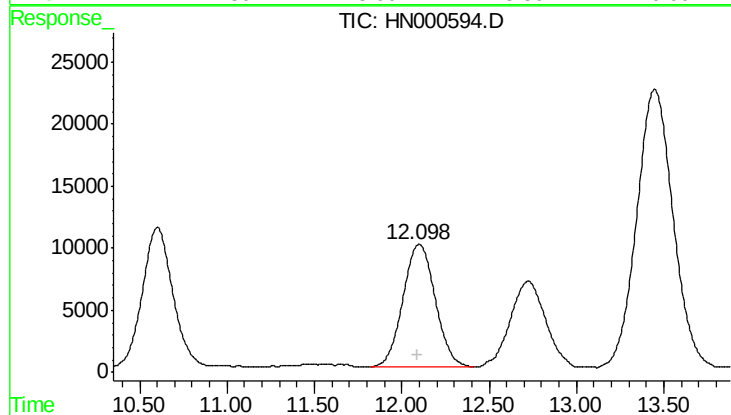

#12 Nitrobenzene


R.T.: 12.100 min
Delta R.T.: 0.008 min
Response: 1273310
Conc: 48.58 ug/L

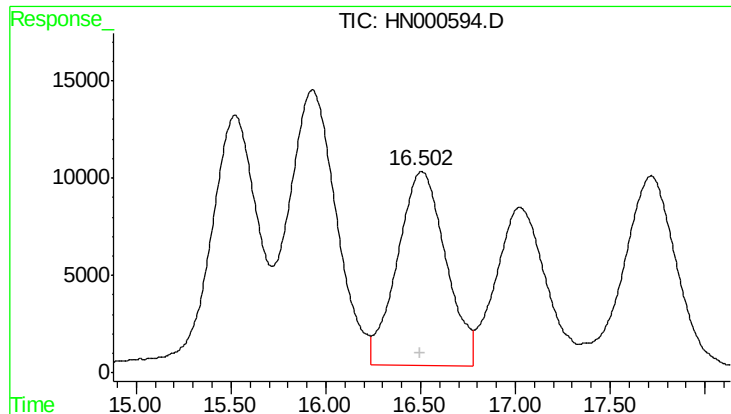

#13 2-Nitrotoluene


R.T.: 16.505 min
Delta R.T.: 0.008 min
Response: 1771545
Conc: 104.82 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-2

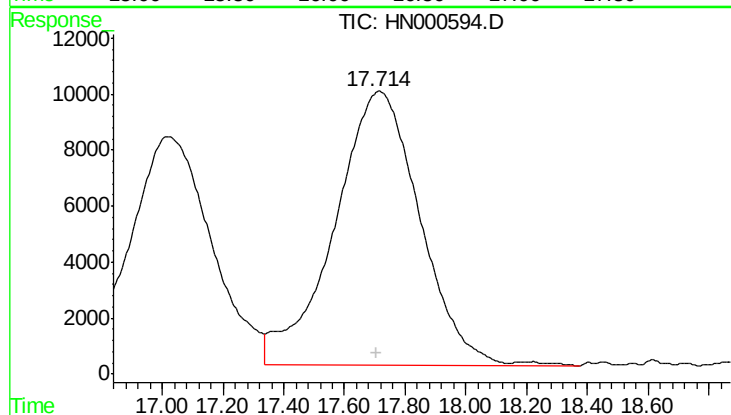


#14 3-Nitrotoluene

R.T.: 17.716 min
Delta R.T.: 0.011 min
Response: 1917621
Conc: 105.81 ug/L

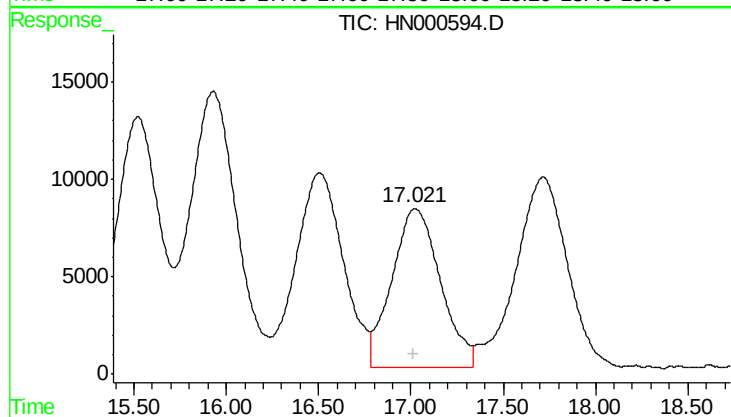

#15 4-Nitrotoluene

R.T.: 17.023 min
Delta R.T.: 0.005 min
Response: 1493292
Conc: 107.11 ug/L

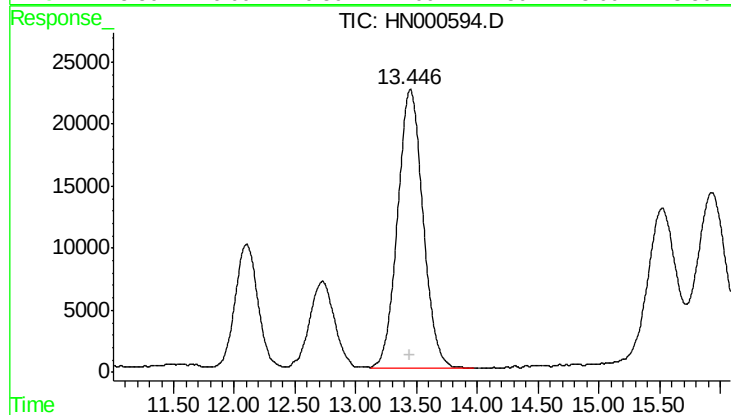

#16 3,5-Dinitroaniline

R.T.: 13.448 min
Delta R.T.: 0.007 min
Response: 3265030
Conc: 97.82 ug/L