

Data Path : S:\HPCHEM1\HPLC_N\Data\HN112012\
 Data File : HN000595.D
 Signal(s) : VWD1A.CH
 Acq On : 20-Nov-2012, 17:10
 Operator : HLM
 Sample : 8330-1
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 HPLC_N
 LabSampleId :
 8330-1

Integration File: events.e
 Quant Time: Nov 22 03:09:48 2012
 Quant Method : S:\HPCHEM1\HPLC_N\Method\HN112012.M
 Quant Title : SW8330 / 8330A confirmation
 QLast Update : Wed Nov 21 16:37:45 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	7.576	219351	21.755 ug/L
Target Compounds			
3) T RDX	10.602	283797	20.581 ug/L
7) T 2-Amino-4,6-dinitroto...	15.916	535213	11.223 ug/L
8) T 4-Amino-2,6-dinitroto...	15.916	535213	11.157 ug/L
9) T 2,4-Dinitrotoluene	21.410	404832	10.538 ug/L
11) T 1,3-Dinitrobenzene	15.519	473040	11.196 ug/L
12) T Nitrobenzene	12.092	268256	10.235 ug/L
13) T 2-Nitrotoluene	16.495	405012	23.963 ug/L
14) T 3-Nitrotoluene	17.721	466494	25.741 ug/L
16) T 3,5-Dinitroaniline	13.445	715887	21.447 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_N\Data\HN112012\
Data File : HN000595.D
Signal(s) : VWD1A.CH
Acq On : 20-Nov-2012, 17:10
Operator : HLM
Sample : 8330-1
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
HPLC_N
LabSampleId :
8330-1

Integration File: events.e
Quant Time: Nov 22 03:09:48 2012
Quant Method : S:\HPCHEM1\HPLC_N\Method\HN112012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Wed Nov 21 16:37:45 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

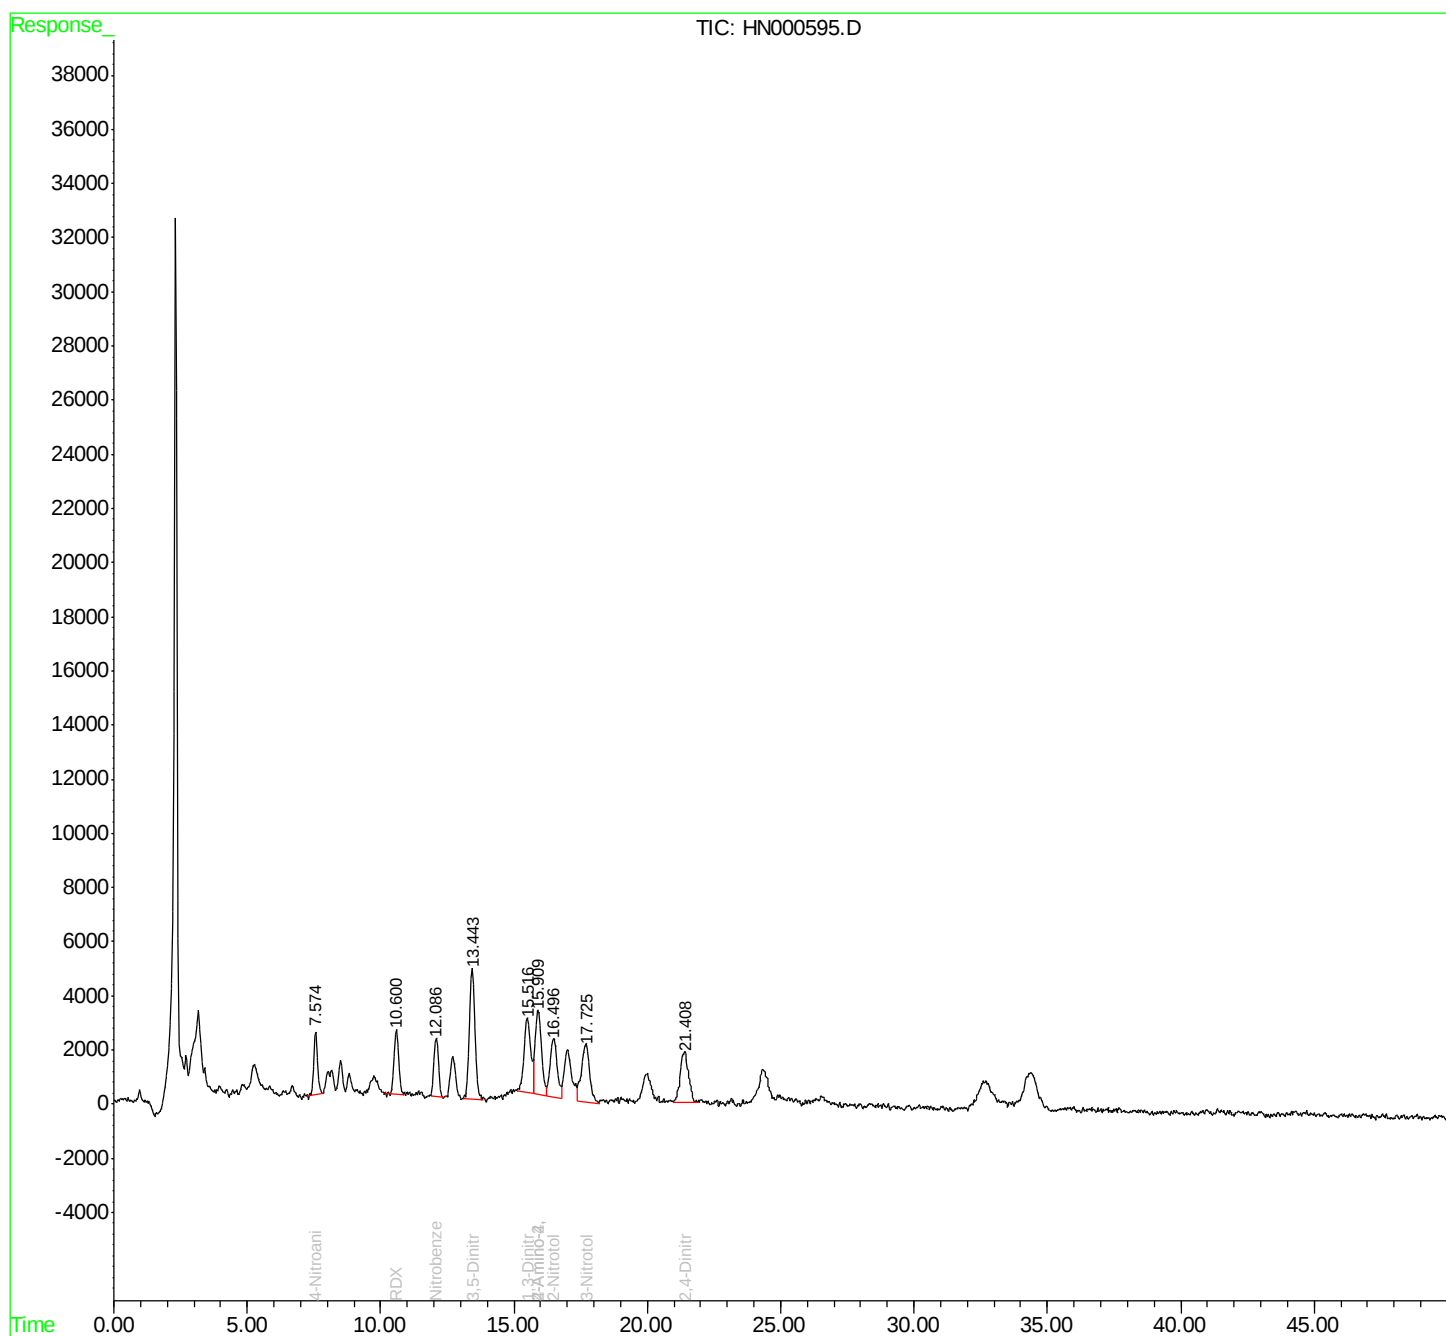


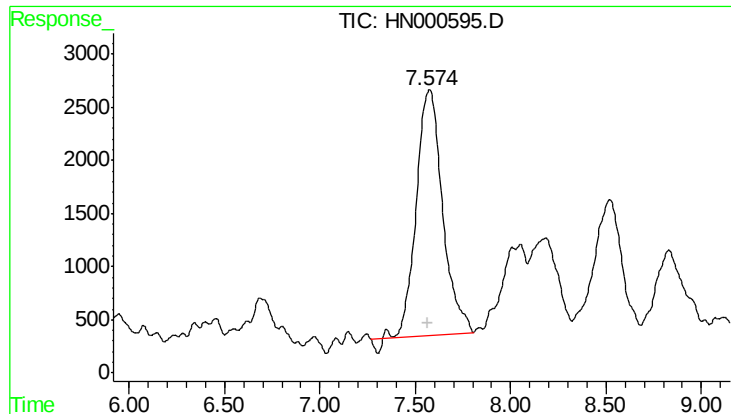

#1 4-Nitroaniline


R.T.: 7.576 min
Delta R.T.: 0.010 min
Response: 219351
Conc: 21.76 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-1

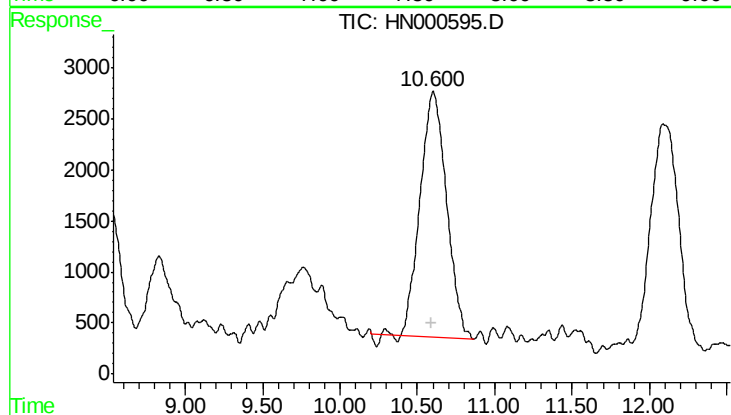


#3 RDX

R.T.: 10.602 min
Delta R.T.: 0.009 min
Response: 283797
Conc: 20.58 ug/L

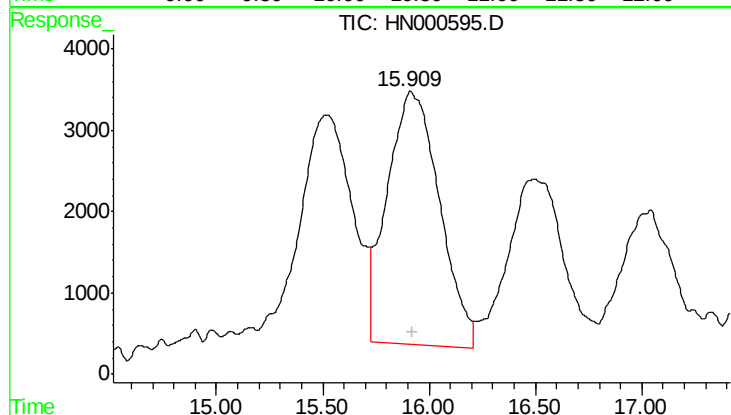


#7 2-Amino-4,6-dinitrotoluene

R.T.: 15.916 min
Delta R.T.: -0.005 min
Response: 535213
Conc: 11.22 ug/L

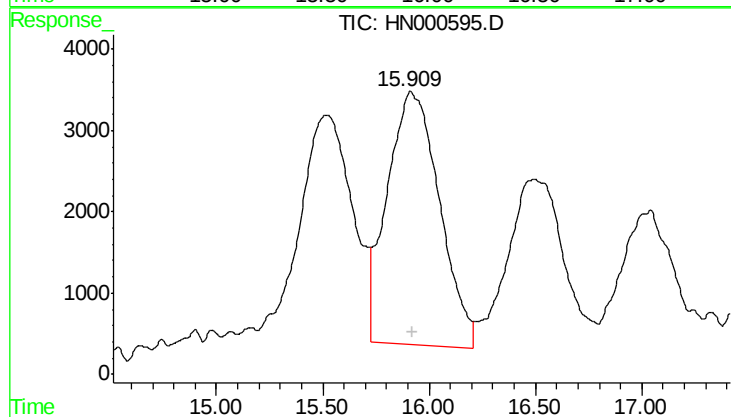

#8 4-Amino-2,6-dinitrotoluene


R.T.: 15.916 min
Delta R.T.: -0.005 min
Response: 535213
Conc: 11.16 ug/L

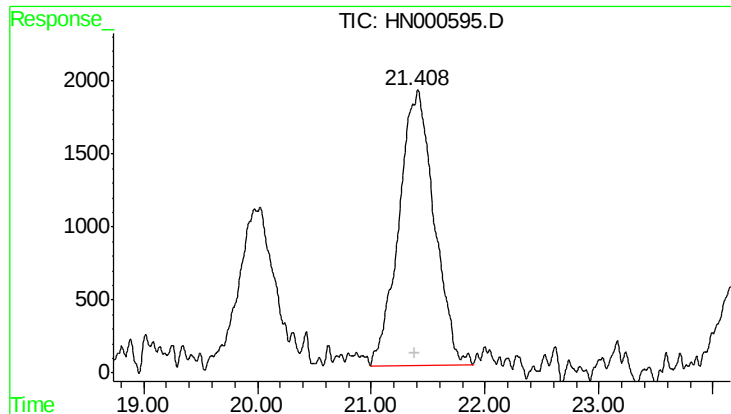

#9 2,4-Dinitrotoluene


R.T.: 21.410 min
Delta R.T.: 0.027 min
Response: 404832
Conc: 10.54 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-1

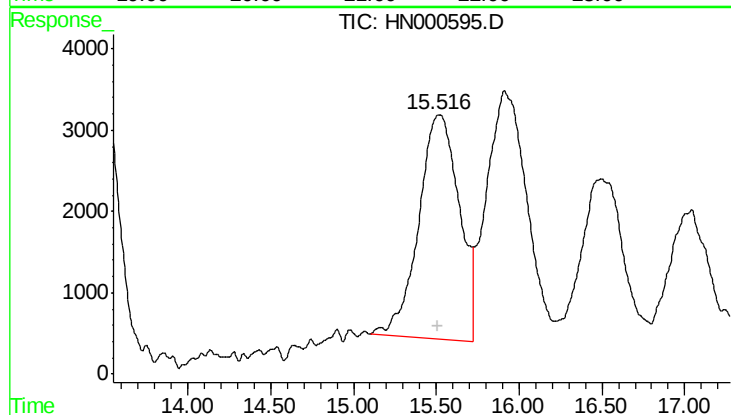


#11 1,3-Dinitrobenzene

R.T.: 15.519 min
Delta R.T.: 0.007 min
Response: 473040
Conc: 11.20 ug/L

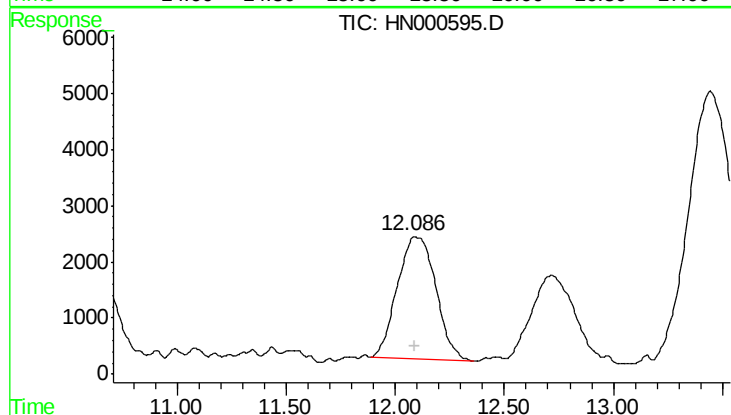


#12 Nitrobenzene

R.T.: 12.092 min
Delta R.T.: 0.000 min
Response: 268256
Conc: 10.24 ug/L

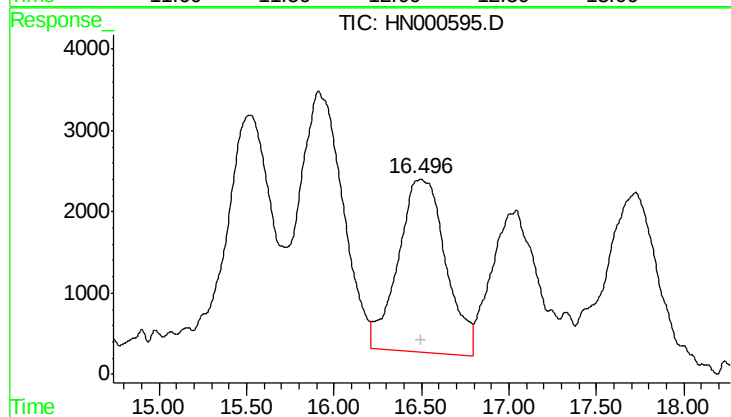

#13 2-Nitrotoluene


R.T.: 16.495 min
Delta R.T.: -0.002 min
Response: 405012
Conc: 23.96 ug/L

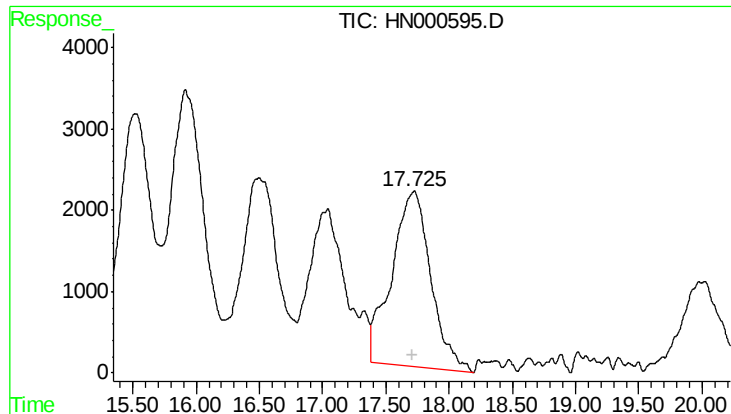

#14 3-Nitrotoluene

R.T.: 17.721 min
Delta R.T.: 0.016 min
Response: 466494
Conc: 25.74 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-1

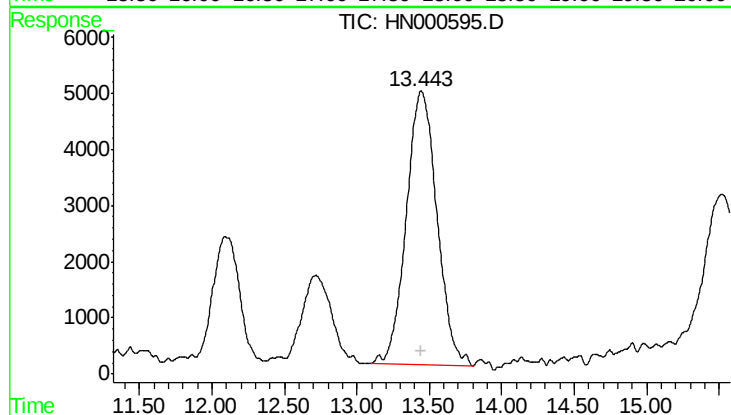

#16 3,5-Dinitroaniline

R.T.: 13.445 min
Delta R.T.: 0.004 min
Response: 715887
Conc: 21.45 ug/L