

Data Path : S:\HPCHEM1\HPLC_N\Data\HN112012\
 Data File : HN000600.D
 Signal(s) : VWD1A.CH
 Acq On : 20-Nov-2012, 21:33
 Operator : HLM
 Sample : 8330-ICV
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 HPLC_N
 LabSampleId :
 8330-ICV

Integration File: events.e
 Quant Time: Nov 22 03:09:56 2012
 Quant Method : S:\HPCHEM1\HPLC_N\Method\HN112012.M
 Quant Title : SW8330 / 8330A confirmation
 QLast Update : Wed Nov 21 16:37:45 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc	Units

System Monitoring Compounds				
Target Compounds				
2) T HMX	12.765	10348397	1026.095	ug/L
3) T RDX	10.625	14382365	1043.037	ug/L
4) T 1,3,5-Trinitrobenzene	24.428	29772219	1065.815	ug/L
5) T Tetryl	34.486	23280631	1079.349	ug/L
6) T 2,4,6-Trinitrotoluene	32.740	29000384	1070.310	ug/L
7) T 2-Amino-4,6-dinitroto...	15.972	48999477	1027.451	ug/L
8) T 4-Amino-2,6-dinitroto...	15.972	48999477	1021.472	ug/L
9) T 2,4-Dinitrotoluene	21.450	37058603	964.657	ug/L
10) T 2,6-Dinitrotoluene	20.043	19790307	973.991	ug/L
11) T 1,3-Dinitrobenzene	15.554	40730815	964.029	ug/L
12) T Nitrobenzene	12.119	26848472	1024.394	ug/L
13) T 2-Nitrotoluene	16.539	17350390	1026.558	ug/L
14) T 3-Nitrotoluene	17.750	18260728	1007.624	ug/L
15) T 4-Nitrotoluene	17.061	14500591	1040.057	ug/L
16) T 3,5-Dinitroaniline	13.482	33142250	992.890	ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_N\Data\HN112012\
Data File : HN000600.D
Signal(s) : VWD1A.CH
Acq On : 20-Nov-2012, 21:33
Operator : HLM
Sample : 8330-ICV
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
HPLC_N
LabSampleId :
8330-ICV

Integration File: events.e
Quant Time: Nov 22 03:09:56 2012
Quant Method : S:\HPCHEM1\HPLC_N\Method\HN112012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Wed Nov 21 16:37:45 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

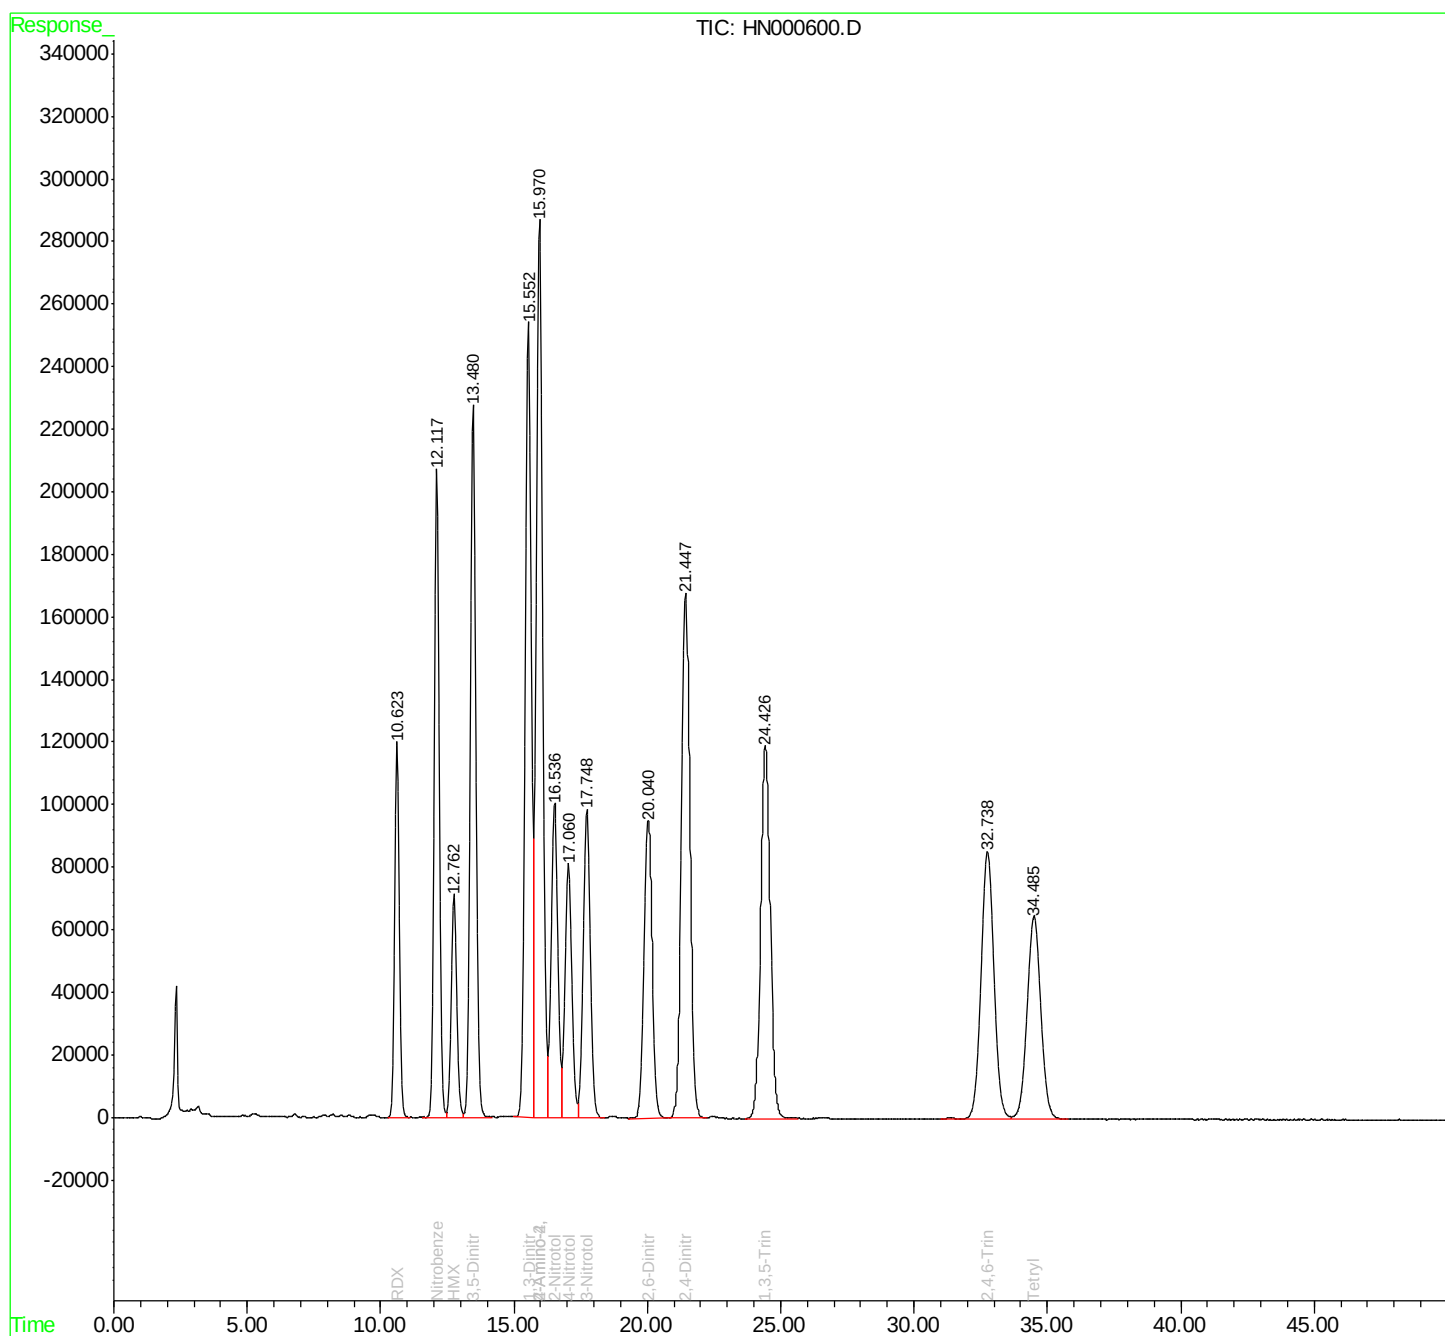


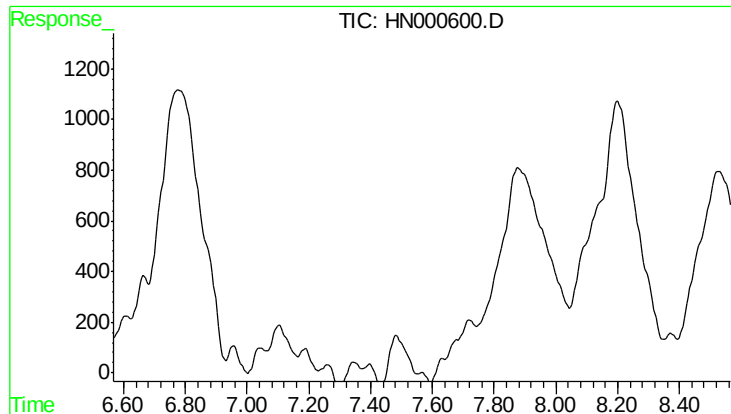

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 7.566 min
Response: 0
Conc: N.D.

Instrument :
HPLC_N
LabSampleId :
8330-ICV

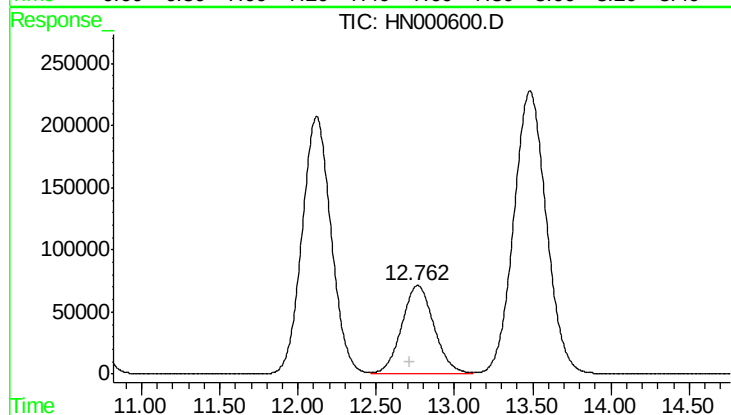


#2 HMX

R.T.: 12.765 min
Delta R.T.: 0.050 min
Response: 10348397
Conc: 1026.10 ug/L

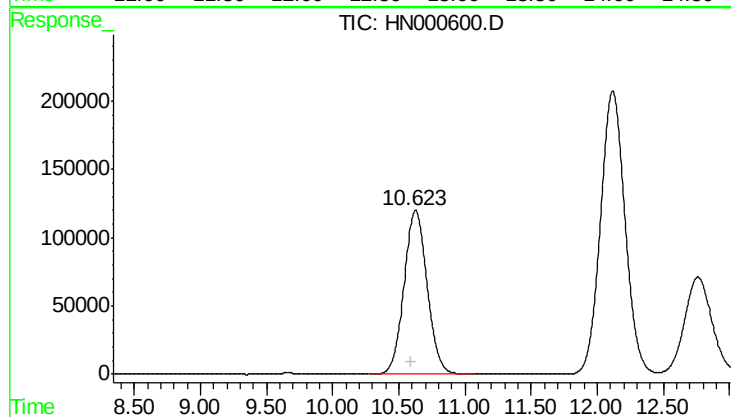


#3 RDX

R.T.: 10.625 min
Delta R.T.: 0.031 min
Response: 14382365
Conc: 1043.04 ug/L

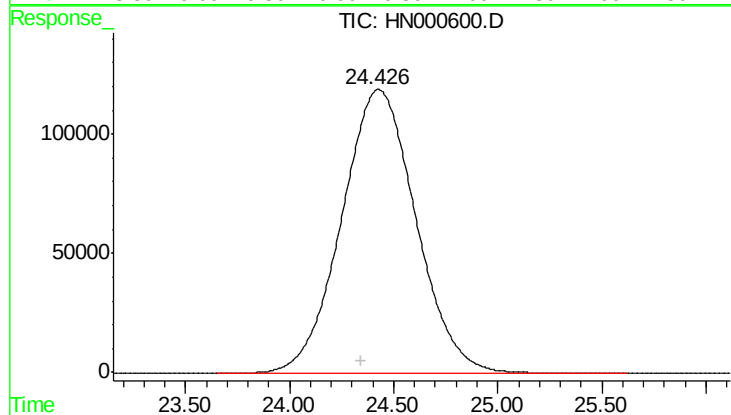

#4 1,3,5-Trinitrobenzene


R.T.: 24.428 min
Delta R.T.: 0.087 min
Response: 29772219
Conc: 1065.81 ug/L

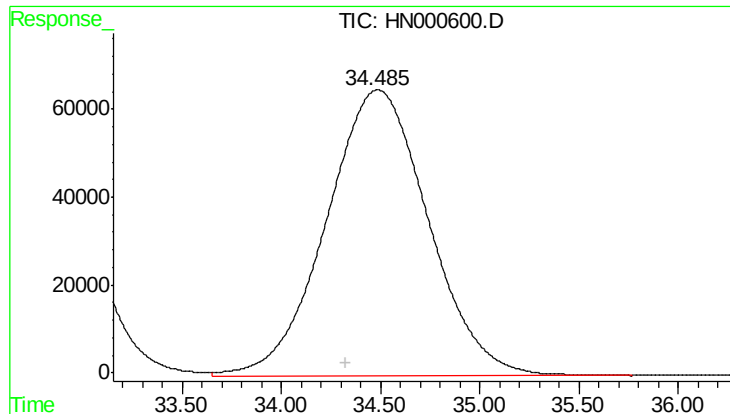

#5 Tetryl


R.T.: 34.486 min
Delta R.T.: 0.164 min
Response: 23280631
Conc: 1079.35 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-ICV

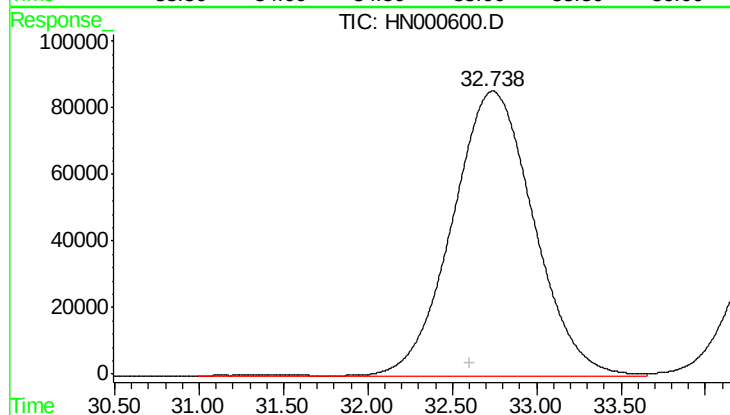


#6 2,4,6-Trinitrotoluene

R.T.: 32.740 min
Delta R.T.: 0.138 min
Response: 29000384
Conc: 1070.31 ug/L

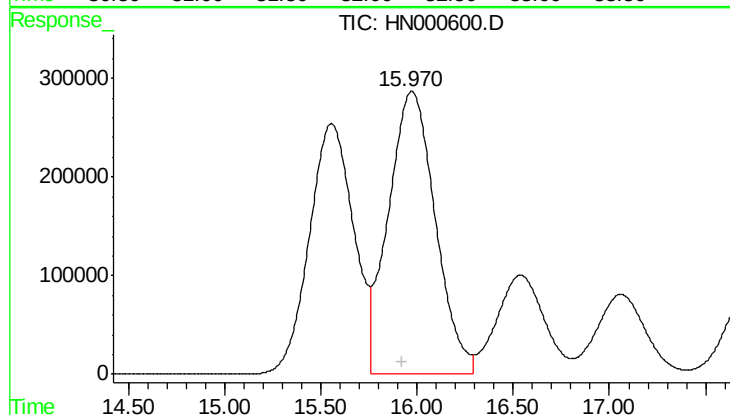


#7 2-Amino-4,6-dinitrotoluene

R.T.: 15.972 min
Delta R.T.: 0.052 min
Response: 48999477
Conc: 1027.45 ug/L

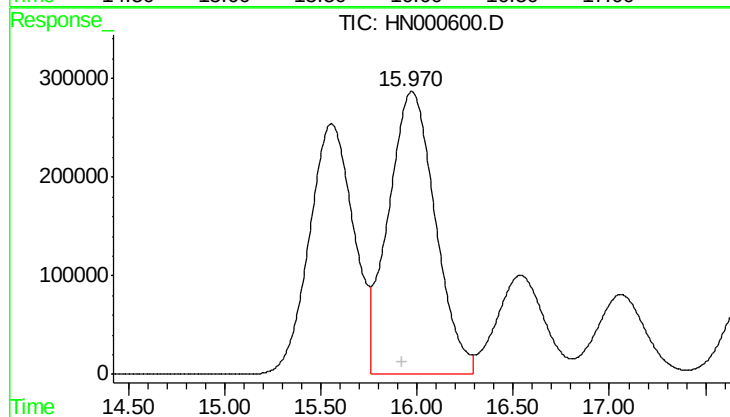

#8 4-Amino-2,6-dinitrotoluene


R.T.: 15.972 min
Delta R.T.: 0.052 min
Response: 48999477
Conc: 1021.47 ug/L

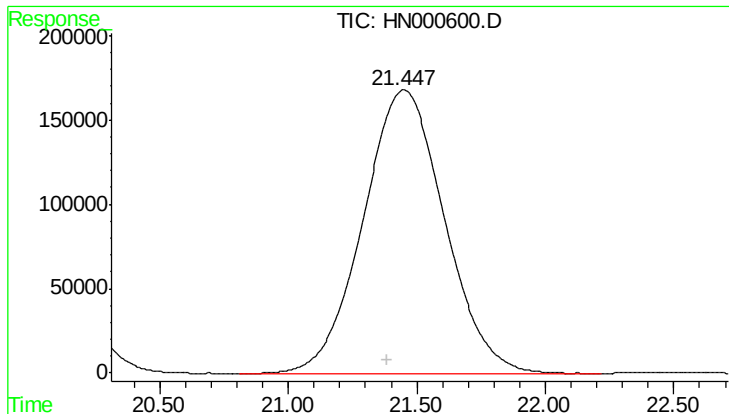

#9 2,4-Dinitrotoluene


R.T.: 21.450 min
Delta R.T.: 0.067 min
Response: 37058603
Conc: 964.66 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-ICV

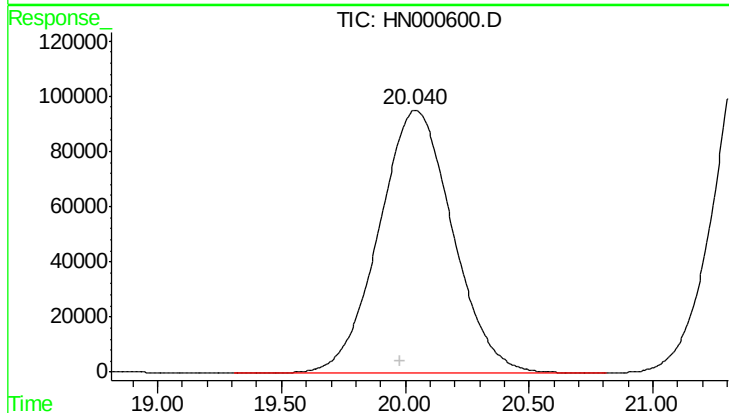


#10 2,6-Dinitrotoluene

R.T.: 20.043 min
Delta R.T.: 0.061 min
Response: 19790307
Conc: 973.99 ug/L

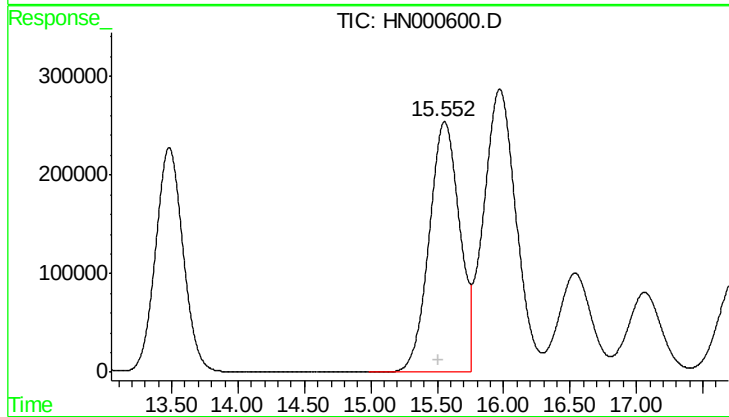


#11 1,3-Dinitrobenzene

R.T.: 15.554 min
Delta R.T.: 0.042 min
Response: 40730815
Conc: 964.03 ug/L

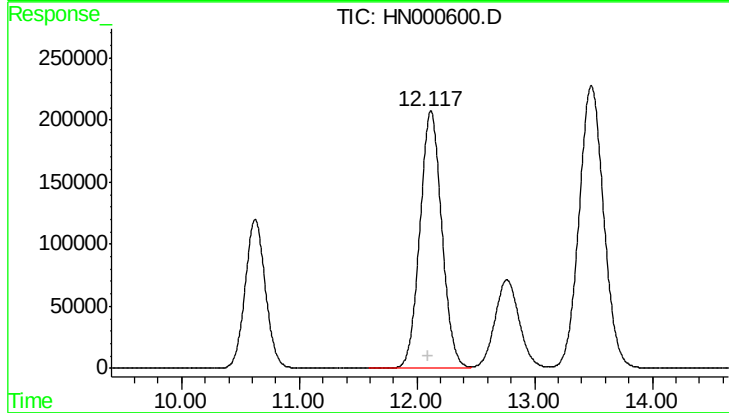

#12 Nitrobenzene


R.T.: 12.119 min
Delta R.T.: 0.027 min
Response: 26848472
Conc: 1024.39 ug/L

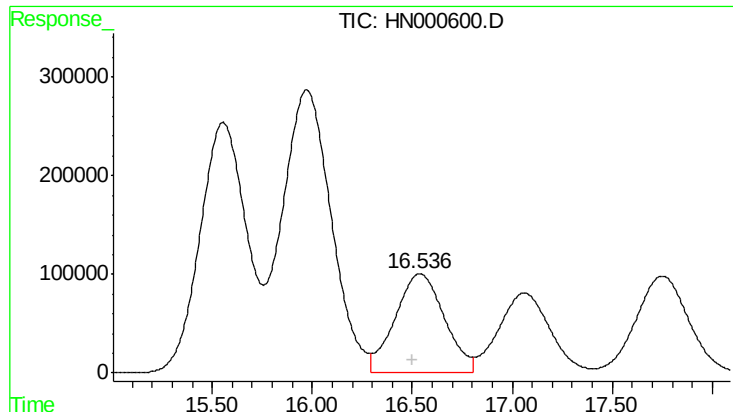

#13 2-Nitrotoluene


R.T.: 16.539 min
 Delta R.T.: 0.041 min
 Response: 17350390
 Conc: 1026.56 ug/L

Instrument :
 HPLC_N
 LabSampleId :
 8330-ICV

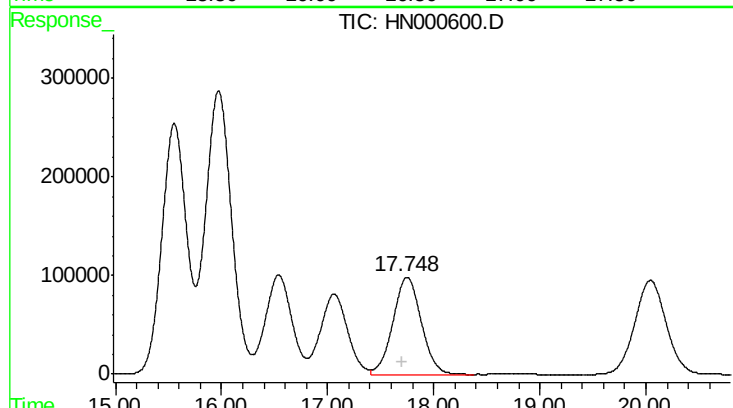


#14 3-Nitrotoluene

R.T.: 17.750 min
 Delta R.T.: 0.045 min
 Response: 18260728
 Conc: 1007.62 ug/L

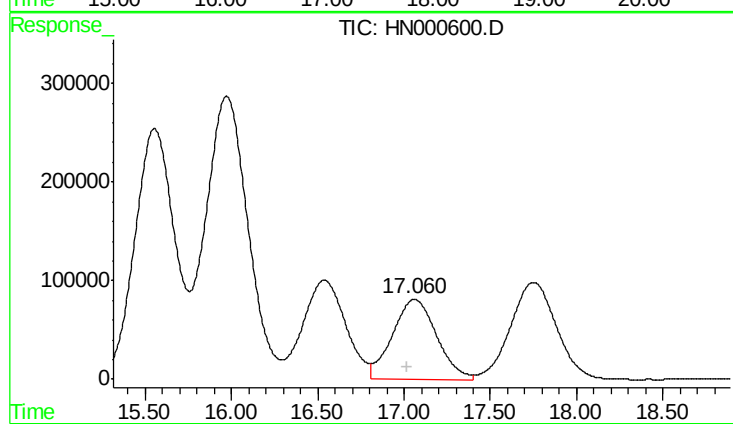

#15 4-Nitrotoluene

R.T.: 17.061 min
 Delta R.T.: 0.043 min
 Response: 14500591
 Conc: 1040.06 ug/L

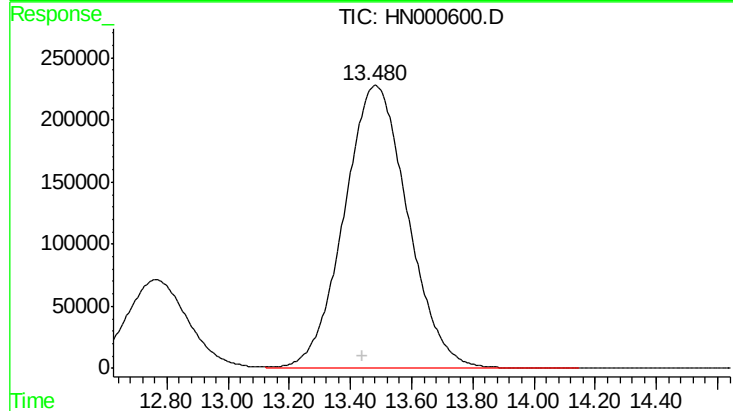

#16 3,5-Dinitroaniline

R.T.: 13.482 min
 Delta R.T.: 0.041 min
 Response: 33142250
 Conc: 992.89 ug/L