

Data Path : S:\HPCHEM1\HPLC_N\Data\HN112012\
 Data File : HN000593.D
 Signal(s) : VWD1A.CH
 Acq On : 20-Nov-2012, 15:25
 Operator : HLM
 Sample : 8330-3
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 HPLC_N
 LabSampleId :
 8330-3

Integration File: events.e
 Quant Time: Nov 22 03:01:25 2012
 Quant Method : H:\VOL1\HPLC\HPLC_N\METHODS\HN112012.M
 Quant Title : SW8330 / 8330A confirmation
 QLast Update : Wed Nov 21 16:28:41 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	7.568	4972104	480.575 ug/L
Target Compounds				
2) T	HMX	12.714	5043140	488.351 ug/L
3) T	RDX	10.595	6873305	493.293 ug/L
4) T	1,3,5-Trinitrobenzene	24.342	7018228	251.843 ug/L
5) T	Tetryl	34.329	10739526	496.922 ug/L
6) T	2,4,6-Trinitrotoluene	32.609	6669982	248.395 ug/L
7) T	2-Amino-4,6-dinitroto...	15.922	11981964	256.650 ug/L
8) T	4-Amino-2,6-dinitroto...	15.922	11981964	256.650 ug/L
9) T	2,4-Dinitrotoluene	21.385	9482262	250.335 ug/L
10) T	2,6-Dinitrotoluene	19.983	4885137	249.070 ug/L
11) T	1,3-Dinitrobenzene	15.514	10241028	253.127 ug/L
12) T	Nitrobenzene	12.094	6500196	248.852 ug/L
13) T	2-Nitrotoluene	16.500	8618358	539.216 ug/L
14) T	3-Nitrotoluene	17.709	9133243	490.969 ug/L
15) T	4-Nitrotoluene	17.021	7276982	533.215 ug/L
16) T	3,5-Dinitroaniline	13.442	16471612	492.573 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_N\Data\HN112012\
Data File : HN000593.D
Signal(s) : VWD1A.CH
Acq On : 20-Nov-2012, 15:25
Operator : HLM
Sample : 8330-3
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
HPLC_N
LabSampleId :
8330-3

Integration File: events.e
Quant Time: Nov 22 03:01:25 2012
Quant Method : H:\VOL1\HPLC\HPLC_N\METHODS\HN112012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Wed Nov 21 16:28:41 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

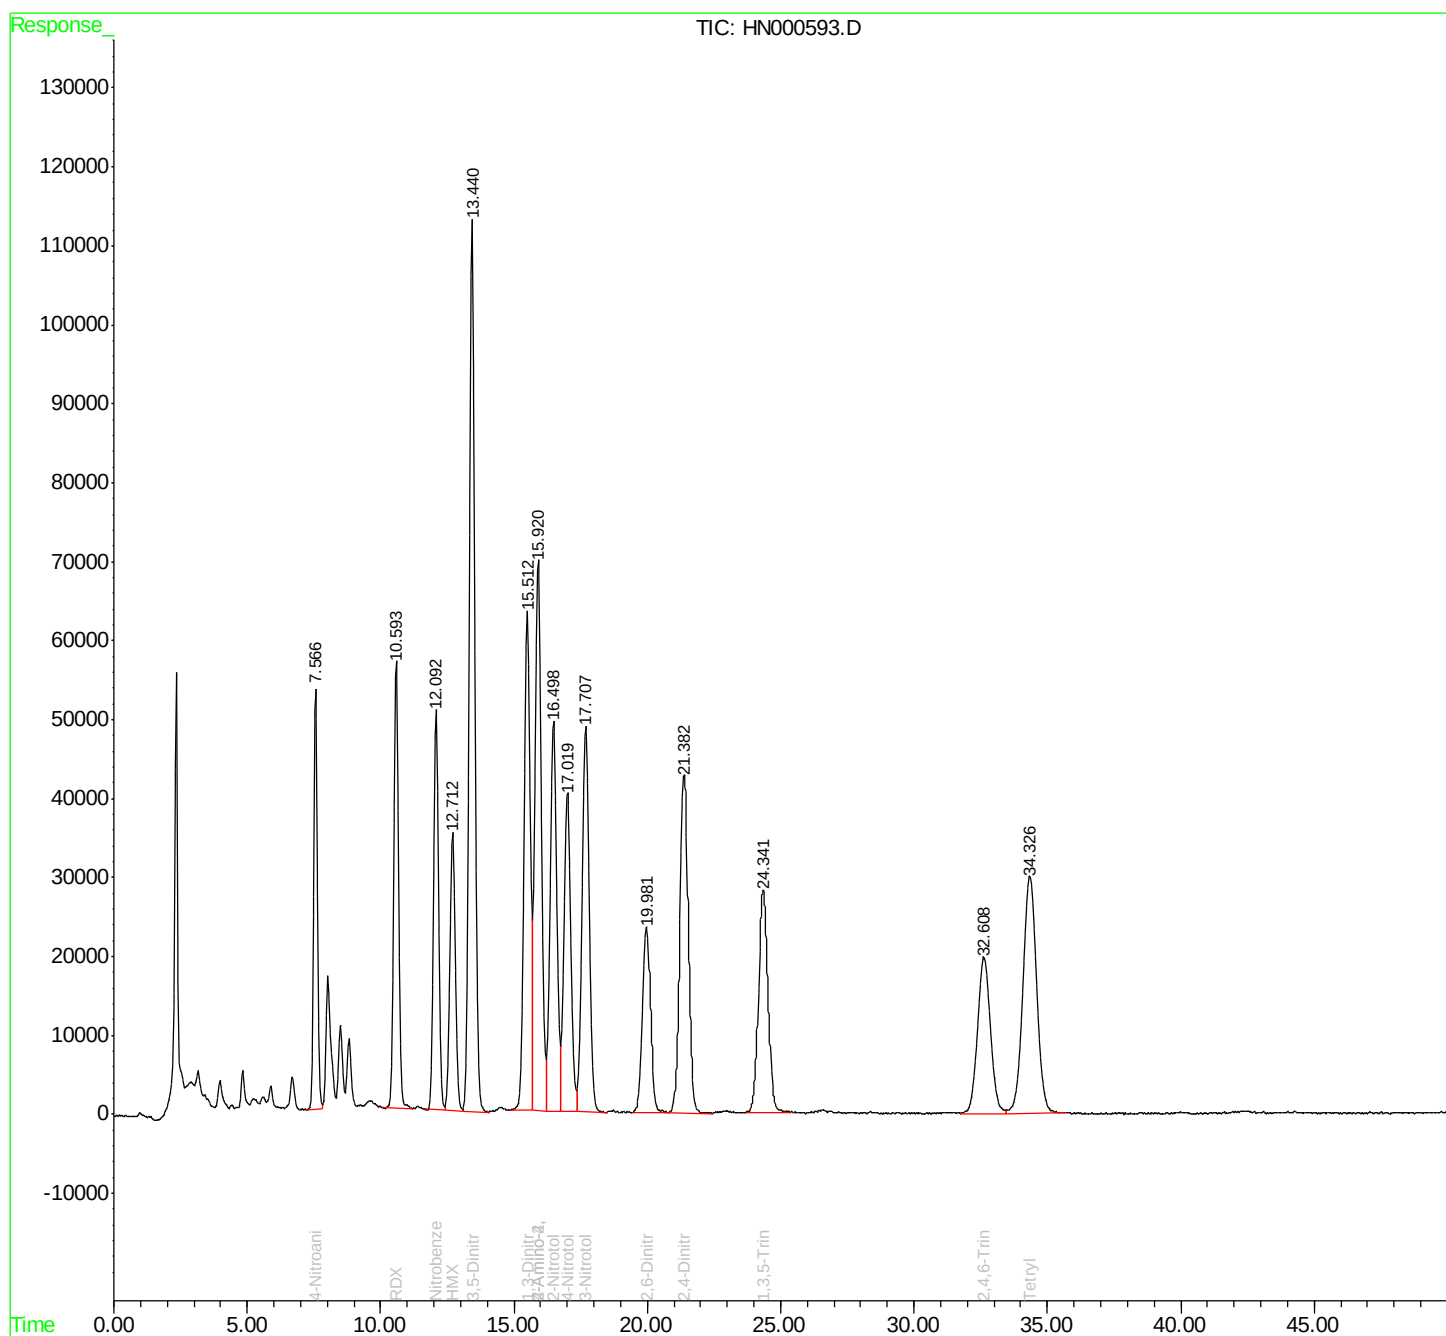


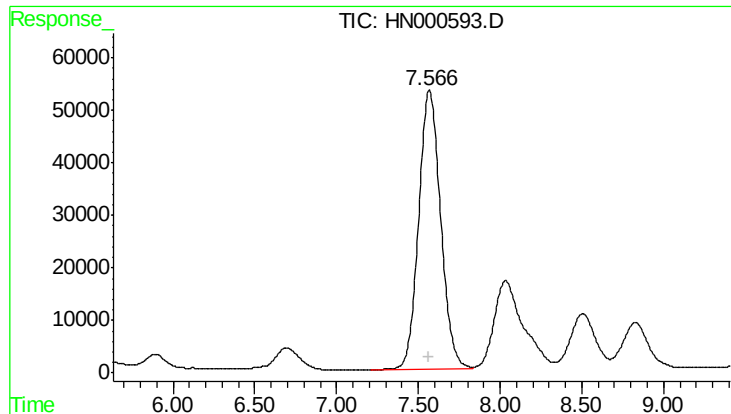

#1 4-Nitroaniline


R.T.: 7.568 min
Delta R.T.: 0.005 min
Response: 4972104
Conc: 480.57 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-3

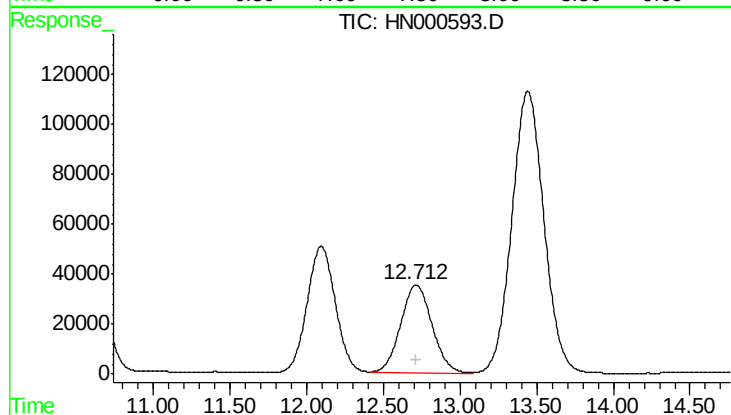


#2 HMX

R.T.: 12.714 min
Delta R.T.: 0.001 min
Response: 5043140
Conc: 488.35 ug/L

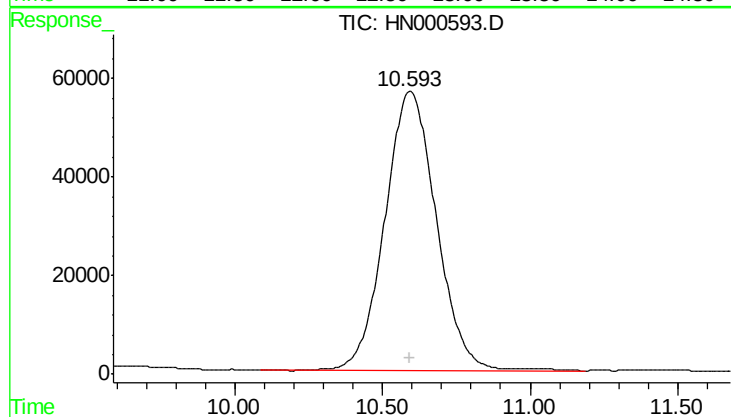


#3 RDX

R.T.: 10.595 min
Delta R.T.: 0.003 min
Response: 6873305
Conc: 493.29 ug/L

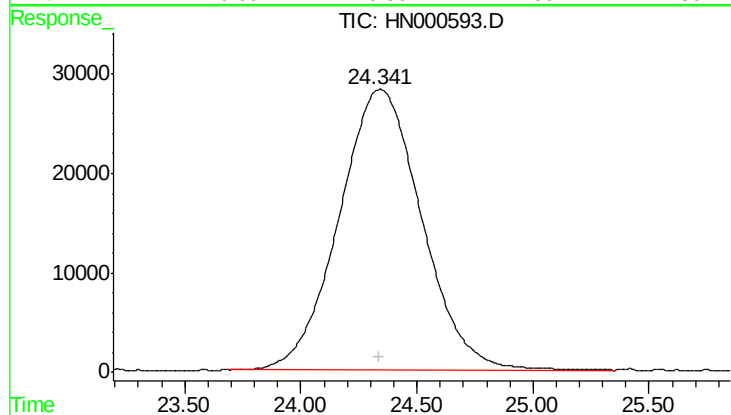

#4 1,3,5-Trinitrobenzene


R.T.: 24.342 min
Delta R.T.: 0.003 min
Response: 7018228
Conc: 251.84 ug/L

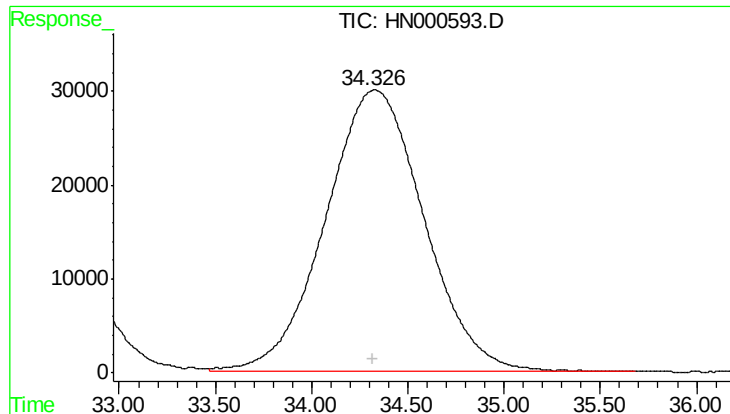

#5 Tetryl


R.T.: 34.329 min
Delta R.T.: 0.009 min
Response: 10739526
Conc: 496.92 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-3

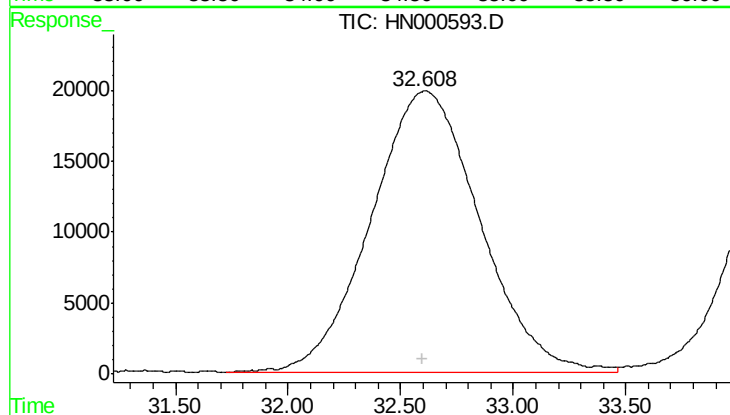


#6 2,4,6-Trinitrotoluene

R.T.: 32.609 min
Delta R.T.: 0.010 min
Response: 6669982
Conc: 248.39 ug/L

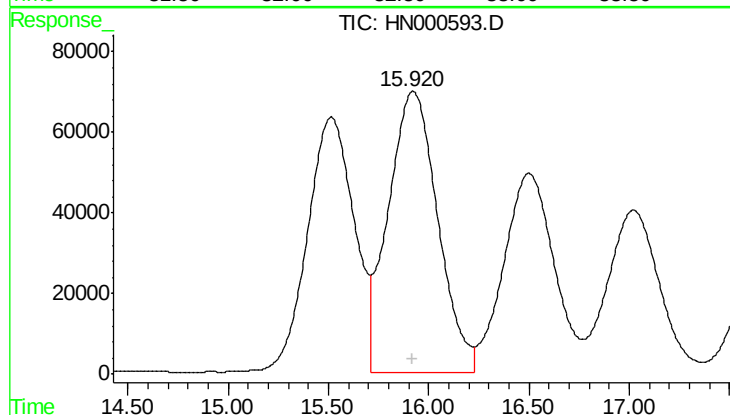


#7 2-Amino-4,6-dinitrotoluene

R.T.: 15.922 min
Delta R.T.: 0.004 min
Response: 11981964
Conc: 256.65 ug/L

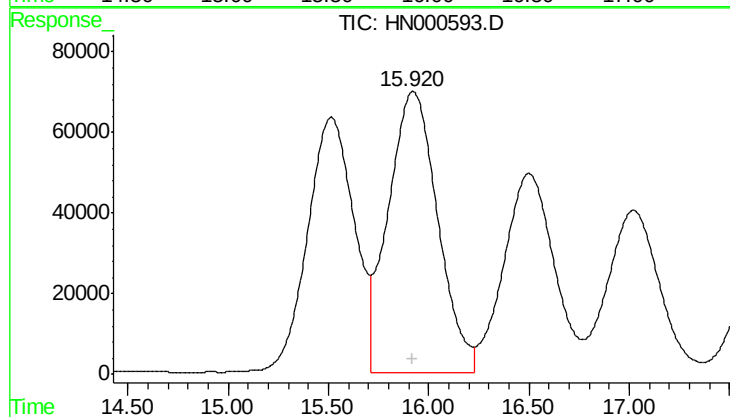

#8 4-Amino-2,6-dinitrotoluene


R.T.: 15.922 min
Delta R.T.: 0.004 min
Response: 11981964
Conc: 256.65 ug/L

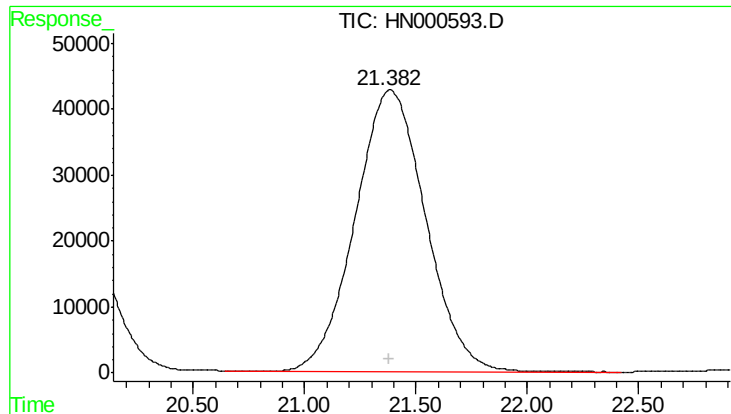

#9 2,4-Dinitrotoluene


R.T.: 21.385 min
Delta R.T.: 0.004 min
Response: 9482262
Conc: 250.34 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-3

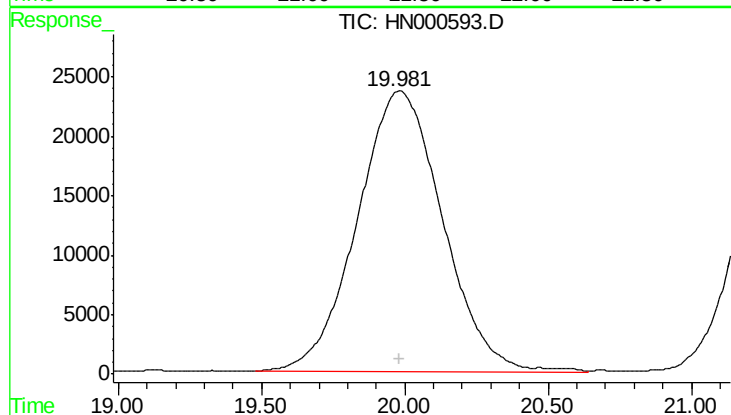


#10 2,6-Dinitrotoluene

R.T.: 19.983 min
Delta R.T.: 0.003 min
Response: 4885137
Conc: 249.07 ug/L

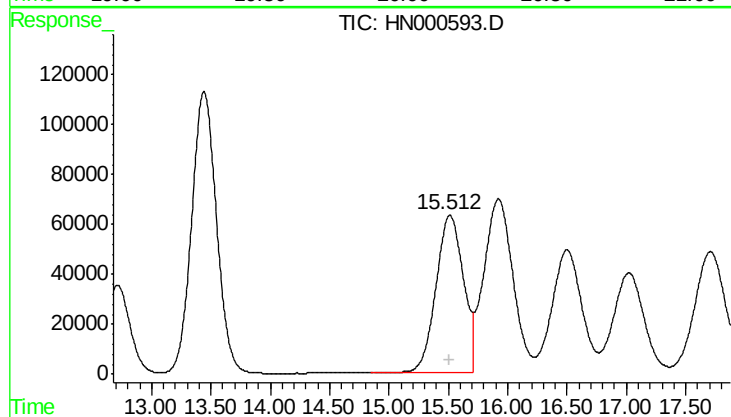


#11 1,3-Dinitrobenzene

R.T.: 15.514 min
Delta R.T.: 0.004 min
Response: 10241028
Conc: 253.13 ug/L

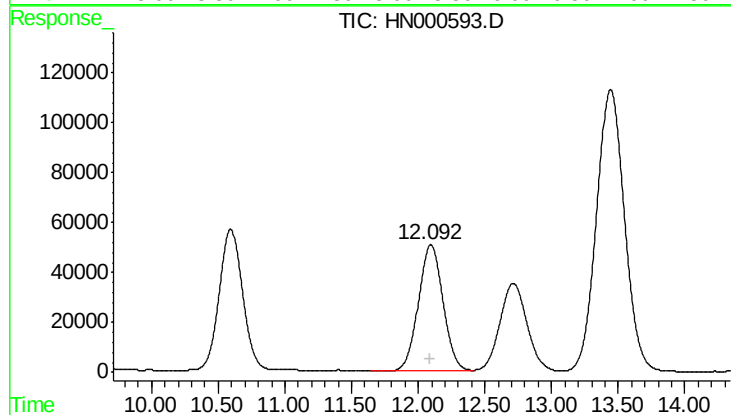

#12 Nitrobenzene


R.T.: 12.094 min
Delta R.T.: 0.004 min
Response: 6500196
Conc: 248.85 ug/L

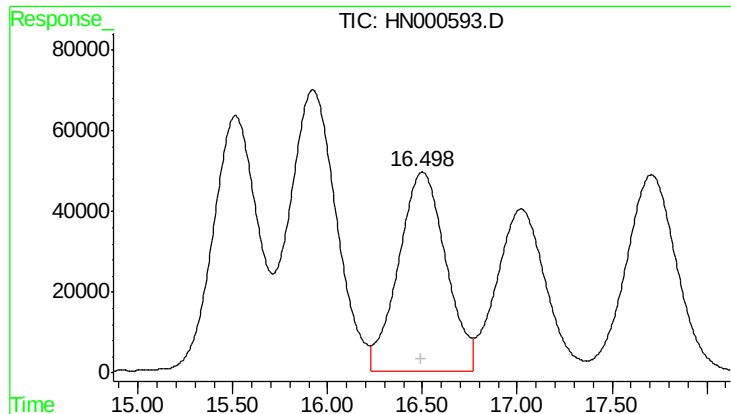

#13 2-Nitrotoluene


R.T.: 16.500 min
Delta R.T.: 0.005 min
Response: 8618358
Conc: 539.22 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-3

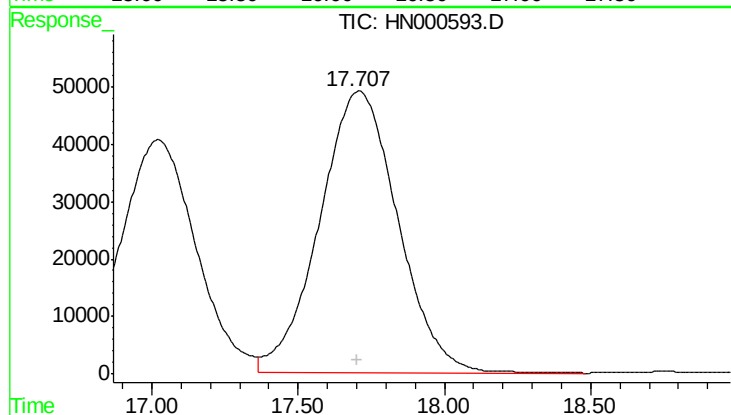


#14 3-Nitrotoluene

R.T.: 17.709 min
Delta R.T.: 0.006 min
Response: 9133243
Conc: 490.97 ug/L

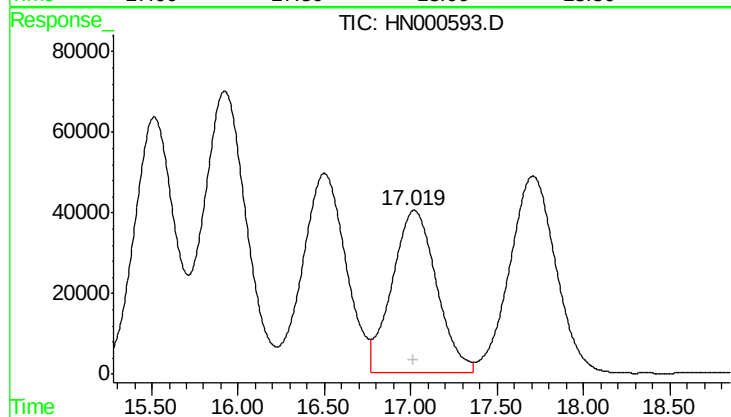

#15 4-Nitrotoluene

R.T.: 17.021 min
Delta R.T.: 0.005 min
Response: 7276982
Conc: 533.21 ug/L

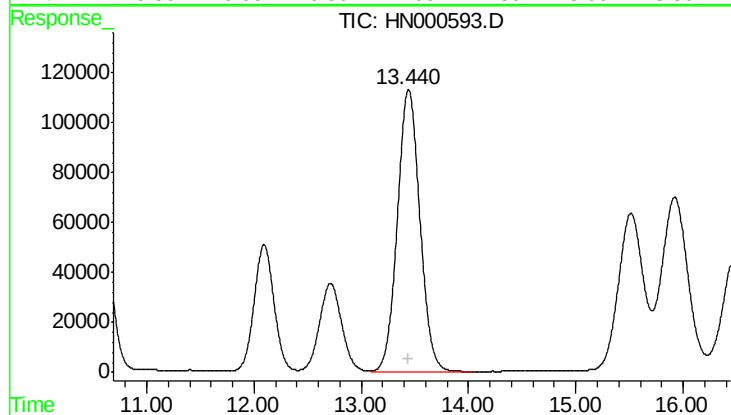

#16 3,5-Dinitroaniline

R.T.: 13.442 min
Delta R.T.: 0.003 min
Response: 16471612
Conc: 492.57 ug/L