

Data Path : S:\HPCHEM1\HPLC_N\Data\HN112012\
 Data File : HN000594.D
 Signal(s) : VWD1A.CH
 Acq On : 20-Nov-2012, 16:18
 Operator : HLM
 Sample : 8330-2
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 HPLC_N
 LabSampleId :
 8330-2

Integration File: events.e
 Quant Time: Nov 22 00:47:48 2012
 Quant Method : H:\VOL1\HPLC\HPLC_N\METHODS\HN112012.M
 Quant Title : SW8330 / 8330A confirmation
 QLast Update : Wed Nov 21 16:28:41 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	7.573	981429	94.859 ug/L
Target Compounds				
2) T	HMX	12.725	989837	95.851 ug/L
3) T	RDX	10.602	1340231	96.188 ug/L
4) T	1,3,5-Trinitrobenzene	24.356	1390182	49.885 ug/L
5) T	Tetryl	34.341	2209828	102.250 ug/L
6) T	2,4,6-Trinitrotoluene	32.645	1414071	52.661 ug/L
7) T	2-Amino-4,6-dinitroto...	15.929	2457806	52.646 ug/L
8) T	4-Amino-2,6-dinitroto...	15.929	2457806	52.646 ug/L
9) T	2,4-Dinitrotoluene	21.397	1935250	51.091 ug/L
10) T	2,6-Dinitrotoluene	19.984	1033673	52.702 ug/L
11) T	1,3-Dinitrobenzene	15.522	2185182	54.011 ug/L
12) T	Nitrobenzene	12.100	1273310	48.747 ug/L
13) T	2-Nitrotoluene	16.505	1771545	110.838 ug/L
14) T	3-Nitrotoluene	17.716	1917621	94.784 ug/L
15) T	4-Nitrotoluene	17.023	1493292	109.420 ug/L
16) T	3,5-Dinitroaniline	13.448	3265030	97.639 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_N\Data\HN112012\
Data File : HN000594.D
Signal(s) : VWD1A.CH
Acq On : 20-Nov-2012, 16:18
Operator : HLM
Sample : 8330-2
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
HPLC_N
LabSampleId :
8330-2

Integration File: events.e
Quant Time: Nov 22 00:47:48 2012
Quant Method : H:\VOL1\HPLC\HPLC_N\METHODS\HN112012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Wed Nov 21 16:28:41 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

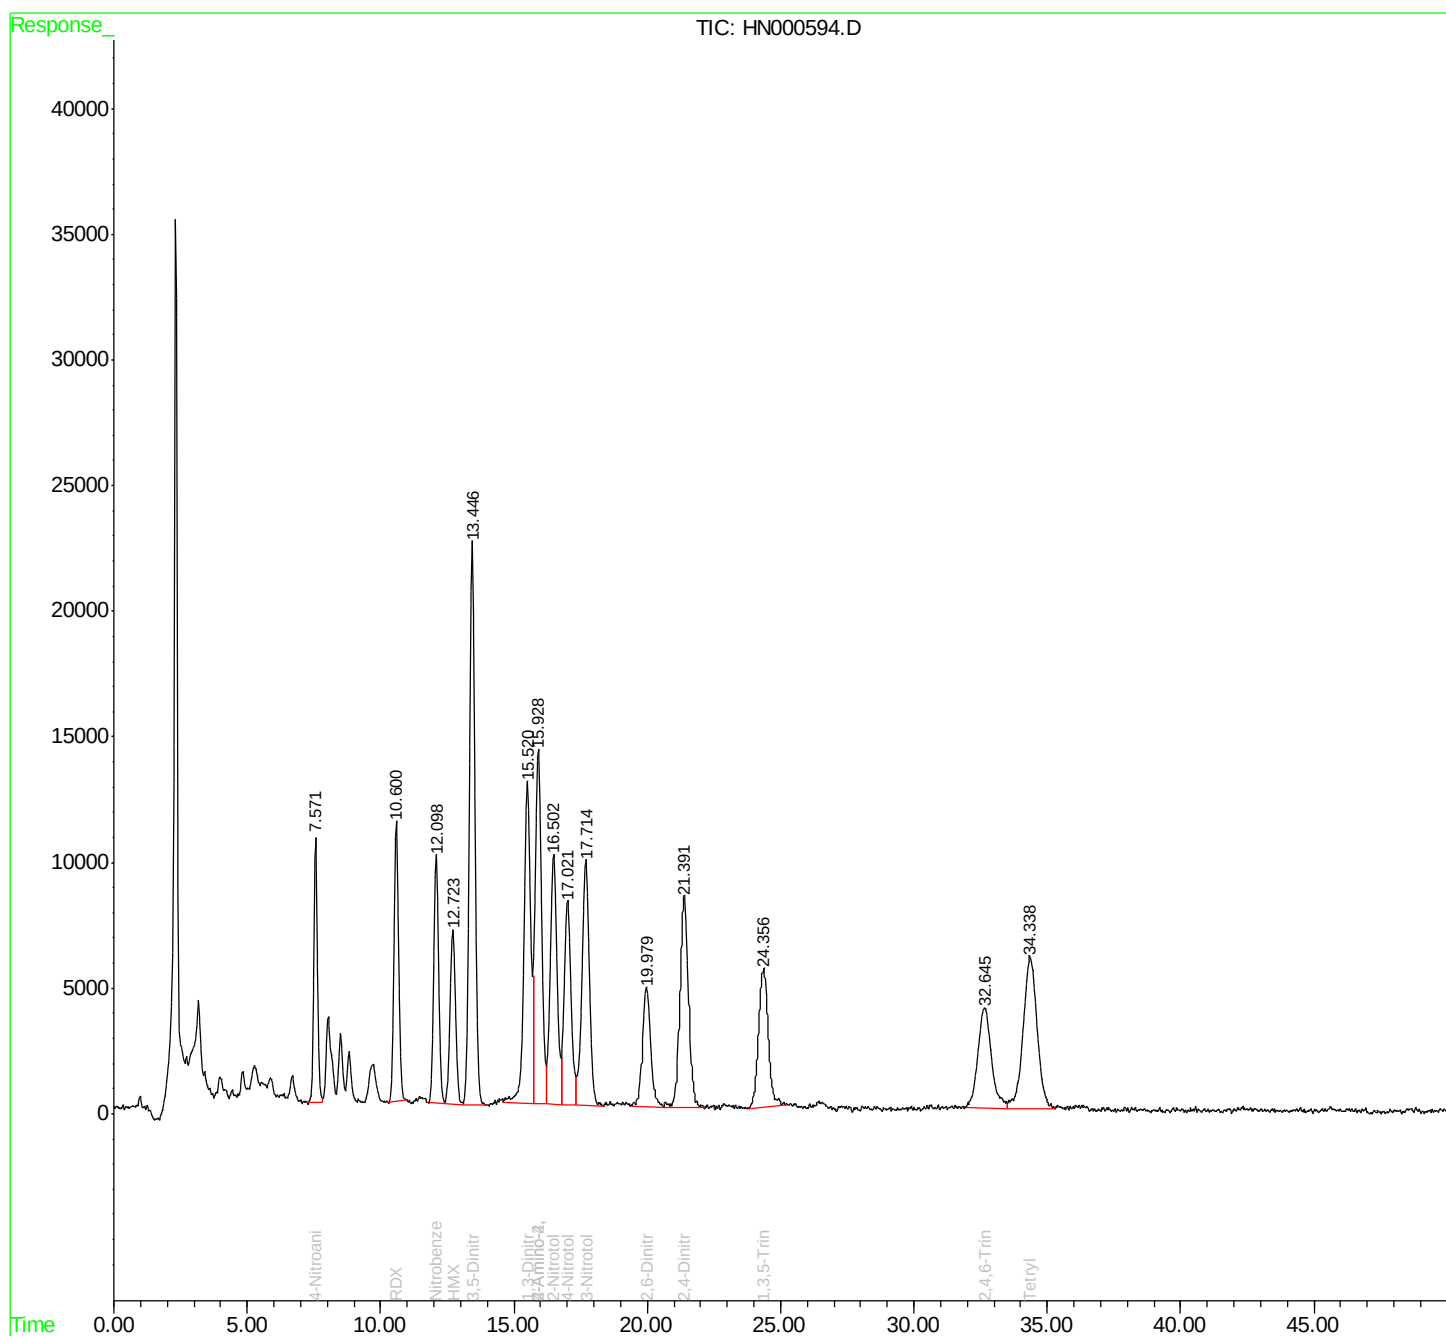


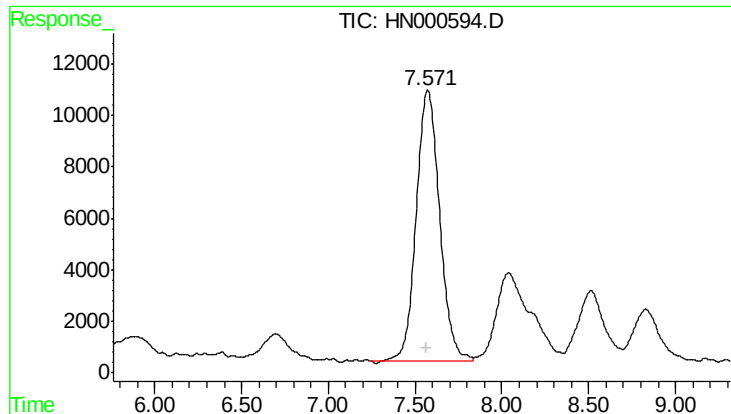

#1 4-Nitroaniline


R.T.: 7.573 min
Delta R.T.: 0.009 min
Response: 981429
Conc: 94.86 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-2

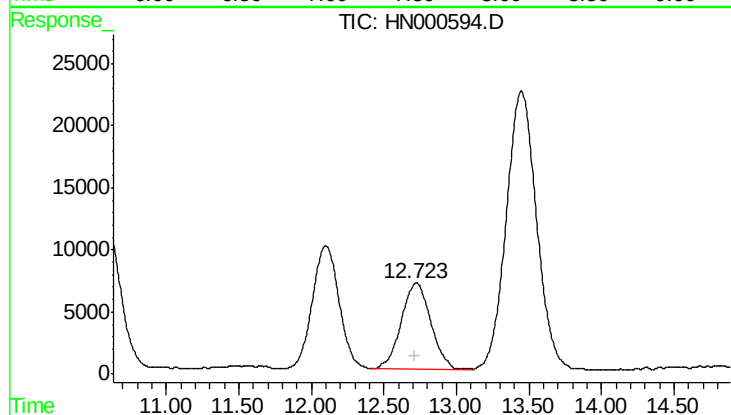


#2 HMX

R.T.: 12.725 min
Delta R.T.: 0.013 min
Response: 989837
Conc: 95.85 ug/L

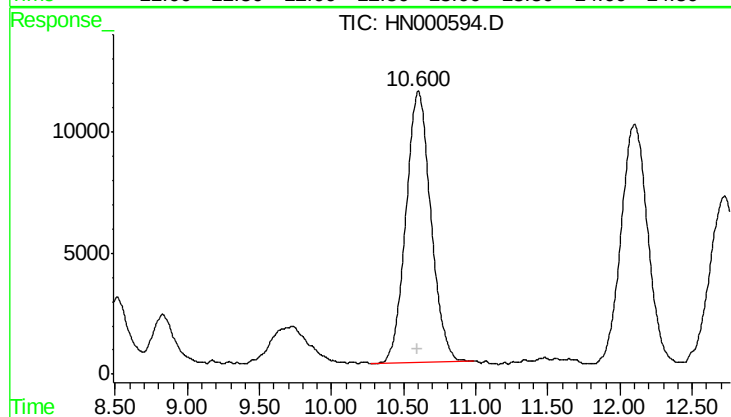


#3 RDX

R.T.: 10.602 min
Delta R.T.: 0.011 min
Response: 1340231
Conc: 96.19 ug/L

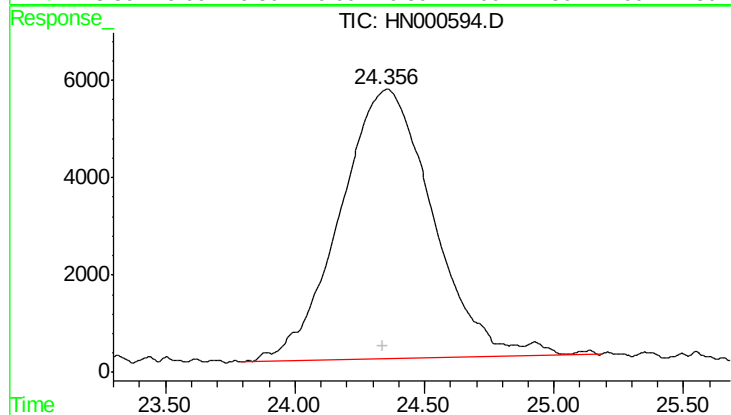

#4 1,3,5-Trinitrobenzene


R.T.: 24.356 min
Delta R.T.: 0.017 min
Response: 1390182
Conc: 49.89 ug/L

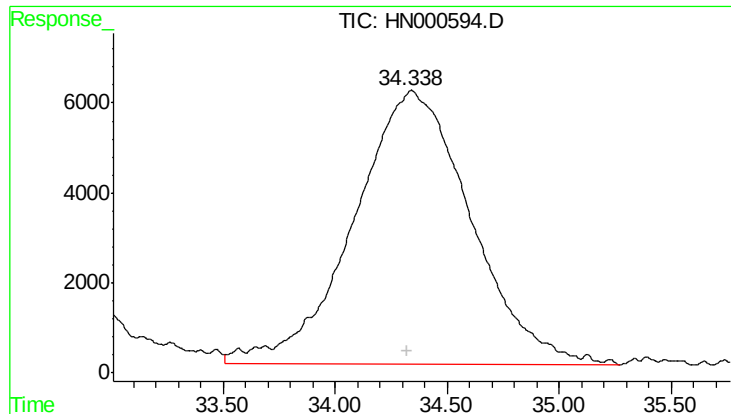

#5 Tetryl


R.T.: 34.341 min
Delta R.T.: 0.022 min
Response: 2209828
Conc: 102.25 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-2

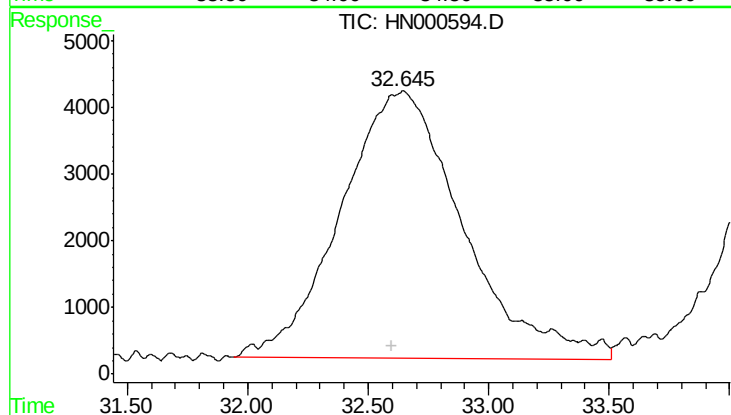


#6 2,4,6-Trinitrotoluene

R.T.: 32.645 min
Delta R.T.: 0.046 min
Response: 1414071
Conc: 52.66 ug/L

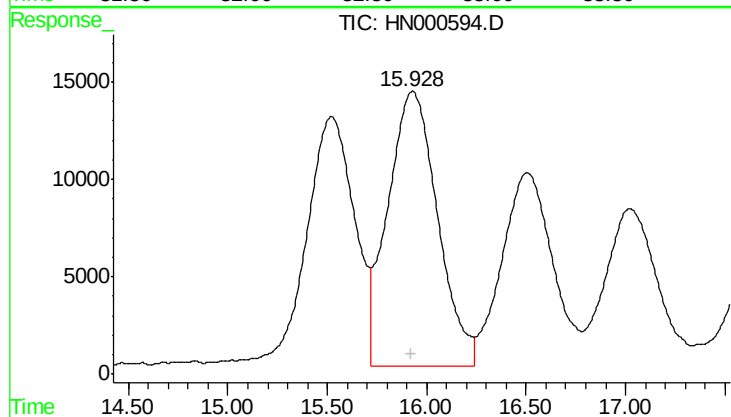


#7 2-Amino-4,6-dinitrotoluene

R.T.: 15.929 min
Delta R.T.: 0.011 min
Response: 2457806
Conc: 52.65 ug/L

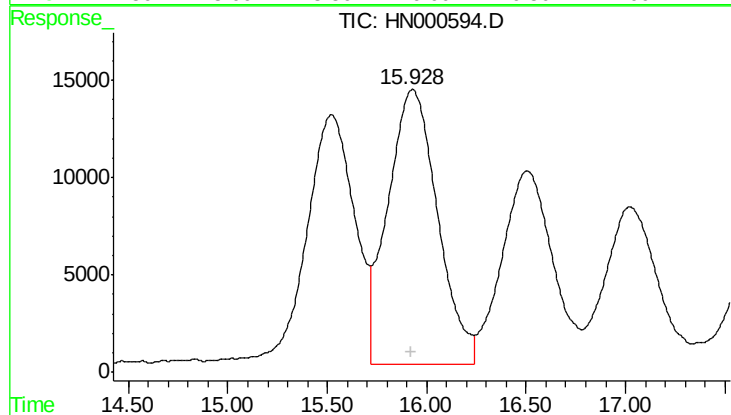

#8 4-Amino-2,6-dinitrotoluene


R.T.: 15.929 min
Delta R.T.: 0.011 min
Response: 2457806
Conc: 52.65 ug/L

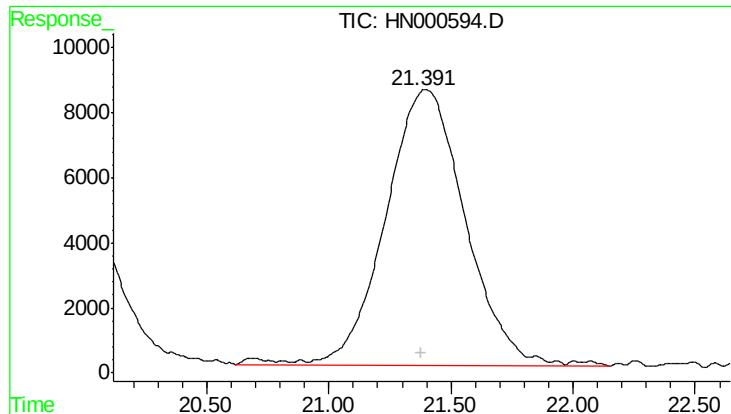

#9 2,4-Dinitrotoluene


R.T.: 21.397 min
Delta R.T.: 0.016 min
Response: 1935250
Conc: 51.09 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-2

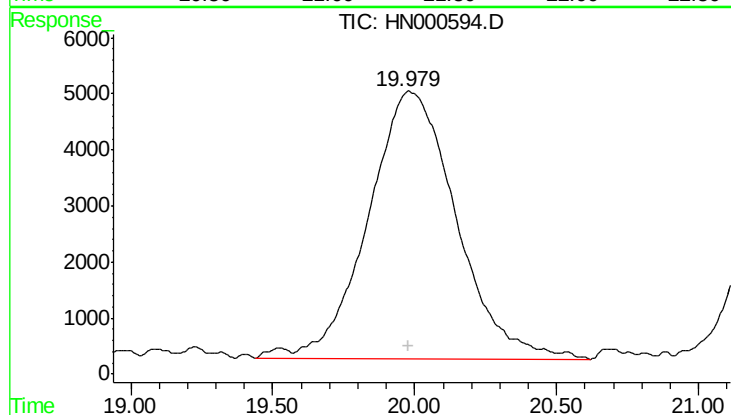


#10 2,6-Dinitrotoluene

R.T.: 19.984 min
Delta R.T.: 0.005 min
Response: 1033673
Conc: 52.70 ug/L

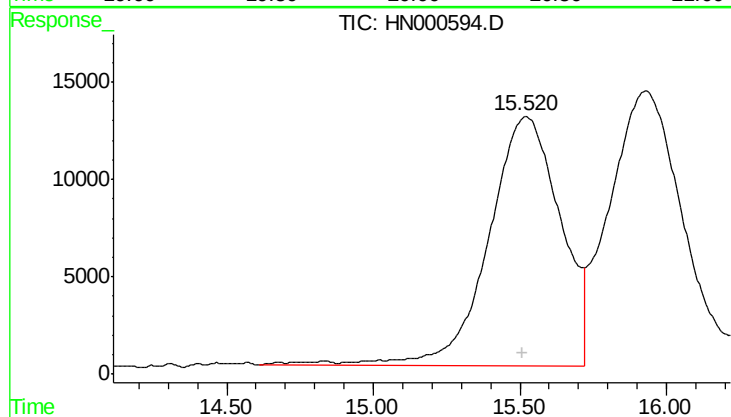


#11 1,3-Dinitrobenzene

R.T.: 15.522 min
Delta R.T.: 0.012 min
Response: 2185182
Conc: 54.01 ug/L

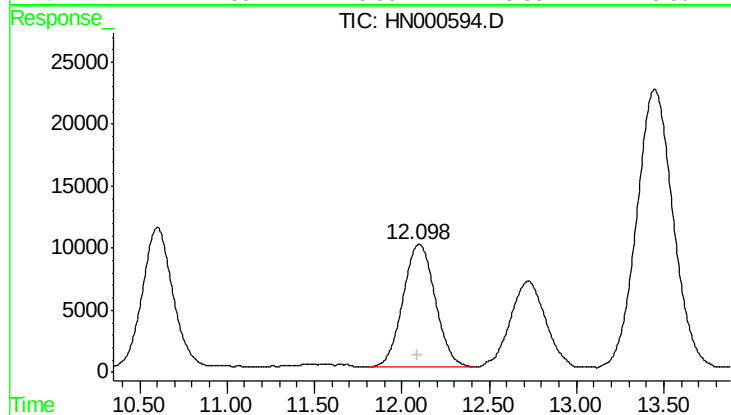

#12 Nitrobenzene


R.T.: 12.100 min
Delta R.T.: 0.010 min
Response: 1273310
Conc: 48.75 ug/L

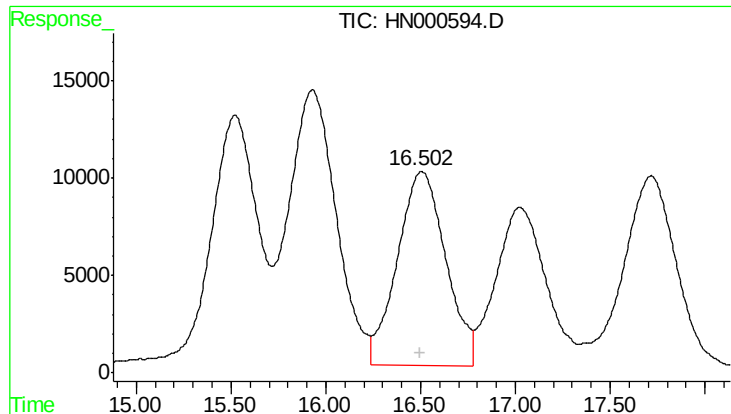

#13 2-Nitrotoluene


R.T.: 16.505 min
Delta R.T.: 0.011 min
Response: 1771545
Conc: 110.84 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-2

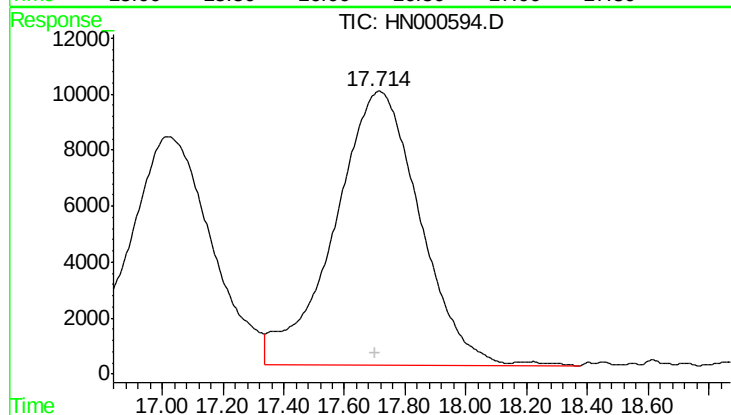


#14 3-Nitrotoluene

R.T.: 17.716 min
Delta R.T.: 0.013 min
Response: 1917621
Conc: 94.78 ug/L

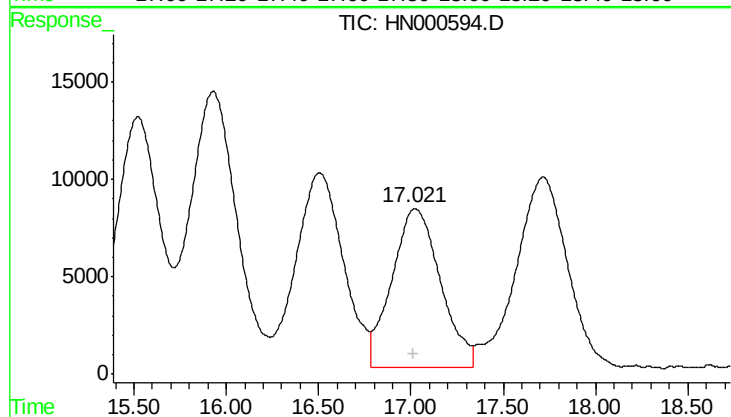

#15 4-Nitrotoluene

R.T.: 17.023 min
Delta R.T.: 0.007 min
Response: 1493292
Conc: 109.42 ug/L

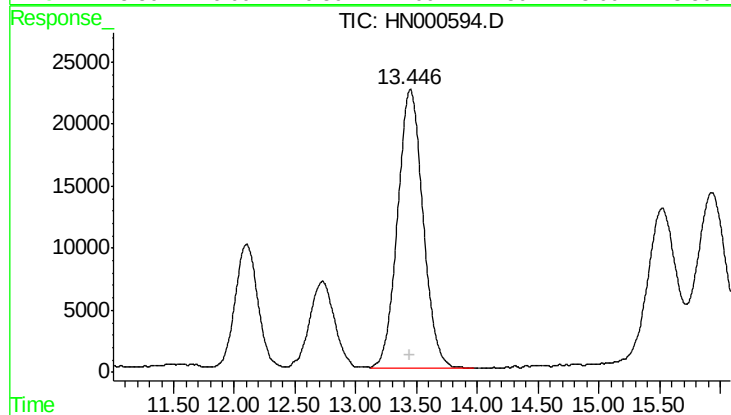

#16 3,5-Dinitroaniline

R.T.: 13.448 min
Delta R.T.: 0.009 min
Response: 3265030
Conc: 97.64 ug/L