

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN010715\HN007200.D\VWD1A.CH Vial: 10
Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN010715\HN007200.D\VWD1A.CH
Acq On : 07-Jan-2015, 18:37 Operator: TP
Sample : PB81205BL Inst : G1314A
Misc : Multiplr: 1.00
IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
Quant Time: Jan 8 10:52 2015 Quant Results File: HN010715.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN010715.M
Title :
Last Update : Thu Jan 08 10:28:20 2015
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.31	2031240	501.157 ug/L m
Target Compounds			

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____ Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.



HN007200.D HN010715.M Mon Jan 12 15:03:57 2015


Quantitation Report

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN010715\HN007200.D\VWD1A.CH Vial: 10
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN010715\HN007200.D\VWD1A.CH
 Acq On : 07-Jan-2015, 18:37 Operator: TP
 Sample : PB81205BL Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
 Quant Time: Jan 8 10:52 2015 Quant Results File: HN010715.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN010715.M
 Title :
 Last Update : Thu Jan 08 10:28:20 2015
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

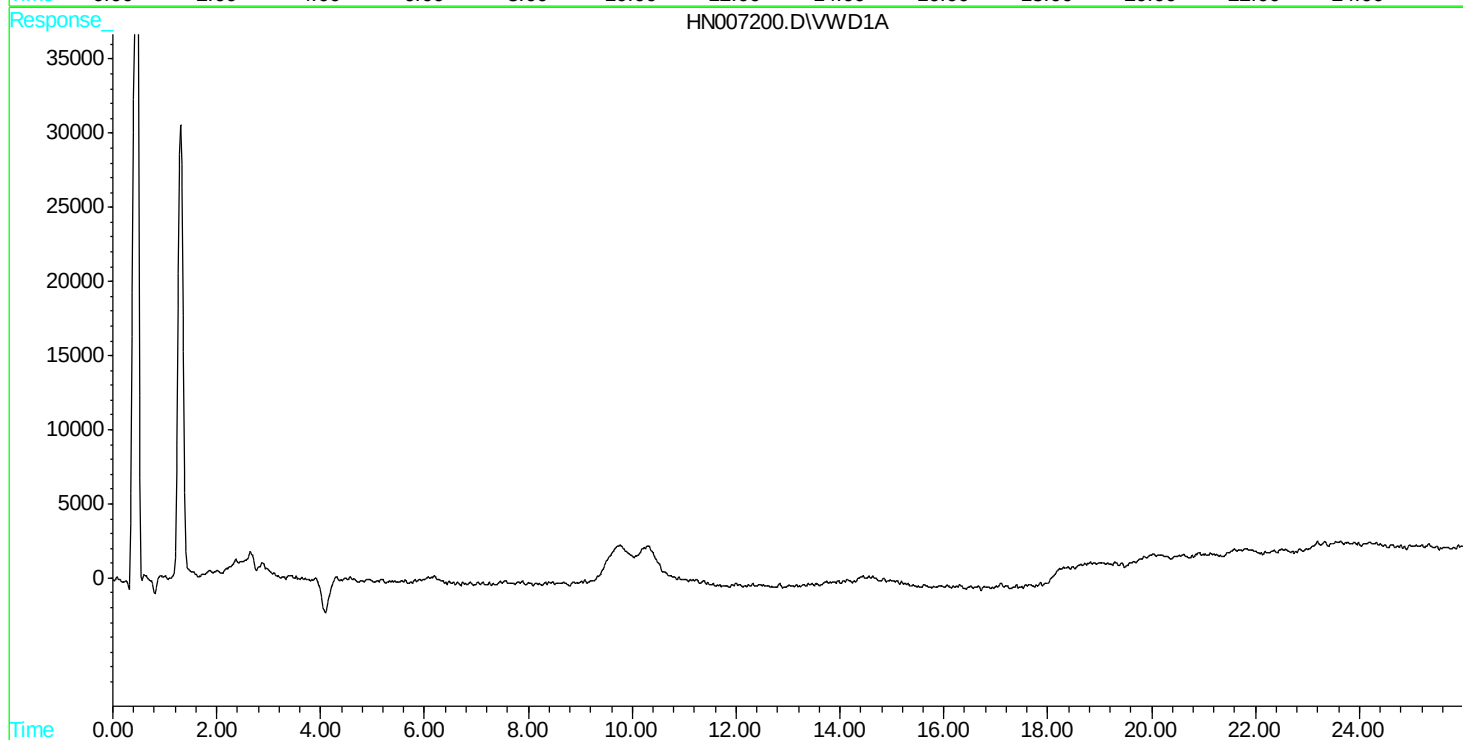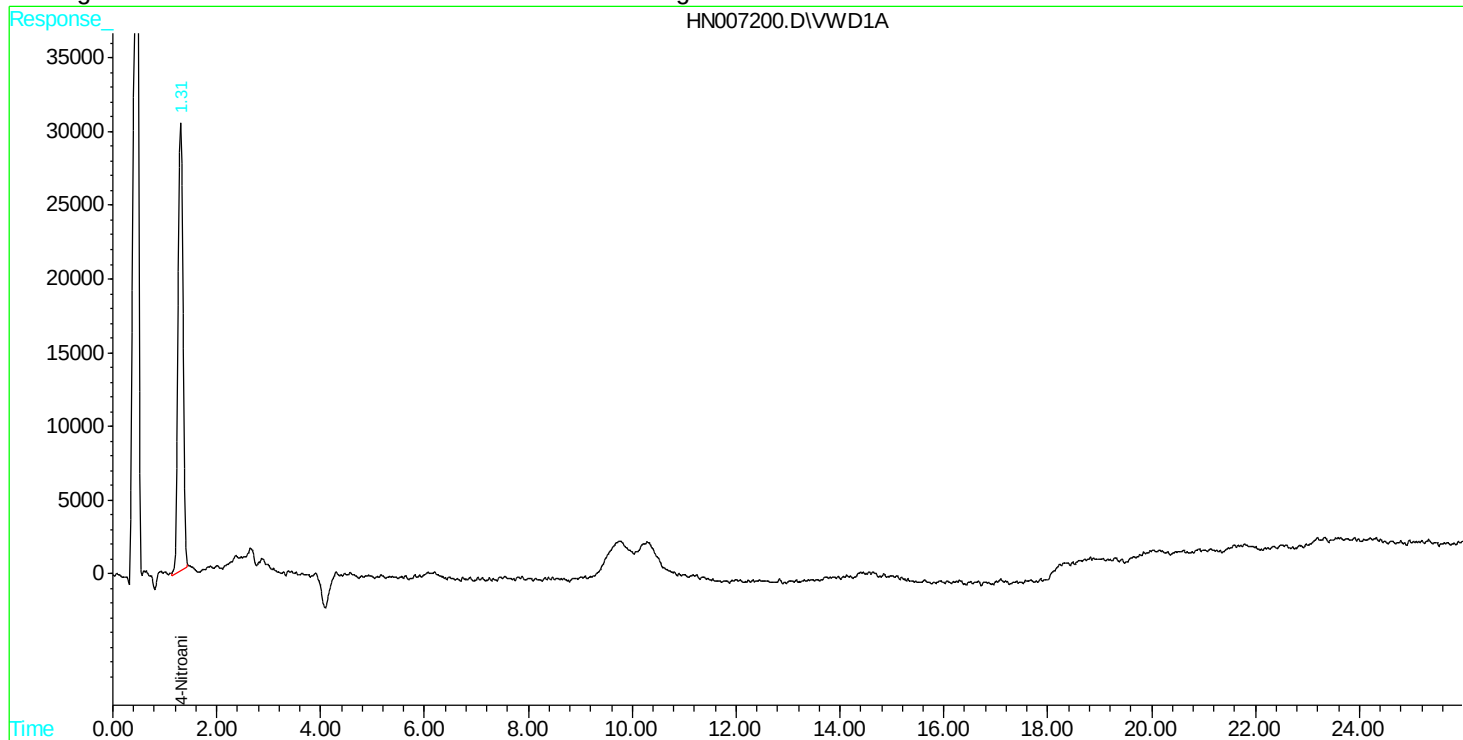

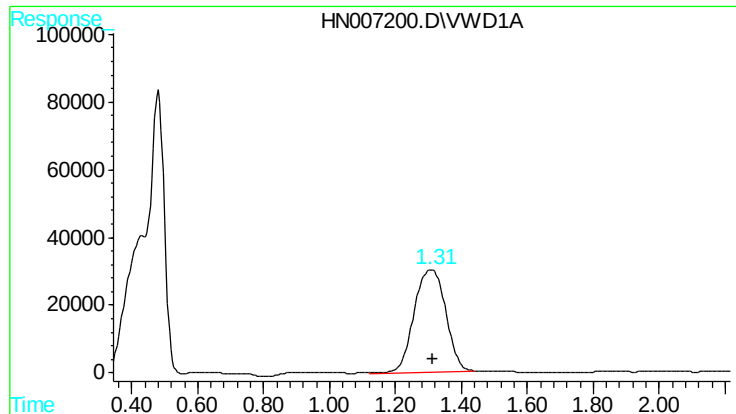

#1 4-Nitroaniline

R.T.: 1.307 min
Delta R.T.: -0.006 min
Response: 2031240
Conc: 501.16 ug/L m