

Data File : S:\HPCHEM1\HPLC_N\DATA\HN012114\HN005789.D Vial: 9
Acq On : 21-Jan-2014, 16:26 Operator: QM
Sample : PB74516BL Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jan 23 3:28 2014 Quant Results File: HN0121NG.RES

Instrument :
HPLC_N
ClientSampleId :
PB74516BL

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN0121NG.M
Title :
Last Update : Tue Jan 21 14:02:23 2014
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.30	665799	0.165 ng/ul

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005789.D HN0121NG.M

Sat Jan 25 00:49:07 2014

RPT1


Quantitation Report


Data File : S:\HPCHEM1\HPLC_N\DATA\HN012114\HN005789.D Vial: 9
Acq On : 21-Jan-2014, 16:26 Operator: QM
Sample : PB74516BL Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jan 23 3:28 2014 Quant Results File: HN0121NG.RES

Instrument :
HPLC_N
ClientSampleId :
PB74516BL

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN0121NG.M
Title :
Last Update : Tue Jan 21 14:02:23 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

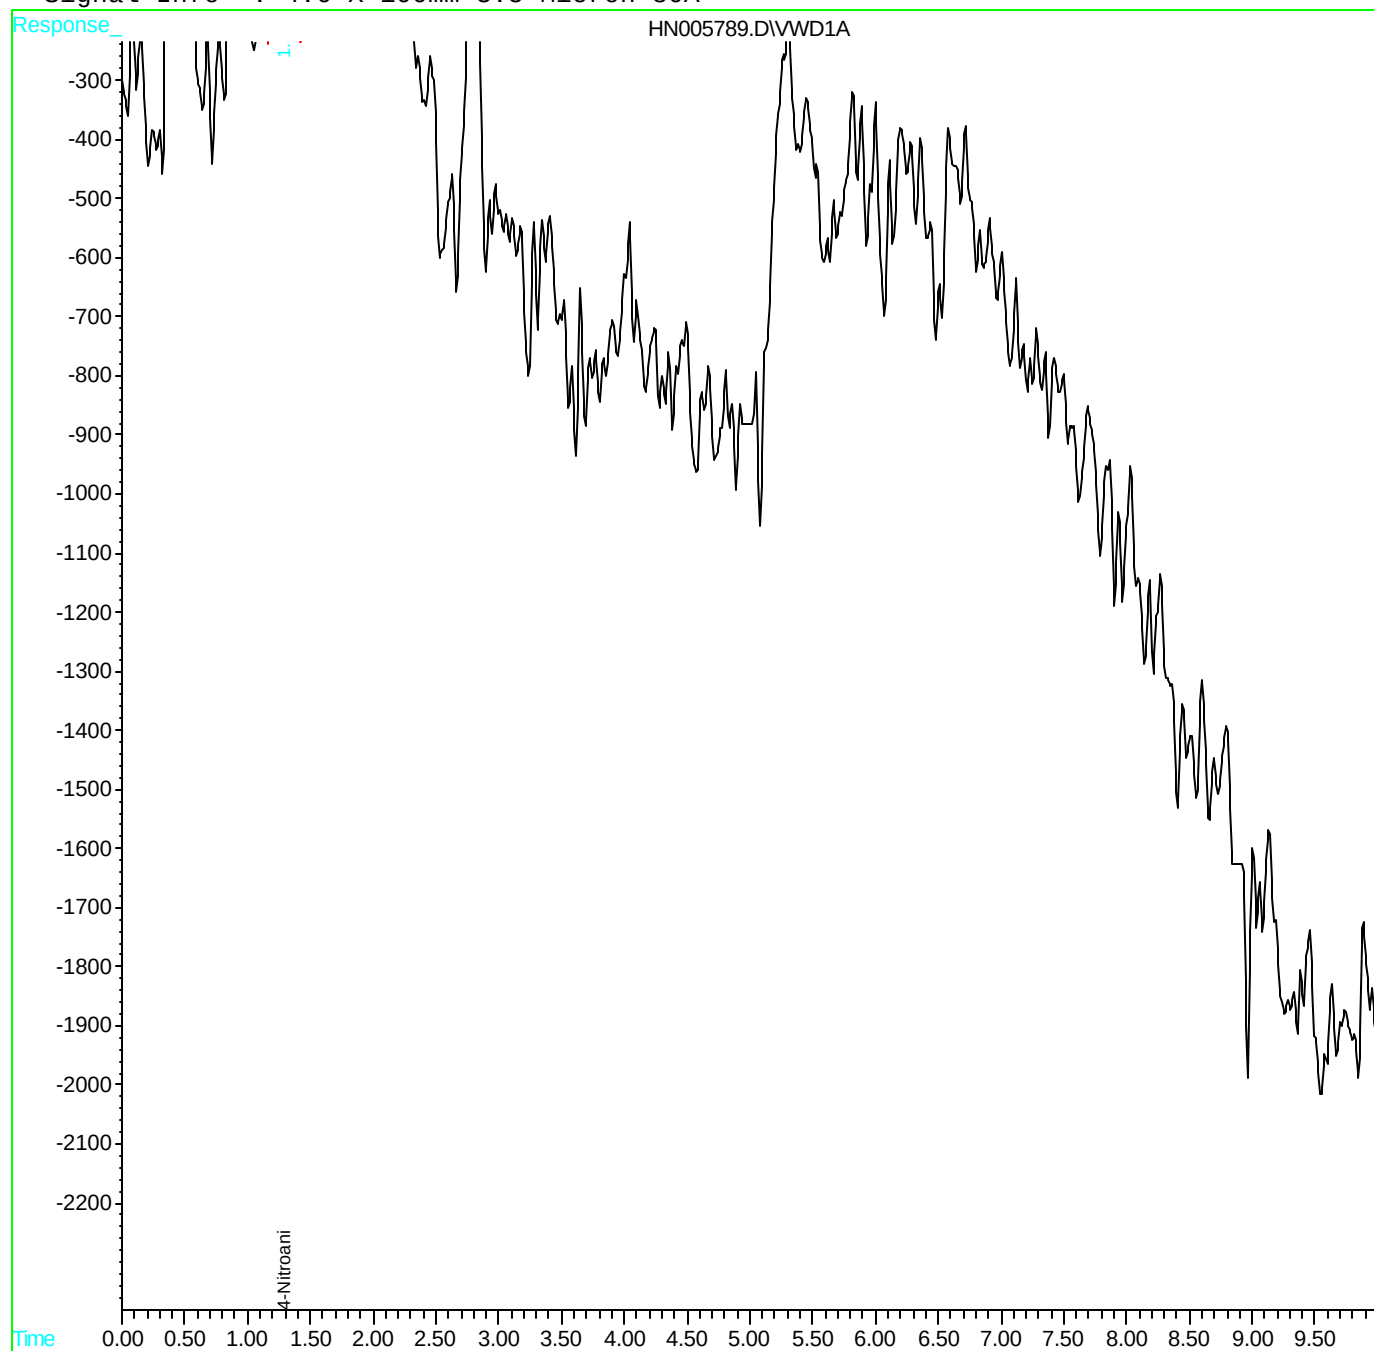

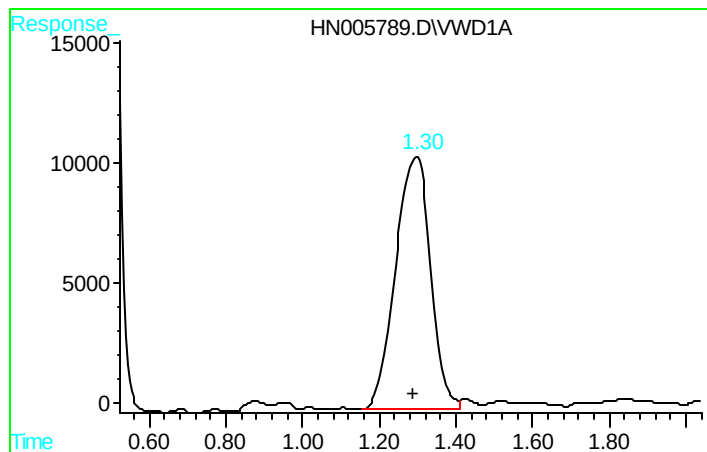

#1 4-Nitroaniline

R.T.: 1.298 min
Delta R.T.: 0.008 min
Response: 665799
Conc: 0.17 ng/ul

Instrument :
HPLC_N
ClientSampleId :
PB74516BL