

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN030316\
Data File : HN007643.D
Signal(s) : vwd1A.ch
Acq On : 03-Mar-2016, 15:52
Operator : UM/MA
Sample : HSTDICC050
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
SSTDICC050

Integration File: AUTOINT1.E
Quant Time: Mar 03 17:27:37 2016
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN0303NG.M
Quant Title :
QLast Update : Thu Mar 03 17:27:09 2016
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.327	205192150	50.079 ng/ul
Target Compounds			
2) T Nitroglycerin	5.954	401747849	48.124 ng/ul

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN030316\
Data File : HN007643.D
Signal(s) : vwd1A.ch
Acq On : 03-Mar-2016, 15:52
Operator : UM/MA
Sample : HSTDICC050
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
SSTDICC050

Integration File: AUTOINT1.E
Quant Time: Mar 03 17:27:37 2016
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN0303NG.M
Quant Title :
QLast Update : Thu Mar 03 17:27:09 2016
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

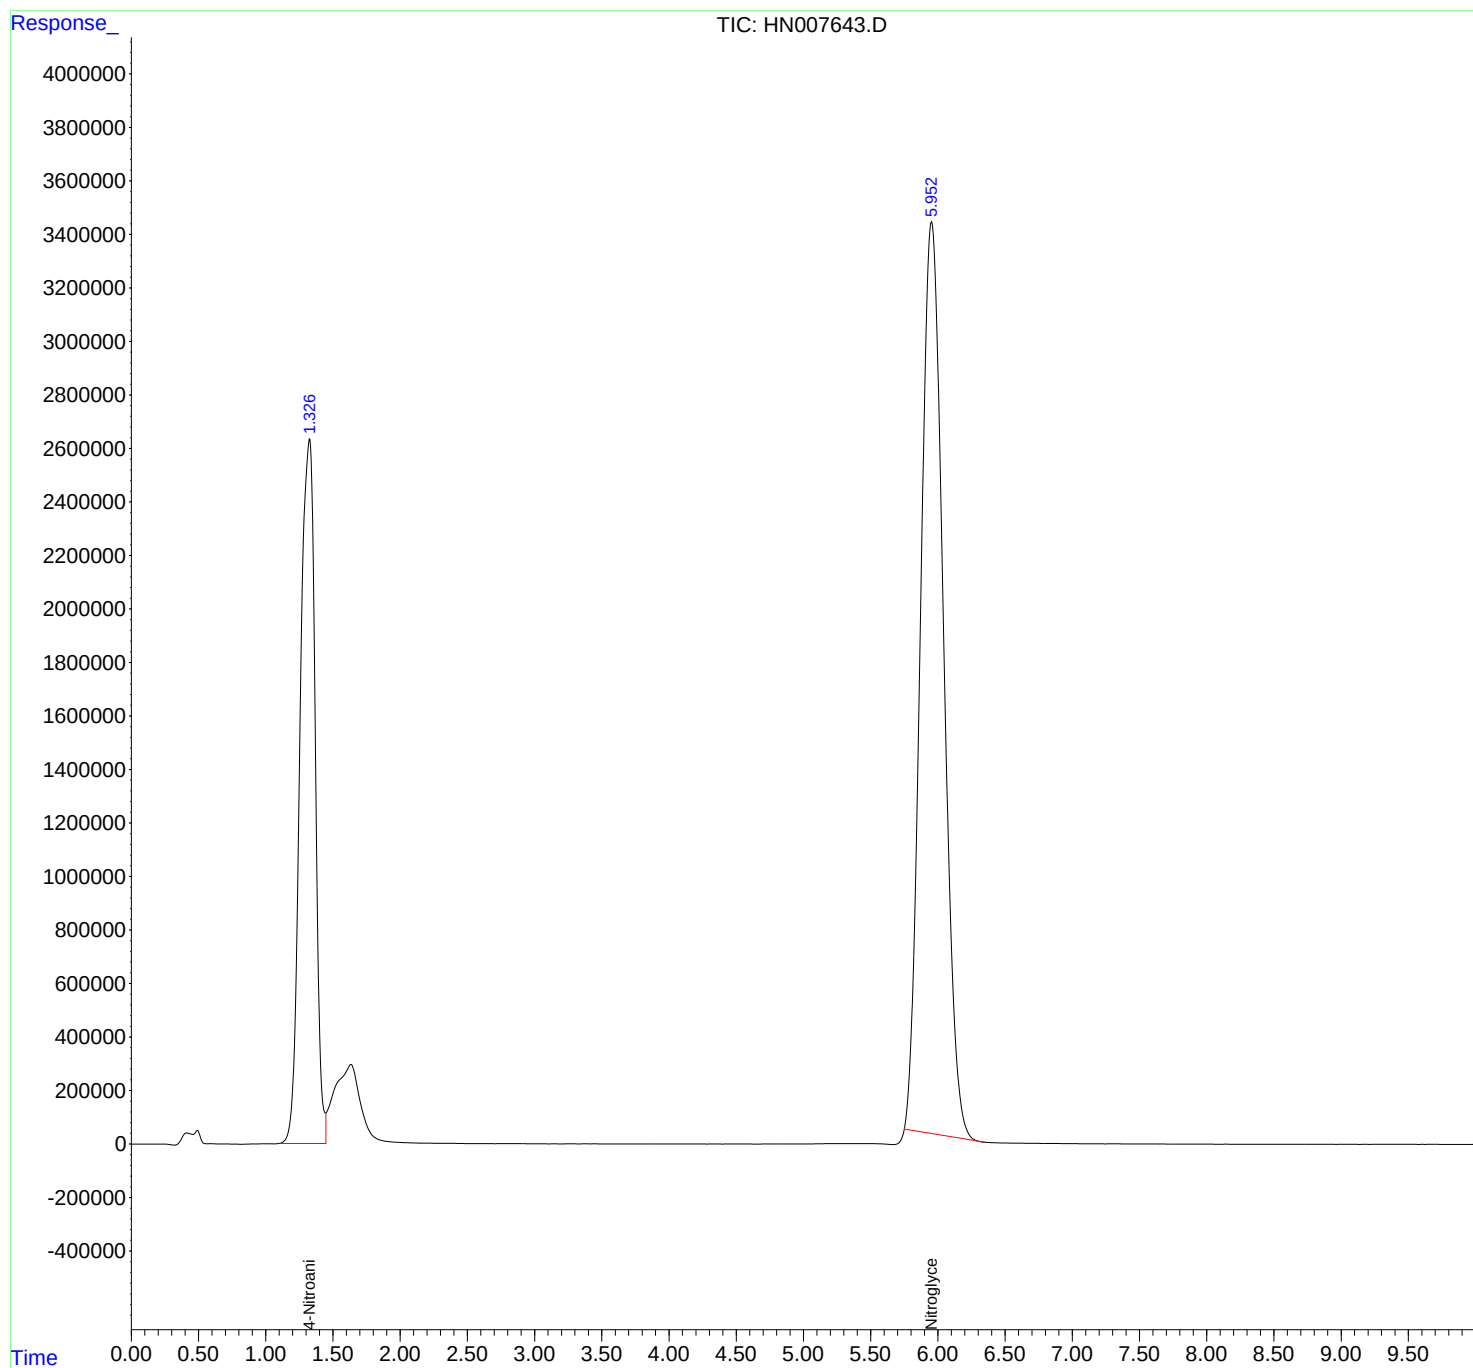


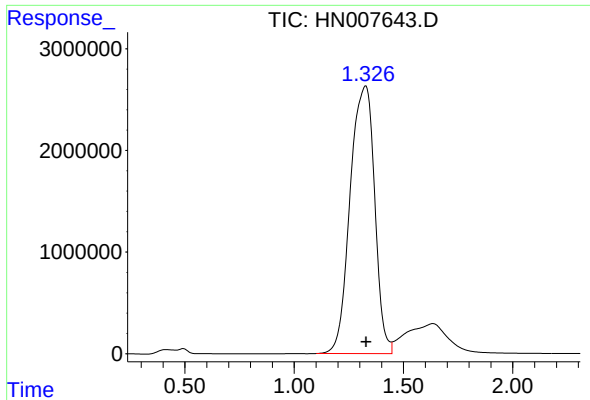

#1 4-Nitroaniline

R.T.: 1.327 min
Delta R.T.: -0.002 min
Response: 205192150
Conc: 50.08 ng/ul

Instrument :
HPLC_N
ClientSampleId :
SSTDIC050

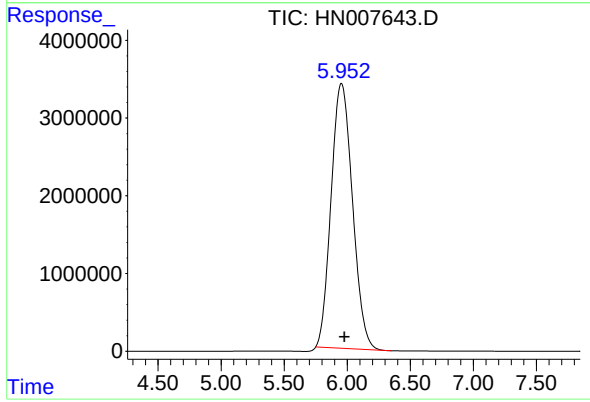

#2 Nitroglycerin

R.T.: 5.954 min
Delta R.T.: -0.024 min
Response: 401747849
Conc: 48.12 ng/ul