

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN033115\
 Data File : HN007293.D
 Signal(s) : vwd1A.ch
 Acq On : 31-Mar-2015, 15:44
 Operator : TP/IZ
 Sample : HSTDCCC0500
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 02 12:33:10 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN031315.M
 Quant Title :
 QLast Update : Thu Apr 02 12:19:18 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S 4-Nitroaniline	1.294	2054517	537.165 ug/L
---------------------	-------	---------	--------------

Target Compounds

2) T HMX	0.874	1935732	422.188 ug/L
3) T RDX	1.670	2425838	436.382 ug/L
4) T 1,3,5-Trinitrobenzene	2.644	4819893	429.801 ug/L
5) T 1,3-Dinitrobenzene	3.505	7552012	447.344 ng/ml
6) T 3,5-Dinitroaniline	3.863	6021154	449.220 ug/L
7) T Nitrobenzene	4.742	4378329	439.399 ug/L
8) T Tetryl	6.263	2747803	341.498 ug/L
9) T 2,4,6-Trinitrotoluene	6.496	5063022	455.489 ug/L
10) T 2-Amino-4,6-dinitroto...	7.015	4832756	435.323 ug/L
11) T 4-Amino-2,6-dinitroto...	7.382	3228656	461.474 ug/L
12) T 2,4-Dinitrotoluene	8.142	6765367	446.048 ug/L
13) T 2,6-Dinitrotoluene	8.554	3858835	457.842 ug/L
14) T 2-Nitrotoluene	11.863	2876300	421.839 ug/L
15) T 4-Nitrotoluene	12.585	2263126	352.020 ug/L
16) T 3-Nitrotoluene	13.889	2906134	432.073 ug/L
17) T PETN	19.200	3765791	385.876 ug/L


(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\HPCHEM1\HPLC_NData\HN033115\
Data File : HN007293.D
Signal(s) : vwd1A.ch
Acq On : 31-Mar-2015, 15:44
Operator : TP/IZ
Sample : HSTDCCC0500
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 02 12:33:10 2015
Quant Method : Z:\HPCHEM1\HPLC_NMETHODS\HN031315.M
Quant Title :
QLast Update : Thu Apr 02 12:19:18 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

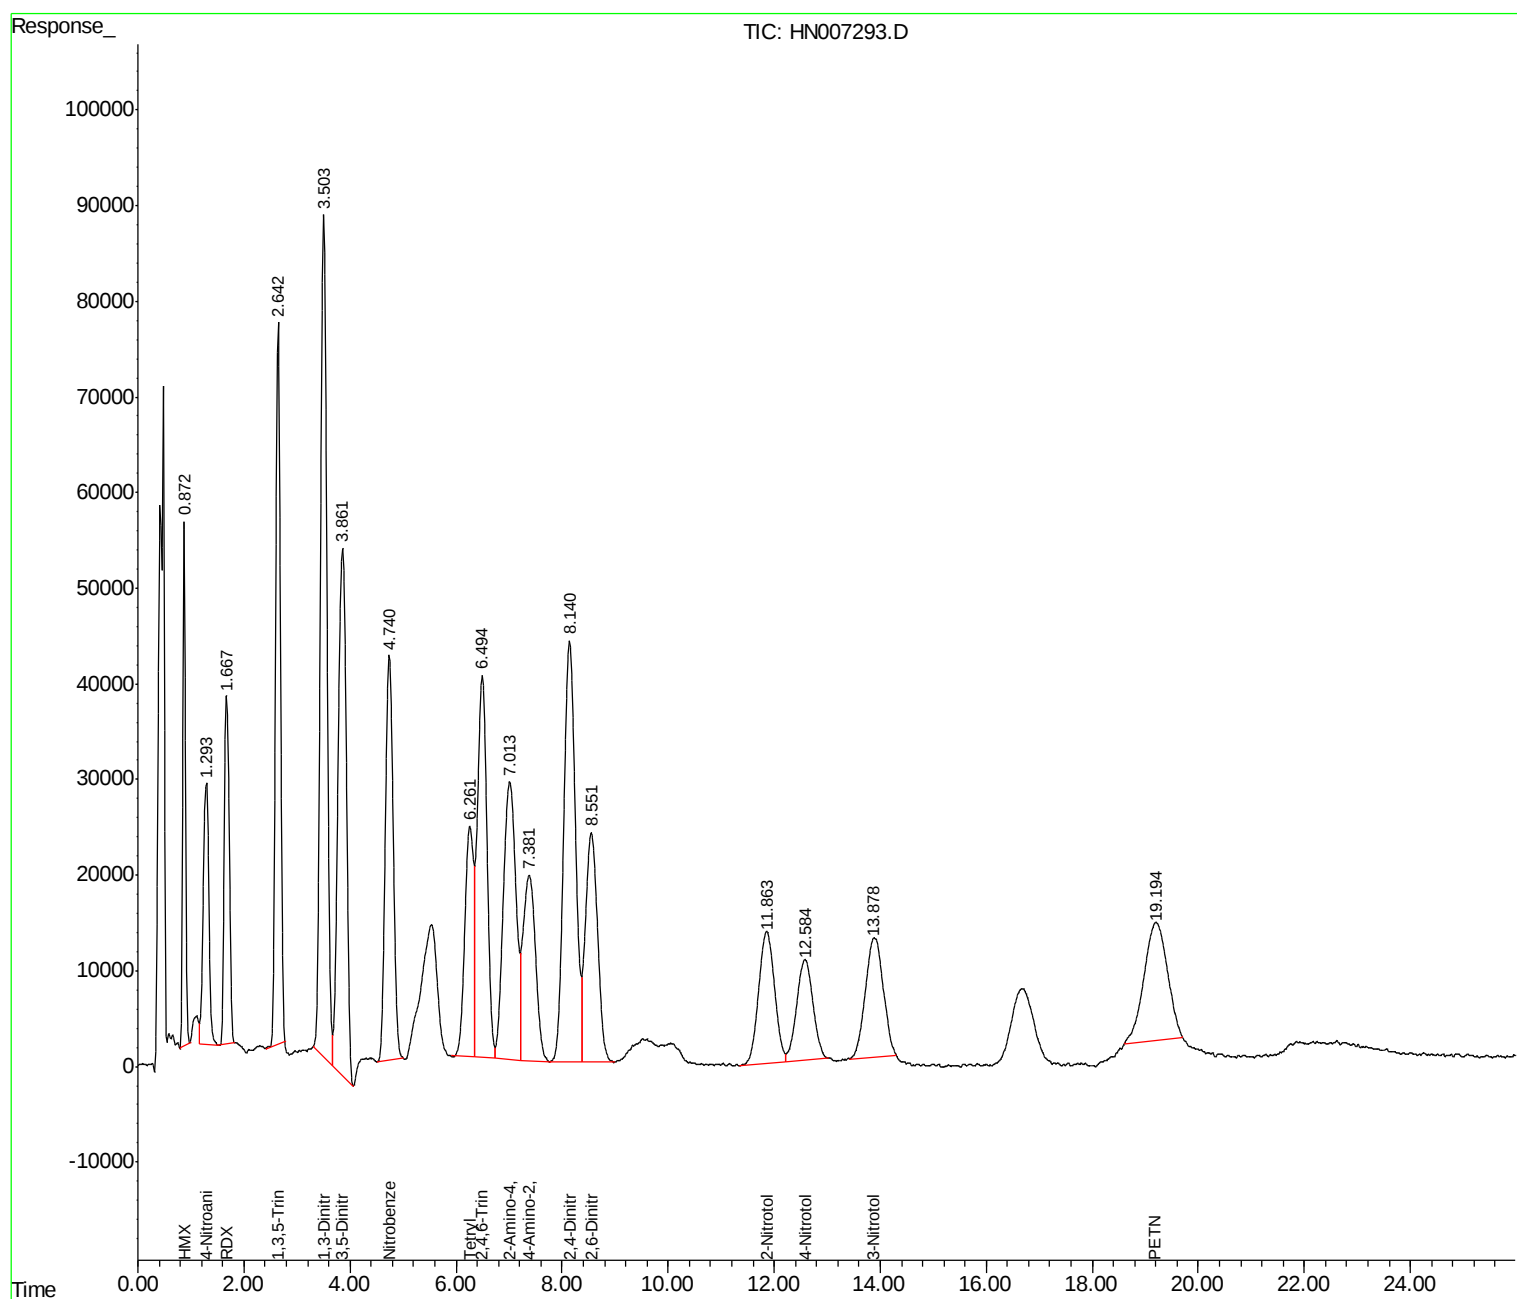

The printer must be in Portrait mode.