

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN042314\
Data File : HN005835.D
Signal(s) : VWD1A.CH
Acq On : 23-Apr-2014, 14:50
Operator : JDU
Sample : HSTDICC2000
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDICC2000

Integration File: autoint1.e
Quant Time: Apr 30 11:15:38 2014
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN042314.M
Quant Title :
QLast Update : Thu Apr 24 15:16:33 2014
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.352	1504925	2675.251 ug/L
Target Compounds			
2) T RDX	1.733	2300585	1441.230 ug/L
3) T Tetryl	6.383	3296640	1711.601 ug/L
4) T 2,4,6-Trinitrotoluene	6.683	4495140	2114.859 ug/L
5) T PETN	19.159	3084496	2824.375 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN042314\
Data File : HN005835.D
Signal(s) : VWD1A.CH
Acq On : 23-Apr-2014, 14:50
Operator : JDU
Sample : HSTDICC2000
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDICC2000

Integration File: autoint1.e
Quant Time: Apr 30 11:15:38 2014
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN042314.M
Quant Title :
QLast Update : Thu Apr 24 15:16:33 2014
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

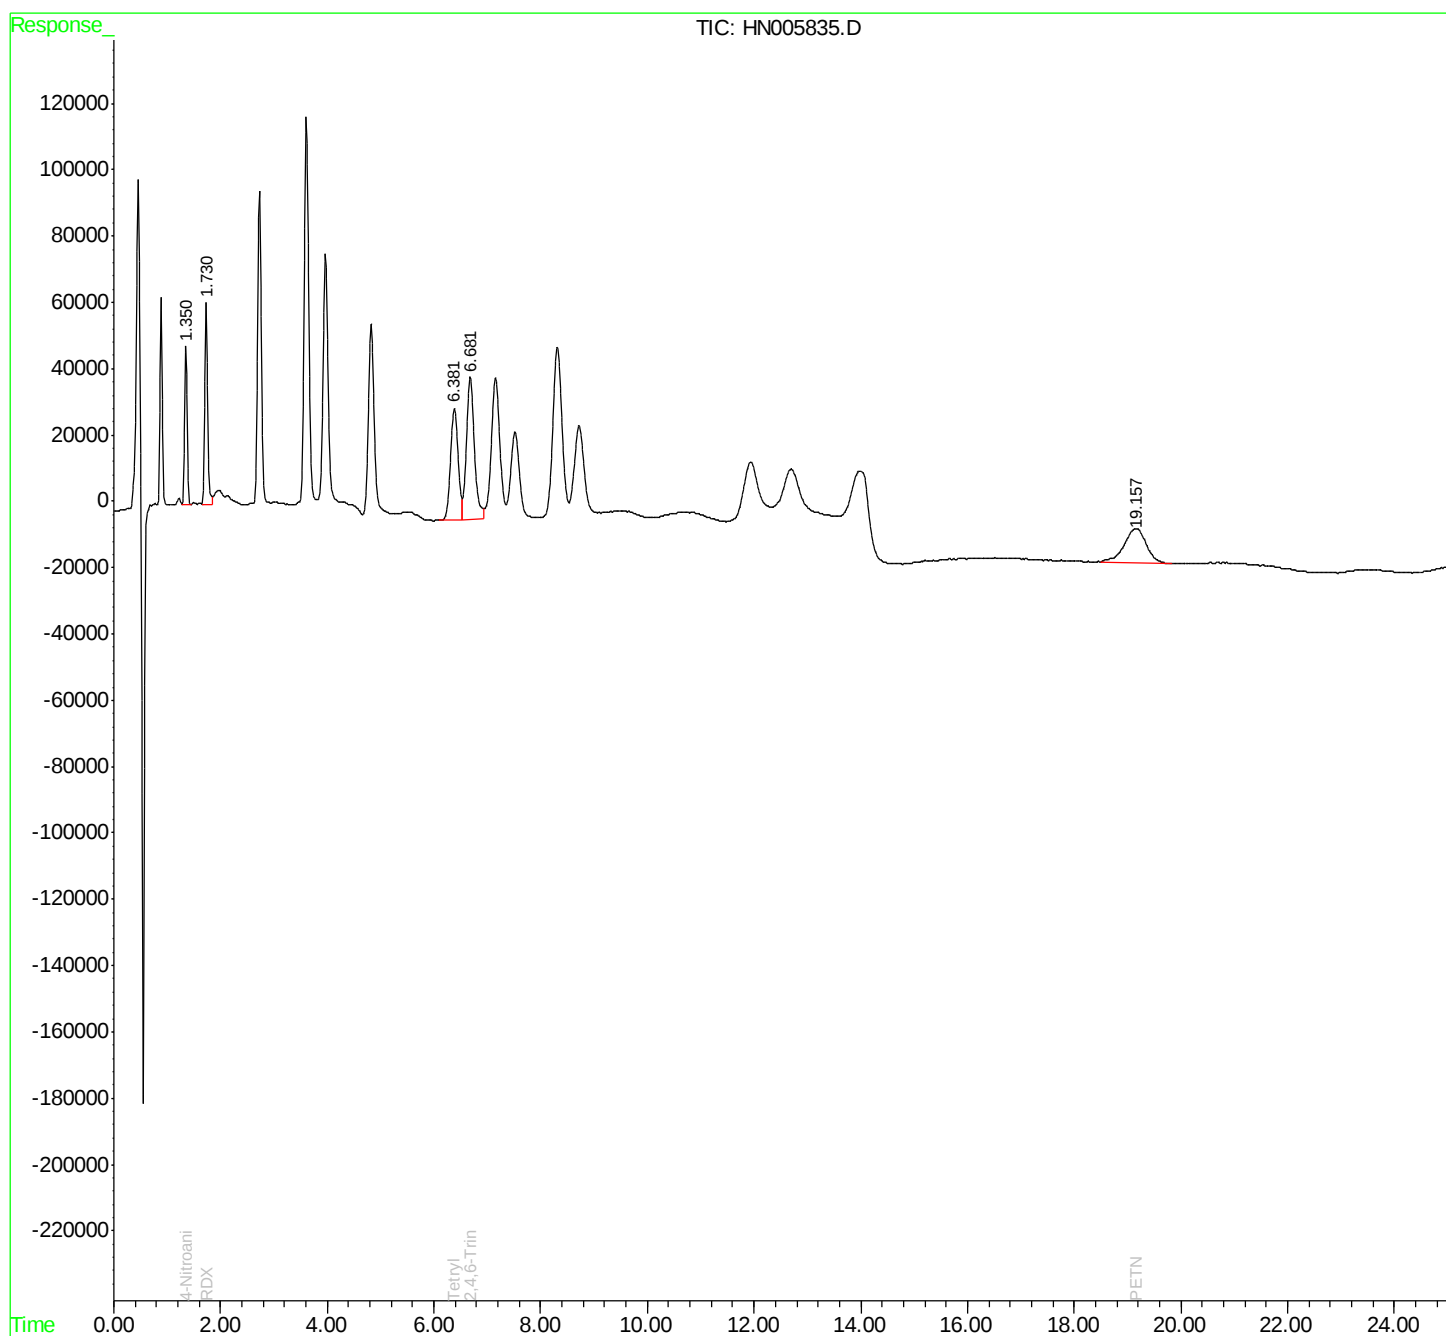


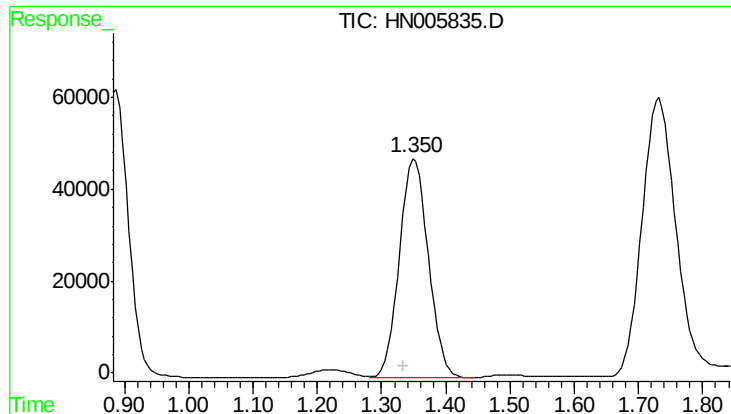

#1 4-Nitroaniline


R.T.: 1.352 min
Delta R.T.: 0.018 min
Response: 1504925
Conc: 2675.25 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDICC2000

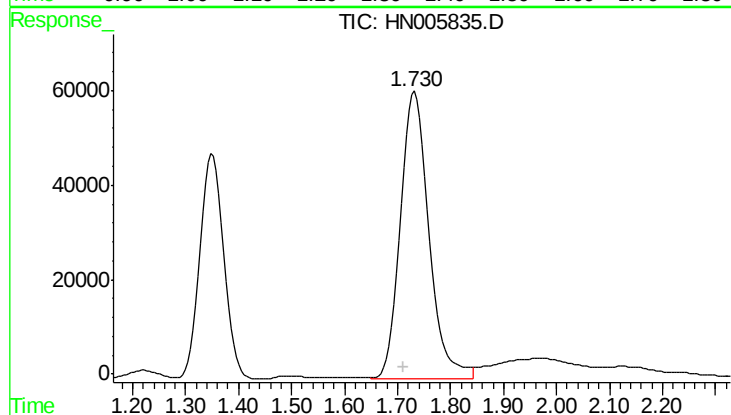


#2 RDX

R.T.: 1.733 min
Delta R.T.: 0.022 min
Response: 2300585
Conc: 1441.23 ug/L

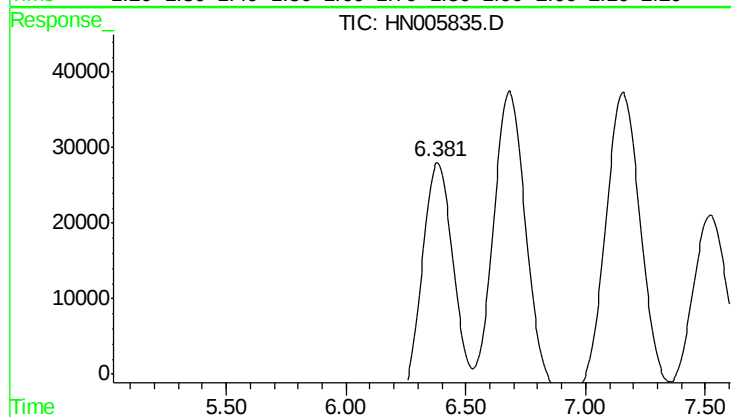


#3 Tetryl

R.T.: 6.383 min
Delta R.T.: 0.063 min
Response: 3296640
Conc: 1711.60 ug/L

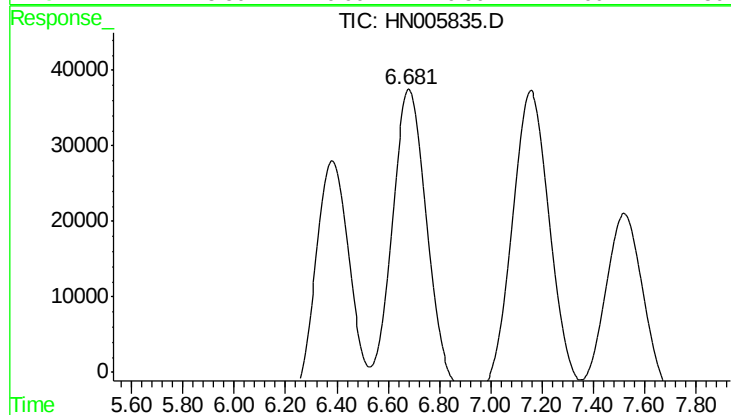

#4 2,4,6-Trinitrotoluene

R.T.: 6.683 min
Delta R.T.: 0.064 min
Response: 4495140
Conc: 2114.86 ug/L

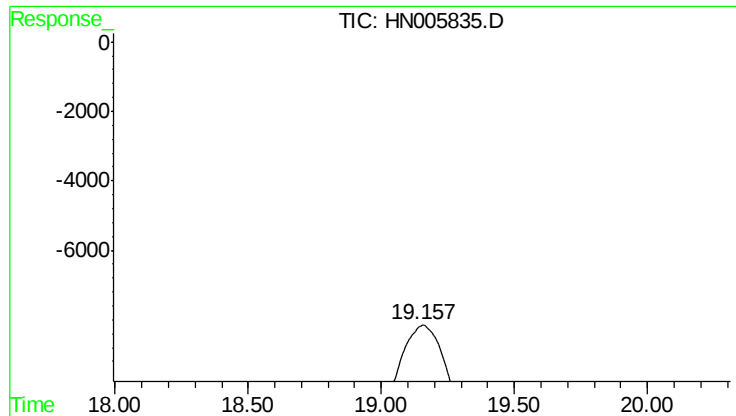

#5 PETN

R.T.: 19.159 min
Delta R.T.: 0.059 min
Response: 3084496
Conc: 2824.37 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDICC2000