

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN042314\
Data File : HN005836.D
Signal(s) : VWD1A.CH
Acq On : 23-Apr-2014, 15:17
Operator : JDU
Sample : HSTDICC1000
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDICC1000

Integration File: autoint1.e
Quant Time: Apr 30 11:17:25 2014
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN042314.M
Quant Title :
QLast Update : Thu Apr 24 15:16:33 2014
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.331	594259	1056.393 ug/L
Target Compounds			
2) T RDX	1.706	1226878	768.593 ug/L
3) T Tetryl	6.301	1813045	941.325 ug/L
4) T 2,4,6-Trinitrotoluene	6.597	2513174	1182.390 ug/L
5) T PETN	19.149	1296584	1187.241 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN042314\
Data File : HN005836.D
Signal(s) : VWD1A.CH
Acq On : 23-Apr-2014, 15:17
Operator : JDU
Sample : HSTDICC1000
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDICC1000

Integration File: autoint1.e
Quant Time: Apr 30 11:17:25 2014
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN042314.M
Quant Title :
QLast Update : Thu Apr 24 15:16:33 2014
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

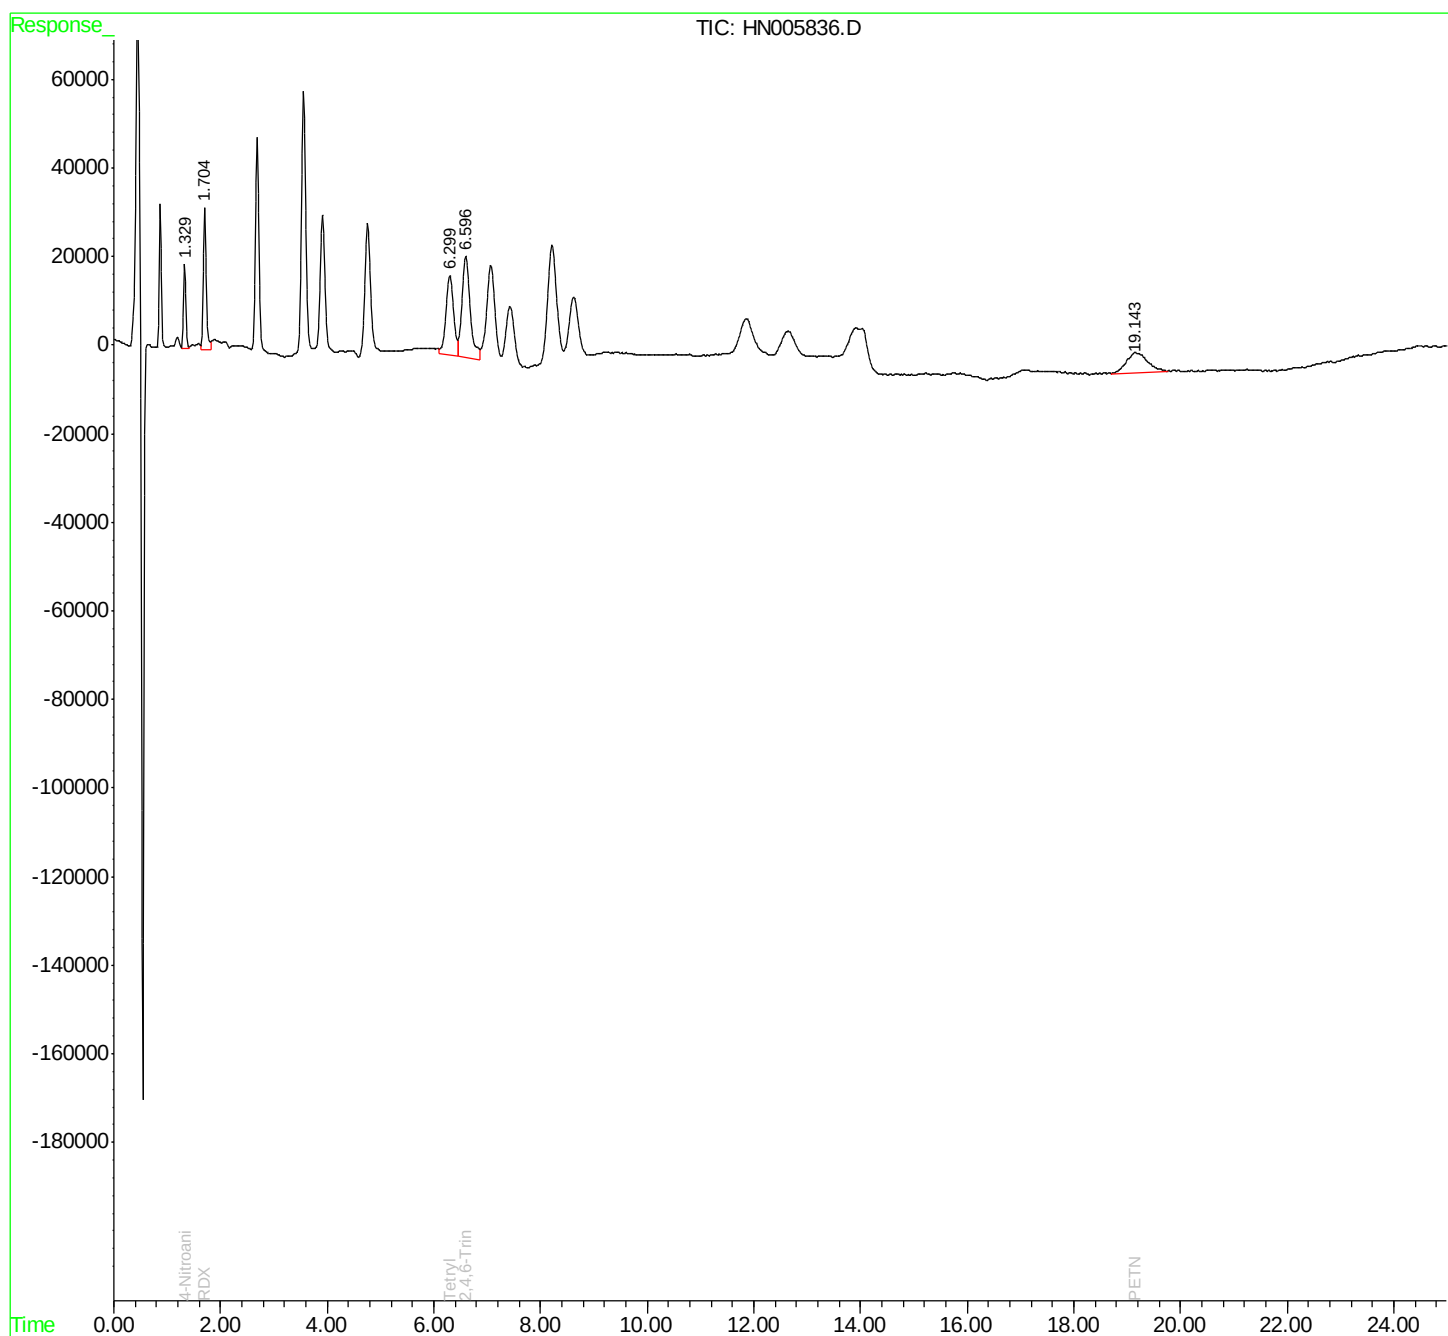


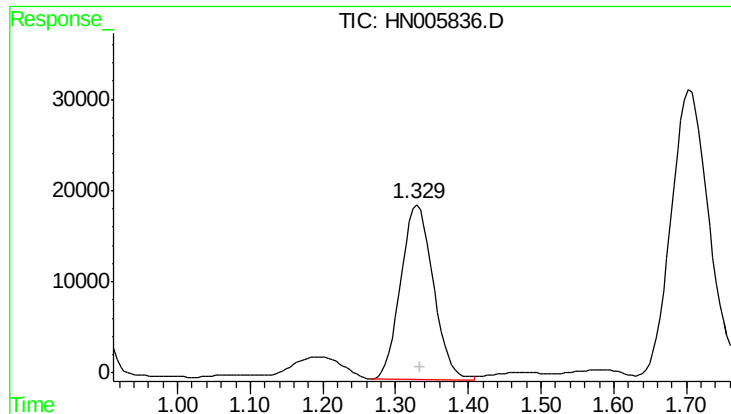

#1 4-Nitroaniline


R.T.: 1.331 min
Delta R.T.: -0.003 min
Response: 594259
Conc: 1056.39 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDICC1000

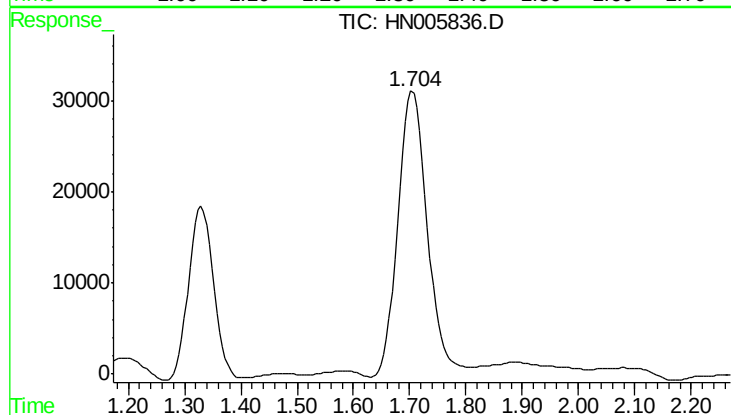


#2 RDX

R.T.: 1.706 min
Delta R.T.: -0.005 min
Response: 1226878
Conc: 768.59 ug/L

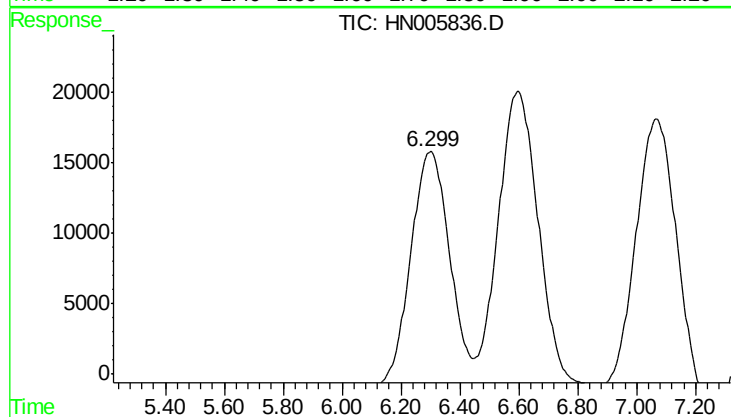


#3 Tetryl

R.T.: 6.301 min
Delta R.T.: -0.019 min
Response: 1813045
Conc: 941.32 ug/L

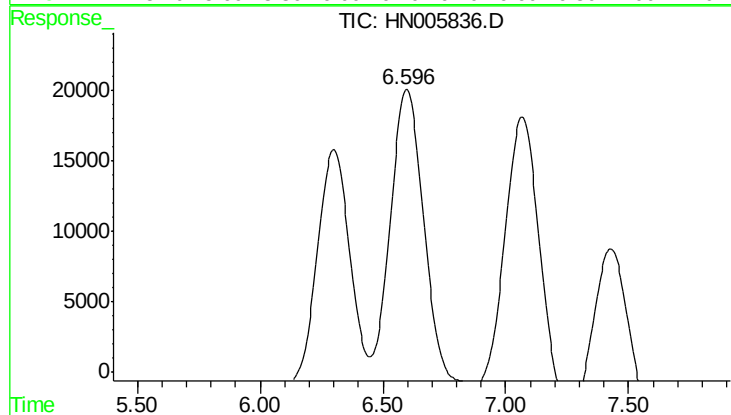

#4 2,4,6-Trinitrotoluene

R.T.: 6.597 min
Delta R.T.: -0.022 min
Response: 2513174
Conc: 1182.39 ug/L

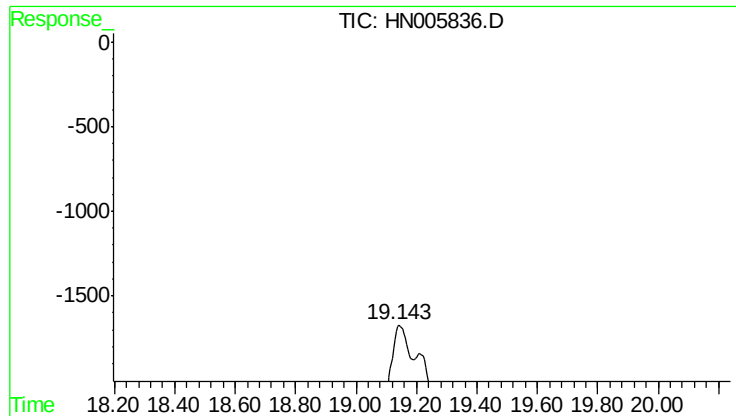

#5 PETN

R.T.: 19.149 min
Delta R.T.: 0.049 min
Response: 1296584
Conc: 1187.24 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDICC1000