

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN042314\
 Data File : HN005845.D
 Signal(s) : VWD1A.CH
 Acq On : 23-Apr-2014, 18:48
 Operator : JDU
 Sample : F1945-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 SS26-MDA01

Integration File: autoint1.e
 Quant Time: Apr 30 11:28:57 2014
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN042314.M
 Quant Title :
 QLast Update : Thu Apr 24 12:12:00 2014
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.336	137298	299.134 ug/L
Target Compounds			
2) T HMX	0.813	5218237	6530.251 ug/L
5) T 1,3-Dinitrobenzene	3.489	18825	15.258 ng/ml
6) T 3,5-Dinitroaniline	3.873	67410	86.882 ug/L
8) T Tetryl	6.076	9514	78.603 ug/L
9) T 2,4,6-Trinitrotoluene	6.386	3858	1.819 ug/L
10) T 2-Amino-4,6-dinitroto...	6.805	7696	3.689 ug/L
11) T 4-Amino-2,6-dinitroto...	7.186	5310	3.685 ug/L
12) T 2,4-Dinitrotoluene	7.975	13241	52.819 ug/L
14) T 2-Nitrotoluene	11.391	6257	89.463 ug/L
17) T PETN	18.521	13986	198.848 ug/L

(f)=RT Delta > 1/2 Window

(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN042314\
Data File : HN005845.D
Signal(s) : VWD1A.CH
Acq On : 23-Apr-2014, 18:48
Operator : JDU
Sample : F1945-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
SS26-MDA01

Integration File: autoint1.e
Quant Time: Apr 30 11:28:57 2014
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN042314.M
Quant Title :
QLast Update : Thu Apr 24 12:12:00 2014
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A




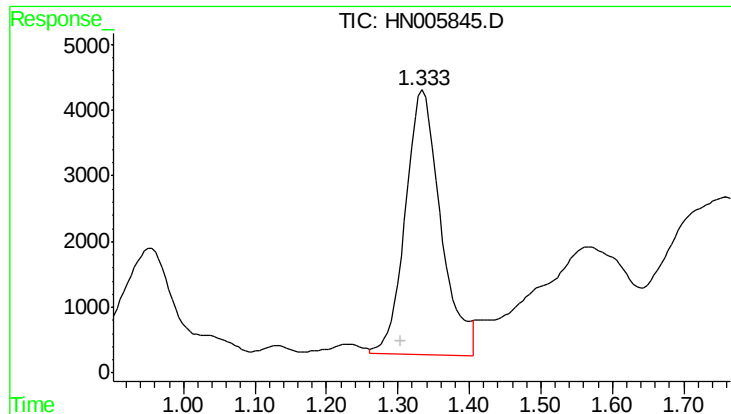

#1 4-Nitroaniline


R.T.: 1.336 min
Delta R.T.: 0.032 min
Response: 137298
Conc: 299.13 ug/L

Instrument :
HPLC_N
ClientSampleId :
SS26-MDA01

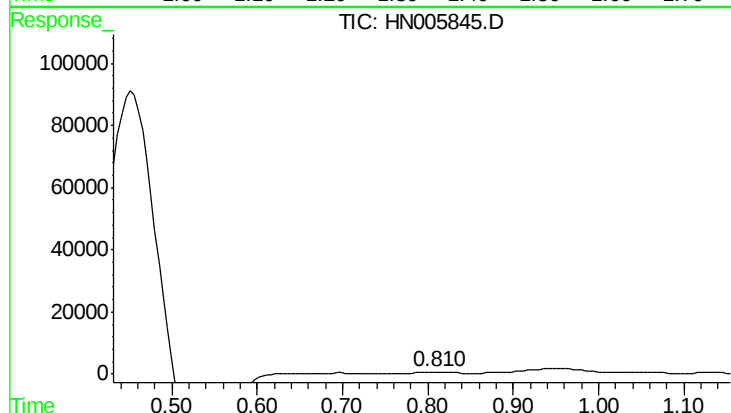


#2 HMX

R.T.: 0.813 min
Delta R.T.: -0.060 min
Response: 5218237
Conc: 6530.25 ug/L

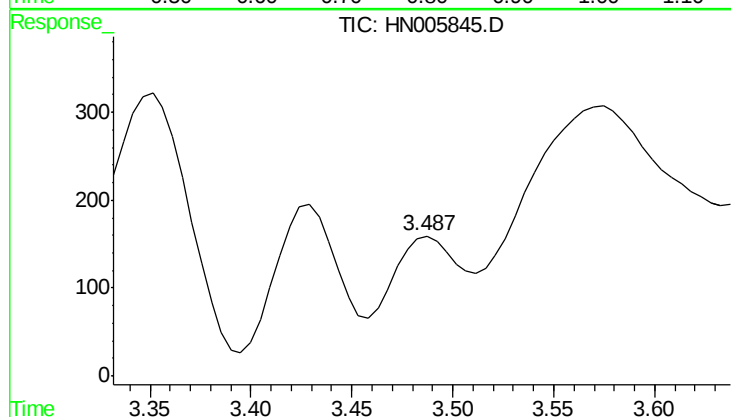


#5 1,3-Dinitrobenzene

R.T.: 3.489 min
Delta R.T.: 0.020 min
Response: 18825
Conc: 15.26 ng/ml

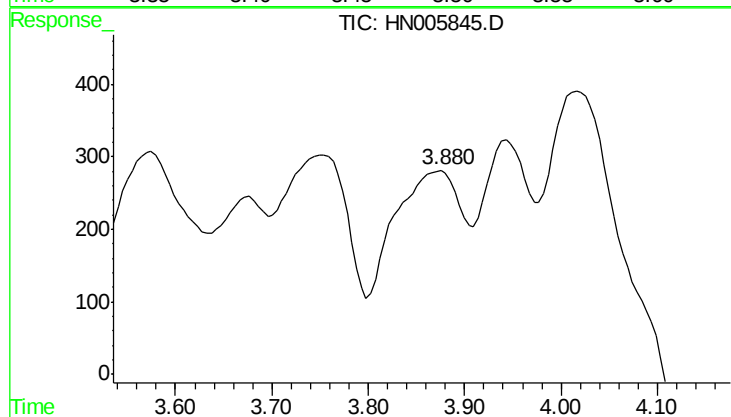

#6 3,5-Dinitroaniline


R.T.: 3.873 min
Delta R.T.: 0.056 min
Response: 67410
Conc: 86.88 ug/L

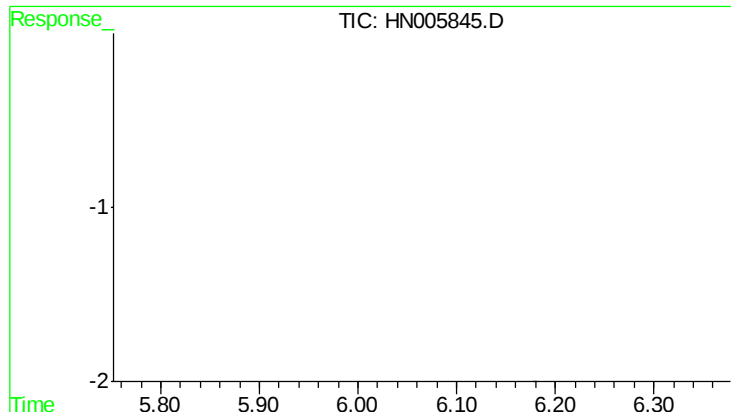

#8 Tetryl


R.T.: 6.076 min
 Delta R.T.: 0.005 min
 Response: 9514
 Conc: 78.60 ug/L

Instrument :
 HPLC_N
 ClientSampleId :
 SS26-MDA01

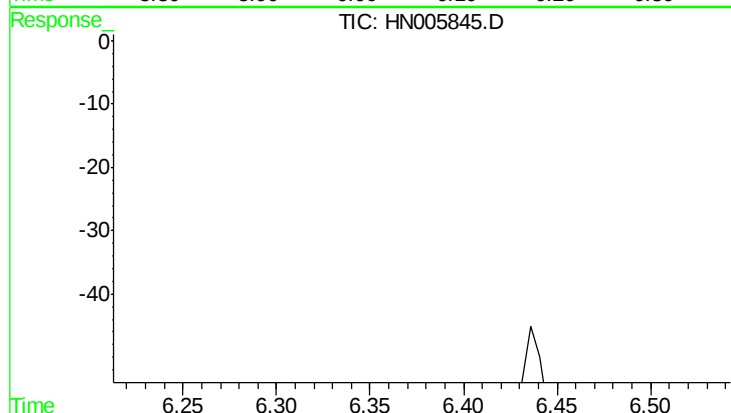


#9 2,4,6-Trinitrotoluene

R.T.: 6.386 min
 Delta R.T.: 0.013 min
 Response: 3858
 Conc: 1.82 ug/L

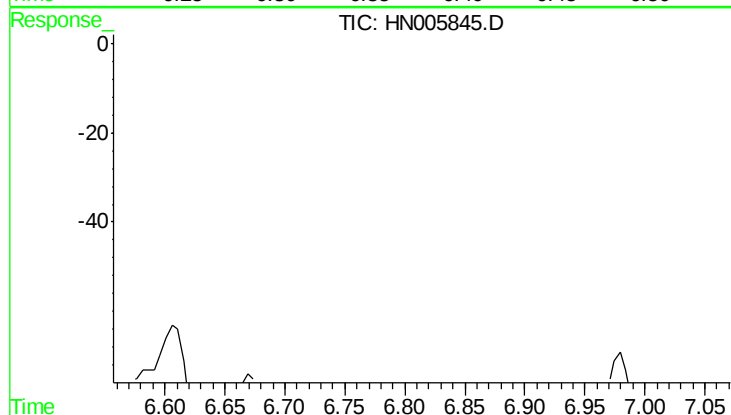


#10 2-Amino-4,6-dinitrotoluene

R.T.: 6.805 min
 Delta R.T.: -0.039 min
 Response: 7696
 Conc: 3.69 ug/L

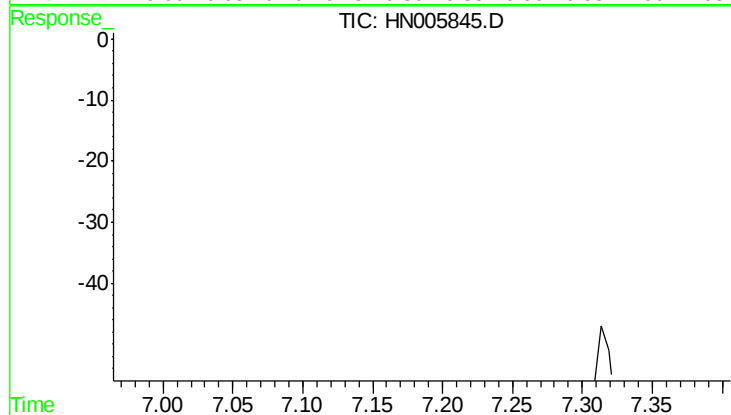

#11 4-Amino-2,6-dinitrotoluene


R.T.: 7.186 min
 Delta R.T.: 0.017 min
 Response: 5310
 Conc: 3.69 ug/L

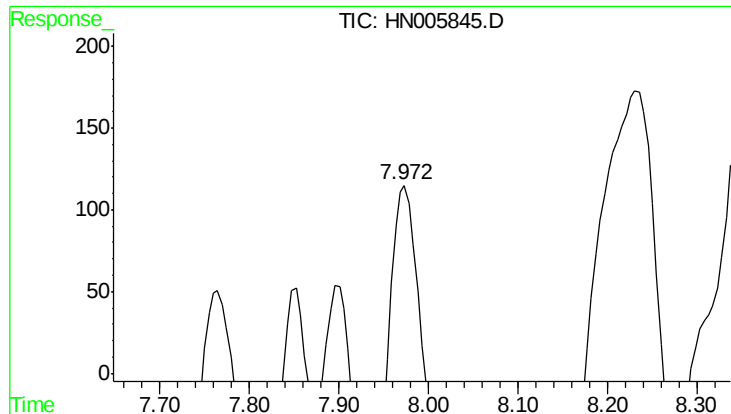

#12 2,4-Dinitrotoluene


R.T.: 7.975 min
Delta R.T.: 0.037 min
Response: 13241
Conc: 52.82 ug/L

Instrument :
HPLC_N
ClientSampleId :
SS26-MDA01

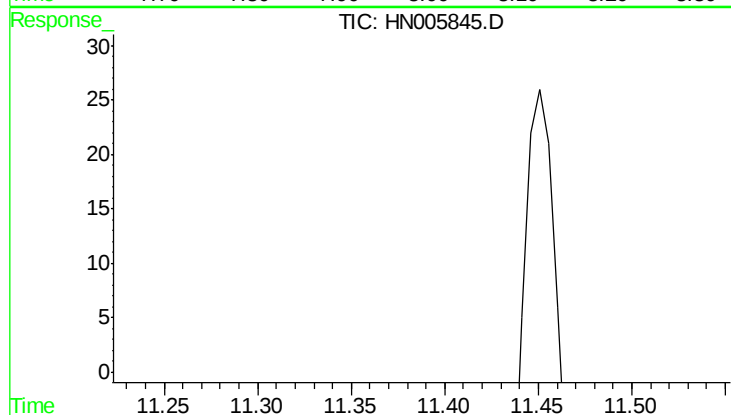

#14 2-Nitrotoluene

R.T.: 11.391 min
Delta R.T.: 0.000 min
Response: 6257
Conc: 89.46 ug/L

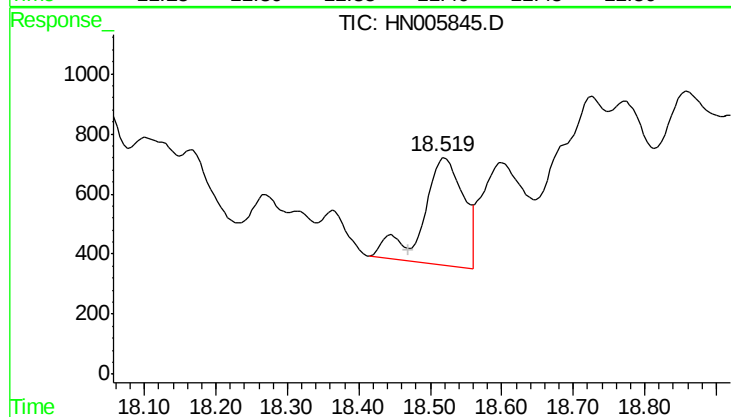

#17 PETN

R.T.: 18.521 min
Delta R.T.: 0.002 min
Response: 13986
Conc: 198.85 ug/L