

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN042314\
 Data File : HN005846.D
 Signal(s) : VWD1A.CH
 Acq On : 23-Apr-2014, 19:14
 Operator : JDU
 Sample : F1945-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 SS26-MDA01D

Integration File: autoint1.e
 Quant Time: Apr 30 11:29:50 2014
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN042314.M
 Quant Title :
 QLast Update : Thu Apr 24 12:12:00 2014
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	1.332	152319	317.855 ug/L
Target Compounds				
2) T	HMX	0.913	1691475	2116.760 ug/L
4) T	1,3,5-Trinitrobenzene	2.665	11895	43.908 ug/L
5) T	1,3-Dinitrobenzene	3.483	24339	16.865 ng/ml
6) T	3,5-Dinitroaniline	3.760	101242	100.468 ug/L
8) T	Tetryl	6.100	17004	82.590 ug/L
9) T	2,4,6-Trinitrotoluene	6.363	15361	7.244 ug/L
11) T	4-Amino-2,6-dinitroto...	7.151	20036	13.904 ug/L
12) T	2,4-Dinitrotoluene	7.983	30275	57.279 ug/L
14) T	2-Nitrotoluene	11.335	13415	92.923 ug/L
15) T	4-Nitrotoluene	12.143	17007	15.500 ug/L
16) T	3-Nitrotoluene	13.335	7652	8.174 ug/L

(f)=RT Delta > 1/2 Window

(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN042314\
Data File : HN005846.D
Signal(s) : VWD1A.CH
Acq On : 23-Apr-2014, 19:14
Operator : JDU
Sample : F1945-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
SS26-MDA01D

Integration File: autoint1.e
Quant Time: Apr 30 11:29:50 2014
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN042314.M
Quant Title :
QLast Update : Thu Apr 24 12:12:00 2014
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A




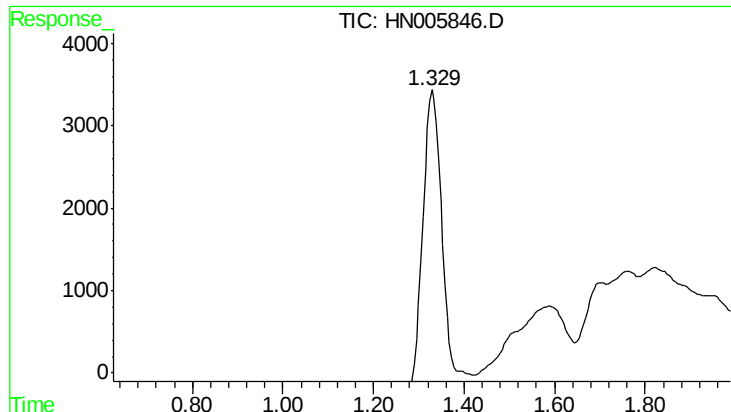

#1 4-Nitroaniline


R.T.: 1.332 min
Delta R.T.: 0.028 min
Response: 152319
Conc: 317.86 ug/L

Instrument :
HPLC_N
ClientSampleId :
SS26-MDA01D

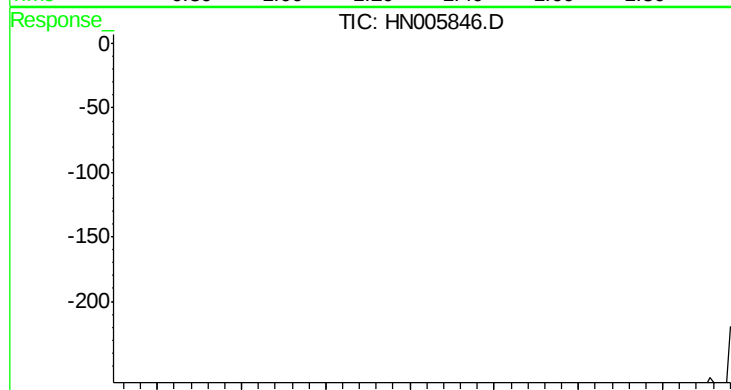


#2 HMX

R.T.: 0.913 min
Delta R.T.: 0.040 min
Response: 1691475
Conc: 2116.76 ug/L

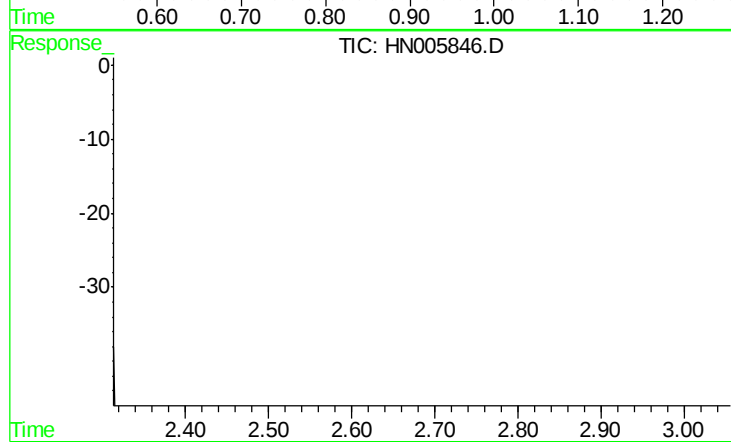


#4 1,3,5-Trinitrobenzene

R.T.: 2.665 min
Delta R.T.: 0.043 min
Response: 11895
Conc: 43.91 ug/L

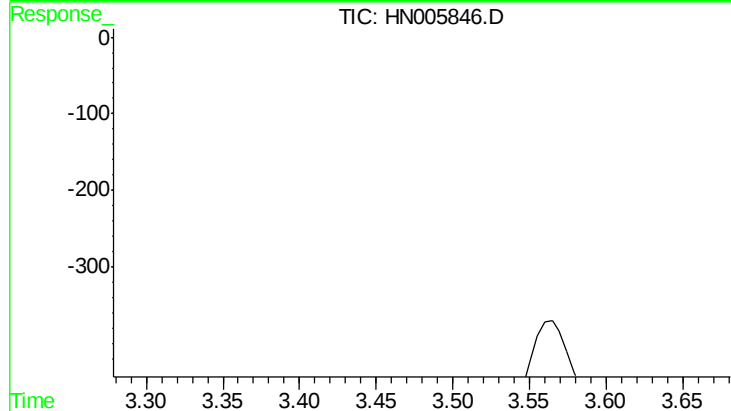

#5 1,3-Dinitrobenzene


R.T.: 3.483 min
Delta R.T.: 0.014 min
Response: 24339
Conc: 16.87 ng/ml

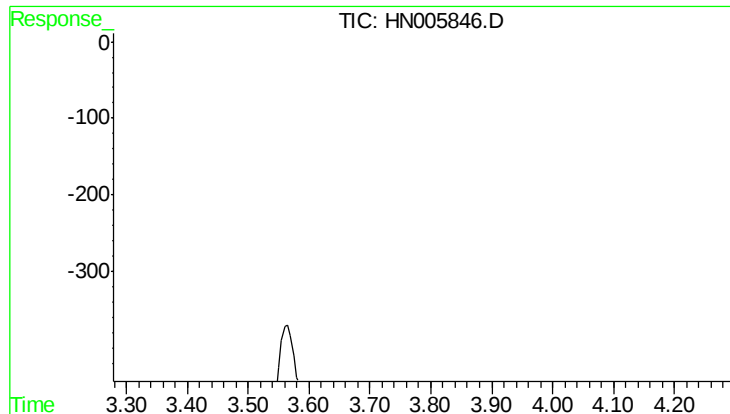

#6 3,5-Dinitroaniline


R.T.: 3.760 min
Delta R.T.: -0.057 min
Response: 101242
Conc: 100.47 ug/L

Instrument :
HPLC_N
ClientSampleId :
SS26-MDA01D

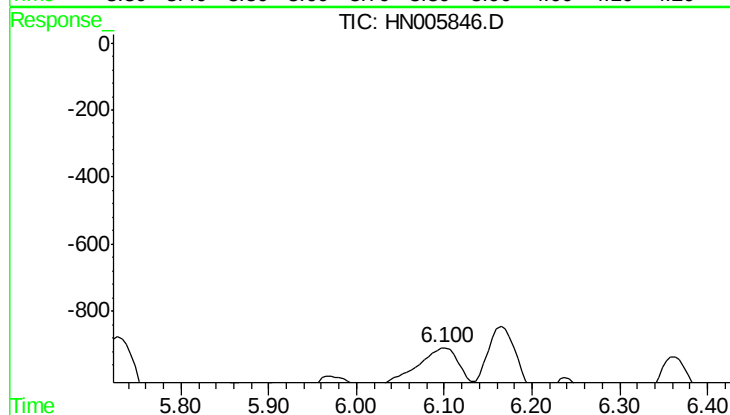


#8 Tetryl

R.T.: 6.100 min
Delta R.T.: 0.029 min
Response: 17004
Conc: 82.59 ug/L

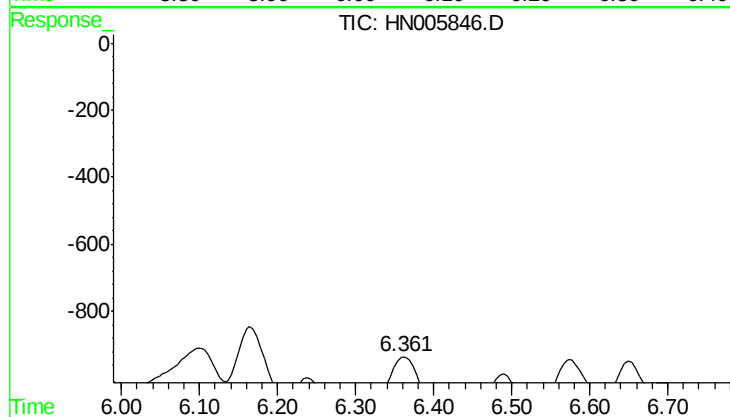


#9 2,4,6-Trinitrotoluene

R.T.: 6.363 min
Delta R.T.: -0.010 min
Response: 15361
Conc: 7.24 ug/L

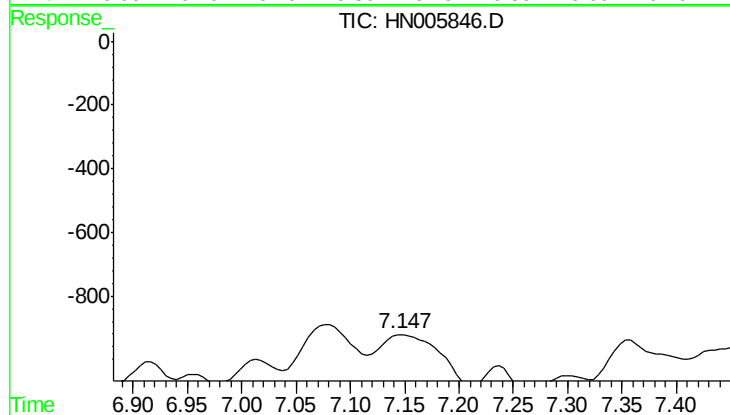

#11 4-Amino-2,6-dinitrotoluene


R.T.: 7.151 min
Delta R.T.: -0.018 min
Response: 20036
Conc: 13.90 ug/L

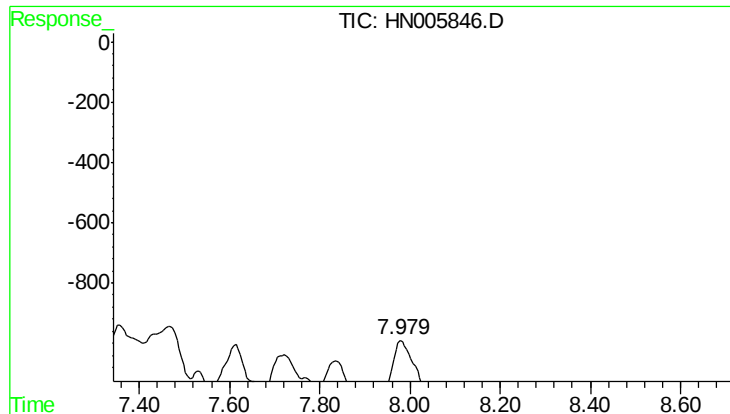

#12 2,4-Dinitrotoluene


R.T.: 7.983 min
Delta R.T.: 0.045 min
Response: 30275
Conc: 57.28 ug/L

Instrument :
HPLC_N
ClientSampleId :
SS26-MDA01D

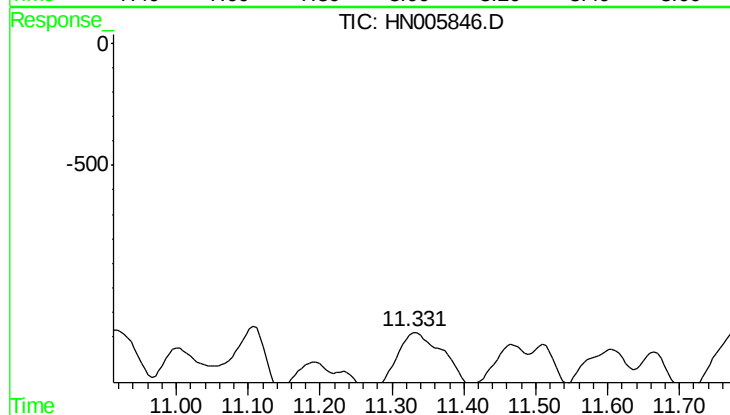


#14 2-Nitrotoluene

R.T.: 11.335 min
Delta R.T.: -0.056 min
Response: 13415
Conc: 92.92 ug/L

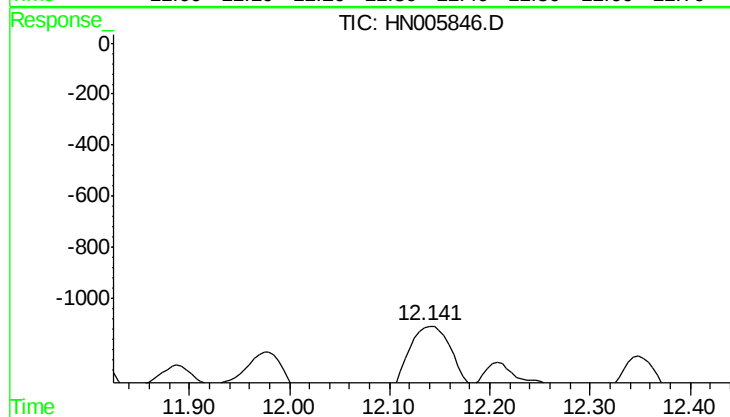

#15 4-Nitrotoluene

R.T.: 12.143 min
Delta R.T.: 0.009 min
Response: 17007
Conc: 15.50 ug/L

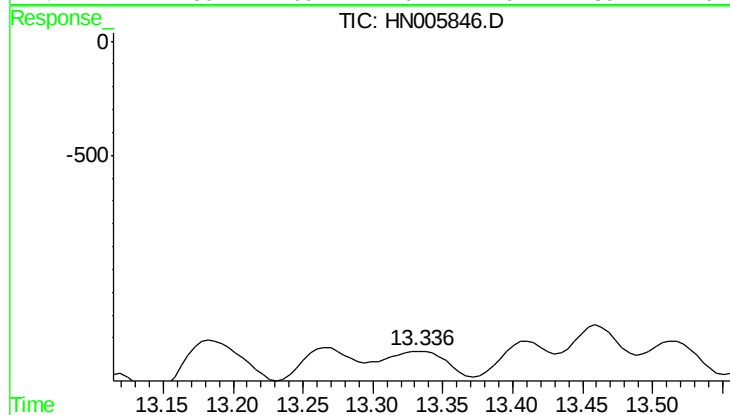

#16 3-Nitrotoluene

R.T.: 13.335 min
Delta R.T.: -0.024 min
Response: 7652
Conc: 8.17 ug/L