

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN052115\
 Data File : HN007380.D
 Signal(s) : vwd1A.ch
 Acq On : 21-May-2015, 19:41
 Operator : TP/IZ
 Sample : G2078-19
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 22 03:58:17 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN052115.M
 Quant Title :
 QLast Update : Fri May 22 03:56:44 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.330	2152951	502.246 ug/L
Target Compounds			
2) T HMX	0.890	2506442	548.251 ug/L
3) T RDX	1.710	1606772	286.677 ug/L
4) T 1,3,5-Trinitrobenzene	2.658	3567317	318.042 ug/L
5) T 1,3-Dinitrobenzene	3.532	4406350	256.203 ng/ml
6) T 3,5-Dinitroaniline	3.922	2067614	150.801 ug/L
7) T Nitrobenzene	4.715	6159371	593.199 ug/L
9) T 2,4,6-Trinitrotoluene	6.493	9081397	779.230 ug/L
10) T 2-Amino-4,6-dinitroto...	7.067	7194082	620.248 ug/L
11) T 4-Amino-2,6-dinitroto...	7.411	1322411	165.817 ug/L
12) T 2,4-Dinitrotoluene	8.122	15290243	923.343 ug/L
13) T 2,6-Dinitrotoluene	8.517	8322768	906.551 ug/L
14) T 2-Nitrotoluene	11.662	7133390	1080.096 ug/L
15) T 4-Nitrotoluene	12.411	5158182	955.754 ug/L
16) T 3-Nitrotoluene	13.663	4745410	680.201 ug/L
17) T PETN	18.605f	2963774	319.355 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN052115\
Data File : HN007380.D
Signal(s) : vwd1A.ch
Acq On : 21-May-2015, 19:41
Operator : TP/IZ
Sample : G2078-19
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 22 03:58:17 2015
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN052115.M
Quant Title :
QLast Update : Fri May 22 03:56:44 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 uL
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

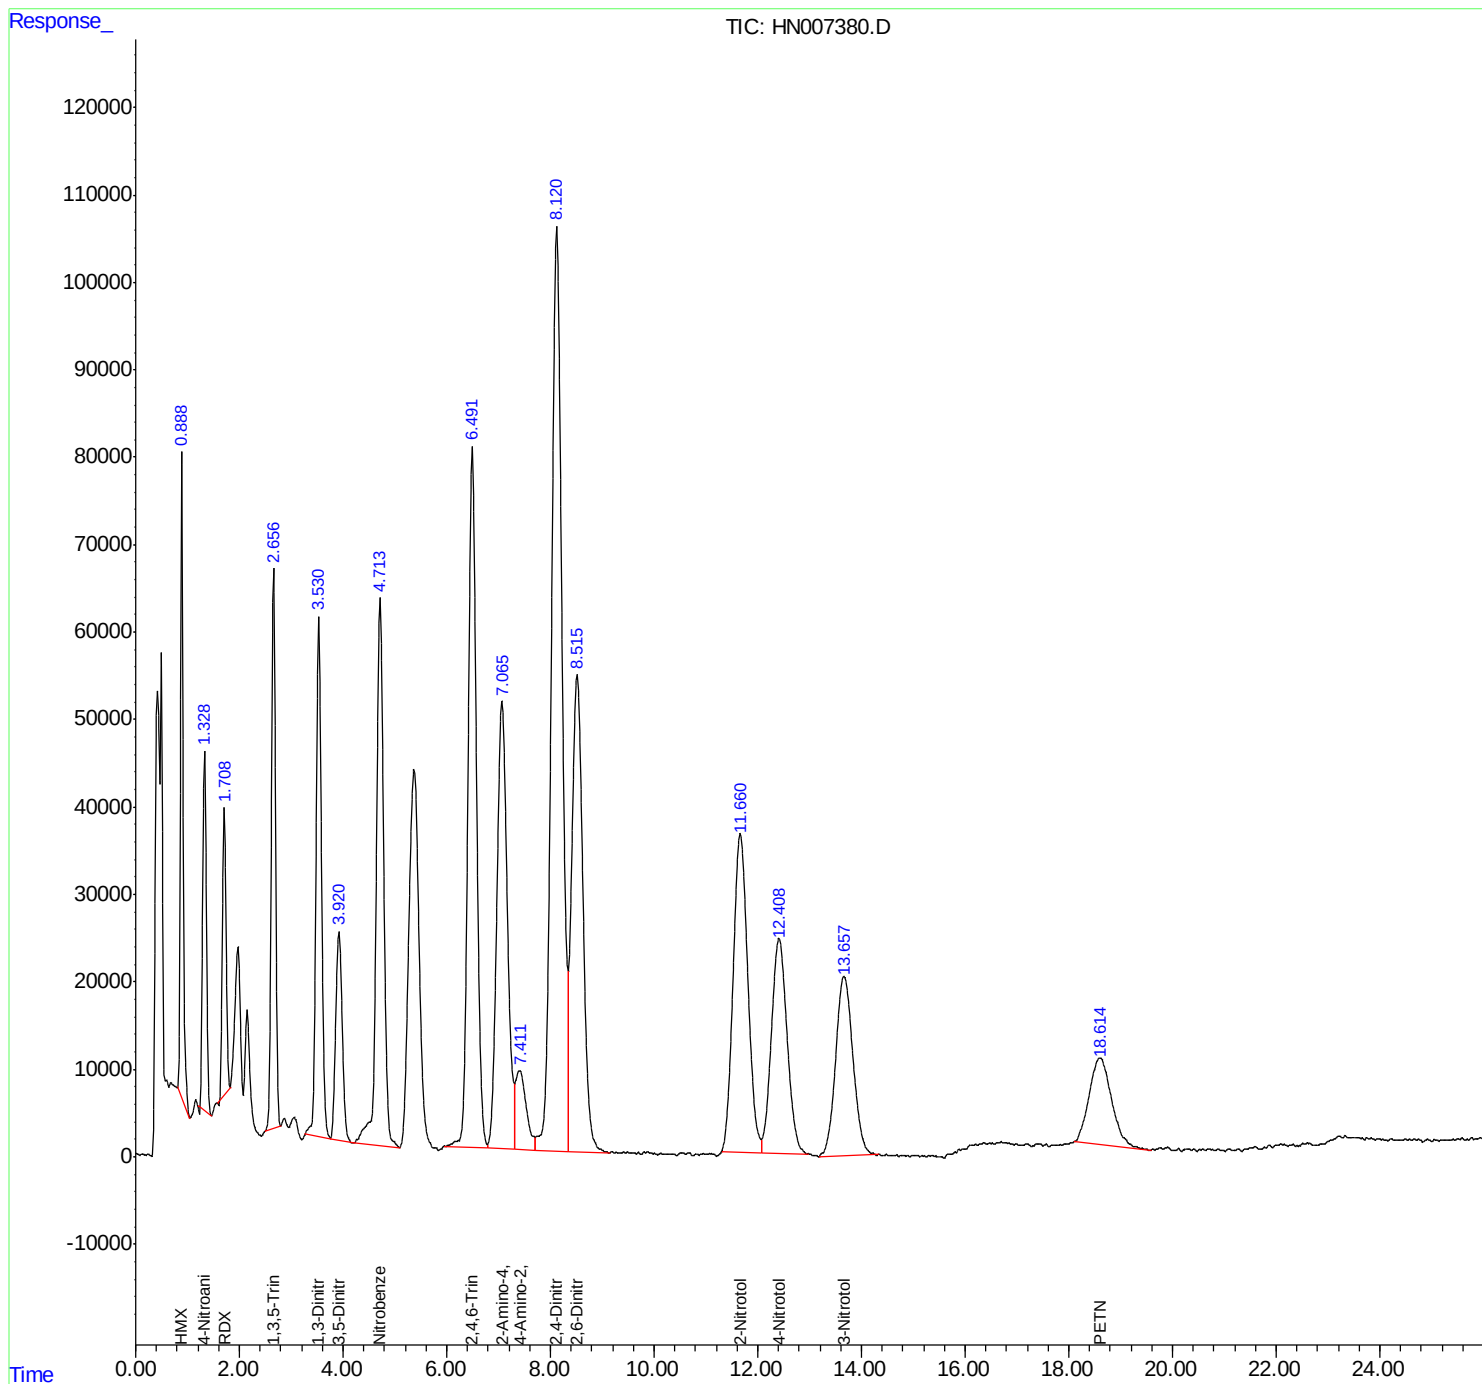


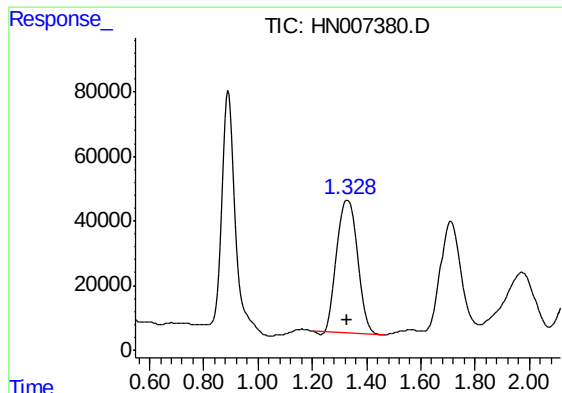

#1 4-Nitroaniline


R.T.: 1.330 min
Delta R.T.: 0.001 min
Response: 2152951
Conc: 502.25 ug/L

Instrument :
HPLC_N
ClientSampleId :

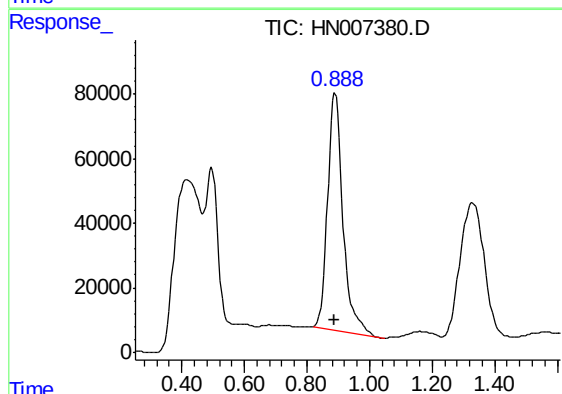


#2 HMX

R.T.: 0.890 min
Delta R.T.: 0.003 min
Response: 2506442
Conc: 548.25 ug/L

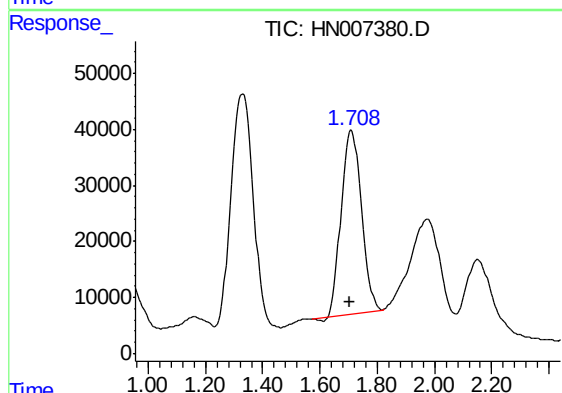


#3 RDX

R.T.: 1.710 min
Delta R.T.: 0.005 min
Response: 1606772
Conc: 286.68 ug/L

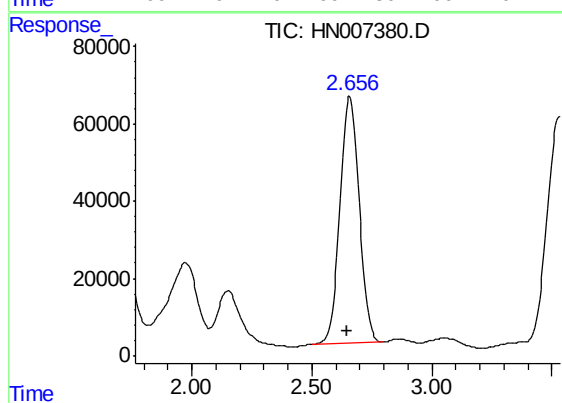

#4 1,3,5-Trinitrobenzene


R.T.: 2.658 min
Delta R.T.: 0.010 min
Response: 3567317
Conc: 318.04 ug/L

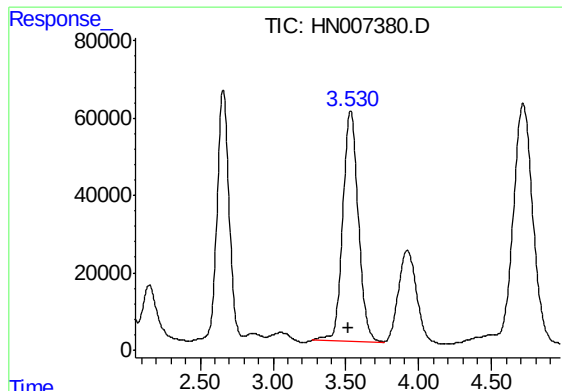

#5 1,3-Dinitrobenzene


R.T.: 3.532 min
Delta R.T.: 0.015 min
Response: 4406350
Conc: 256.20 ng/ml

Instrument :
HPLC_N
ClientSampleId :

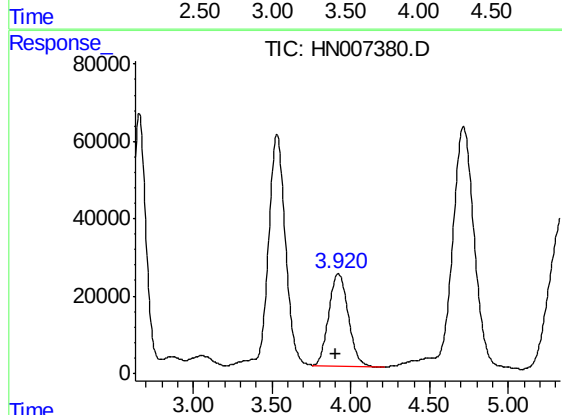


#6 3,5-Dinitroaniline

R.T.: 3.922 min
Delta R.T.: 0.017 min
Response: 2067614
Conc: 150.80 ug/L

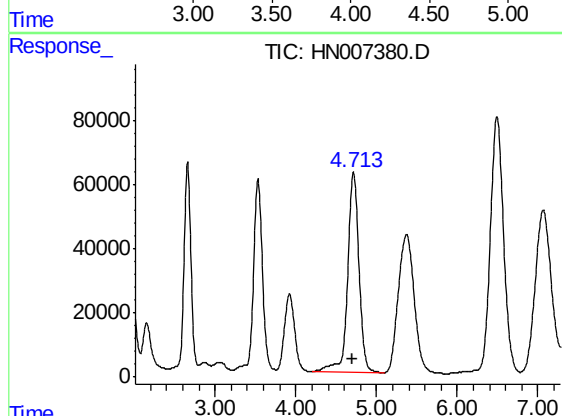


#7 Nitrobenzene

R.T.: 4.715 min
Delta R.T.: 0.020 min
Response: 6159371
Conc: 593.20 ug/L

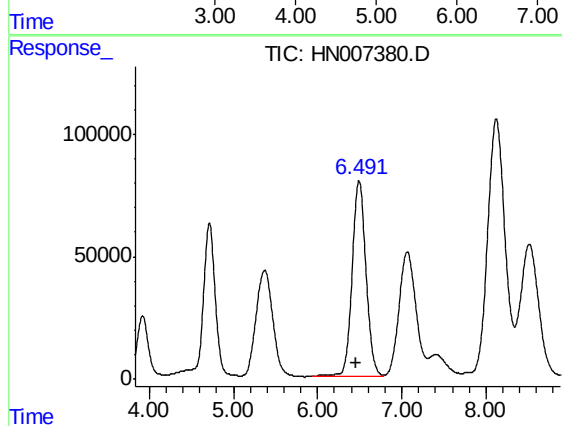

#9 2,4,6-Trinitrotoluene


R.T.: 6.493 min
Delta R.T.: 0.026 min
Response: 9081397
Conc: 779.23 ug/L

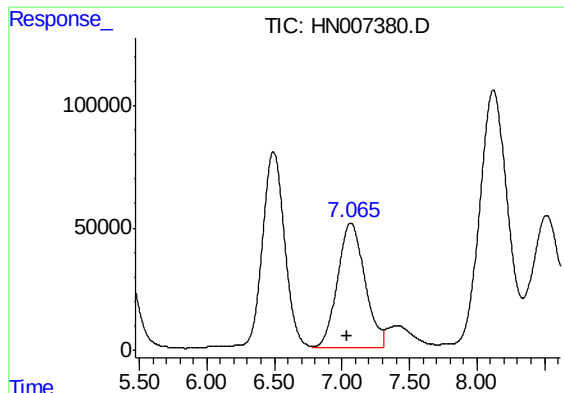

#10 2-Amino-4,6-dinitrotoluene


R.T.: 7.067 min
Delta R.T.: 0.029 min
Response: 7194082
Conc: 620.25 ug/L

Instrument :
HPLC_N
ClientSampleId :

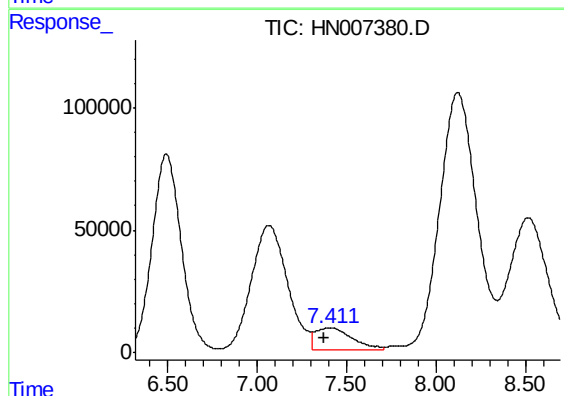


#11 4-Amino-2,6-dinitrotoluene

R.T.: 7.411 min
Delta R.T.: 0.032 min
Response: 1322411
Conc: 165.82 ug/L

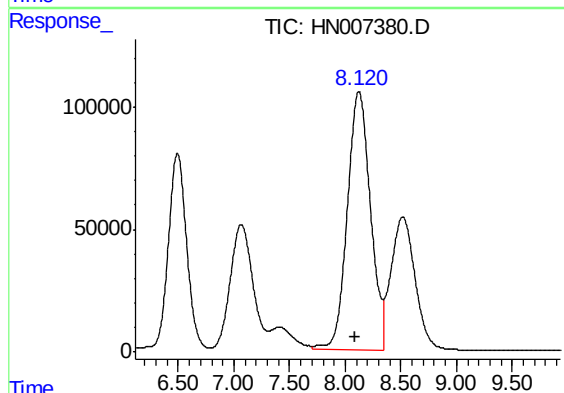


#12 2,4-Dinitrotoluene

R.T.: 8.122 min
Delta R.T.: 0.032 min
Response: 15290243
Conc: 923.34 ug/L

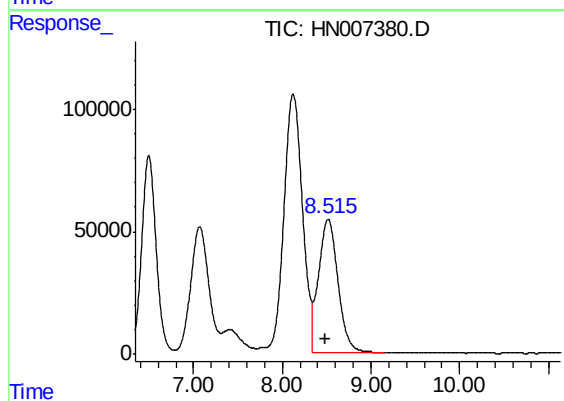

#13 2,6-Dinitrotoluene


R.T.: 8.517 min
Delta R.T.: 0.035 min
Response: 8322768
Conc: 906.55 ug/L

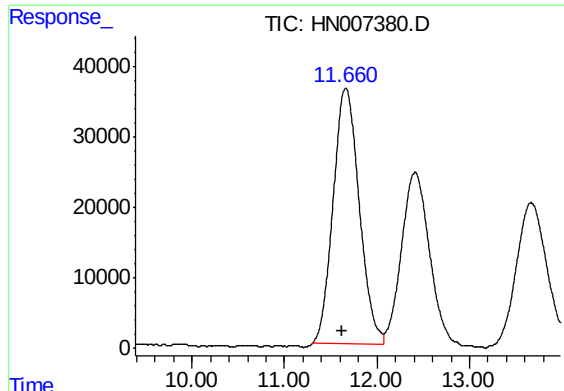

#14 2-Nitrotoluene


R.T.: 11.662 min
Delta R.T.: 0.045 min
Response: 7133390
Conc: 1080.10 ug/L

Instrument :
HPLC_N
ClientSampleId :

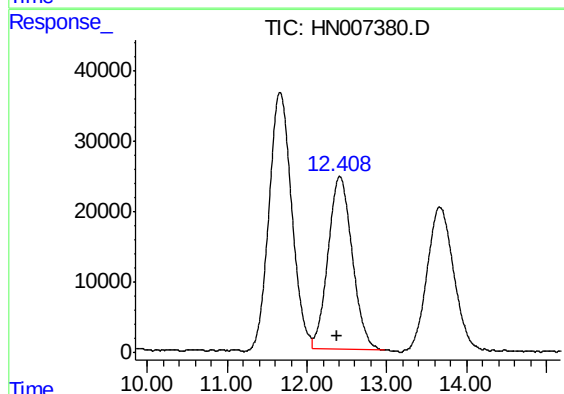


#15 4-Nitrotoluene

R.T.: 12.411 min
Delta R.T.: 0.039 min
Response: 5158182
Conc: 955.75 ug/L

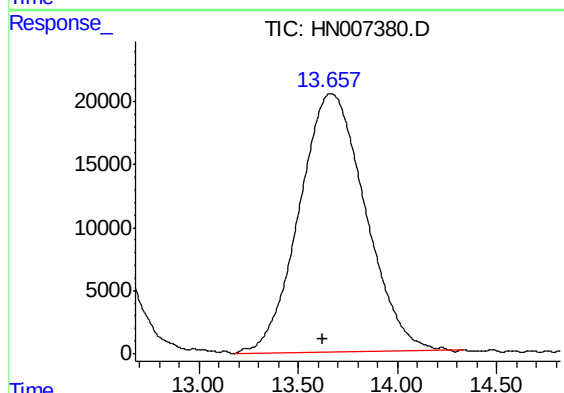

#16 3-Nitrotoluene

R.T.: 13.663 min
Delta R.T.: 0.042 min
Response: 4745410
Conc: 680.20 ug/L

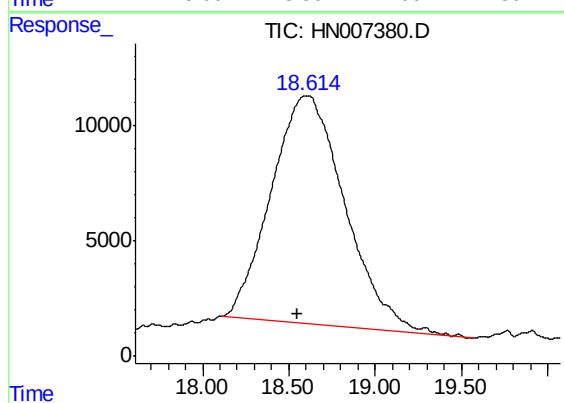

#17 PETN

R.T.: 18.605 min
Delta R.T.: 0.059 min
Response: 2963774
Conc: 319.36 ug/L